
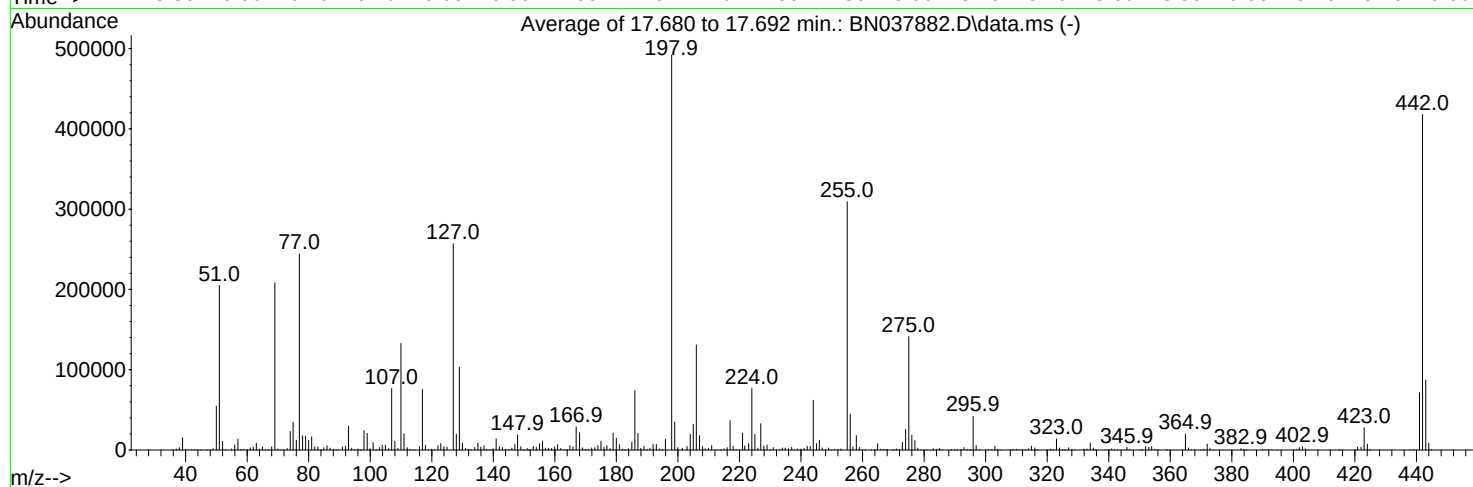


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092525\
Data File : BN037882.D
Acq On : 25 Sep 2025 10:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 24 11:00:01 2025

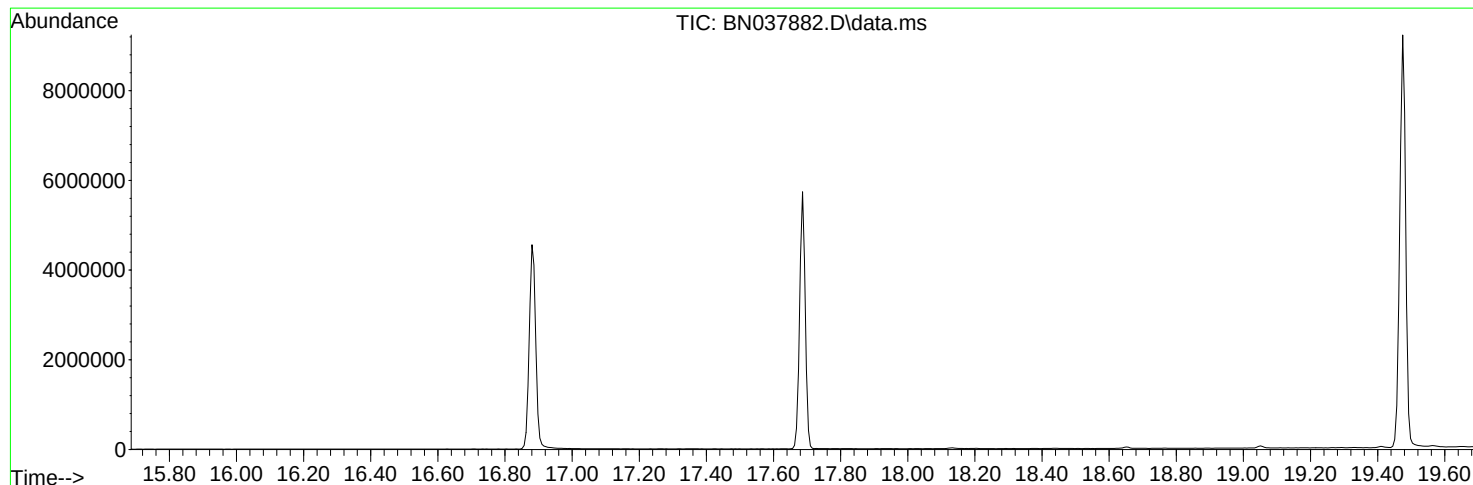




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	3756	PASS
69	69	100	100	100.0	208299	PASS
70	69	0.00	2	0.5	1072	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	491925	PASS
199	198	5	9	7.1	34720	PASS
365	198	1	100	4.0	19900	PASS
441	443	0.01	150	81.7	71253	PASS
442	442	100	100	100.0	417920	PASS
443	442	15	24	20.9	87163	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092525\
Data File : BN037882.D
Acq On : 25 Sep 2025 10:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 25 13:12:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 20 01:53:13 2025
Response via : Initial Calibration

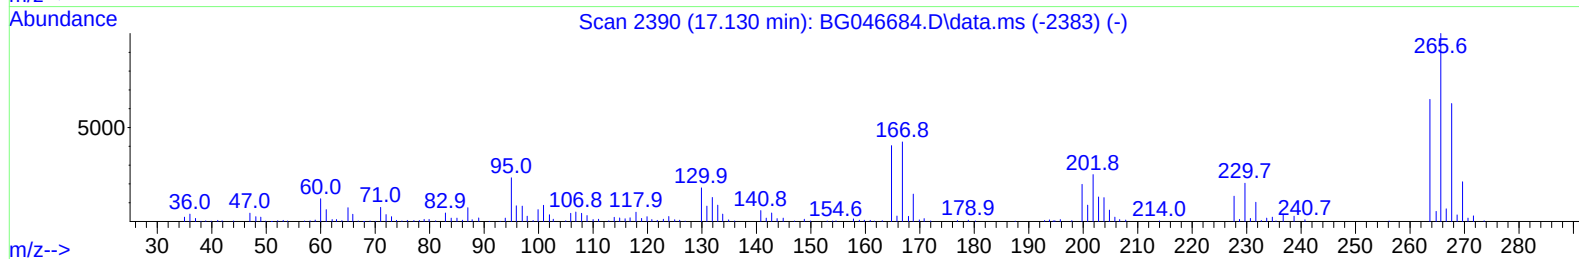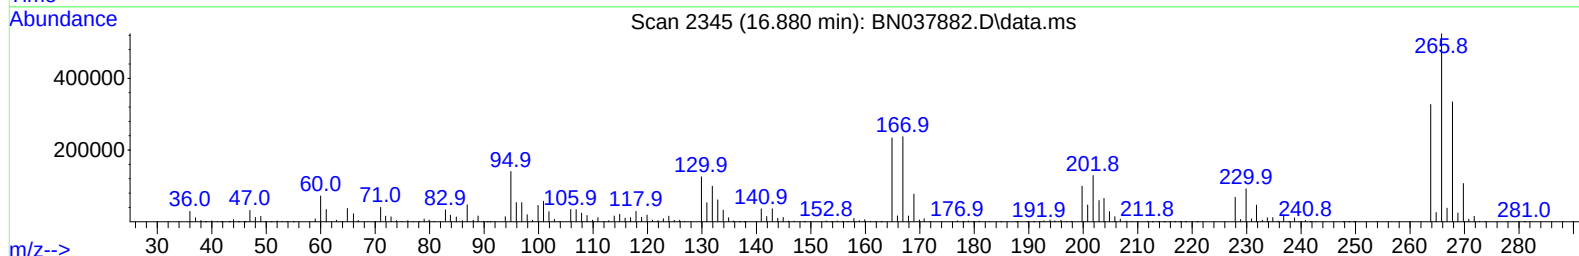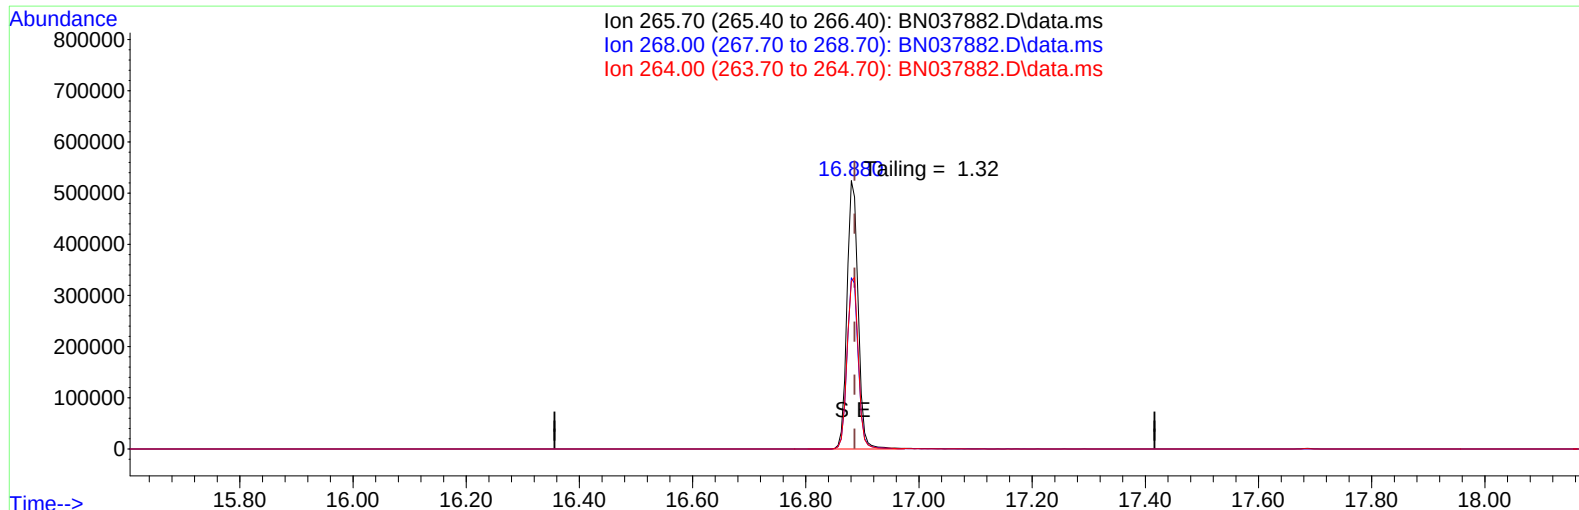

TIC: BN037882.D\data.ms

(70) Pentachlorophenol (C)

16.880min (-0.006) 31548.12 ng




response 718482

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.80
264.00	61.60	62.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092525\
Data File : BN037882.D
Acq On : 25 Sep 2025 10:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 25 13:12:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 20 01:53:13 2025
Response via : Initial Calibration

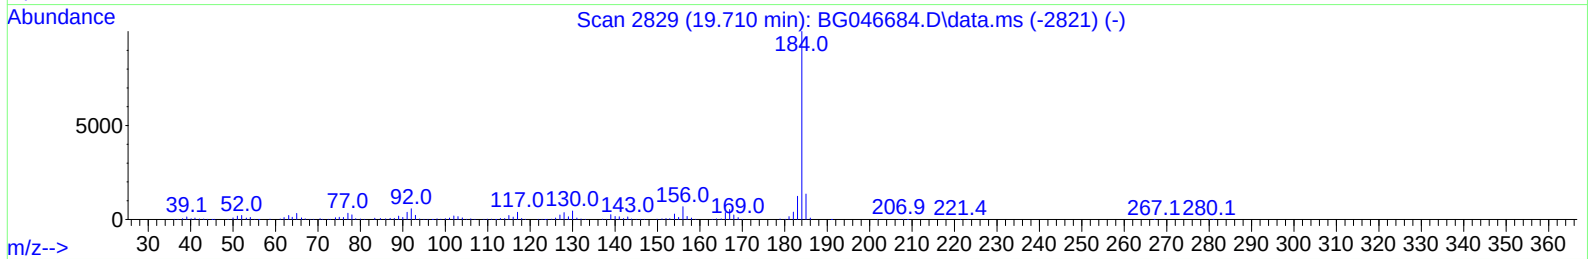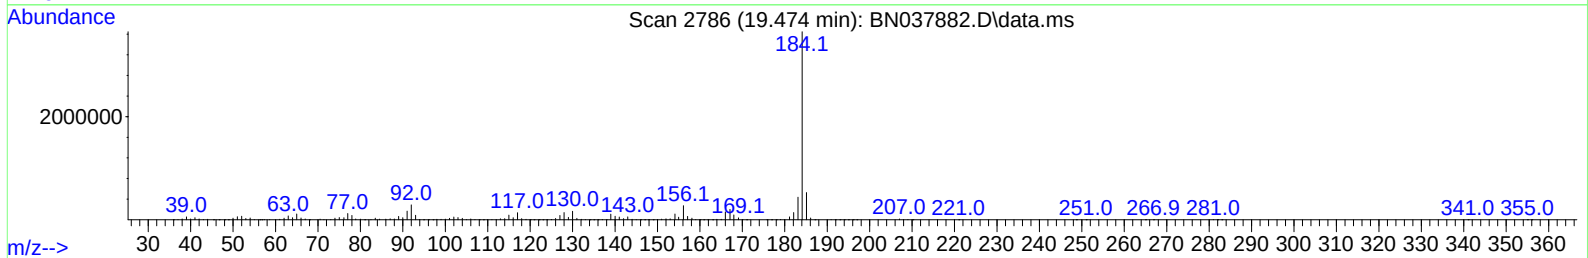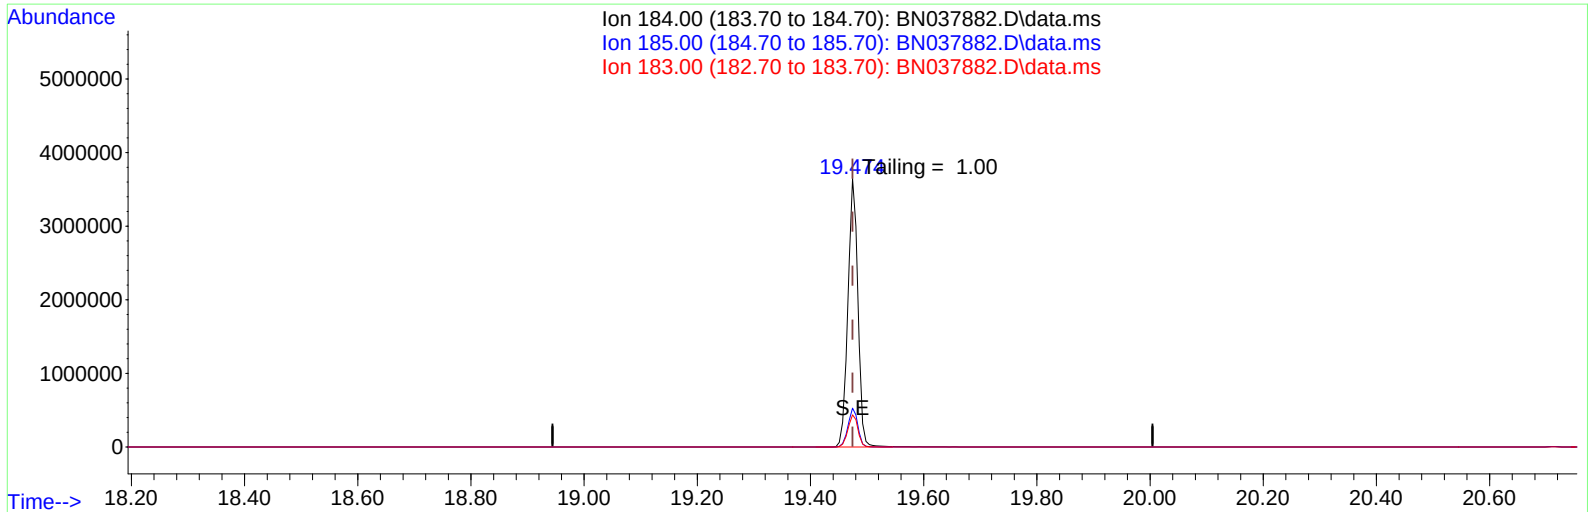

TIC: BN037882.D\data.ms

(77) Benzidine

19.474min (+ 0.000) 0.00 ng

response 4502688

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.51
183.00	13.20	12.03
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/25/2025	BNA_N	<u>BN037882.D</u>
Compound Name	Response	Retention Time
DDT	1891737	20.716
DDD	7741	20.327
DDE	257	19.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7998	1899735	0.42

Instrument :
BNA_N
ClientSampleId :
DFTPP