


Daily Analysis Runlog
J2 SCIENTIFIC PREPLINE GPC System GPC/2

Start Date: 9/23/25 End Date: 9/23/25 Analyst: EH Review By: RJ

STD. Name	STD REF. #	Check Standard	Data File and Date	Reagent		
GPC Calibration	EP 2638	BNA Blank Check		Methylene Chloride		
Pest Check Std	PP 21421 10.0 mL	Pesticide Blank Check		Reagent Reference #		
PCB Check Std	NA	Pesticide Check		E-3973		
CALIB. DATE:	9/23/25	PCB Check				
Port #	Sample ID	Volume Collected	GPC Date	BNA	PEST	Comments
1	Column cleaned		9/23/25	-	-	
2	GPC Calibration		1	-	-	
1	Q-3143-10 Pest SW	85	9/23/25	-	-	Q 3143 Ant Pest.
2	Q-3143-09 Pest SW	85	1	-	-	
3	Q-3143-08 Pest SW	116	1	-	-	
				</		

Doc Control # A3041250

152

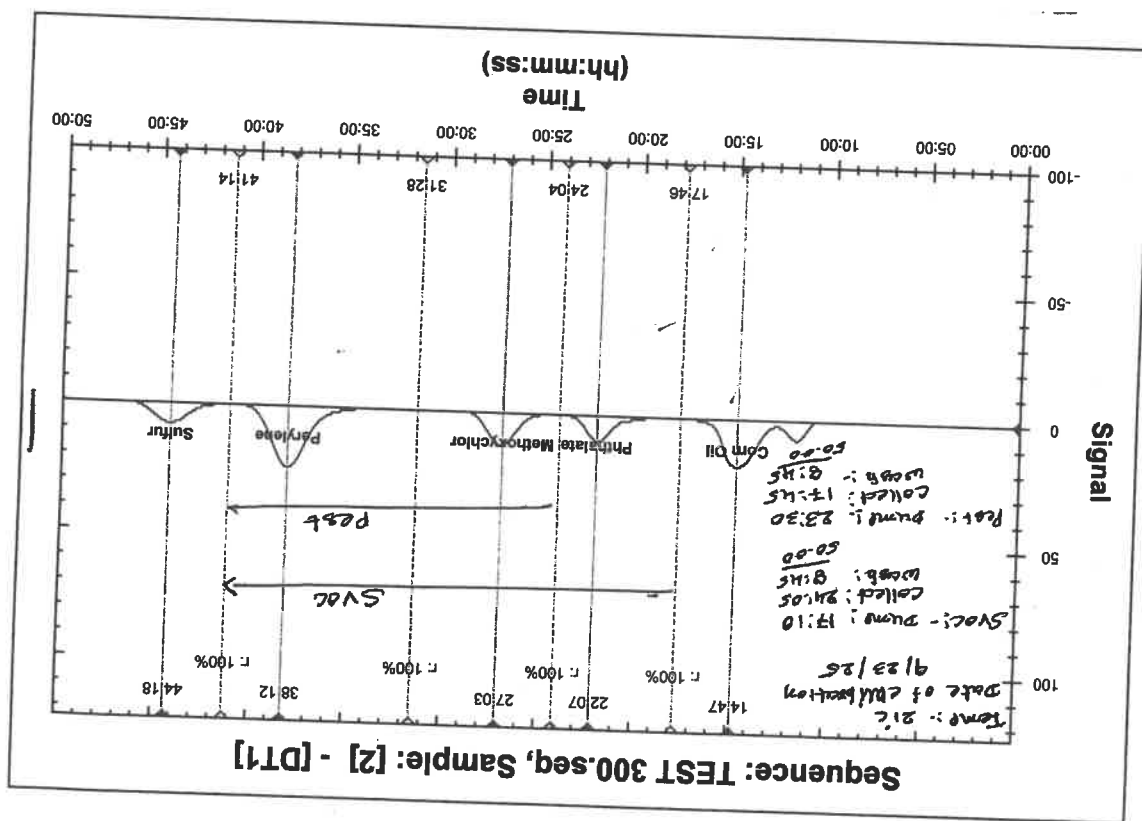

151

Doc Control # A3041250