

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092225\
 Data File : VN087915.D
 Acq On : 22 Sep 2025 12:26
 Operator : JC\MD
 Sample : VN0922WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0922WBL01

Quant Time: Sep 23 04:51:20 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N090425W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri Sep 05 03:29:53 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	7.794	128	53463	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	9.082	114	267356	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.841	117	245968	30.000	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.559	65	131878	28.876	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	96.267%
60) 4-Bromofluorobenzene	12.829	95	100591	25.434	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	84.767%
63) Toluene-d8	10.547	98	329123	28.772	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	95.900%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092225\
Data File : VN087915.D
Acq On : 22 Sep 2025 12:26
Operator : JC\MD
Sample : VN0922WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0922WBL01

Quant Time: Sep 23 04:51:20 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N090425W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri Sep 05 03:29:53 2025
Response via : Initial Calibration




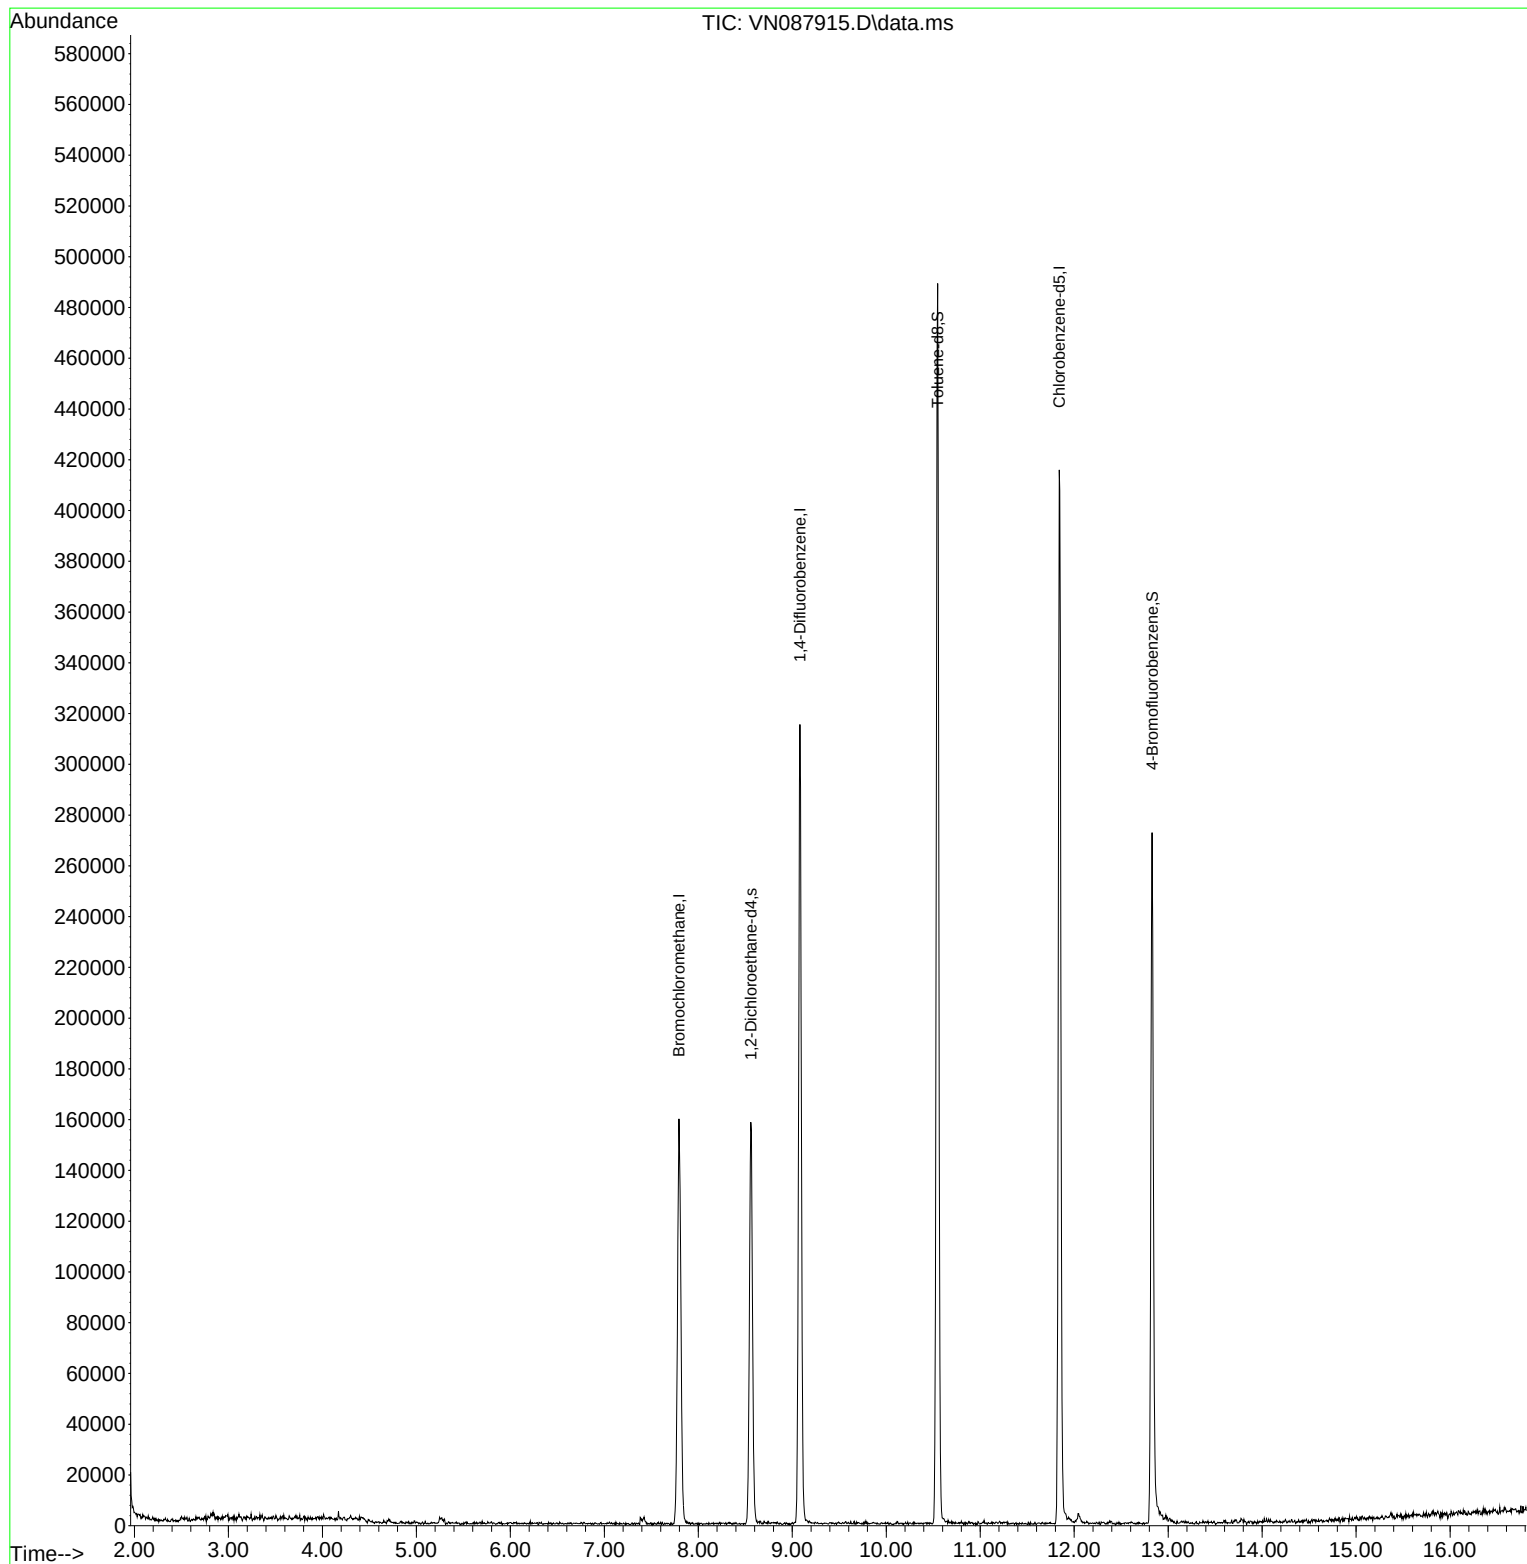


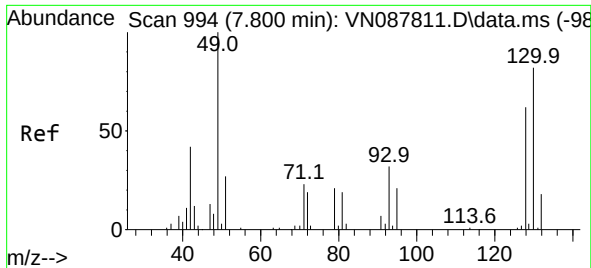

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.794 min Scan# 994
Delta R.T. 0.000 min
Lab File: VN087915.D
Acq: 22 Sep 2025 12:26




Instrument :
MSVOA_N
ClientSampleId :
VN0922WBL01


Tgt Ion:128 Resp: 53463
Ion Ratio Lower Upper
128 100
49 173.1 0.0 464.3
130 136.5 0.0 300.5

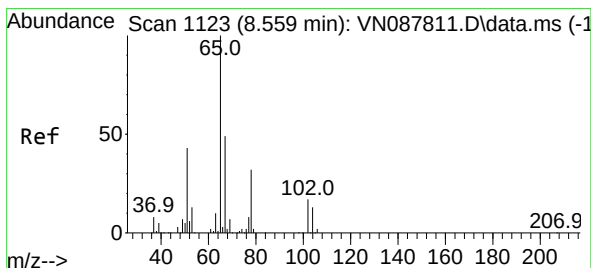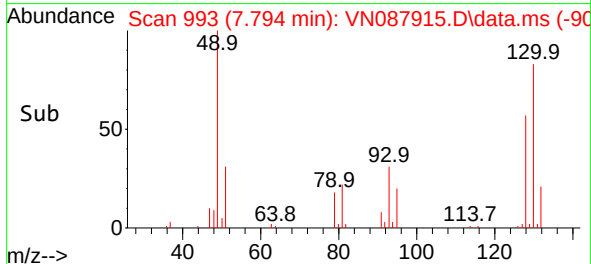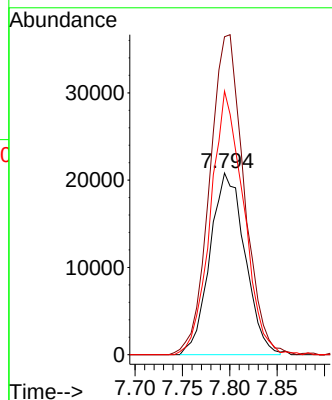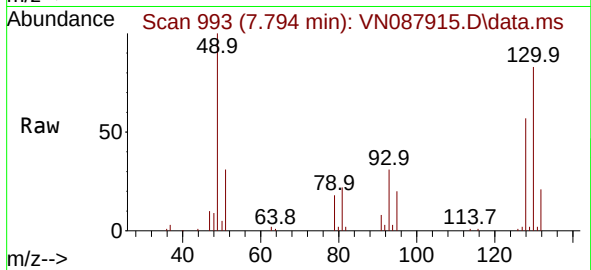

#27
1,2-Dichloroethane-d4
Concen: 28.876 ug/l
RT: 8.559 min Scan# 1123
Delta R.T. -0.000 min
Lab File: VN087915.D
Acq: 22 Sep 2025 12:26

Tgt Ion: 65 Resp: 131878
Ion Ratio Lower Upper
65 100
67 49.9 39.6 59.4

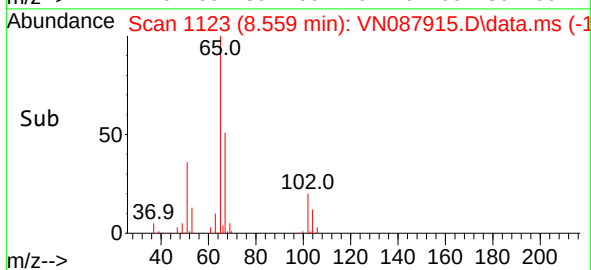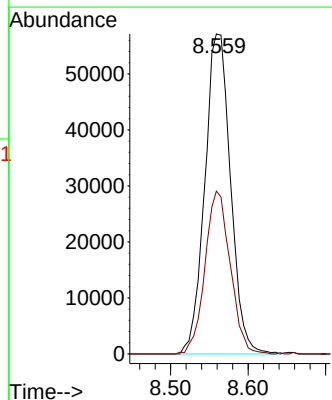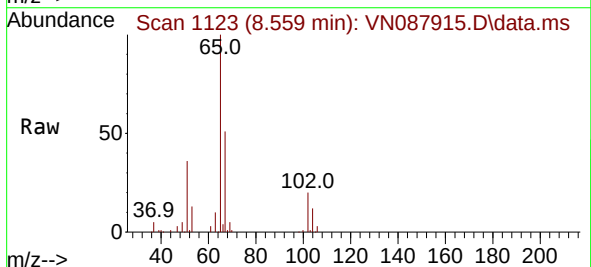

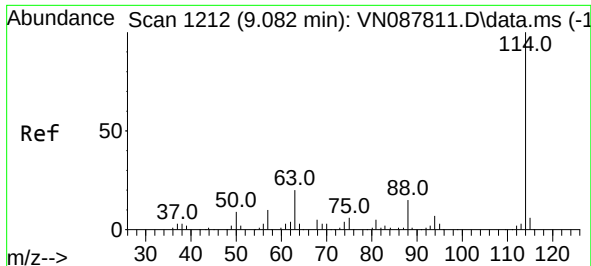

#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 9.082 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN087915.D

Acq: 22 Sep 2025 12:26

Instrument :

MSVOA_N

ClientSampleId :

VN0922WBL01





Tgt Ion:114 Resp: 267356

Ion Ratio Lower Upper

114 100

63 20.3 18.3 27.5

88 14.8 12.4 18.6

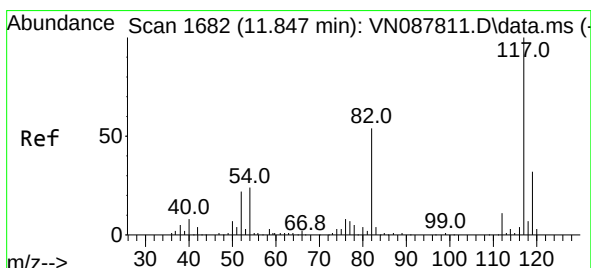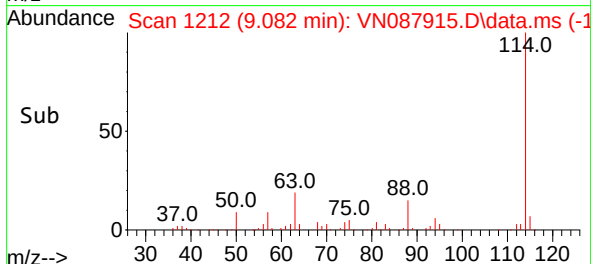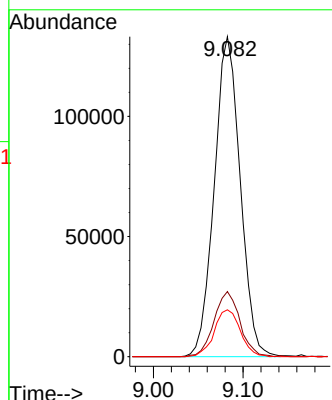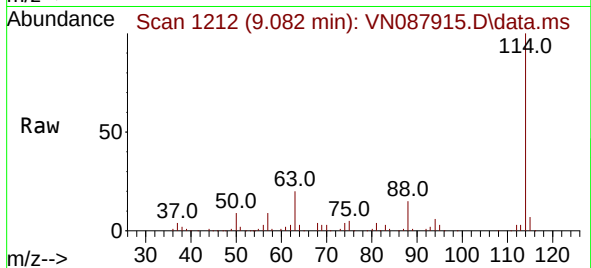

#57

Chlorobenzene-d5

Concen: 30.000 ug/l

RT: 11.841 min Scan# 1681

Delta R.T. -0.000 min

Lab File: VN087915.D

Acq: 22 Sep 2025 12:26




Tgt Ion:117 Resp: 245968


Ion Ratio Lower Upper

117 100

82 54.2 45.9 68.9

119 31.8 25.3 37.9


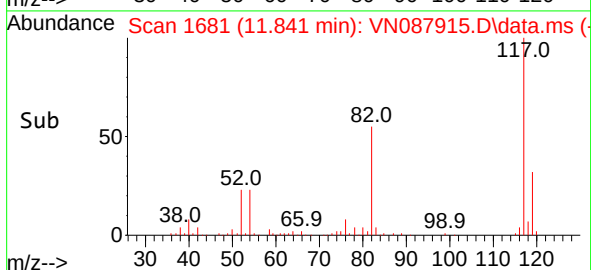
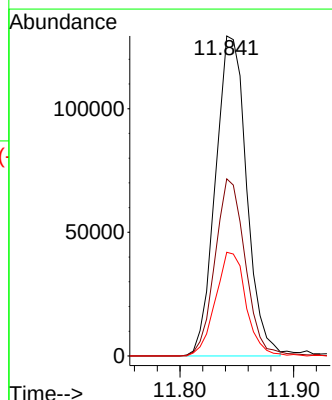
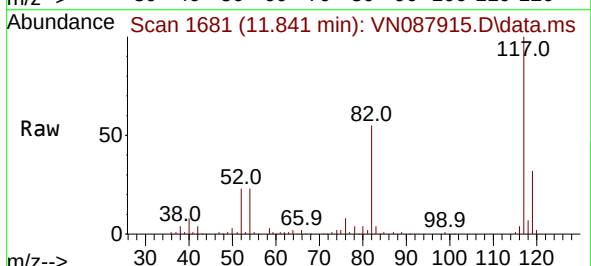


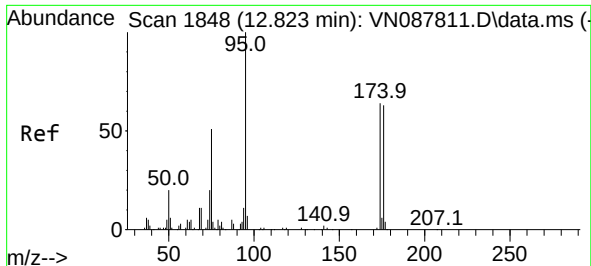

#60
4-Bromofluorobenzene
Concen: 25.434 ug/l
RT: 12.829 min Scan# 1849
Delta R.T. -0.000 min
Lab File: VN087915.D
Acq: 22 Sep 2025 12:26

Instrument :
MSVOA_N
ClientSampleId :
VN0922WBL01

Tgt Ion: 95 Resp: 100591
Ion Ratio Lower Upper
95 100
174 75.8 55.4 83.0
176 69.3 51.5 77.3

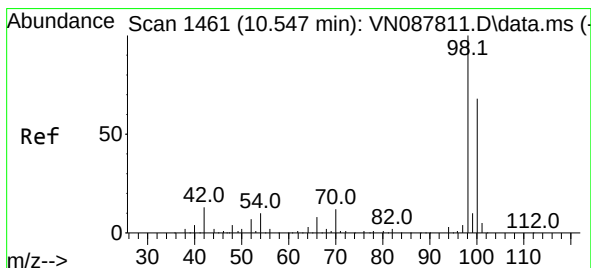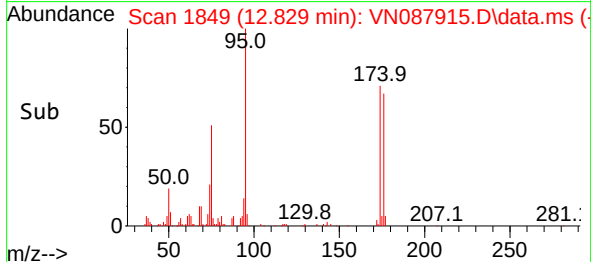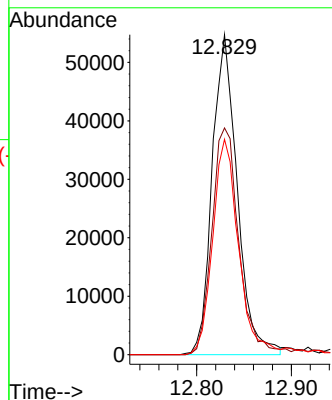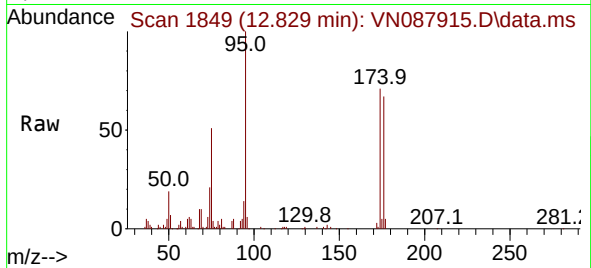

#63
Toluene-d8
Concen: 28.772 ug/l
RT: 10.547 min Scan# 1461
Delta R.T. -0.000 min
Lab File: VN087915.D
Acq: 22 Sep 2025 12:26

Tgt Ion: 98 Resp: 329123
Ion Ratio Lower Upper
98 100
100 65.1 50.6 76.0

