
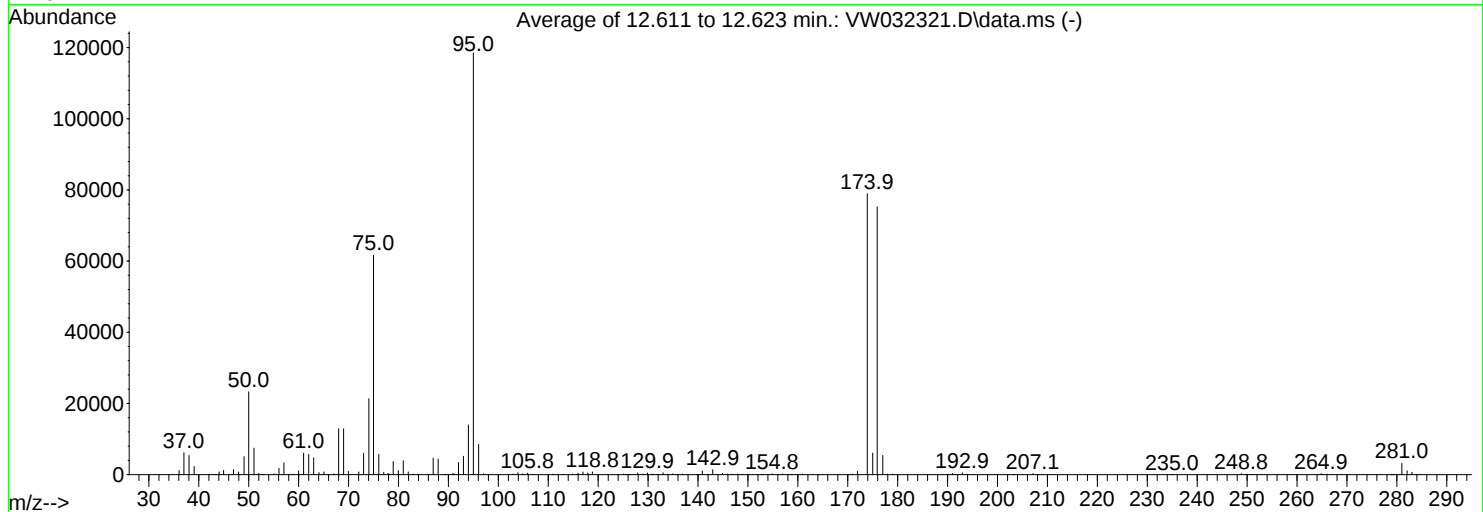


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100225\
Data File : VW032321.D
Acq On : 02 Oct 2025 09:19
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5mL/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W100125S.M
Title : SW846 8260
Last Update : Thu Oct 02 21:24:16 2025

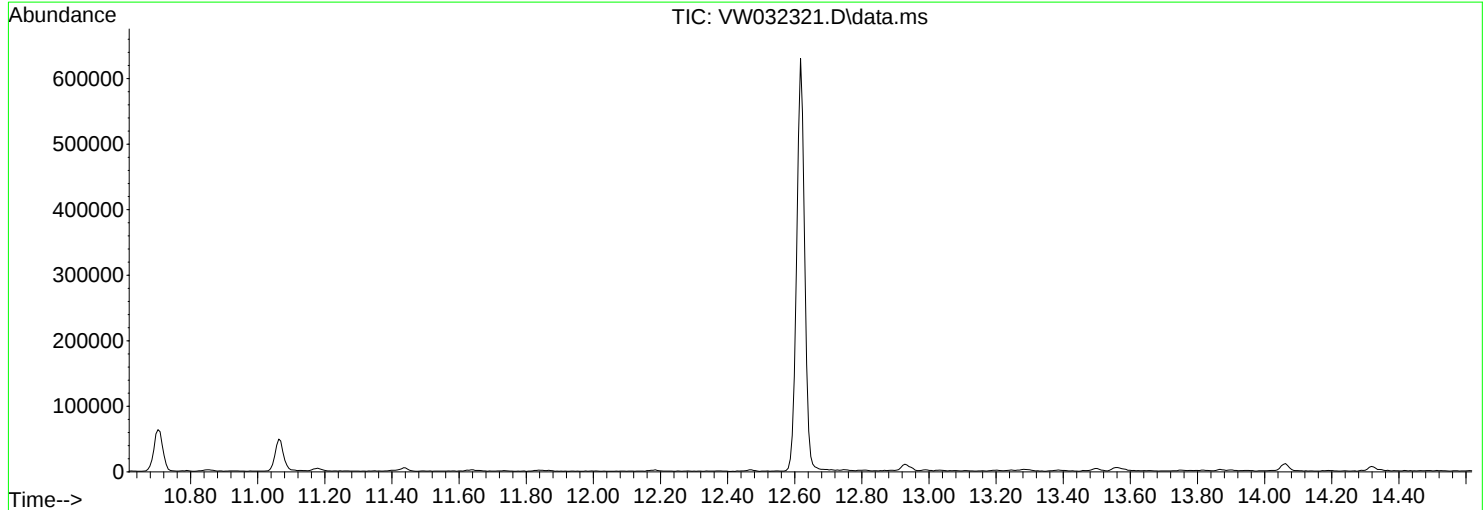

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	23304	PASS
75	95	30	60	52.1	61706	PASS
95	95	100	100	100.0	118515	PASS
96	95	5	9	7.2	8499	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	66.6	78939	PASS
175	174	5	9	7.7	6079	PASS
176	174	95	101	95.3	75219	PASS
177	176	5	9	7.2	5404	PASS