


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL092425\
Data File : VL043000.D
Acq On : 24 Sep 2025 08:20
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL092225AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Sep 23 02:39:16 2025

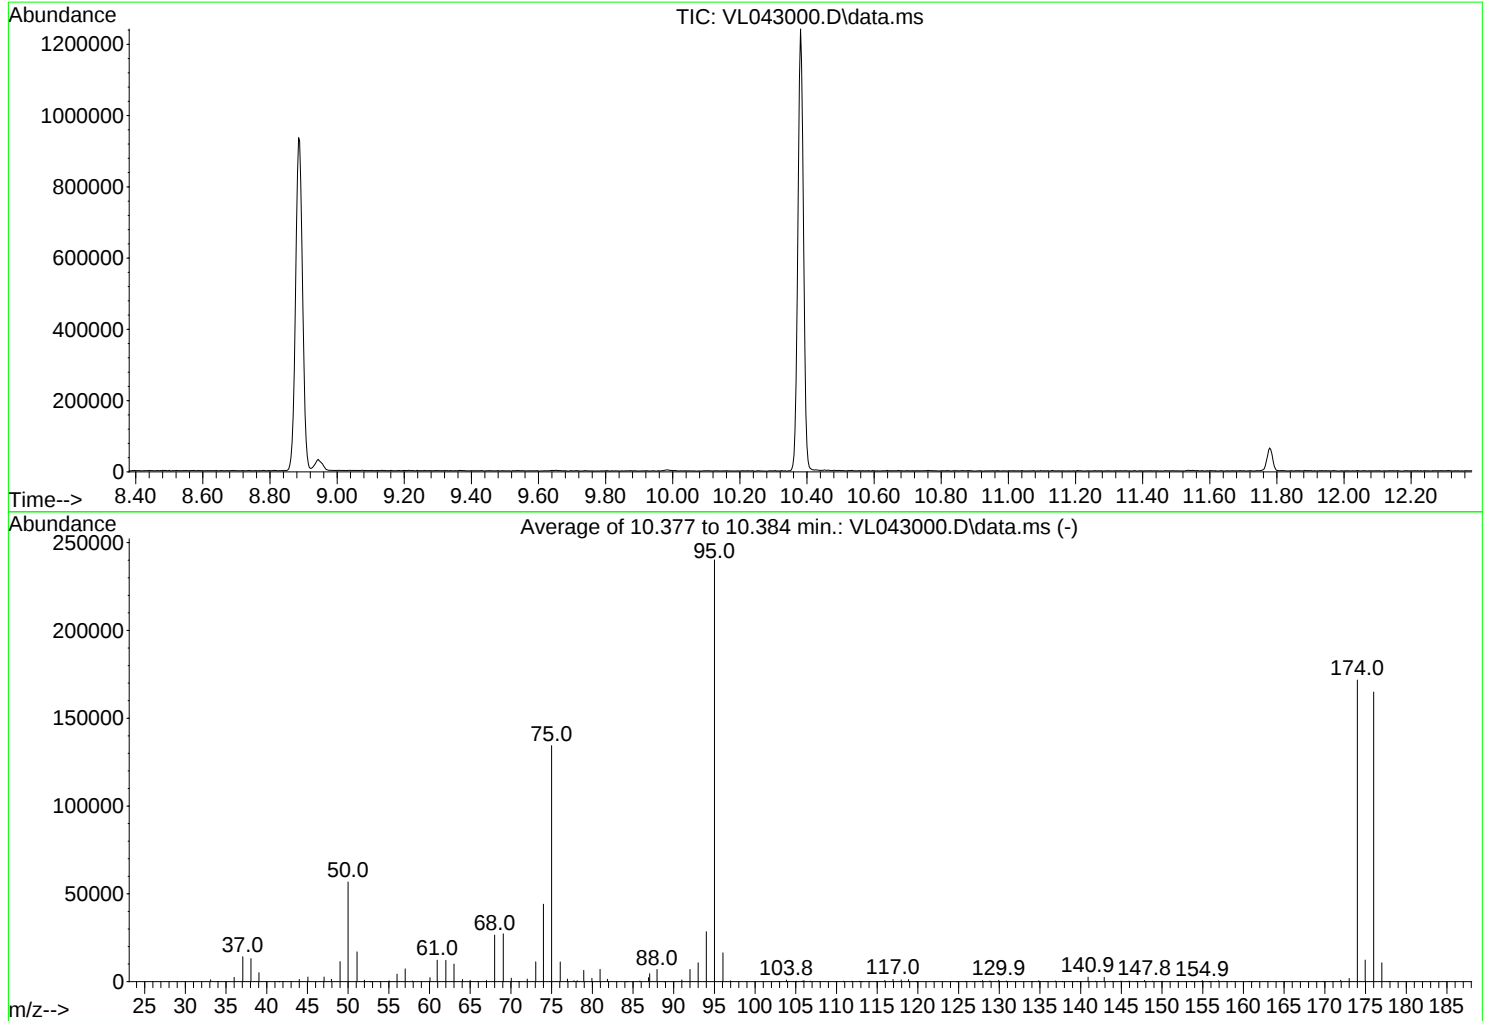

AutoFind: Scans 3179, 3180, 3181; Background Corrected with Scan 3165

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.6	56740	PASS
75	95	30	66	56.0	134448	PASS
95	95	100	100	100.0	240213	PASS
96	95	5	9	6.8	16381	PASS
173	174	0.00	2	1.1	1850	PASS
174	95	50	120	71.5	171733	PASS
175	174	4	9	7.2	12288	PASS
176	174	93	101	96.0	164928	PASS
177	176	5	9	6.5	10768	PASS

Average of 10.377 to 10.384 min.: VL043000.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	1070	45.05	2678	55.05	506	67.00	621
33.95	106	46.00	220	56.00	4297	68.00	2652
36.00	2424	47.05	2644	57.00	7342	69.05	2726
37.05	14192	47.95	1359	57.90	409	70.05	205
38.05	13095	49.00	11393	60.05	2318	70.90	23
39.05	5102	50.00	56740	60.95	12233	72.00	1464
39.95	221	51.10	16989	62.00	12126	73.05	11342
41.50	21	52.00	804	63.00	10000	74.00	44080
42.00	88	52.70	20	64.05	1191	75.00	134448
43.00	204	52.90	76	65.00	706	76.05	11210
44.00	1274	53.85	63	65.90	88	76.95	1482

Average of 10.377 to 10.384 min.: VL043000.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.75	513	87.95	6913	104.70	95	114.90	183
78.15	541	88.80	40	105.05	237	115.95	768
78.95	6431	91.00	1028	105.80	384	116.95	1306
79.95	1959	92.00	6913	106.00	652	117.95	1000
80.95	7004	93.00	10729	106.80	309	118.85	1189
81.85	1412	94.00	28477	107.90	18	119.80	33
82.95	188	95.00	240213	109.90	109	124.05	196
84.20	19	96.05	16381	110.85	246	124.75	36
85.85	340	96.95	419	111.90	279	125.85	173
86.90	2304	102.90	94	112.85	250	126.75	60
87.05	4509	103.85	954	113.10	45	127.70	207

Average of 10.377 to 10.384 min.: VL043000.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
127.95	668	139.90	29	150.00	313	160.70	174
128.85	434	140.90	2596	152.00	181	161.00	36
129.95	801	141.85	296	152.95	139	168.90	17
130.90	350	142.90	2472	153.60	54	169.80	98
134.00	20	143.90	165	153.95	58	170.95	97
134.85	515	144.20	74	154.95	614	171.95	803
135.85	64	144.95	409	155.75	40	173.00	1850
136.90	371	145.95	389	156.95	584	174.00	171733
137.70	20	146.85	167	157.90	61	174.95	12288
139.05	81	147.85	743	158.55	102	176.00	164928
139.60	90	148.85	237	158.95	108	177.00	10768

Average of 10.377 to 10.384 min.: VL043000.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
177.80	97						
178.05	179						

Instrument :

MSVOA_L

ClientSampleId :

BFB