

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092225\
 Data File : P0113917.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2025 16:48
 Operator : YP/AJ
 Sample : Q3155-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/23/2025
 Supervised By :mohammad ahmed 09/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 01:42:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:49:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.650	188.7E6	107.5E6	21.397	20.134
2) SA Decachlor...	8.669	8.612	109.2E6	39085020	16.315m	18.721

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO092225\
Data File : PO113917.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2025 16:48
Operator : YP/AJ
Sample : Q3155-03
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_0
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/23/2025
Supervised By :mohammad ahmed 09/24/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 01:42:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

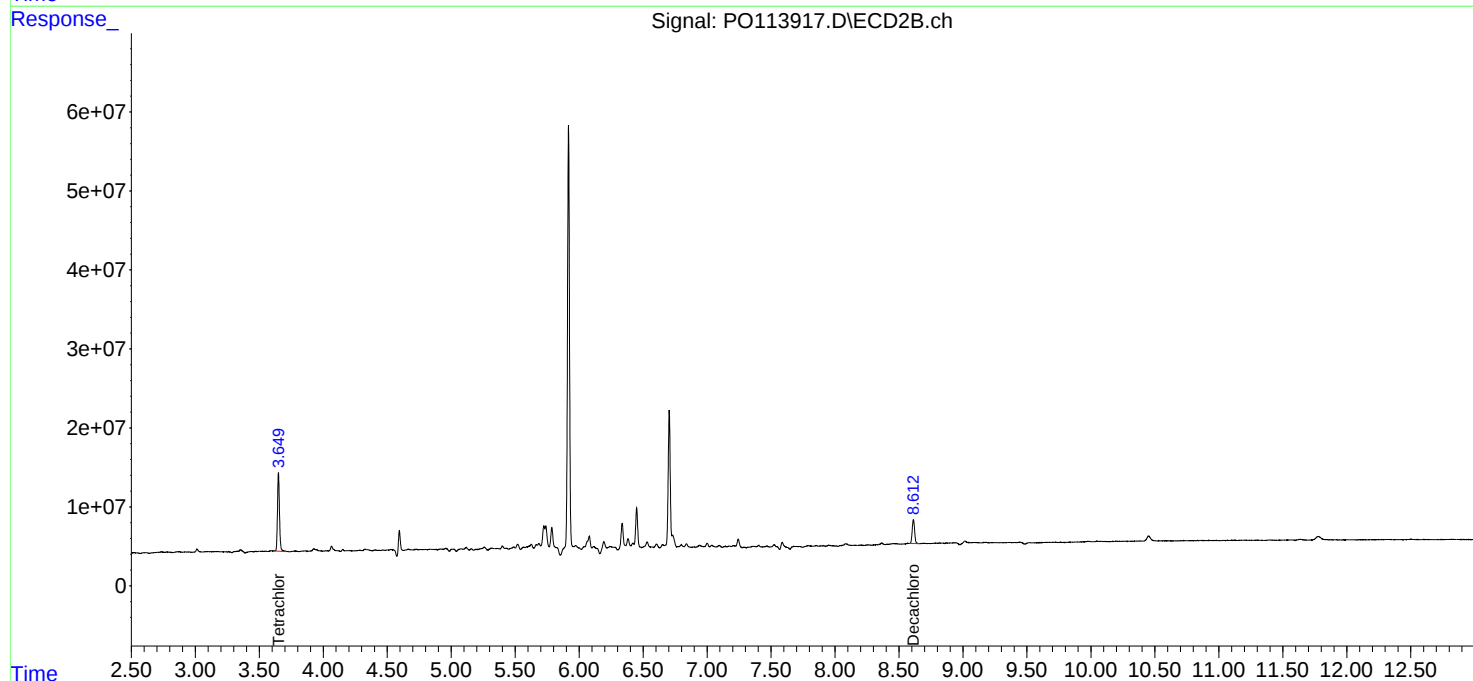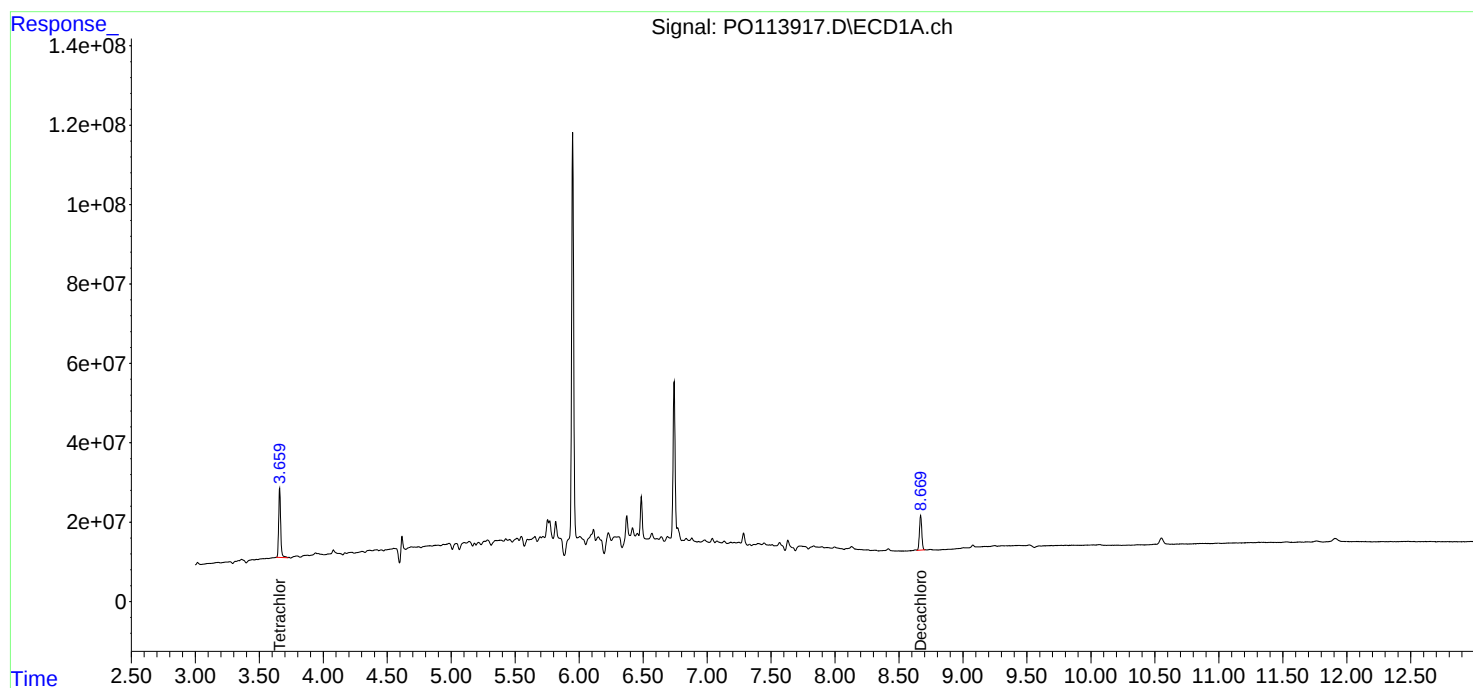

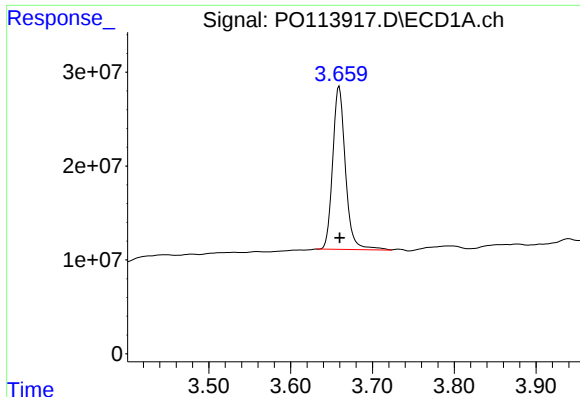


#1 Tetrachloro-m-xylene

R.T.: 3.659 min
Delta R.T.: 0.000 min
Response: 188712849
Conc: 21.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/23/2025
Supervised By :mohammad ahmed 09/24/2025

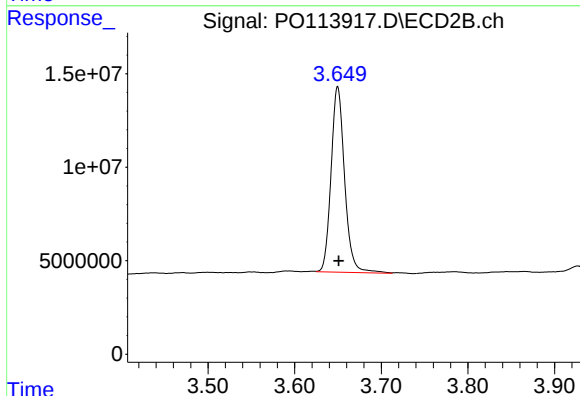


#1 Tetrachloro-m-xylene

R.T.: 3.650 min
Delta R.T.: -0.001 min
Response: 107533912
Conc: 20.13 ng/ml

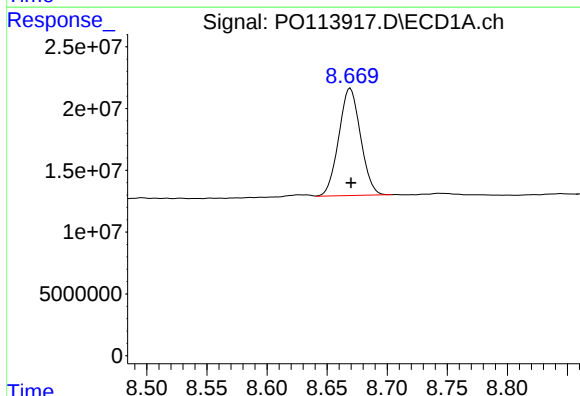

#2 Decachlorobiphenyl

R.T.: 8.669 min
Delta R.T.: -0.001 min
Response: 109150613
Conc: 16.31 ng/ml m

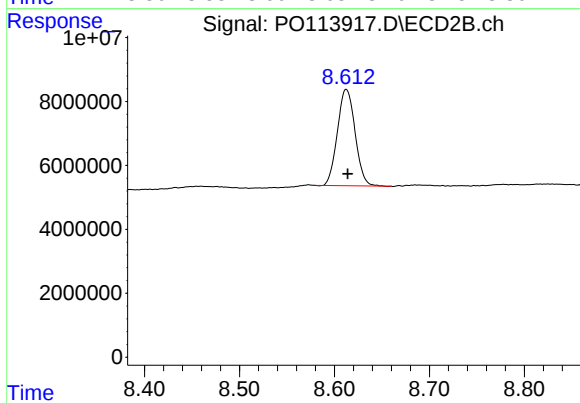

#2 Decachlorobiphenyl

R.T.: 8.612 min
Delta R.T.: -0.001 min
Response: 39085020
Conc: 18.72 ng/ml