

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092525\
 Data File : BN037898.D
 Acq On : 25 Sep 2025 20:41
 Operator : RC/JU
 Sample : Q3156-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE132D2-20250918

Quant Time: Sep 25 23:50:56 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092325.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 24 11:00:01 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.818	152	7601	0.400	ng	0.00
7) Naphthalene-d8	10.626	136	21427	0.400	ng	0.00
13) Acenaphthene-d10	14.473	164	11165	0.400	ng	0.00
19) Phenanthrene-d10	17.223	188	23219	0.400	ng	0.00
29) Chrysene-d12	21.402	240	17732	0.400	ng	0.00
35) Perylene-d12	23.730	264	14515	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.384	112	2798	0.161	ng	0.00
5) Phenol-d6	6.973	99	2293	0.101	ng	0.00
8) Nitrobenzene-d5	8.971	82	5900	0.361	ng	0.00
11) 2-Methylnaphthalene-d10	12.217	152	9997	0.336	ng	0.00
14) 2,4,6-Tribromophenol	15.969	330	1536	0.363	ng	0.00
15) 2-Fluorobiphenyl	13.094	172	15765	0.345	ng	0.00
27) Fluoranthene-d10	19.252	212	23968	0.410	ng	0.00
31) Terphenyl-d14	19.852	244	17629	0.499	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.290	88	47437	6.148	ng	98
34) Bis(2-ethylhexyl)phtha...	21.321	149	1516	0.062	ng	# 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092525\
Data File : BN037898.D
Acq On : 25 Sep 2025 20:41
Operator : RC/JU
Sample : Q3156-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE132D2-20250918


Quant Time: Sep 25 23:50:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 24 11:00:01 2025
Response via : Initial Calibration

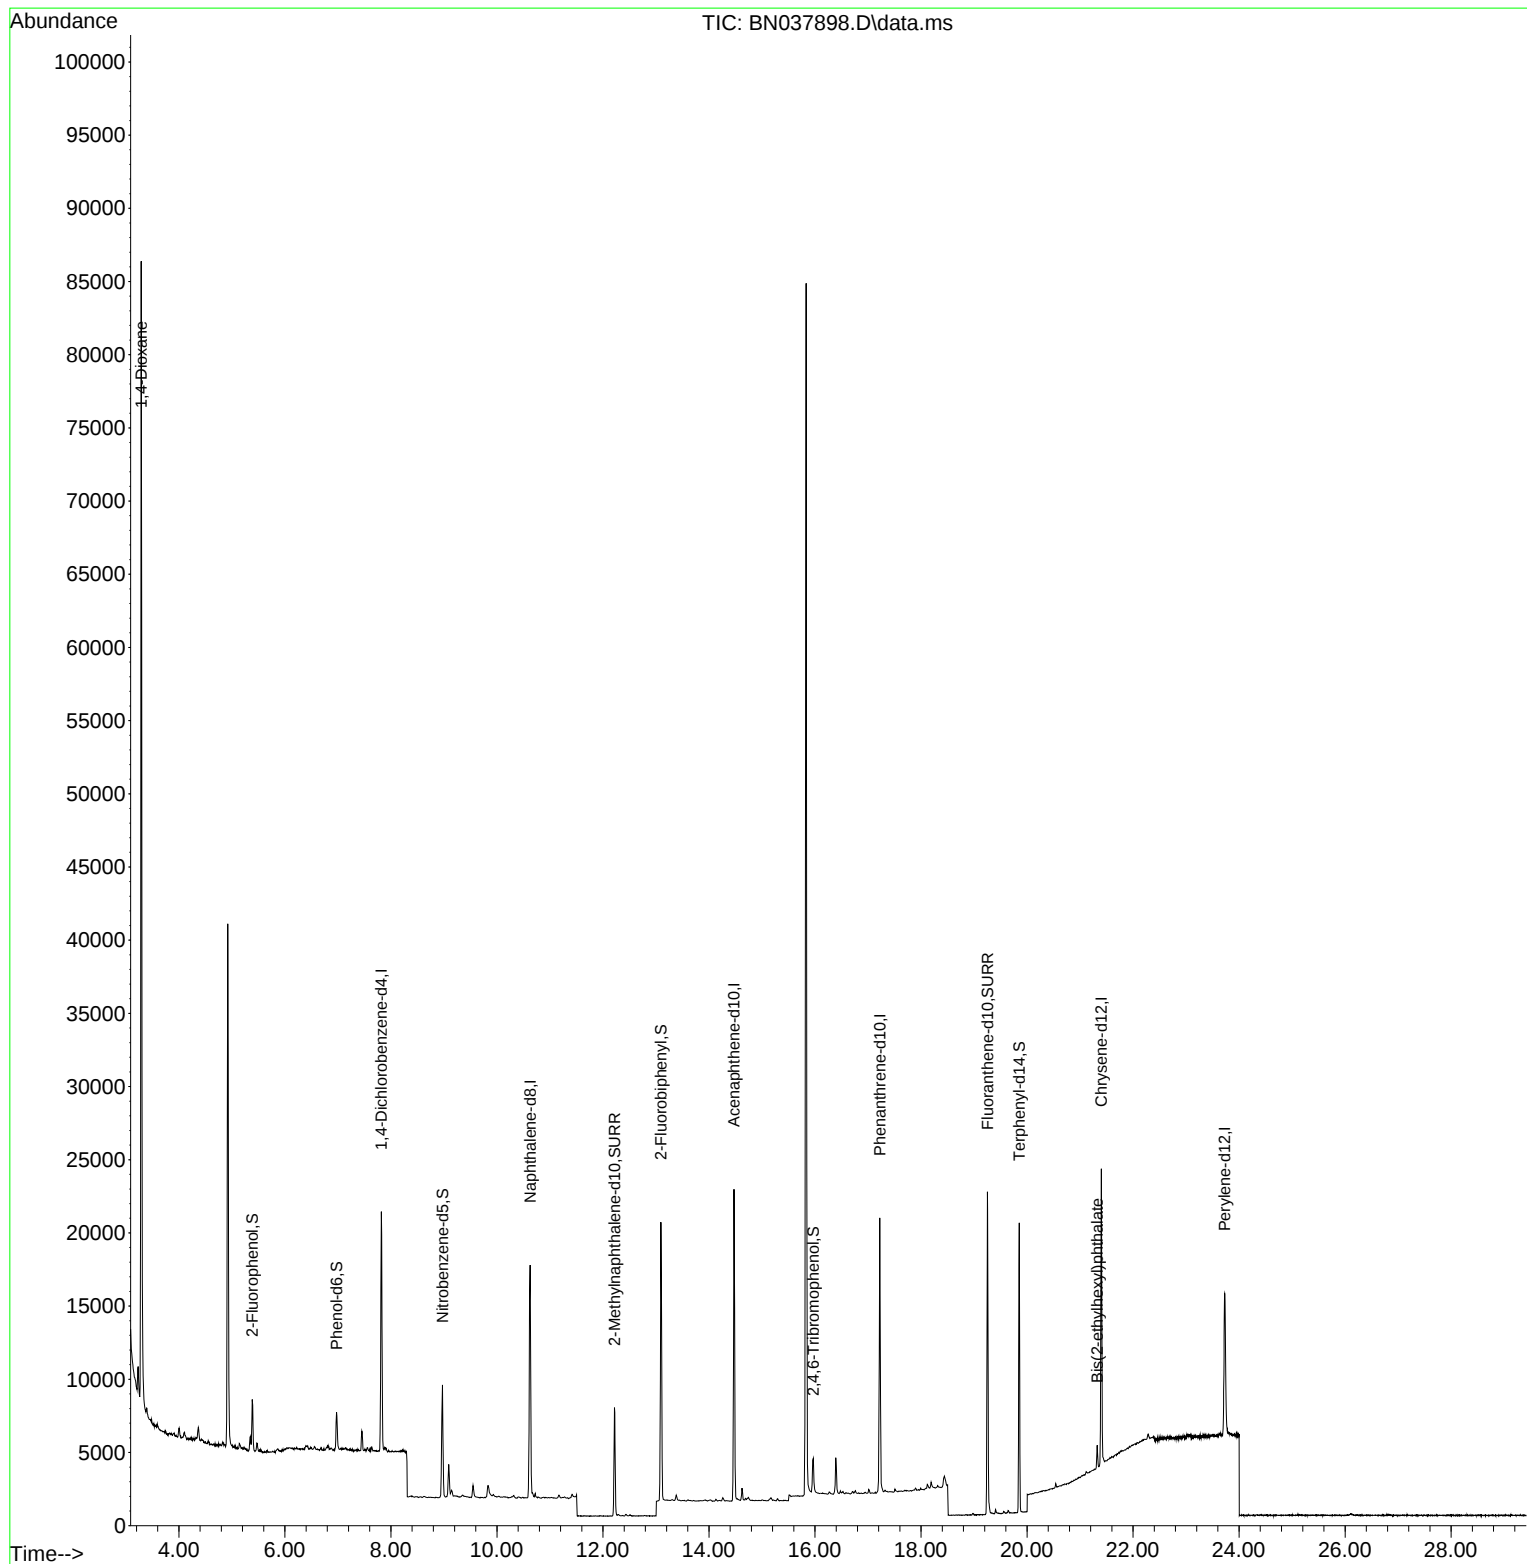



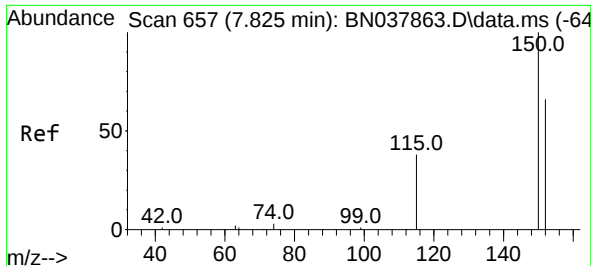


#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.818 min Scan# 61
 Delta R.T. -0.007 min
 Lab File: BN037898.D
 Acq: 25 Sep 2025 20:41


Instrument :
 BNA_N
 ClientSampleId :
 RE132D2-20250918

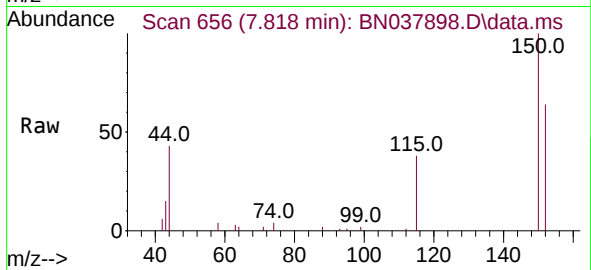



Tgt Ion:152 Resp: 7601
 Ion Ratio Lower Upper
 152 100
 150 155.9 121.0 181.4
 115 59.9 47.4 71.0

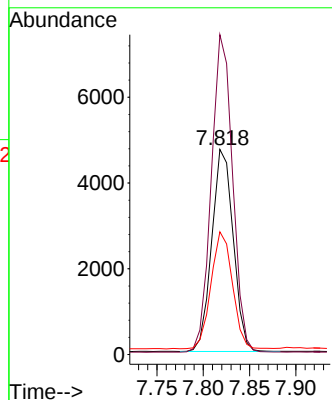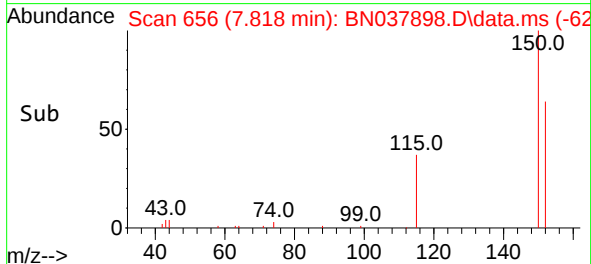


#2
 1,4-Dioxane
 Concen: 6.148 ng
 RT: 3.290 min Scan# 29
 Delta R.T. -0.008 min
 Lab File: BN037898.D
 Acq: 25 Sep 2025 20:41

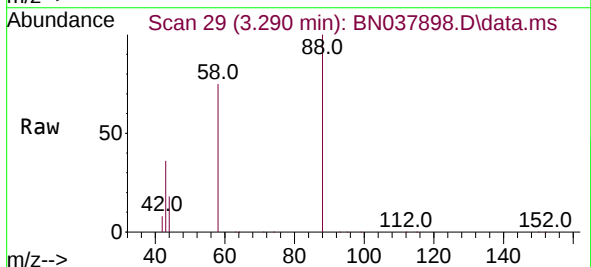

Tgt Ion: 88 Resp: 47437
 Ion Ratio Lower Upper
 88 100
 43 30.6 26.6 39.8
 58 73.4 58.9 88.3



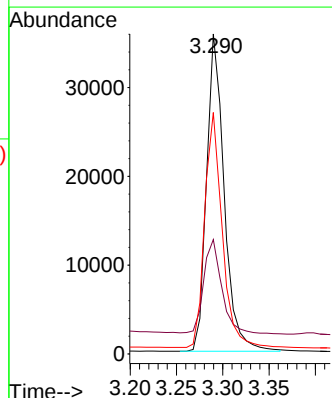



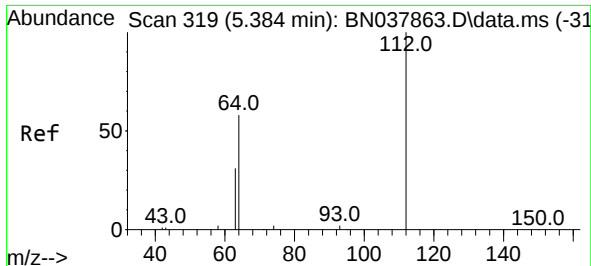

#4
2-Fluorophenol
Concen: 0.161 ng
RT: 5.384 min Scan# 319
Delta R.T. -0.000 min
Lab File: BN037898.D
Acq: 25 Sep 2025 20:41




Instrument :
BNA_N
ClientSampleId :
RE132D2-20250918


Tgt Ion:	112	Resp:	2798
Ion	Ratio	Lower	Upper
112	100		
64	55.8	44.6	66.8
63	30.2	24.9	37.3

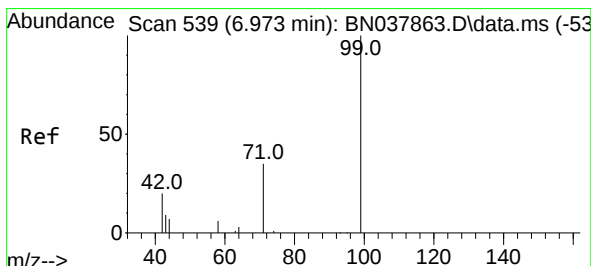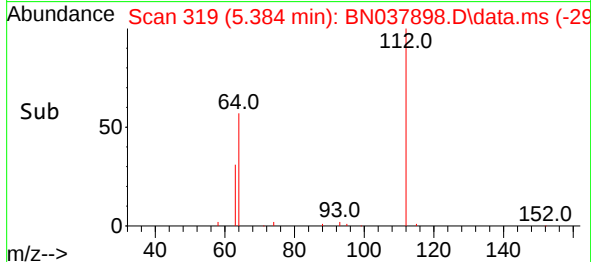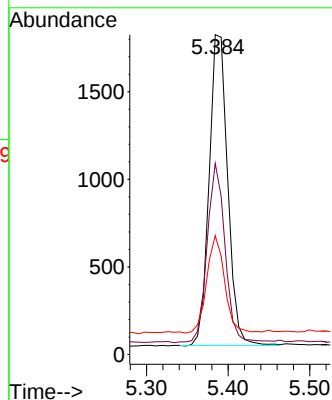

#5
Phenol-d6
Concen: 0.101 ng
RT: 6.973 min Scan# 539
Delta R.T. -0.000 min
Lab File: BN037898.D
Acq: 25 Sep 2025 20:41

Tgt Ion:	99	Resp:	2293
Ion	Ratio	Lower	Upper
99	100		
42	23.2	17.2	25.8
71	35.1	27.3	40.9


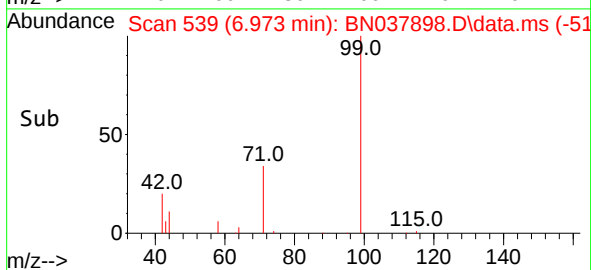
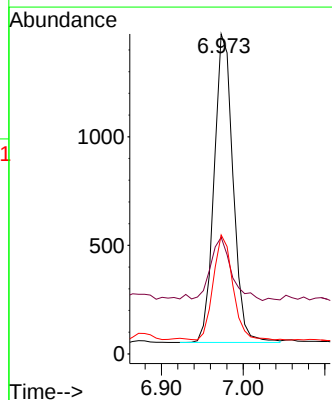
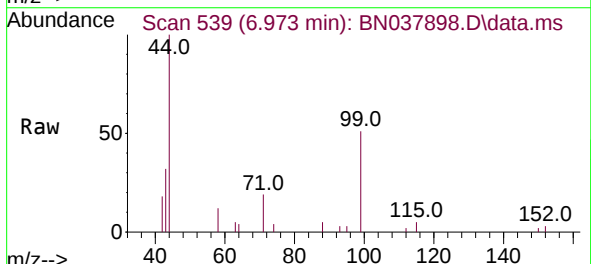


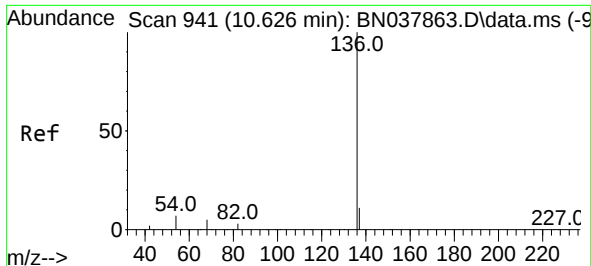

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.626 min Scan# 941
Delta R.T. -0.000 min
Lab File: BN037898.D
Acq: 25 Sep 2025 20:41




Instrument :
BNA_N
ClientSampleId :
RE132D2-20250918


Tgt Ion:	136	Resp:	21427
Ion Ratio	Lower	Upper	
136	100		
137	11.4	9.0	13.4
54	6.5	5.8	8.8
68	5.3	4.3	6.5

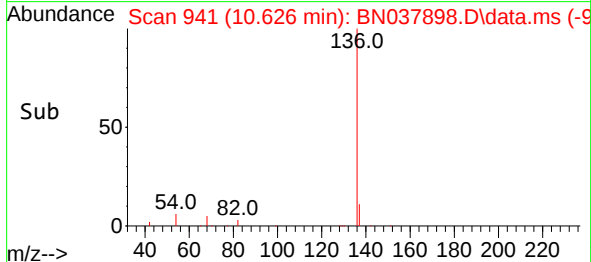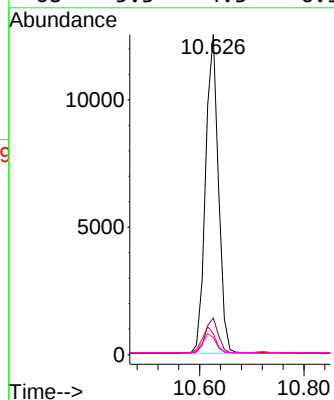

#8
Nitrobenzene-d5
Concen: 0.361 ng
RT: 8.971 min Scan# 786
Delta R.T. -0.000 min
Lab File: BN037898.D
Acq: 25 Sep 2025 20:41

Tgt Ion:	82	Resp:	5900
Ion Ratio	Lower	Upper	
82	100		
128	43.6	34.8	52.2
54	50.6	42.2	63.2


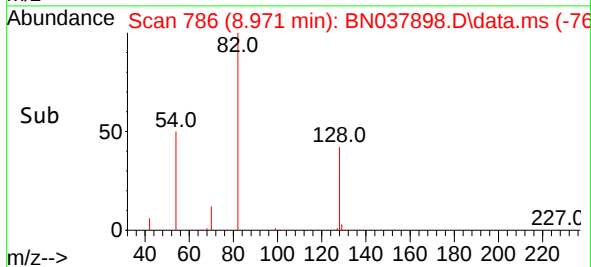
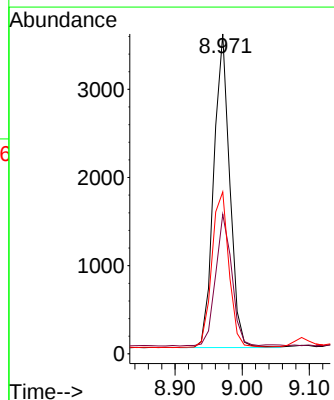
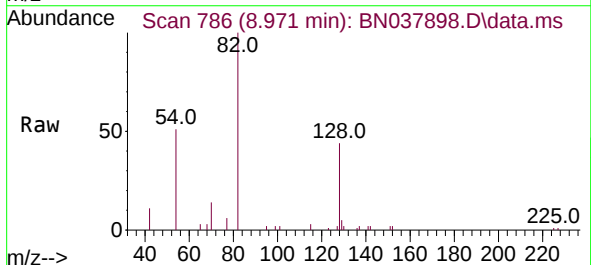


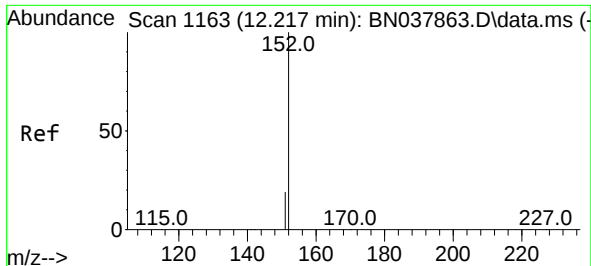

#11
2-Methylnaphthalene-d10
Concen: 0.336 ng
RT: 12.217 min Scan# 1163
Delta R.T. -0.000 min
Lab File: BN037898.D
Acq: 25 Sep 2025 20:41




Instrument :
BNA_N
ClientSampleId :
RE132D2-20250918


Tgt Ion:152 Resp: 9997
Ion Ratio Lower Upper
152 100
151 21.6 17.4 26.2

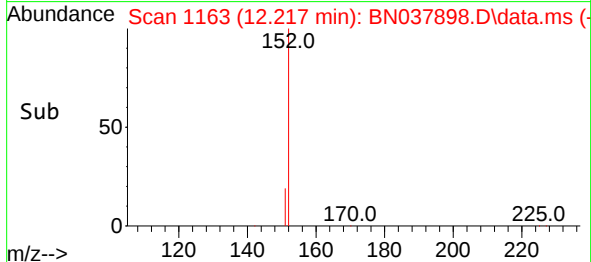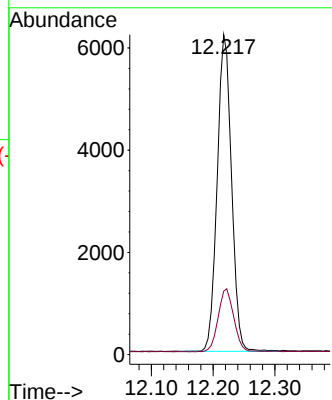

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.473 min Scan# 1456
Delta R.T. -0.000 min
Lab File: BN037898.D
Acq: 25 Sep 2025 20:41


Tgt Ion:164 Resp: 11165
Ion Ratio Lower Upper
164 100
162 106.3 84.8 127.2
160 57.0 46.1 69.1

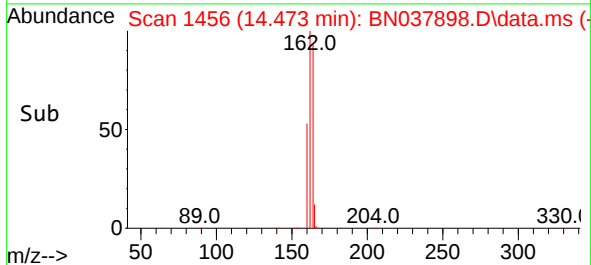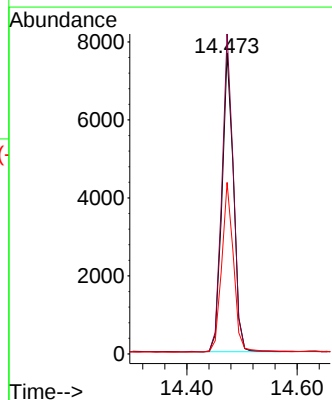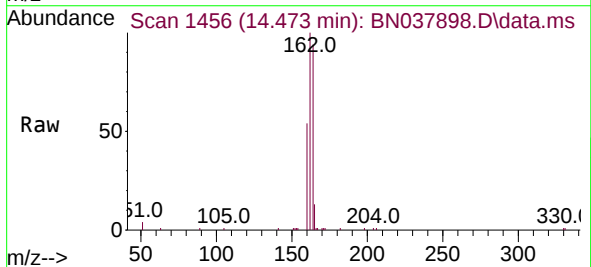



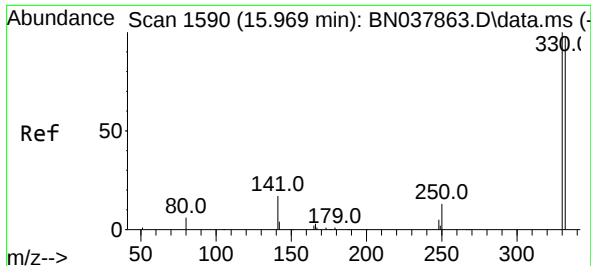


#14
 2,4,6-Tribromophenol
 Concen: 0.363 ng
 RT: 15.969 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BN037898.D
 Acq: 25 Sep 2025 20:41


Instrument :
 BNA_N
 ClientSampleId :
 RE132D2-20250918





Tgt Ion:330 Resp: 1536
 Ion Ratio Lower Upper
 330 100
 332 95.5 77.2 115.8
 141 45.6 37.2 55.8

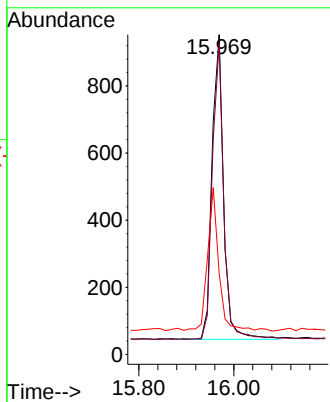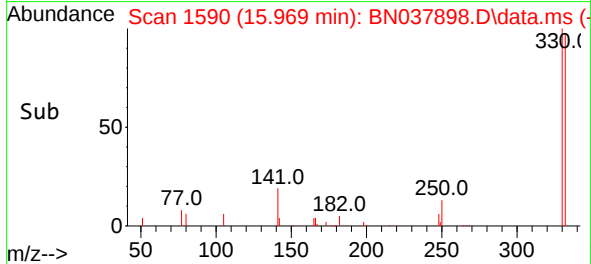


#15
 2-Fluorobiphenyl
 Concen: 0.345 ng
 RT: 13.094 min Scan# 1327
 Delta R.T. -0.000 min
 Lab File: BN037898.D
 Acq: 25 Sep 2025 20:41

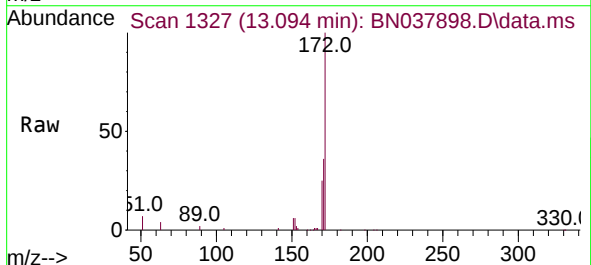

Tgt Ion:172 Resp: 15765
 Ion Ratio Lower Upper
 172 100
 171 36.2 28.6 43.0
 170 25.2 19.7 29.5



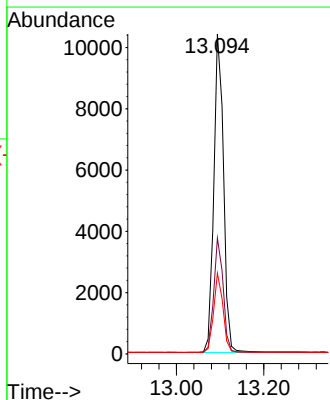
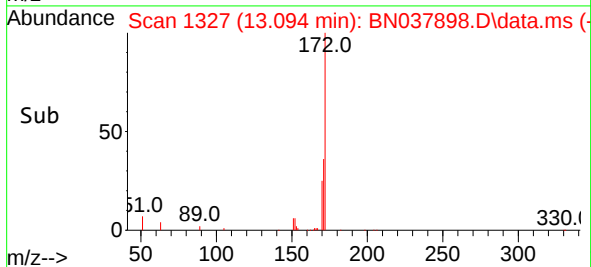


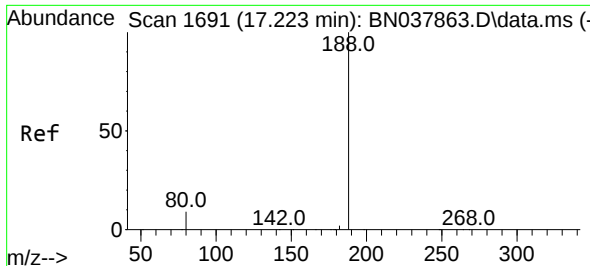

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.223 min Scan# 1691
Delta R.T. -0.000 min
Lab File: BN037898.D
Acq: 25 Sep 2025 20:41




Instrument :
BNA_N
ClientSampleId :
RE132D2-20250918


Tgt Ion:188 Resp: 23219
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.6 7.6 11.4

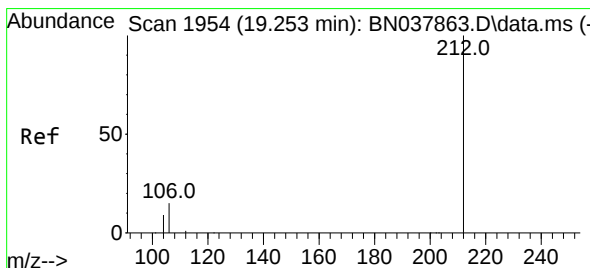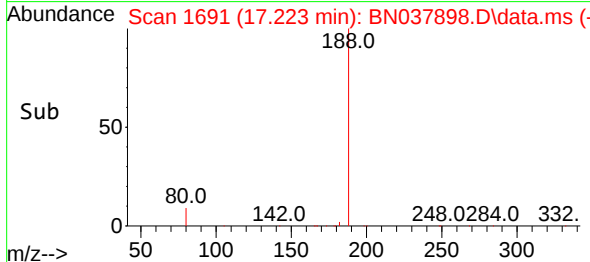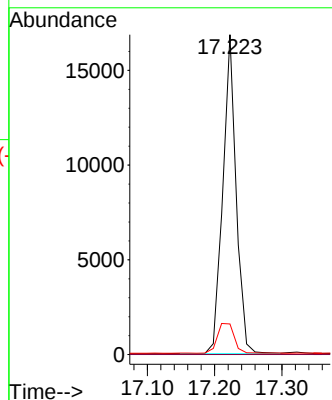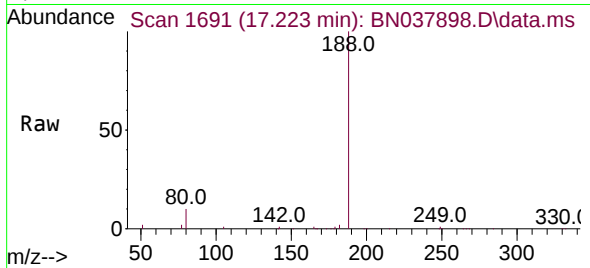

#27
Fluoranthene-d10
Concen: 0.410 ng
RT: 19.252 min Scan# 1954
Delta R.T. -0.000 min
Lab File: BN037898.D
Acq: 25 Sep 2025 20:41

Tgt Ion:212 Resp: 23968
Ion Ratio Lower Upper
212 100
106 15.8 12.6 19.0
104 9.3 7.4 11.0


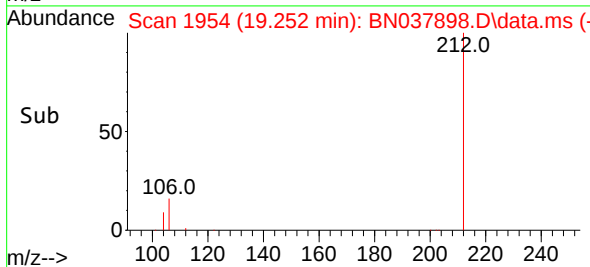
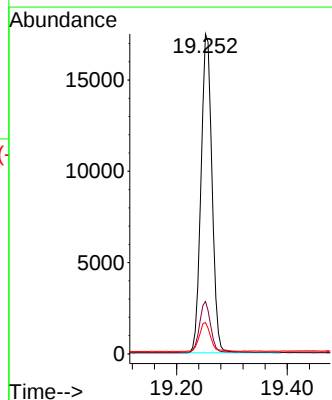
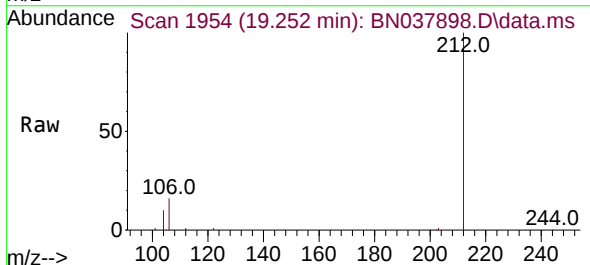




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.402 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN037898.D
Acq: 25 Sep 2025 20:41




Instrument :
BNA_N
ClientSampleId :
RE132D2-20250918


Tgt Ion:240 Resp: 17732
Ion Ratio Lower Upper
240 100
120 14.1 11.4 17.2
236 28.7 23.0 34.6

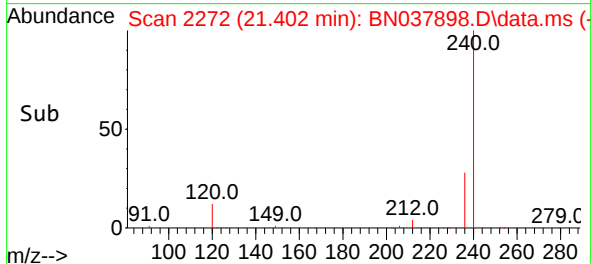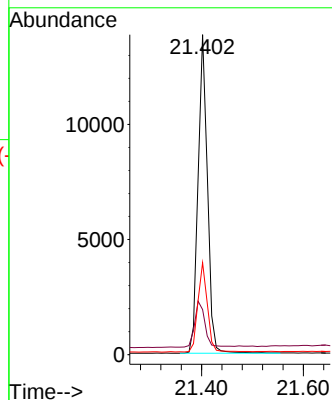

#31
Terphenyl-d14
Concen: 0.499 ng
RT: 19.852 min Scan# 2083
Delta R.T. -0.000 min
Lab File: BN037898.D
Acq: 25 Sep 2025 20:41

Tgt Ion:244 Resp: 17629
Ion Ratio Lower Upper
244 100
212 9.2 7.6 11.4
122 16.9 13.9 20.9


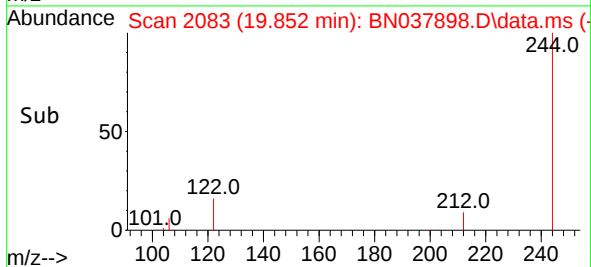
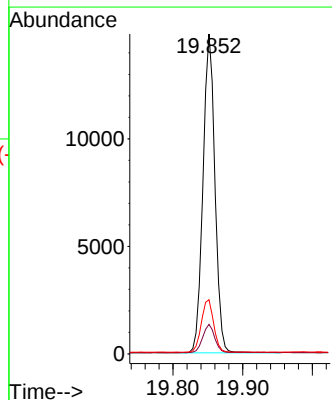
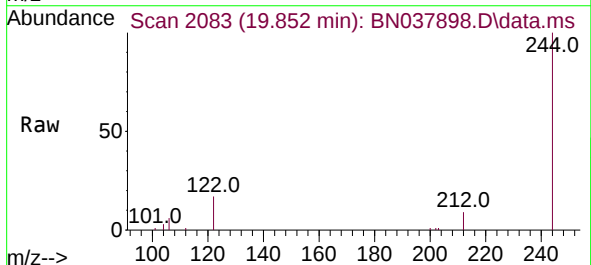


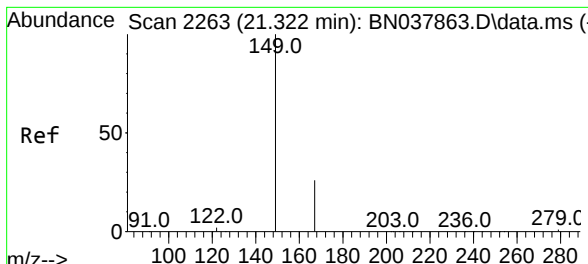

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.062 ng
 RT: 21.321 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN037898.D
 Acq: 25 Sep 2025 20:41

Instrument :
 BNA_N
 ClientSampleId :
 RE132D2-20250918

Tgt Ion:	149	Resp:	1516
Ion Ratio	Lower	Upper	
149	100		
167	29.6	20.4	30.6
279	5.4	2.4	3.6#

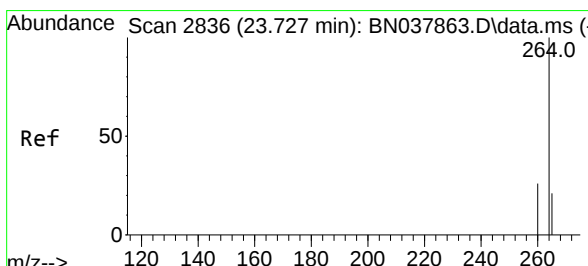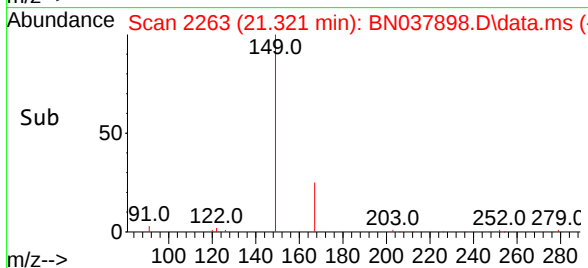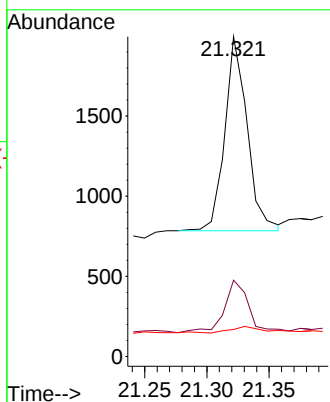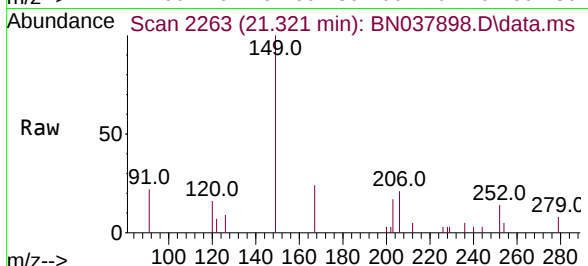

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.730 min Scan# 2837
 Delta R.T. 0.003 min
 Lab File: BN037898.D
 Acq: 25 Sep 2025 20:41

Tgt Ion:	264	Resp:	14515
Ion Ratio	Lower	Upper	
264	100		
260	27.1	21.5	32.3
265	80.8	53.8	80.6#

