
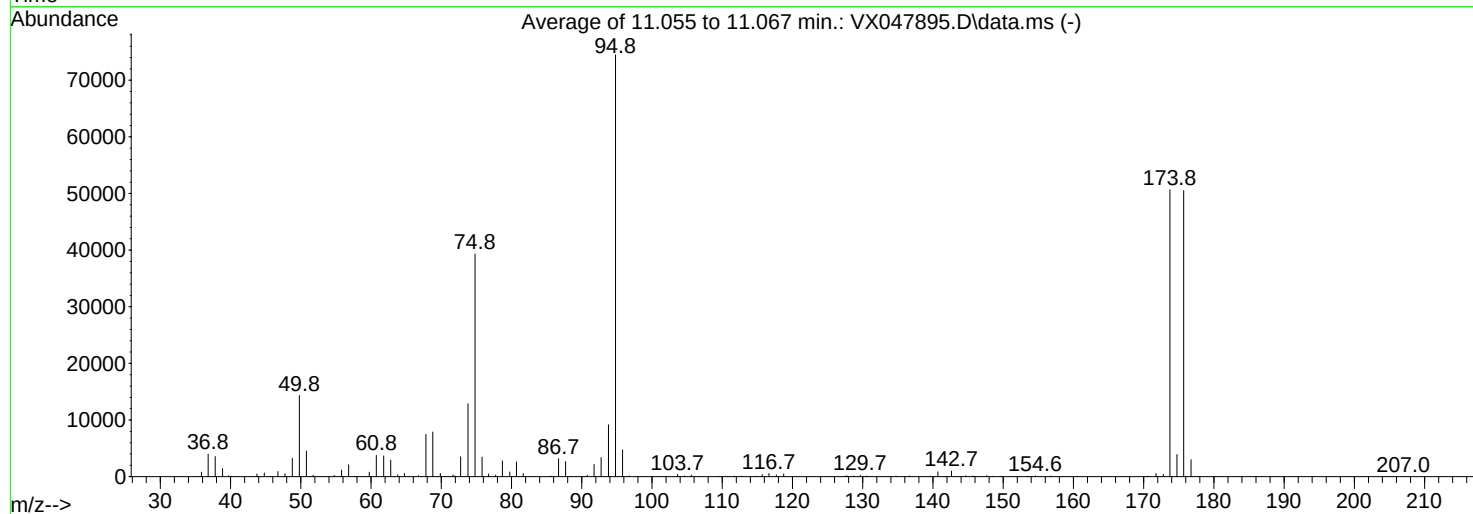


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX093025\
Data File : VX047895.D
Acq On : 30 Sep 2025 08:49
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Title : SW846 8260
Last Update : Wed Sep 17 06:39:58 2025

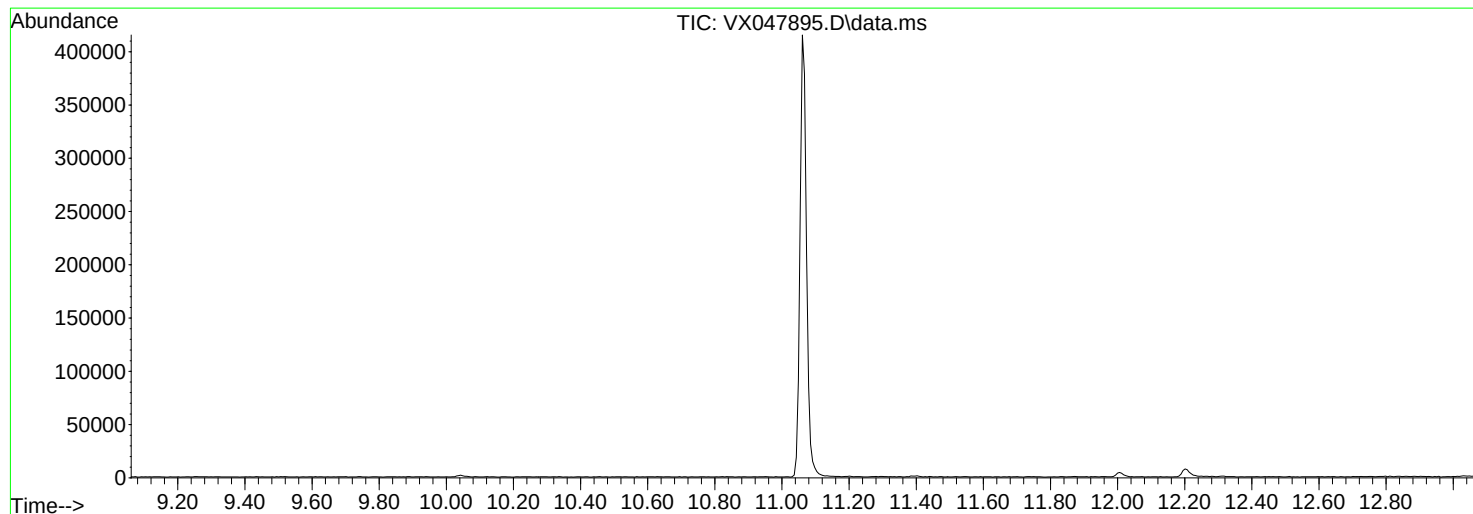

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1630

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.2	14337	PASS
75	95	30	60	52.8	39328	PASS
95	95	100	100	100.0	74483	PASS
96	95	5	9	6.3	4709	PASS
173	174	0.00	2	0.8	407	PASS
174	95	50	100	68.0	50669	PASS
175	174	5	9	7.7	3913	PASS
176	174	95	101	99.7	50504	PASS
177	176	5	9	5.9	2984	PASS