

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092925\
 Data File : VX047883.D
 Acq On : 29 Sep 2025 14:59
 Operator : JC/MD
 Sample : Q3156-23
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RW9-MW01D2-20250919

Quant Time: Sep 30 01:21:42 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 17 06:39:58 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	5.538	168	142790	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.745	114	301628	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	311543	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	162191	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.940	65	129458	56.958	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	113.920%
35) Dibromofluoromethane	5.373	113	102778	50.808	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	101.620%
50) Toluene-d8	8.635	98	346965	49.569	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	99.140%
62) 4-Bromofluorobenzene	11.061	95	151935	57.194	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	114.380%
Target Compounds						
16) Acetone	2.386	43	2333	2.361	ug/l #	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092925\
 Data File : VX047883.D
 Acq On : 29 Sep 2025 14:59
 Operator : JC/MD
 Sample : Q3156-23
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RW9-MW01D2-20250919


Quant Time: Sep 30 01:21:42 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 17 06:39:58 2025
 Response via : Initial Calibration

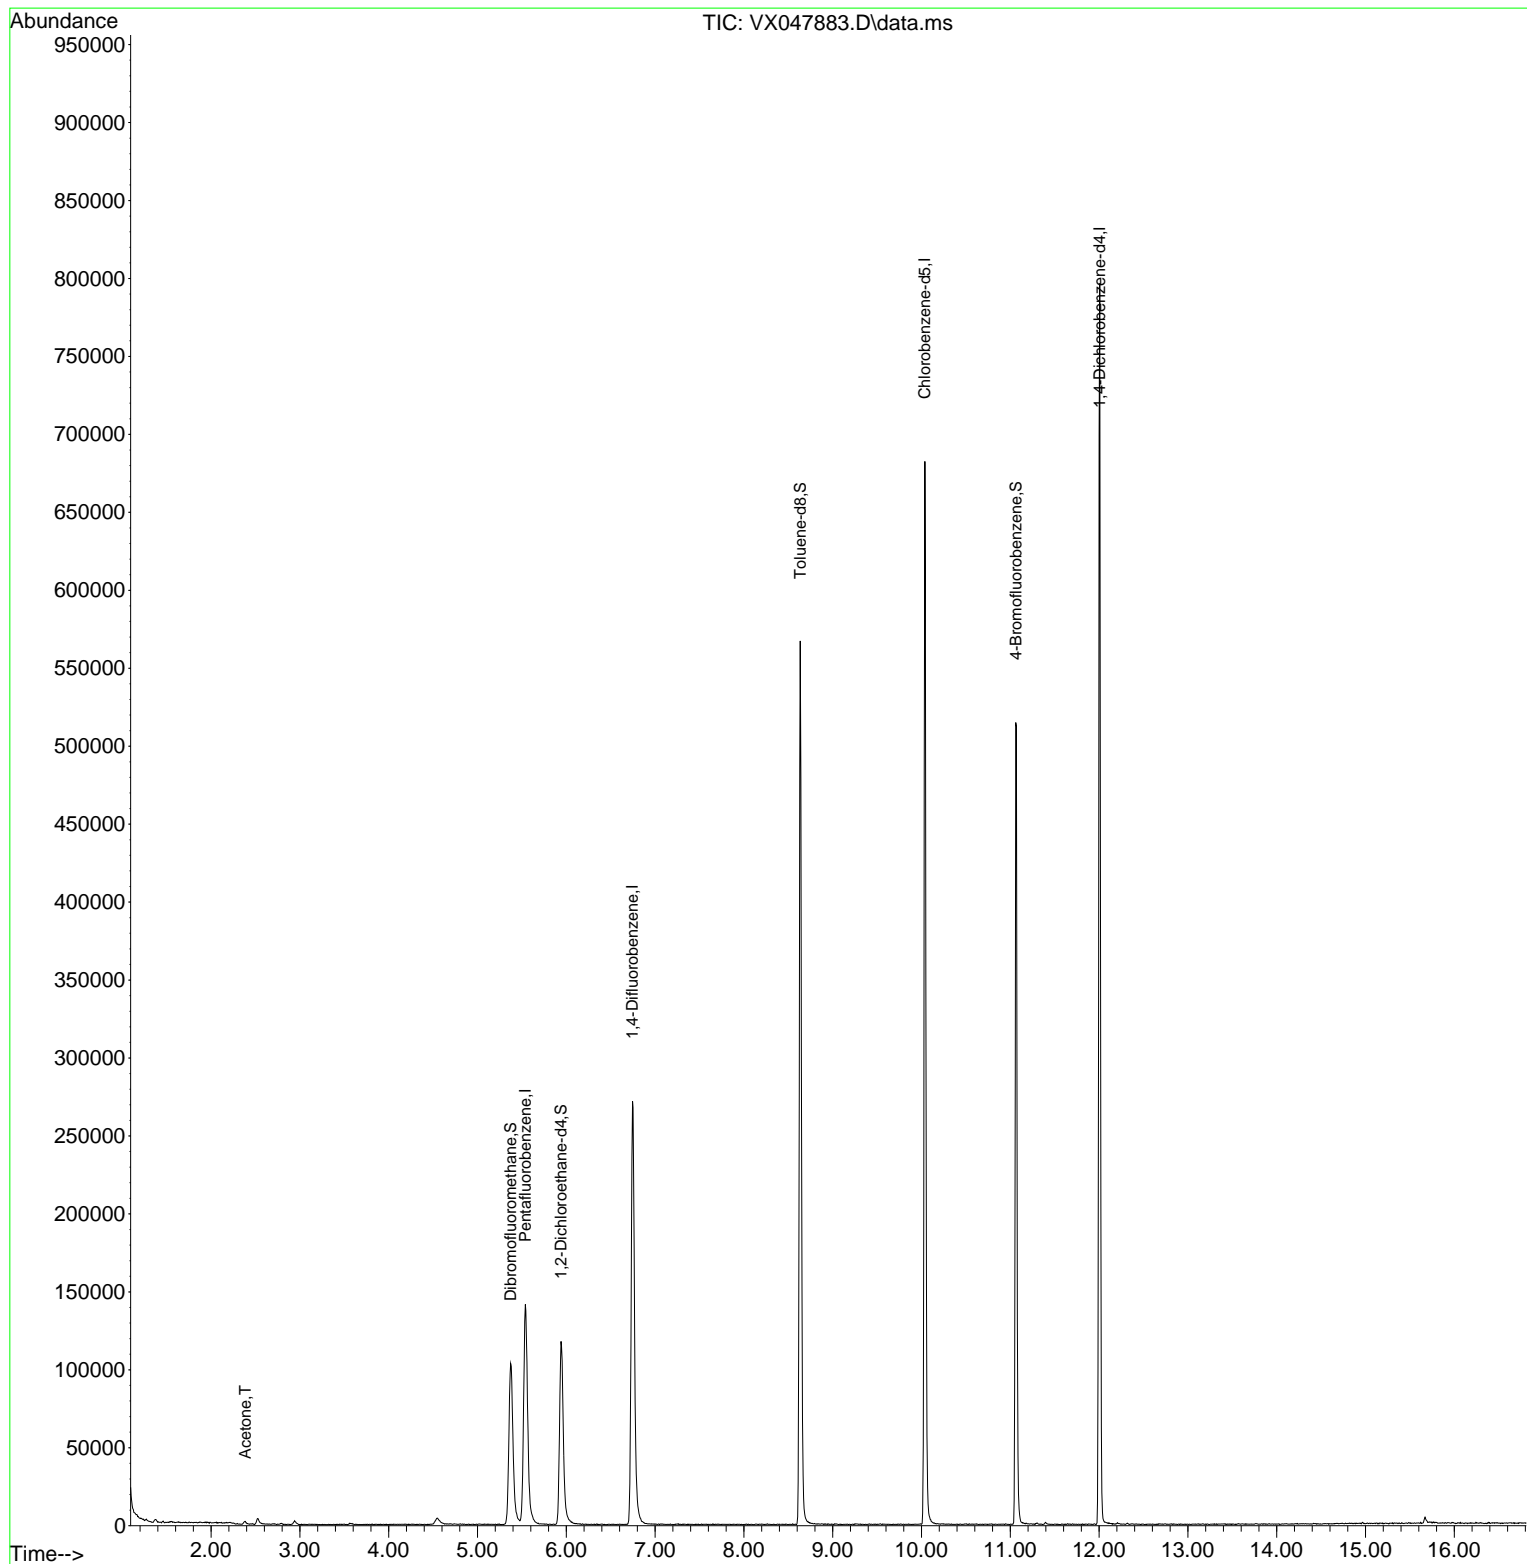



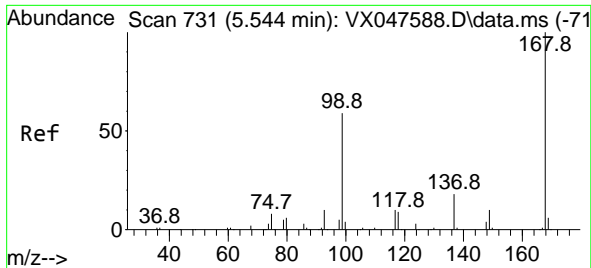


#1
 Pentafluorobenzene
 Concen: 50.000 ug/l
 RT: 5.538 min Scan# 71
 Delta R.T. -0.006 min
 Lab File: VX047883.D
 Acq: 29 Sep 2025 14:59


Instrument : MSVOA_X
 ClientSampleId : RW9-MW01D2-20250919

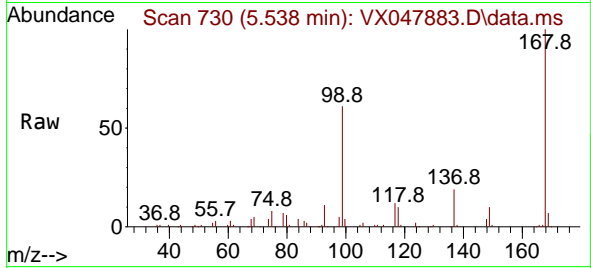



Tgt Ion:168 Resp: 142790
 Ion Ratio Lower Upper
 168 100
 99 61.1 48.8 73.2

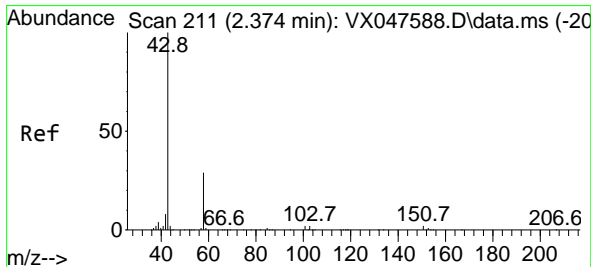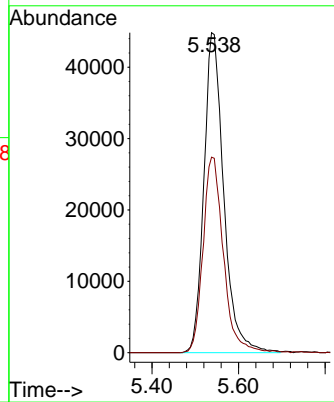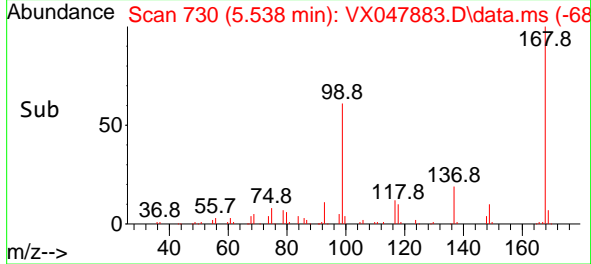


#16
 Acetone
 Concen: 2.361 ug/l
 RT: 2.386 min Scan# 213
 Delta R.T. 0.012 min
 Lab File: VX047883.D
 Acq: 29 Sep 2025 14:59

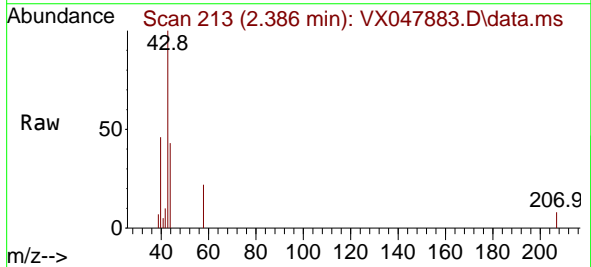

Tgt Ion: 43 Resp: 2333
 Ion Ratio Lower Upper
 43 100
 58 22.4 23.4 35.0#



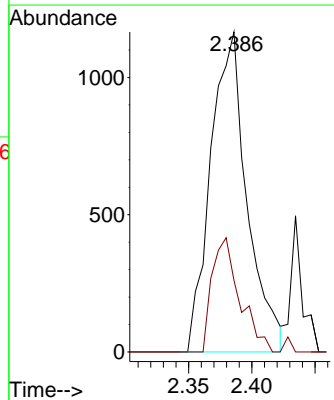
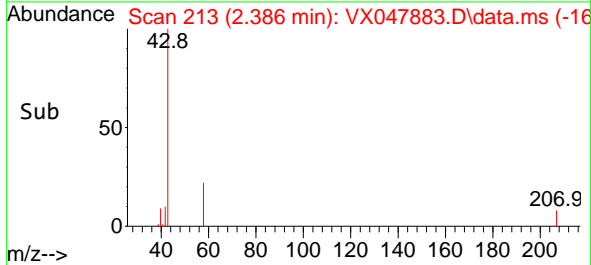


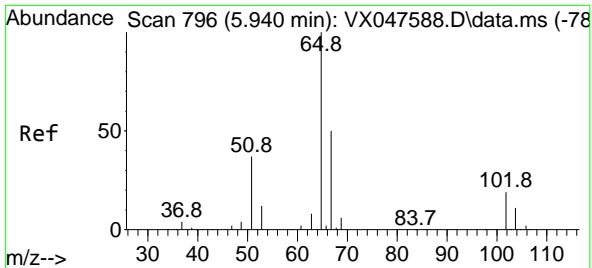

#33
 1,2-Dichloroethane-d4
 Concen: 56.958 ug/l
 RT: 5.940 min Scan# 796
 Delta R.T. -0.000 min
 Lab File: VX047883.D
 Acq: 29 Sep 2025 14:59




Instrument : MSVOA_X
 ClientSampleId : RW9-MW01D2-20250919


Tgt Ion: 65 Resp: 129458
 Ion Ratio Lower Upper
 65 100
 67 51.8 0.0 103.0

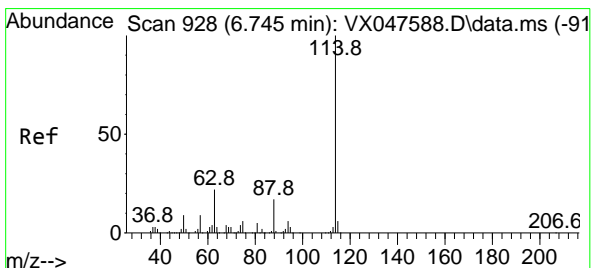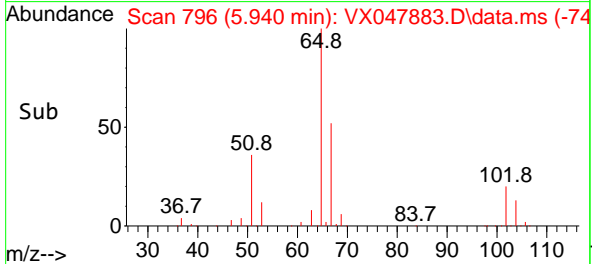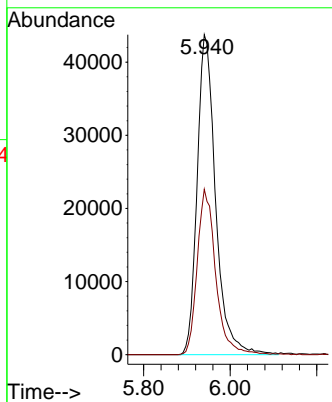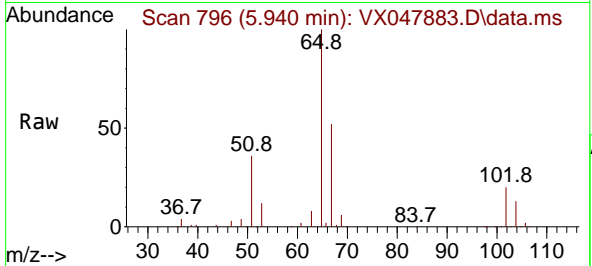

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.745 min Scan# 928
 Delta R.T. -0.000 min
 Lab File: VX047883.D
 Acq: 29 Sep 2025 14:59

Tgt Ion: 114 Resp: 301628
 Ion Ratio Lower Upper
 114 100
 63 21.6 0.0 44.0
 88 16.5 0.0 34.2

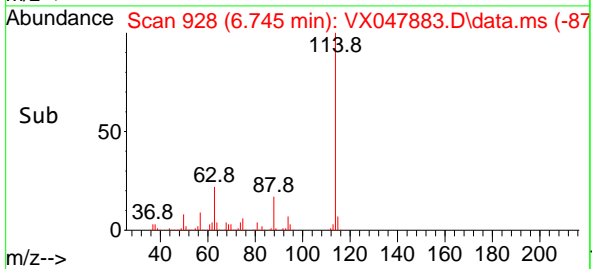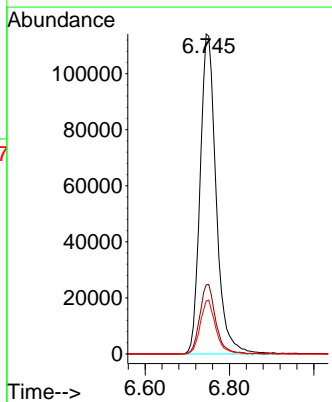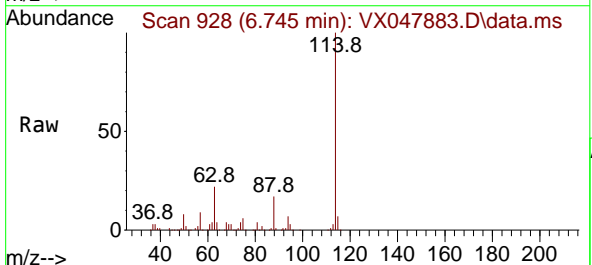




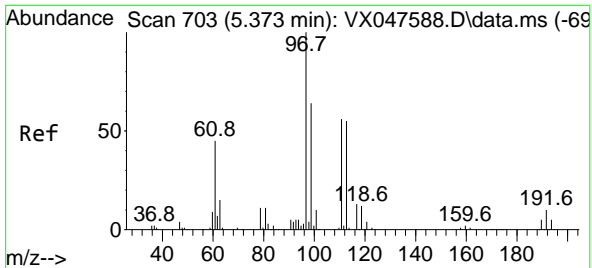


#35
 Dibromofluoromethane
 Concen: 50.808 ug/l
 RT: 5.373 min Scan# 703
 Delta R.T. 0.000 min
 Lab File: VX047883.D
 Acq: 29 Sep 2025 14:59

Instrument :
 MSVOA_X
ClientSampleId :
 RW9-MW01D2-20250919

Tgt Ion: 113 Resp: 102778




Ion	Ratio	Lower	Upper
113	100		
111	102.6	80.9	121.3
192	17.6	14.2	21.4

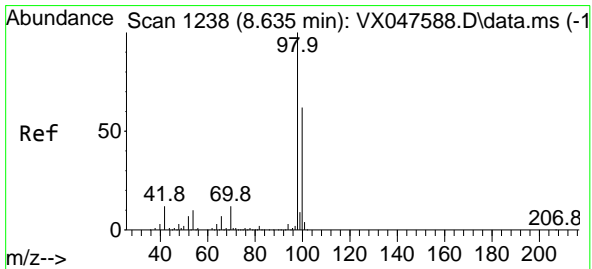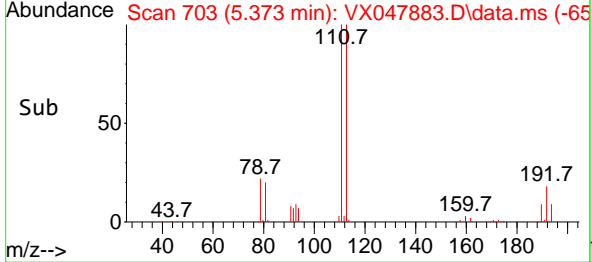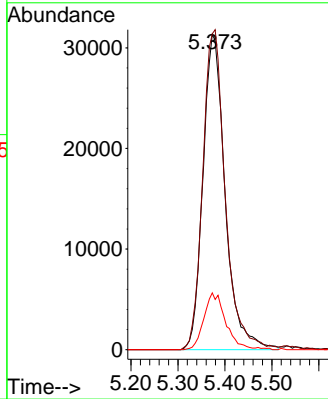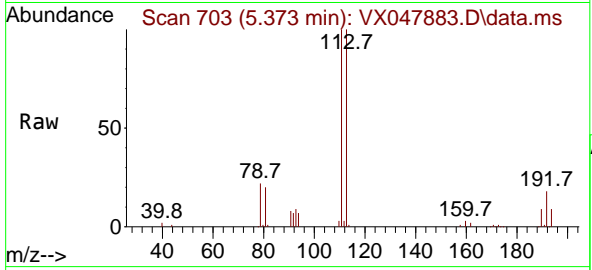


#50
 Toluene-d8
 Concen: 49.569 ug/l
 RT: 8.635 min Scan# 1238
 Delta R.T. -0.000 min
 Lab File: VX047883.D
 Acq: 29 Sep 2025 14:59

Tgt Ion: 98 Resp: 346965

Ion	Ratio	Lower	Upper
98	100		
100	66.4	53.0	79.4


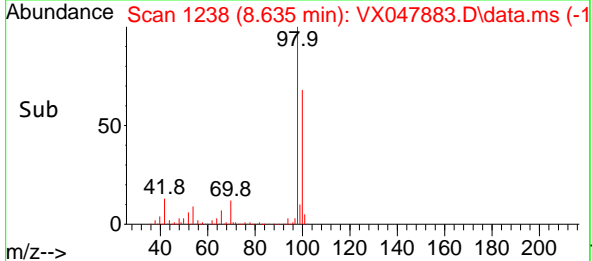
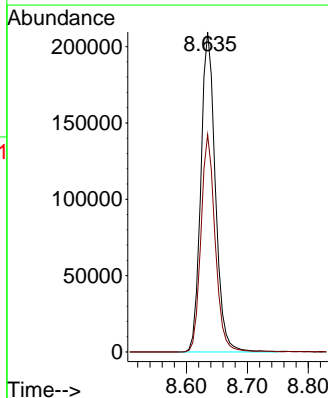
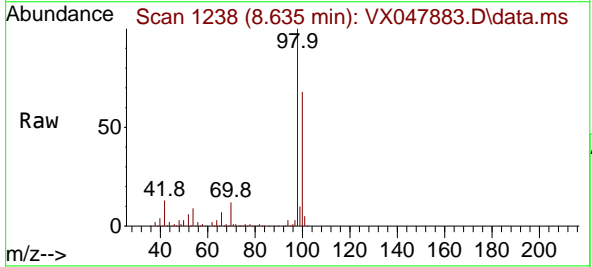


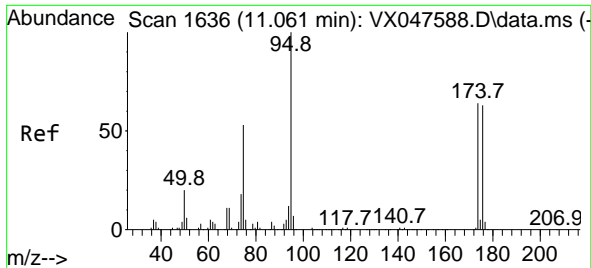

#62
 4-Bromofluorobenzene
 Concen: 57.194 ug/l
 RT: 11.061 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VX047883.D
 Acq: 29 Sep 2025 14:59




Instrument : MSVOA_X
 ClientSampleId : RW9-MW01D2-20250919


Tgt Ion	Resp	Lower	Upper
95	151935		
174	72.9	0.0	141.6
176	70.5	0.0	138.4

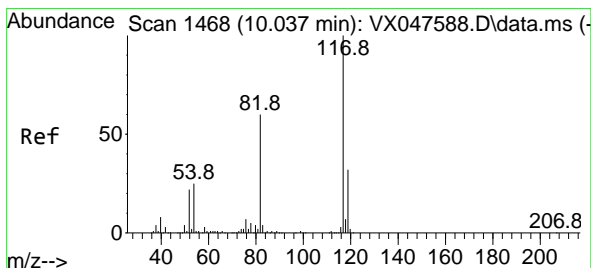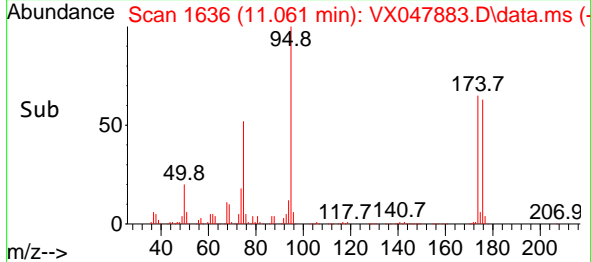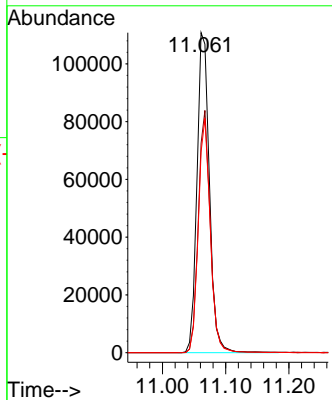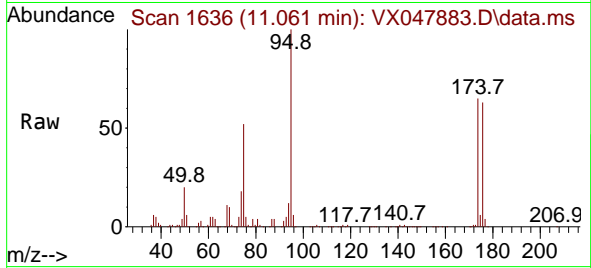

#63
 Chlorobenzene-d5
 Concen: 50.000 ug/l
 RT: 10.037 min Scan# 1468
 Delta R.T. 0.000 min
 Lab File: VX047883.D
 Acq: 29 Sep 2025 14:59


Tgt Ion	Resp	Lower	Upper
117	311543		
82	58.8	47.8	71.6
119	31.9	25.2	37.8

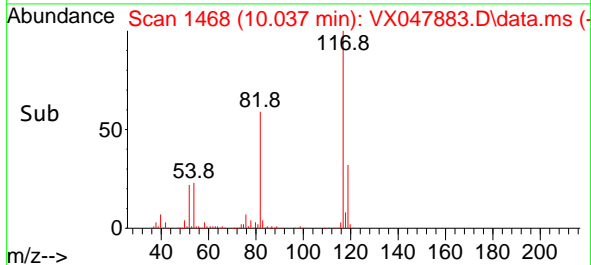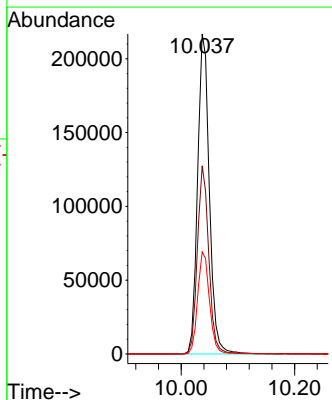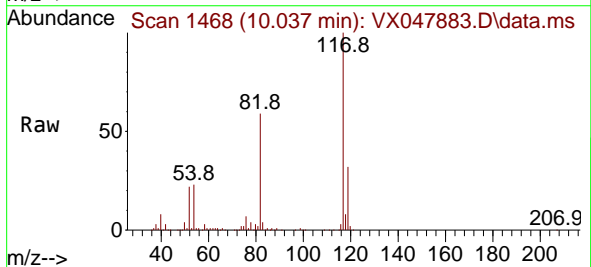

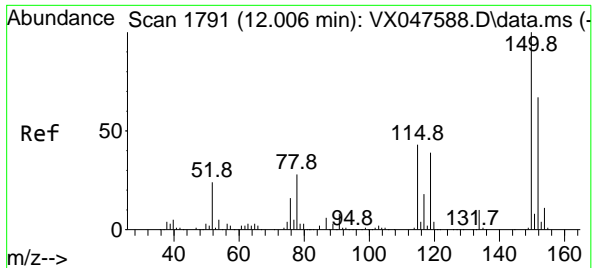

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.006 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VX047883.D
 Acq: 29 Sep 2025 14:59

Instrument :
 MSVOA_X
 ClientSampleId :
 RW9-MW01D2-20250919

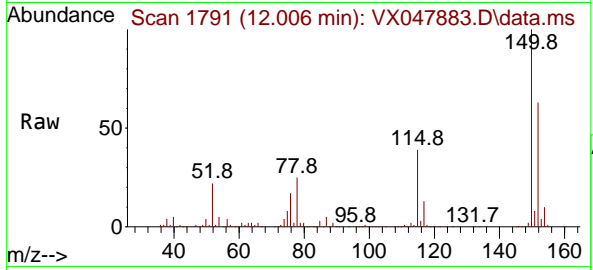

Tgt Ion:152 Resp: 162191

Ion	Ratio	Lower	Upper
152	100		
115	62.4	44.9	134.5
150	158.4	0.0	352.0

