


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092325\
Data File : BP025823.D
Acq On : 23 Sep 2025 09:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 11 16:45:04 2025

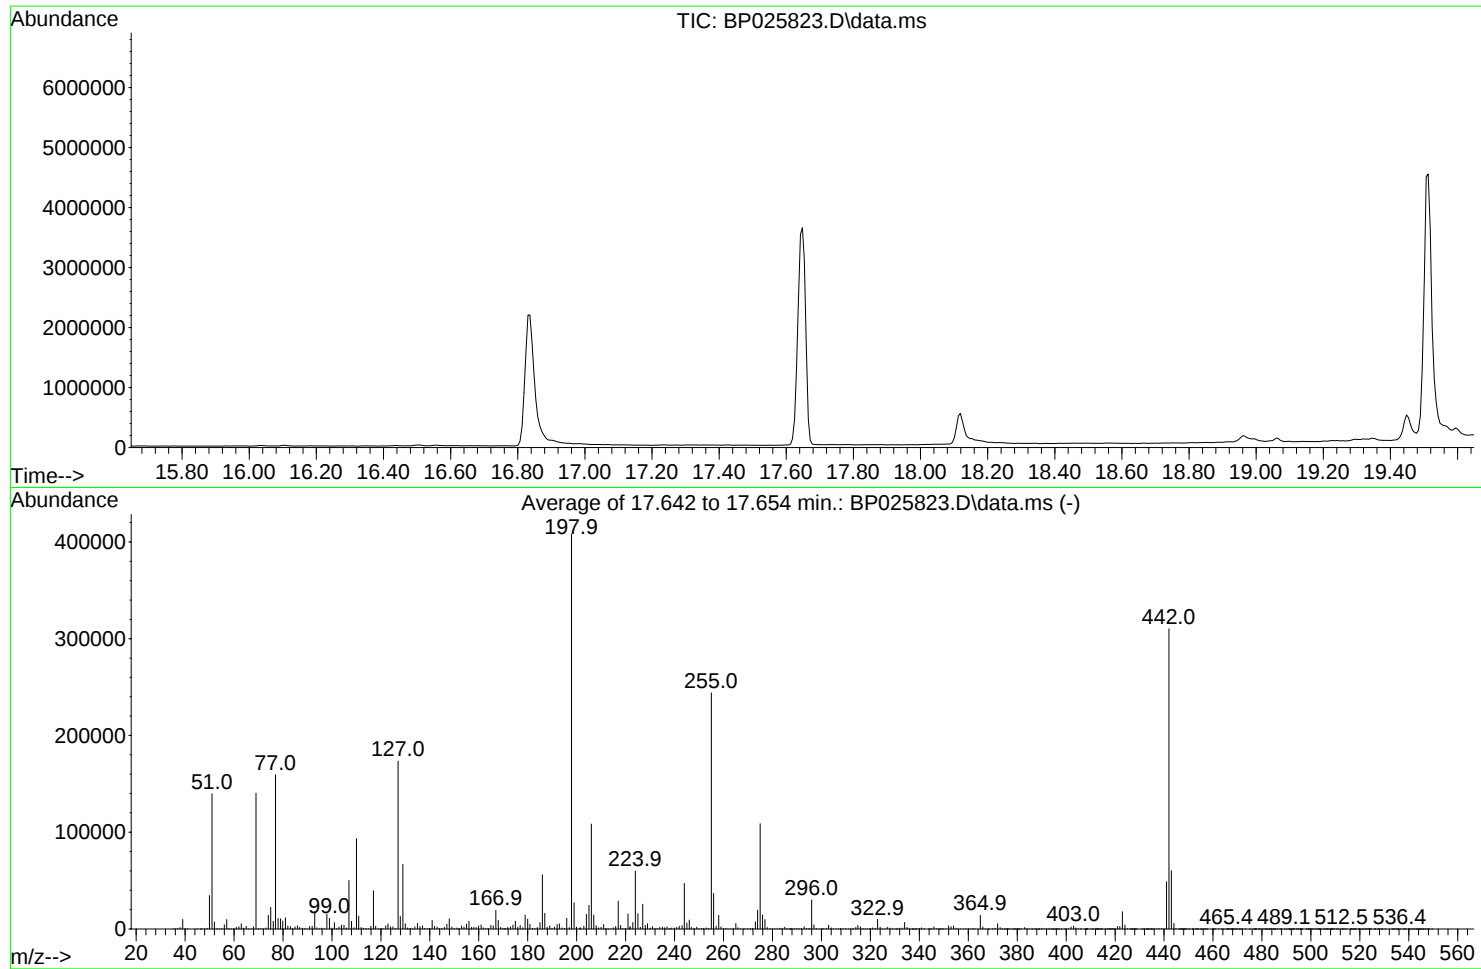


AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2491

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	2328	PASS
69	69	100	100	100.0	140370	PASS
70	69	0.00	2	0.4	543	PASS
197	198	0.00	2	0.3	1363	PASS
198	198	100	100	100.0	408114	PASS
199	198	5	9	6.6	27121	PASS
365	198	1	100	3.5	14163	PASS
441	443	0.01	150	80.8	48712	PASS
442	442	100	100	100.0	310208	PASS
443	442	15	24	19.4	60252	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092325\
Data File : BP025823.D
Acq On : 23 Sep 2025 09:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 23 11:28:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

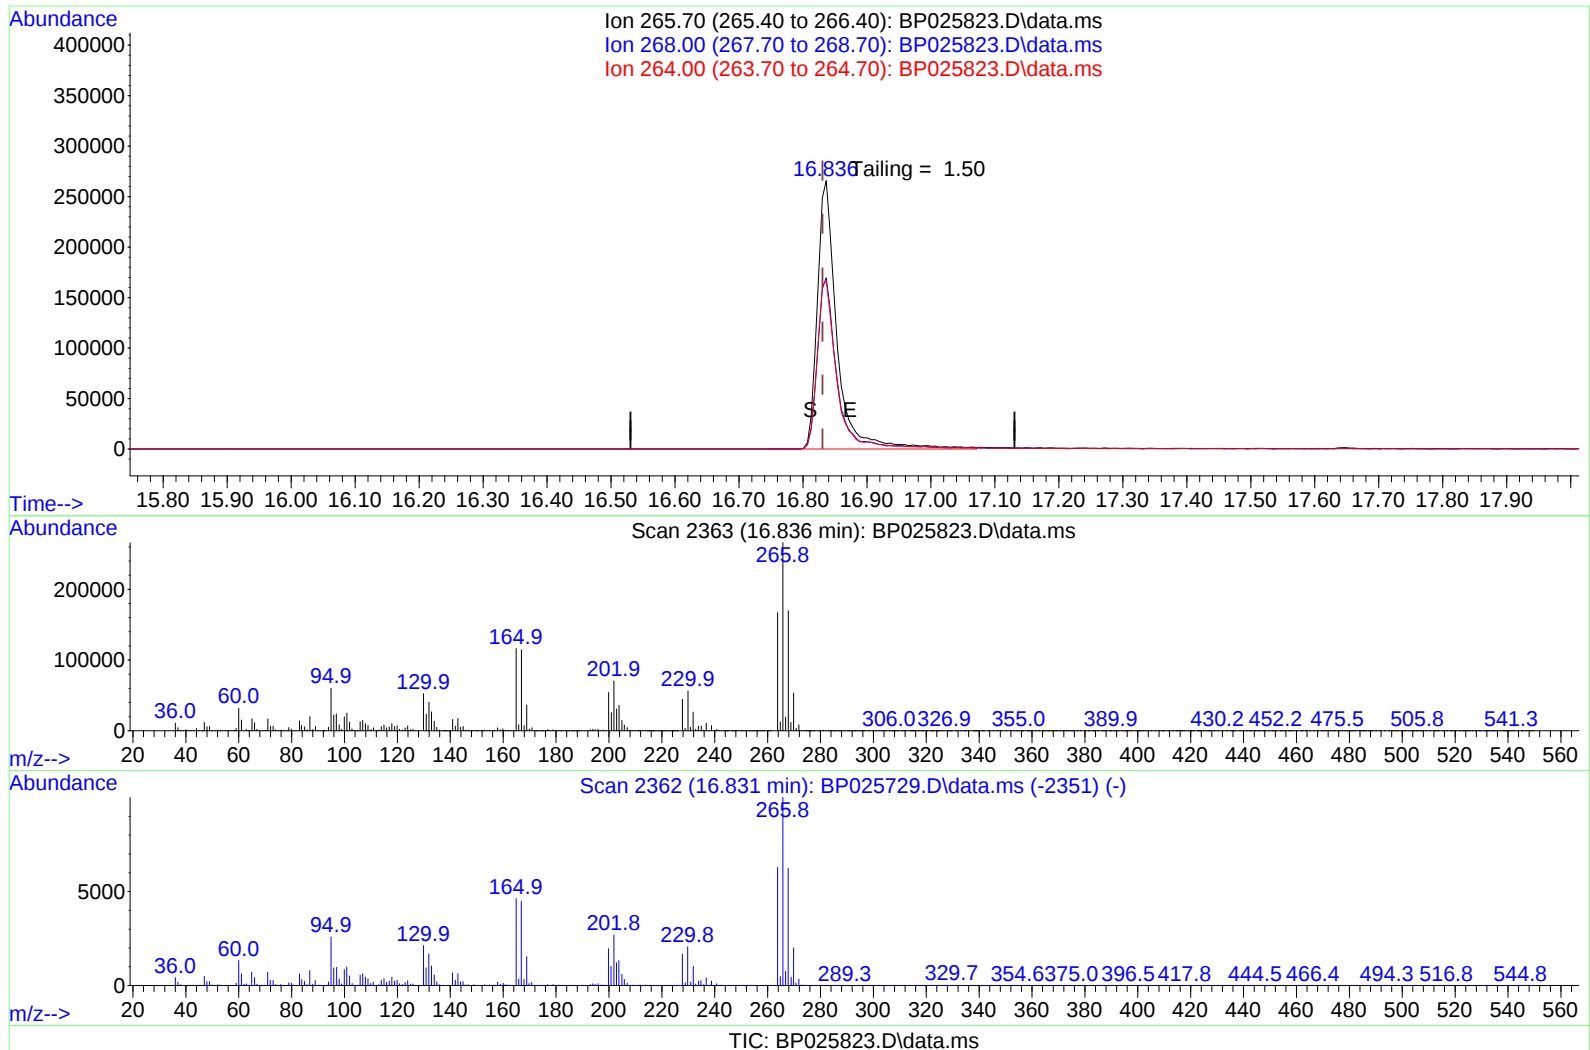

(70) Pentachlorophenol (C)

16.836min (+ 0.006) 4627969.76 ng




response 561305

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.82
264.00	62.70	62.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092325\
Data File : BP025823.D
Acq On : 23 Sep 2025 09:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 23 11:28:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

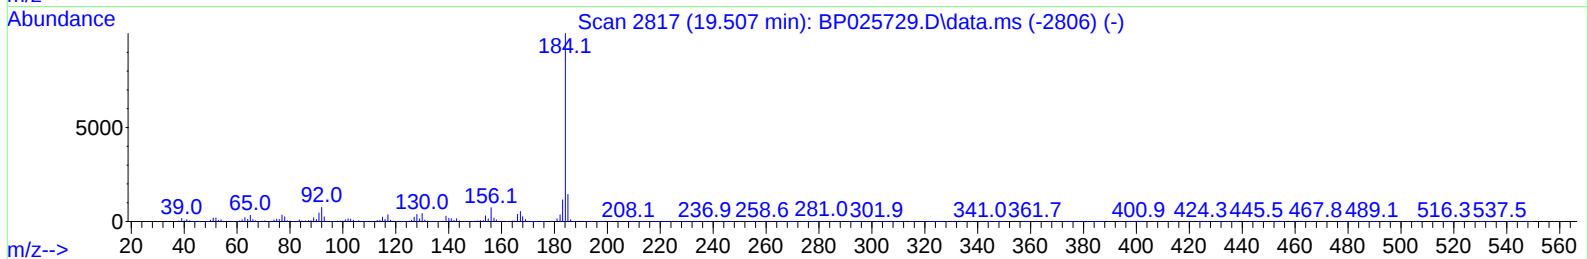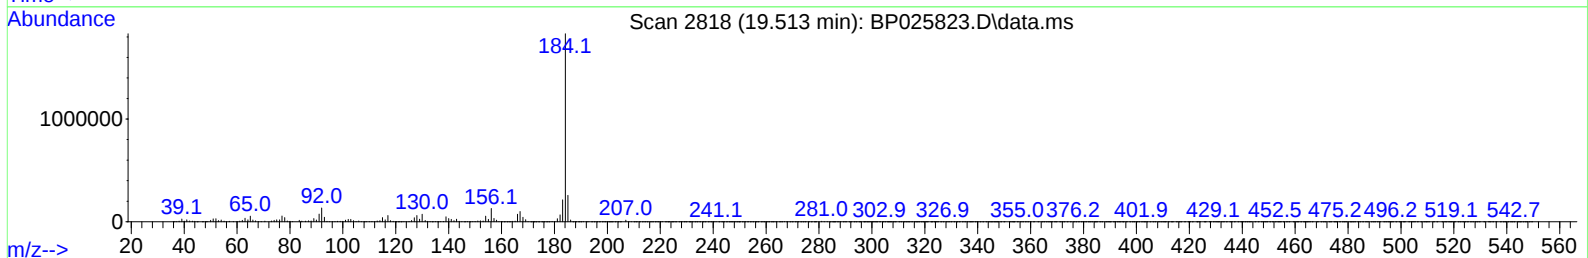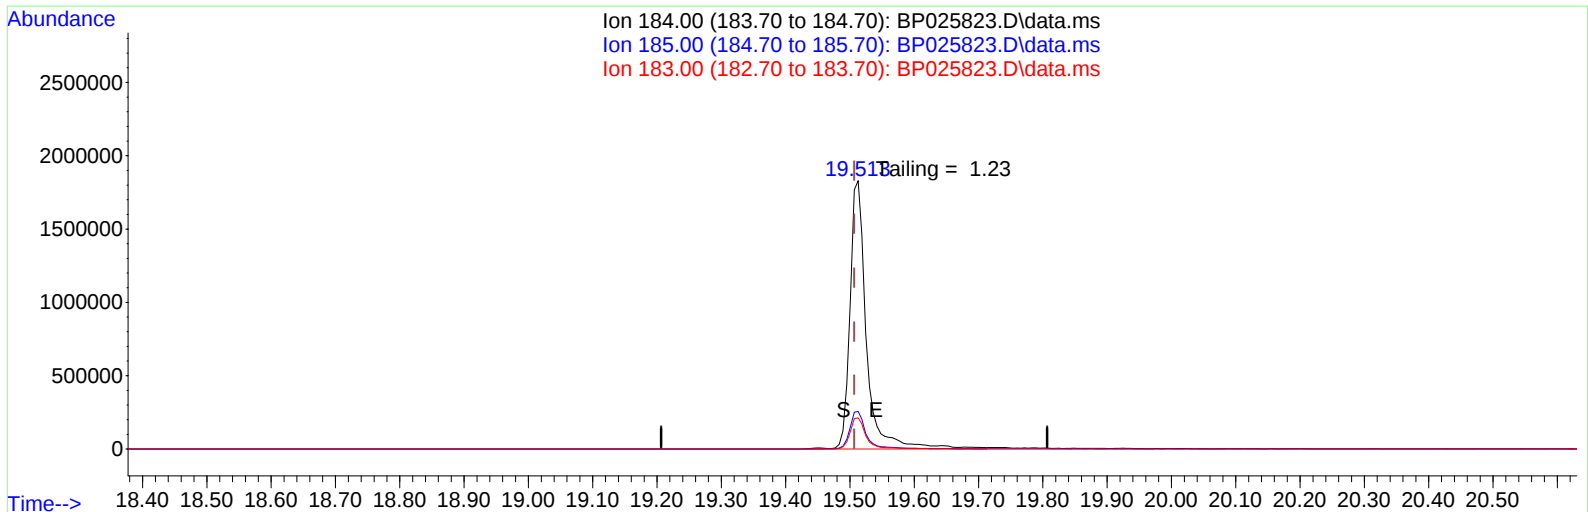

TIC: BP025823.D\data.ms

(77) Benzidine

19.513min (+ 0.006) 1208647.75 ng

response 3203028

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.05
183.00	11.50	11.63
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/23/2025	BNA_P	<u>BP025823.D</u>
Compound Name	Response	Retention Time
DDT	1692869	20.789
DDD	20863	20.33
DDE	303	19.983
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21166	1714035	1.23

Instrument :
BNA_P
ClientSampleId :
DFTPP