

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092325\
 Data File : BP025828.D
 Acq On : 23 Sep 2025 13:48
 Operator : CG/JU
 Sample : PB169774BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB169774BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP025828.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.914	330	336	349	rBV	574471	820813	4.61%	1.164%
2	5.384	409	416	438	rBV	3860382	6244630	35.09%	8.854%
3	6.955	676	683	705	rBV	3334717	6171122	34.68%	8.750%
4	7.749	811	818	829	rBV	827962	1337323	7.51%	1.896%
5	8.896	1005	1013	1043	rBV	2343957	4306005	24.20%	6.105%
6	10.519	1281	1289	1308	rBV	945456	1854218	10.42%	2.629%
7	12.984	1700	1708	1733	rBV	5480868	9382902	52.72%	13.303%
8	14.372	1936	1944	1960	rBV	1382542	2571630	14.45%	3.646%
9	15.895	2194	2203	2222	rBV	4060008	8025980	45.10%	11.379%
10	17.178	2414	2421	2436	rBV	1819891	3493450	19.63%	4.953%
11	19.901	2877	2884	2898	rBV	12325651	17796532	100.00%	25.232%
12	21.636	3172	3179	3191	rBV2	2443982	4576971	25.72%	6.489%
13	25.001	3742	3751	3767	rBV	1224290	3949354	22.19%	5.599%




Sum of corrected areas: 70530930

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092325\
Data File : BP025828.D
Acq On : 23 Sep 2025 13:48
Operator : CG/JU
Sample : PB169774BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB169774BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

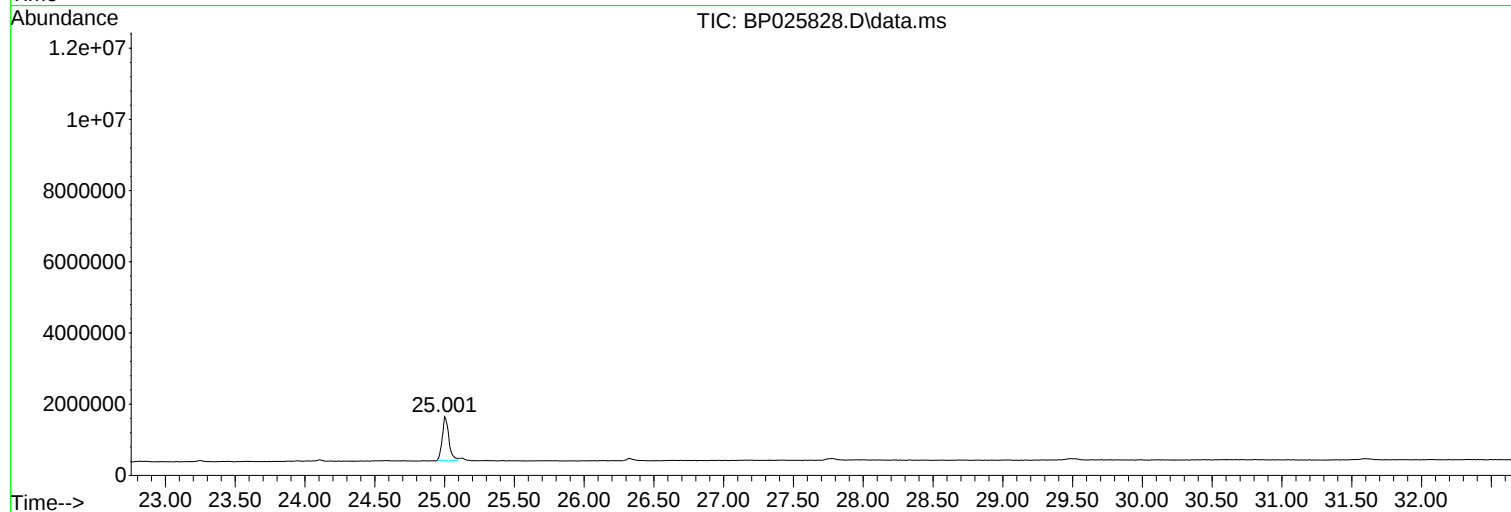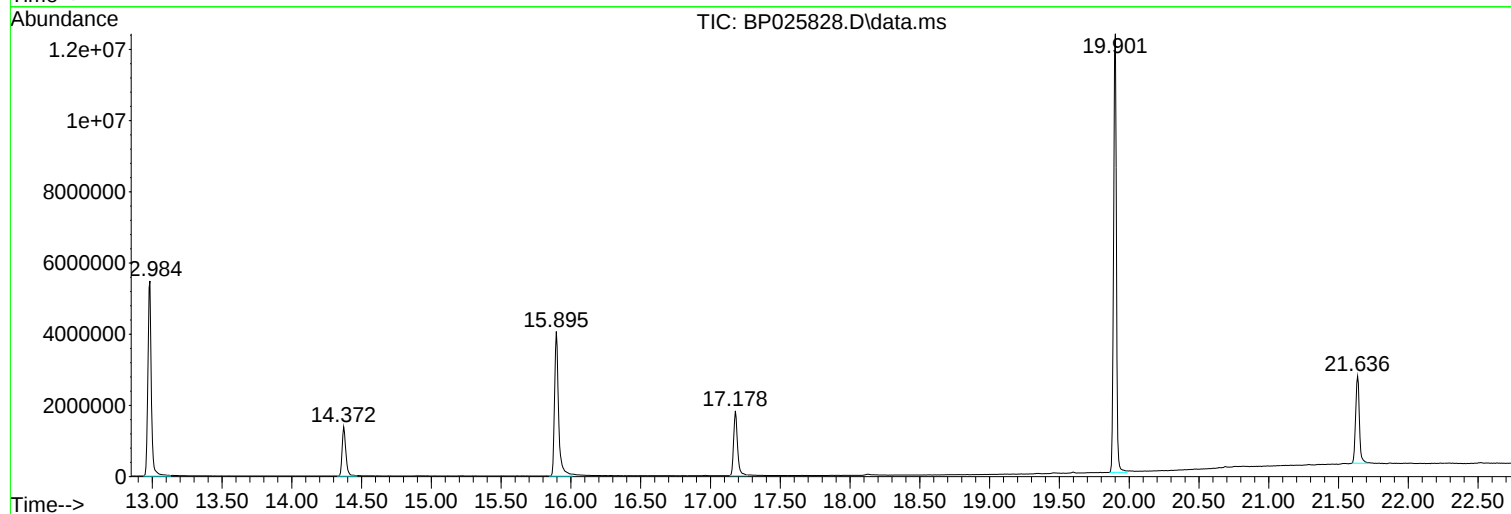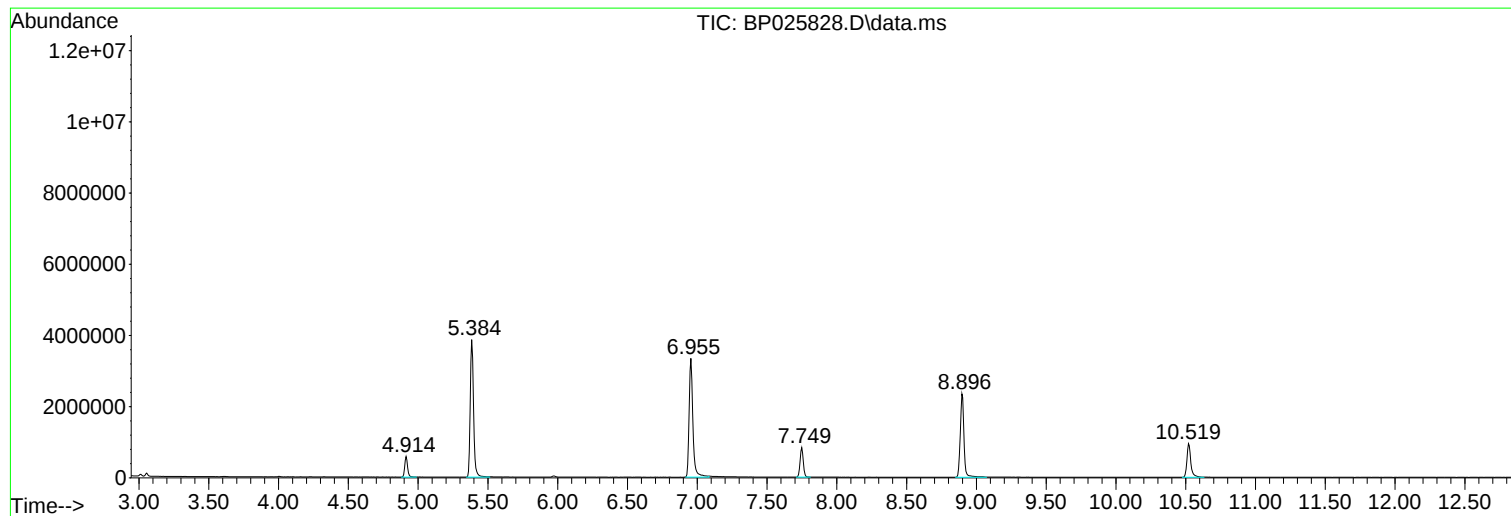

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092325\
Data File : BP025828.D
Acq On : 23 Sep 2025 13:48
Operator : CG/JU
Sample : PB169774BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB169774BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092325\
Data File : BP025828.D
Acq On : 23 Sep 2025 13:48
Operator : CG/JU
Sample : PB169774BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB169774BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------