


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092225\
Data File : BG064417.D
Acq On : 22 Sep 2025 16:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 28 17:41:58 2025

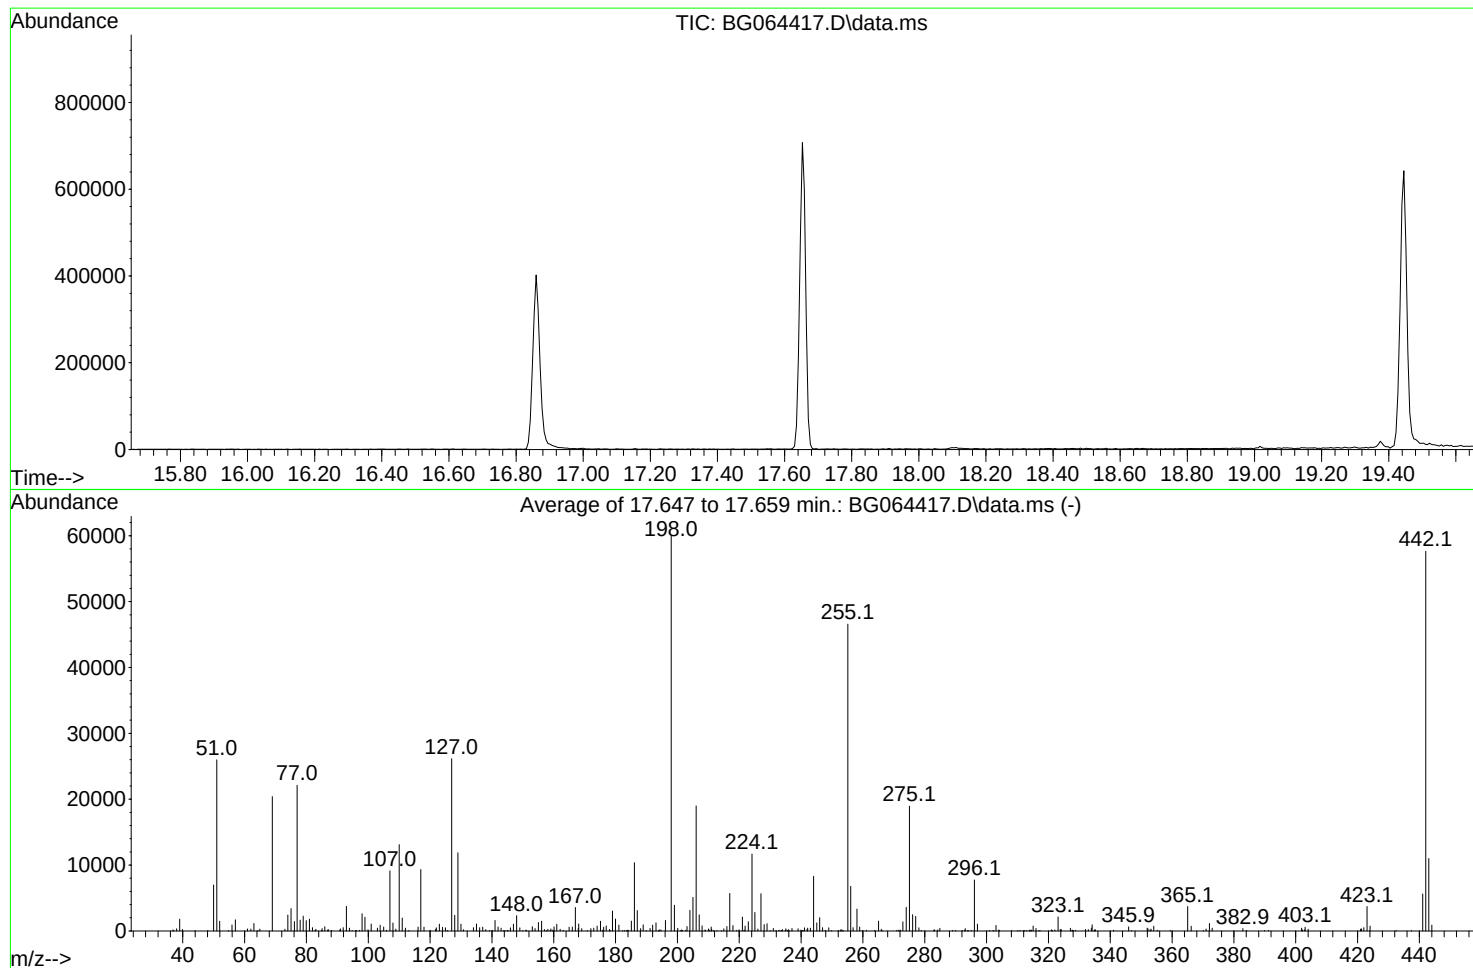

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	20392	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59949	PASS
199	198	5	9	6.5	3908	PASS
365	198	1	100	6.2	3694	PASS
441	443	0.01	150	51.0	5607	PASS
442	442	100	100	100.0	57651	PASS
443	442	15	24	19.1	10987	PASS