
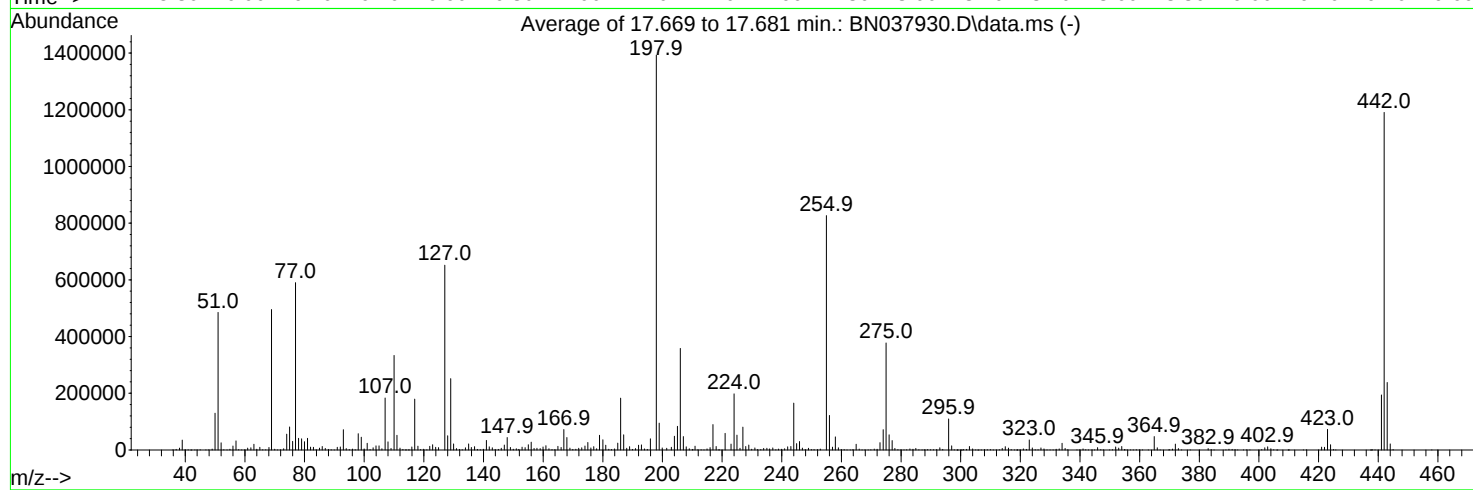


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092925\
Data File : BN037930.D
Acq On : 29 Sep 2025 10:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 24 11:00:01 2025

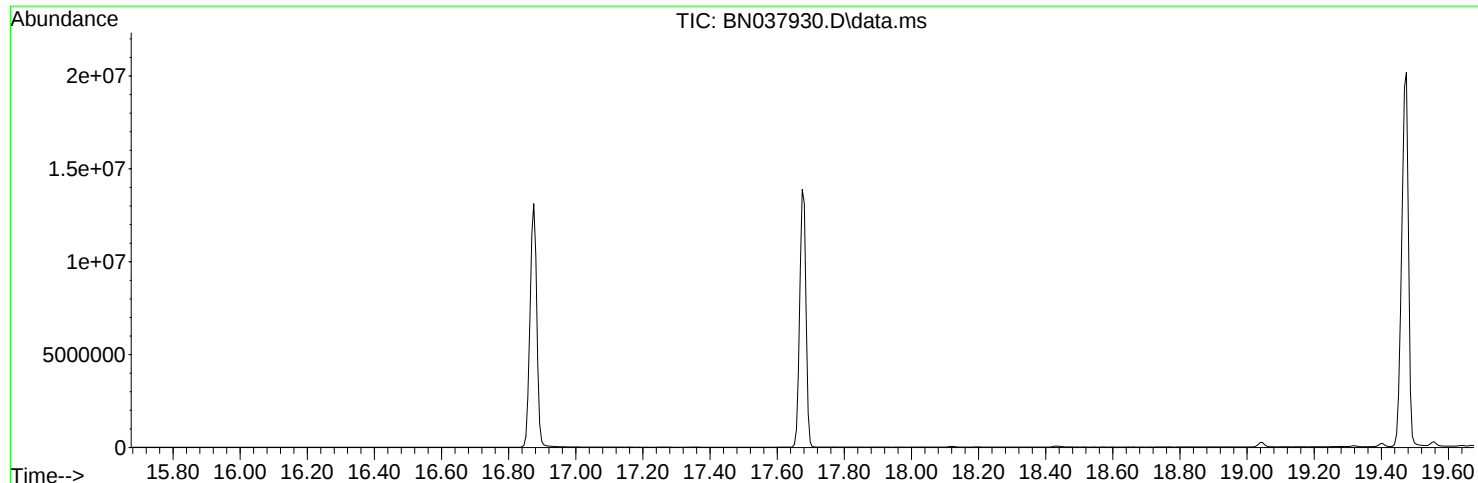




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.8	8960	PASS
69	69	100	100	100.0	495262	PASS
70	69	0.00	2	0.5	2469	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	1392981	PASS
199	198	5	9	6.8	94760	PASS
365	198	1	100	3.4	47144	PASS
441	443	0.01	150	81.6	193963	PASS
442	442	100	100	100.0	1190699	PASS
443	442	15	24	20.0	237845	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092925\
Data File : BN037930.D
Acq On : 29 Sep 2025 10:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 29 11:50:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

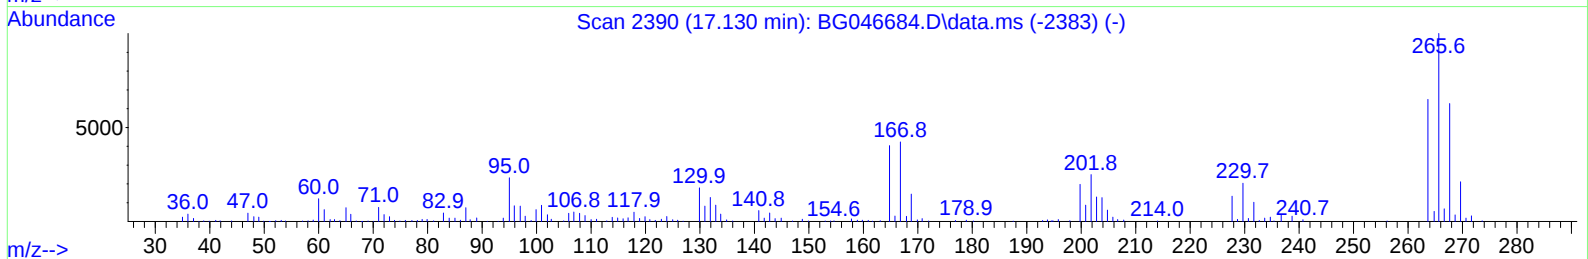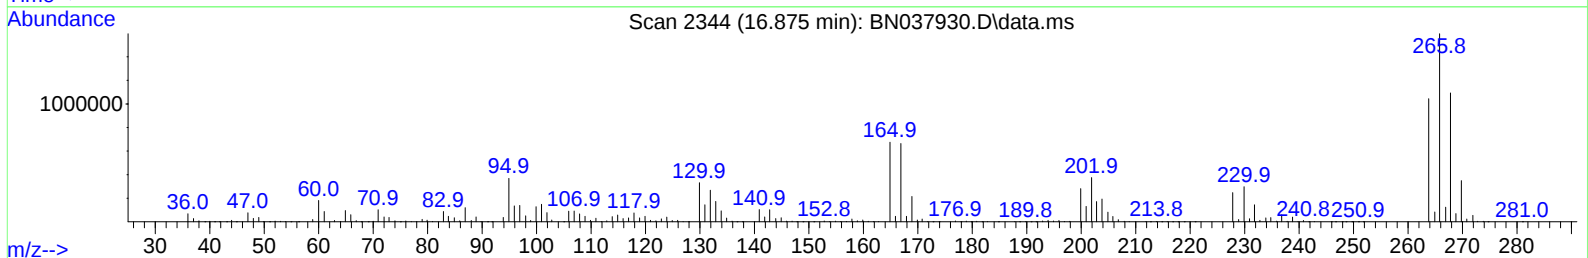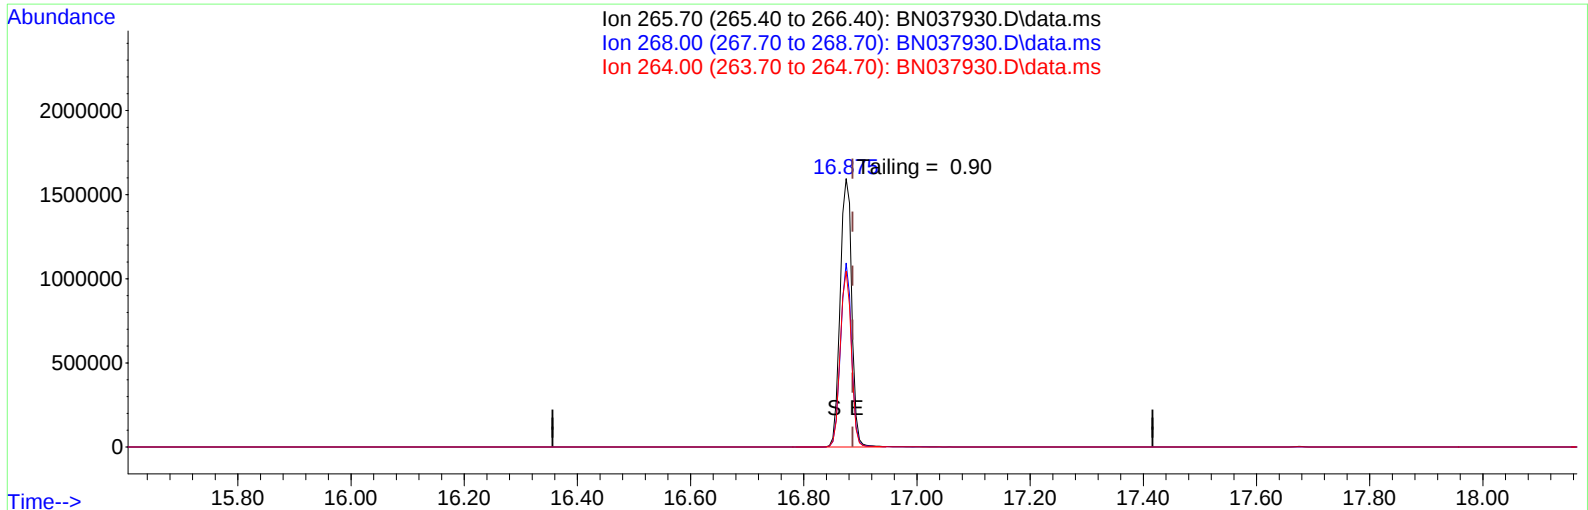

TIC: BN037930.D\data.ms

(70) Pentachlorophenol (C)

16.875min (-0.011) 35044.31 ng




response 2284032

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.49
264.00	61.60	65.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092925\
Data File : BN037930.D
Acq On : 29 Sep 2025 10:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 29 11:50:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

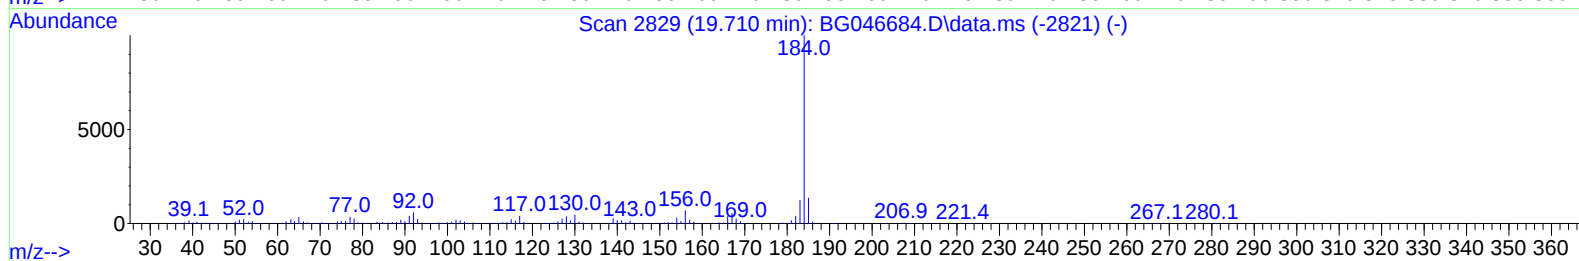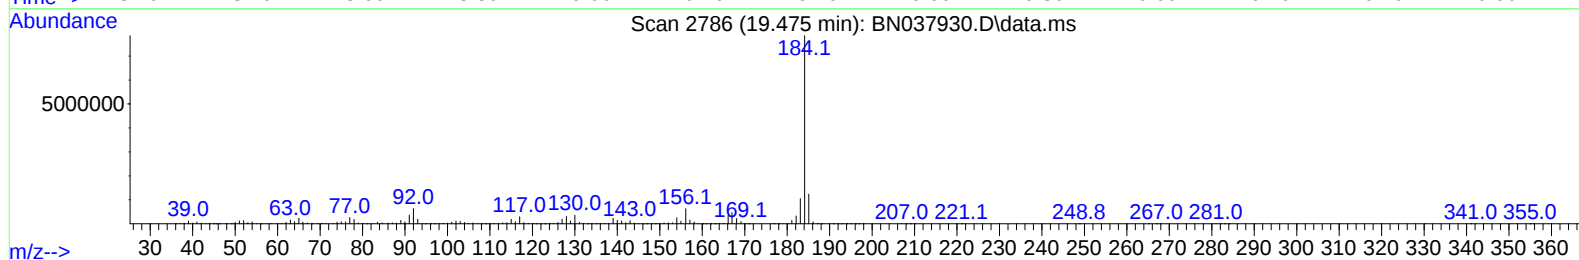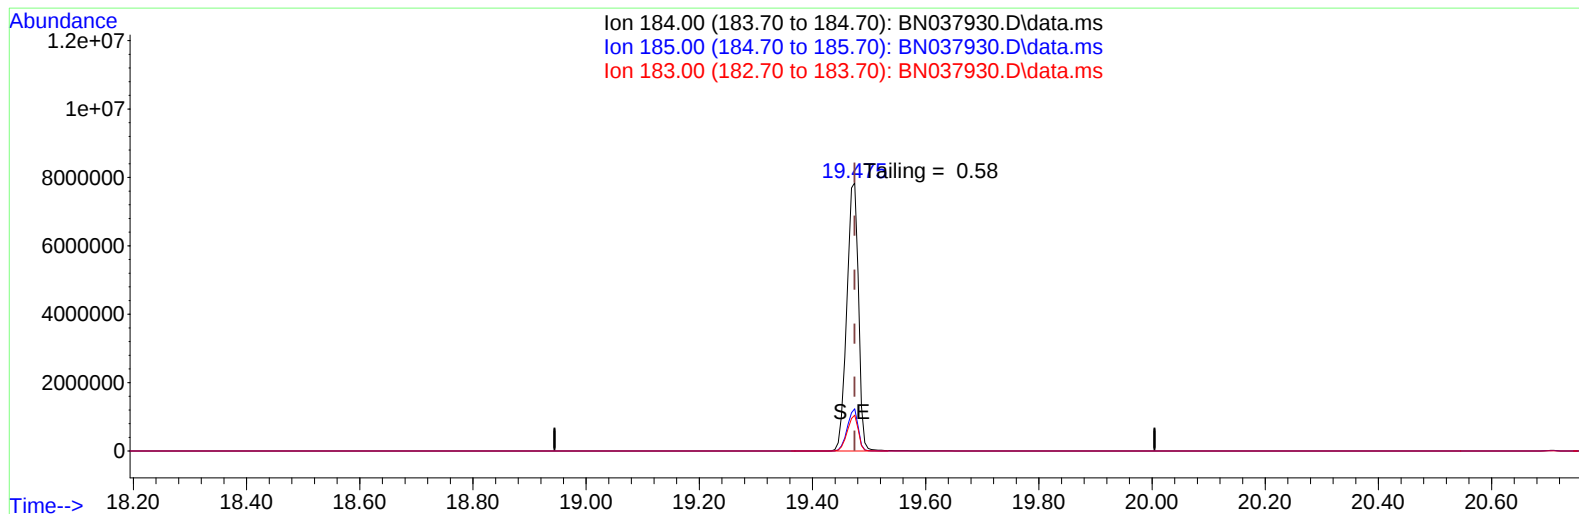

TIC: BN037930.D\data.ms

(77) Benzidine

19.475min (+ 0.001) 0.00 ng

response 11301983

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.77
183.00	13.20	13.39
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/29/2025	BNA_N	<u>BN037930.D</u>
Compound Name	Response	Retention Time
DDT	5429934	20.71
DDD	31482	20.263
DDE	733	19.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
32215	5462149	0.59

Instrument :
BNA_N
ClientSampleId :
DFTPP