

Instrument IC-1		Analyst: RM		Method: 300.0 / 9056A						
Ident	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4	Method name	date time	Initial v Analyst
STD1	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-090925	9/9/2025 10:21	10 RM/IZ
STD2	0.423	0.641	0.632	2.091	0.529	1.063	3.237	IC1-090925	9/9/2025 10:42	10 RM/IZ
STD3	0.794	1.189	1.197	3.984	0.997	2.006	6.010	IC1-090925	9/9/2025 11:25	10 RM/IZ
STD4	0.990	1.475	1.473	4.920	1.228	2.461	7.371	IC1-090925	9/9/2025 11:47	10 RM/IZ
STD5	2.008	3.012	3.027	10.105	2.514	4.978	15.047	IC1-090925	9/9/2025 13:36	10 RM/IZ
STD6	3.935	5.921	5.894	19.658	4.924	9.905	29.203	IC1-090925	9/9/2025 13:58	10 RM/IZ
STD7	5.050	7.561	7.577	25.243	6.308	12.587	37.633	IC1-090925	9/9/2025 14:41	10 RM/IZ
ICV	2.001	2.995	2.988	9.985	2.483	5.041	14.797	IC1-090925	9/9/2025 15:02	10 RM/IZ
ICB	0.000	0.063	0.000	0.000	0.000	0.000	0.000	IC1-090925	9/9/2025 15:45	10 RM/IZ
CCV	1.973	2.936	2.983	10.016	2.431	4.563	14.776	IC1-090925	9/24/2025 9:20	10 RM/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-090925	9/24/2025 9:42	10 RM/IZ
LB137286BLW	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-090925	9/24/2025 10:03	10 RM/IZ
LB137286BSW	2.012	2.938	2.985	10.029	2.434	4.658	14.682	IC1-090925	9/24/2025 10:25	10 RM/IZ
Q3172-01	0.138	164.811	0.000	2.918	0.000	0.000	200.990	IC1-090925	9/24/2025 10:46	10 RM/IZ
Q3168-05	0.053	55.307	0.000	0.000	0.000	0.000	1.690	IC1-090925	9/24/2025 11:08	10 RM/IZ
Q3168-05MS	2.074	56.598	2.963	11.049	2.436	4.980	16.176	IC1-090925	9/24/2025 11:29	10 RM/IZ
Q3168-05MSD	2.051	56.211	2.959	10.965	2.428	5.204	16.108	IC1-090925	9/24/2025 11:51	10 RM/IZ
Q3168-06	0.054	49.652	0.000	1.151	0.000	0.000	1.313	IC1-090925	9/24/2025 12:13	10 RM/IZ
Q3172-01DLX10	0.000	12.707	0.000	0.404	0.000	0.000	16.952	IC1-090925	9/24/2025 12:34	10 RM/IZ
CCV	2.002	2.941	2.996	10.046	2.440	5.051	14.693	IC1-090925	9/24/2025 12:56	10 RM/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-090925	9/24/2025 13:17	10 RM/IZ


Clear table

Instrument ID: IC-2 Analyst: IZ Method: 300.0 / 9056A											
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentratio n HPO4	concentrati on SO4	file name	date time	Initial wt/ Final	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-090925	9/9/2025 10:21	10	RM/IZ
STD2	0.4230	0.6410	0.6320	2.0910	0.5290	1.0630	3.2370	IC1-090925	9/9/2025 10:42	10	RM/IZ
STD3	0.7940	1.1890	1.1970	3.9840	0.9970	2.0060	6.0100	IC1-090925	9/9/2025 11:25	10	RM/IZ
STD4	0.9900	1.4750	1.4730	4.9200	1.2280	2.4610	7.3710	IC1-090925	9/9/2025 11:47	10	RM/IZ
STD5	2.0080	3.0120	3.0270	10.1050	2.5140	4.9780	15.0470	IC1-090925	9/9/2025 13:36	10	RM/IZ
STD6	3.9350	5.9210	5.8940	19.6580	4.9240	9.9050	29.2030	IC1-090925	9/9/2025 13:58	10	RM/IZ
STD7	5.0500	7.5610	7.5770	25.2430	6.3080	12.5870	37.6330	IC1-090925	9/9/2025 14:41	10	RM/IZ

ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000

ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4
STD1							
STD2	5.7500	6.8333	5.3333	4.5500	5.8000	6.3000	7.9000
STD3	-0.7500	-0.9167	-0.2500	-0.4000	-0.3000	0.3000	0.1667
STD4	-1.0000	-1.6667	-1.8000	-1.6000	-1.7600	-1.5600	-1.7200
STD5	0.4000	0.4000	0.9000	1.0500	0.5600	-0.4400	0.3133
STD6	-1.6250	-1.3167	-1.7667	-1.7100	-1.5200	-0.9500	-2.6567
STD7	1.0000	0.8133	1.0267	0.9720	0.9280	0.6960	1.7108

Fluoride (Anions)

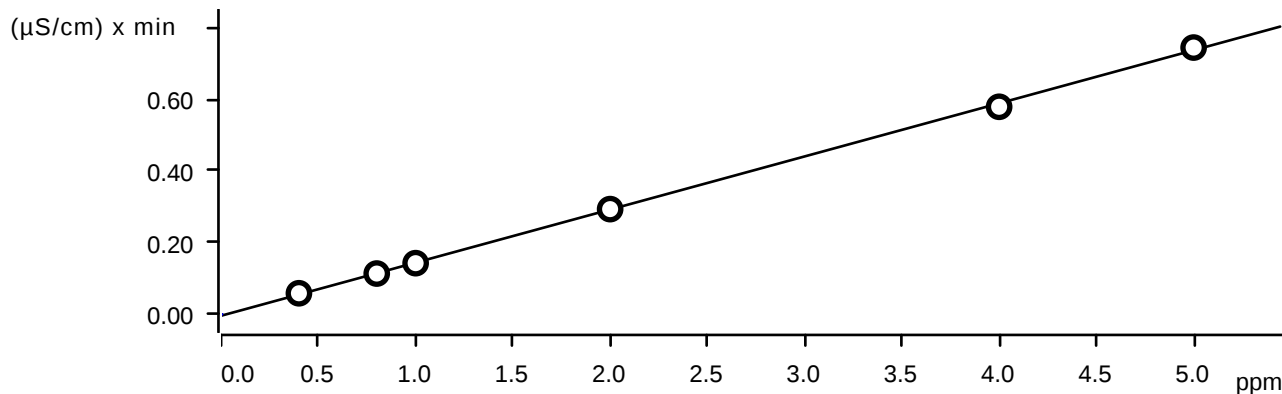


Function: $A = -3.91674E-3 + 0.0148053 \times Q$

Relative standard deviation 1.985504 %

Correlation coefficient 0.999790

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.059	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.114	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.143	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.293	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.579	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.744	STD7	2025-09-09 14:41:06 UTC-4	used

Chloride (Anions)

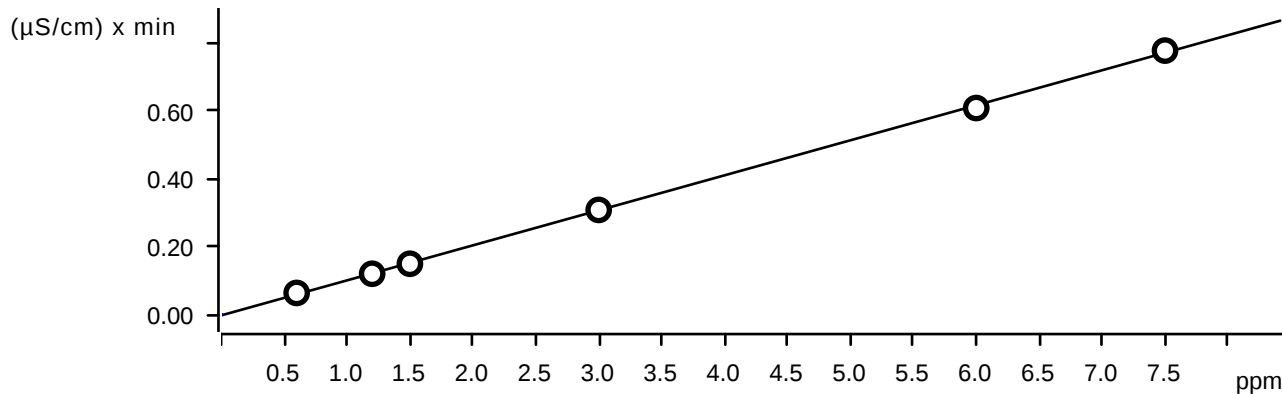


Function: $A = -2.97735E-3 + 0.0103068 \times Q$

Relative standard deviation 1.712968 %

Correlation coefficient 0.999843

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.063	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.120	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.149	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.307	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.607	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.776	STD7	2025-09-09 14:41:06 UTC-4	used

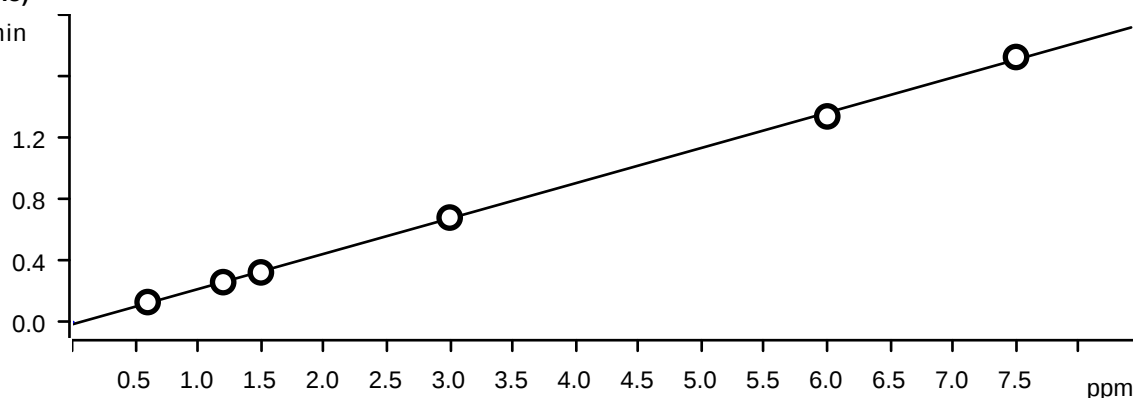Nitrite (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0143669 + 0.0229543 \times Q$


Relative standard deviation 2.170764 %

Correlation coefficient 0.999753

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.131	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.260	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.324	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.681	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.339	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.725	STD7	2025-09-09 14:41:06 UTC-4	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

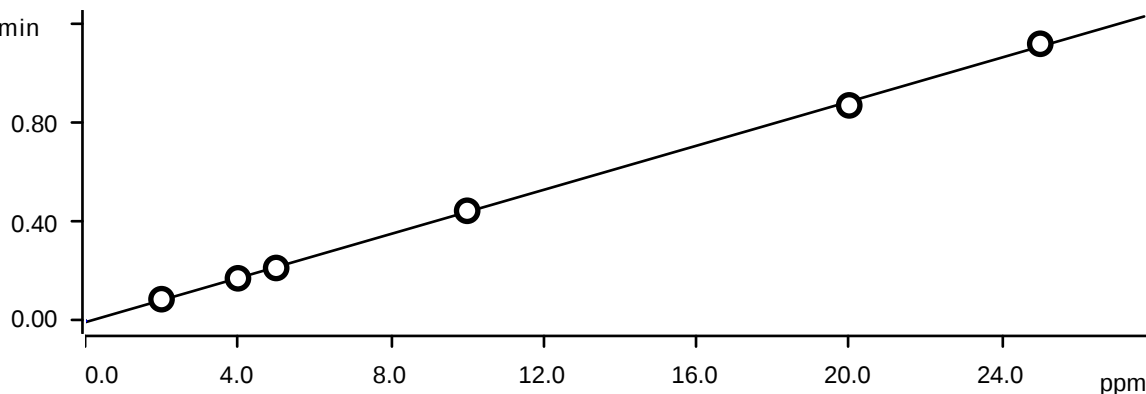

Function: $A = -5.68247E-3 + 4.44287E-3 \times Q$


Relative standard deviation: 2.066849 %

Correlation coefficient: 0.999773

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.087	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.171	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.213	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.443	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.868	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.116	STD7	2025-09-09 14:41:06 UTC-4	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

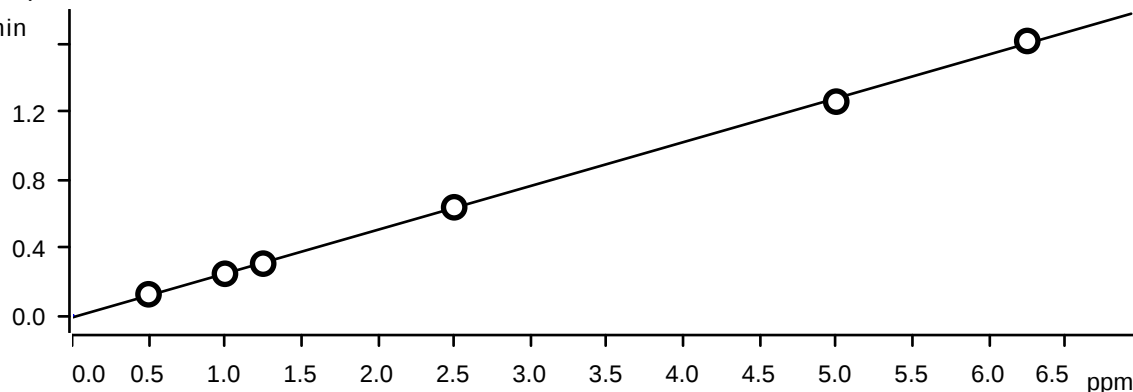


Function: $A = -0.0122982 + 0.0258010 \times Q$

Relative standard deviation: 1.914251 %

Correlation coefficient 0.999807

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.124	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.245	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.305	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.636	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.258	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.615	STD7	2025-09-09 14:41:06 UTC-4	used

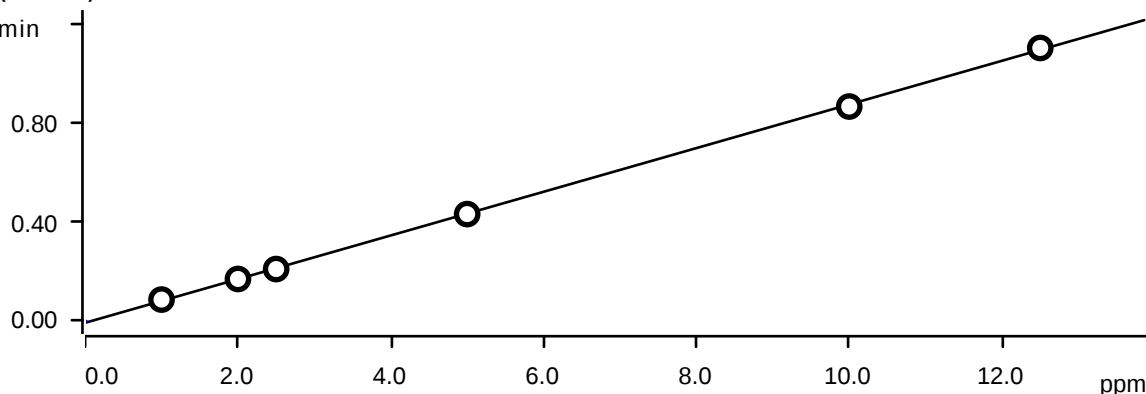
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -6.72192E-3 + 8.79335E-3 \times Q$

Relative standard deviation 1.384046 %

Correlation coefficient 0.999898

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.087	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.170	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.210	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.431	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.864	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.100	STD7	2025-09-09 14:41:06 UTC-4	used

Sulfate (Anions)

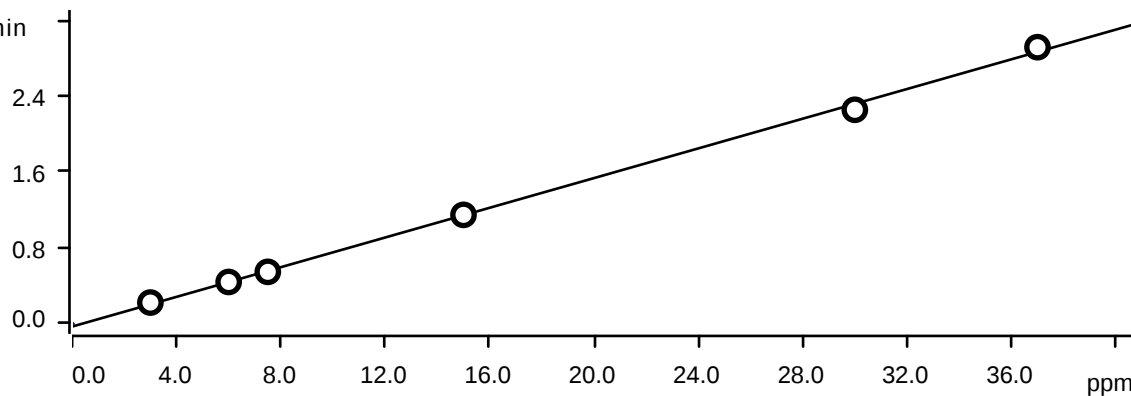 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0295615 + 7.81954E-3 \times Q$

Relative standard deviation 3.285067 %

Correlation coefficient 0.999433

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.224	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.440	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.547	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.147	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.254	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.913	STD7	2025-09-09 14:41:06 UTC-4	used


Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-09-09 10:21:26 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 13.06 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

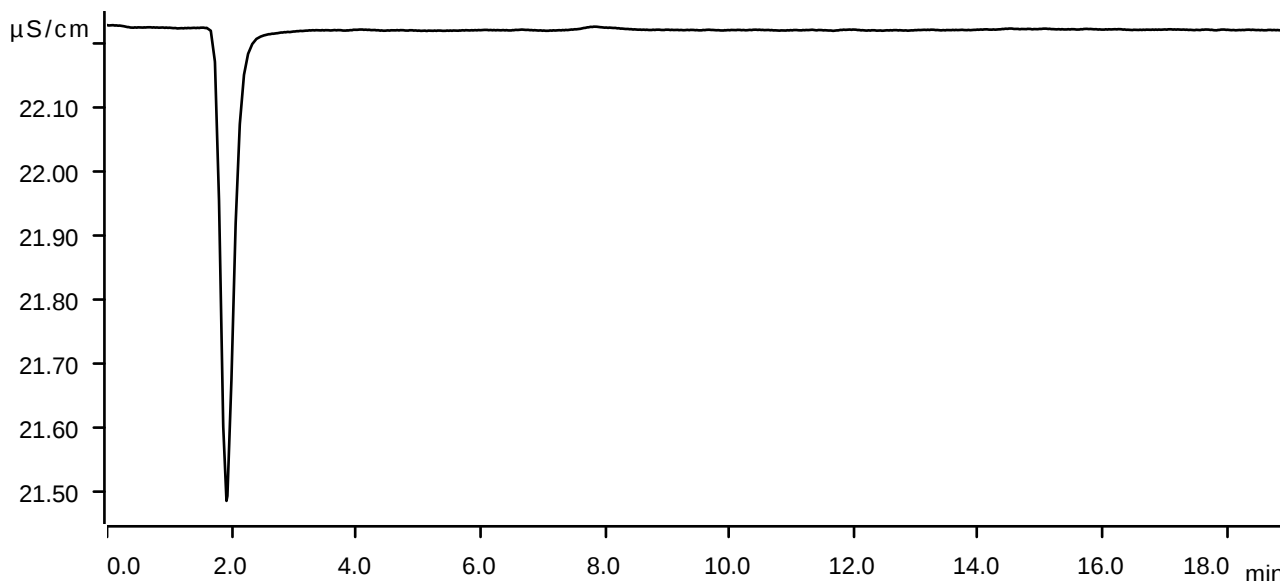


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-09-09 10:42:49 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.84 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

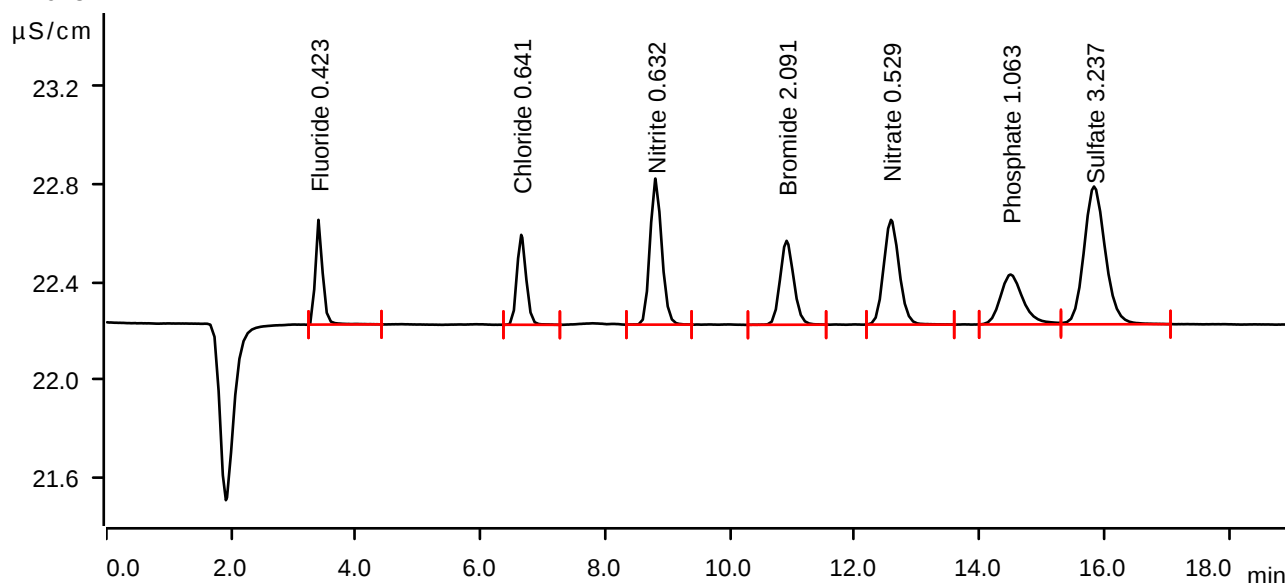

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.400	0.0587	0.429	0.423	Fluoride
2	6.652	0.0631	0.369	0.641	Chloride
3	8.803	0.1306	0.599	0.632	Nitrite
4	10.907	0.0872	0.344	2.091	Bromide
5	12.580	0.1242	0.430	0.529	Nitrate
6	14.497	0.0867	0.205	1.063	Phosphate
7	15.835	0.2236	0.565	3.237	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-09-09 11:25:44 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.67 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

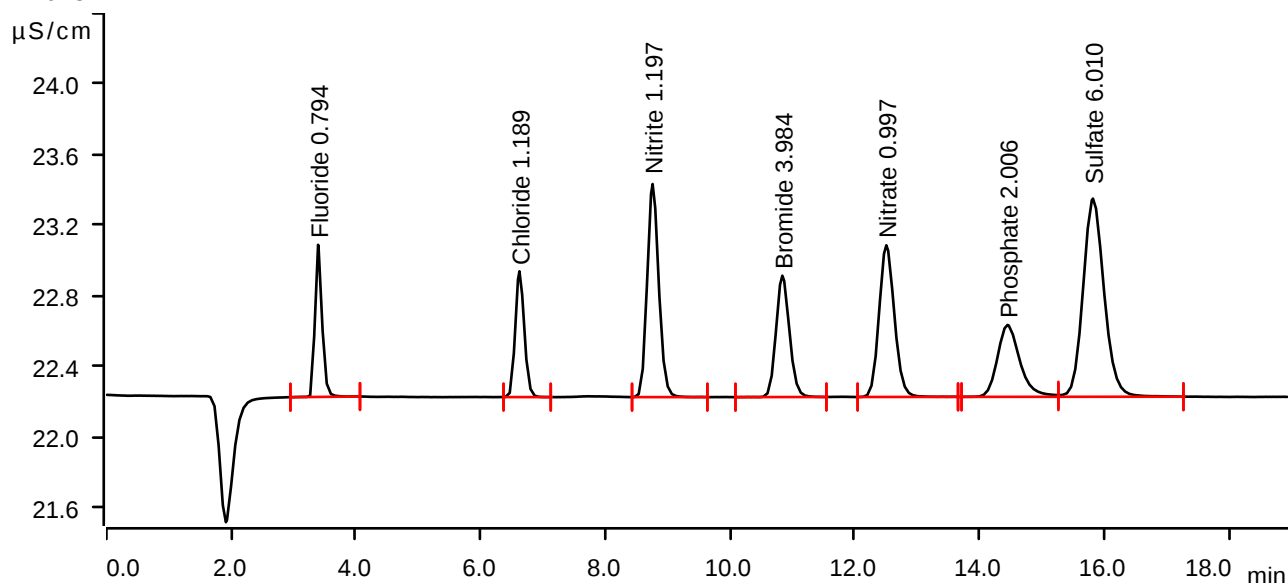

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.395	0.1137	0.861	0.794	Fluoride
2	6.623	0.1196	0.712	1.189	Chloride
3	8.758	0.2603	1.206	1.197	Nitrite
4	10.838	0.1713	0.687	3.984	Bromide
5	12.505	0.2450	0.859	0.997	Nitrate
6	14.448	0.1697	0.407	2.006	Phosphate
7	15.818	0.4404	1.122	6.010	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-09-09 11:47:10 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.61 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

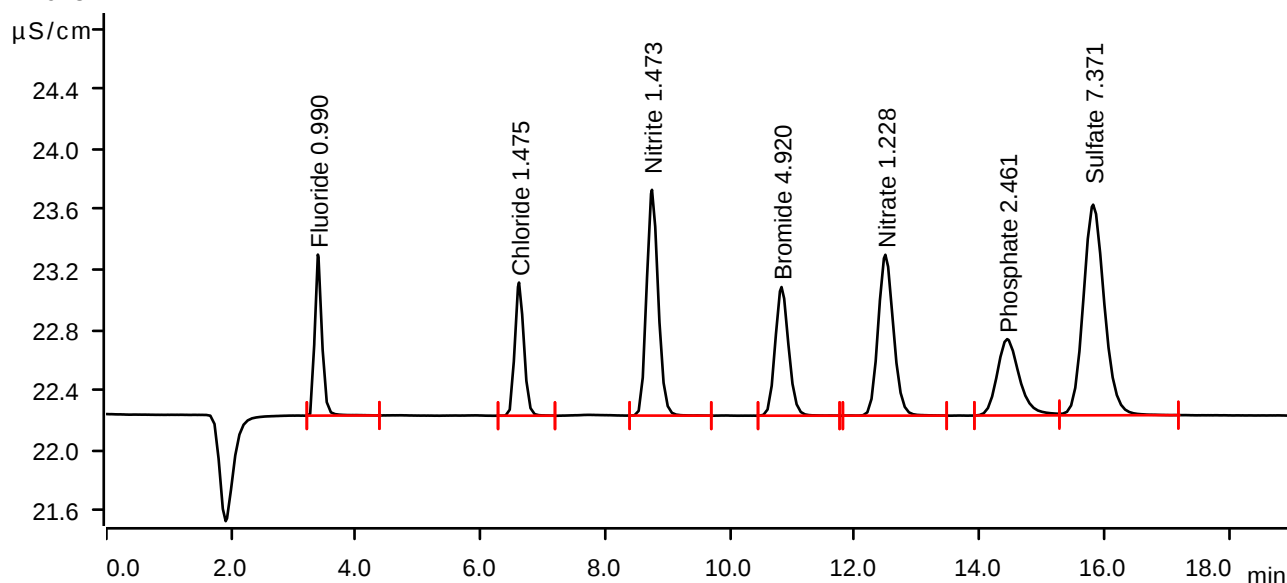

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.392	0.1426	1.068	0.990	Fluoride
2	6.617	0.1490	0.884	1.475	Chloride
3	8.748	0.3238	1.499	1.473	Nitrite
4	10.825	0.2129	0.854	4.920	Bromide
5	12.490	0.3046	1.068	1.228	Nitrate
6	14.443	0.2097	0.507	2.461	Phosphate
7	15.822	0.5468	1.398	7.371	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2025-09-09 13:36:36 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.50 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

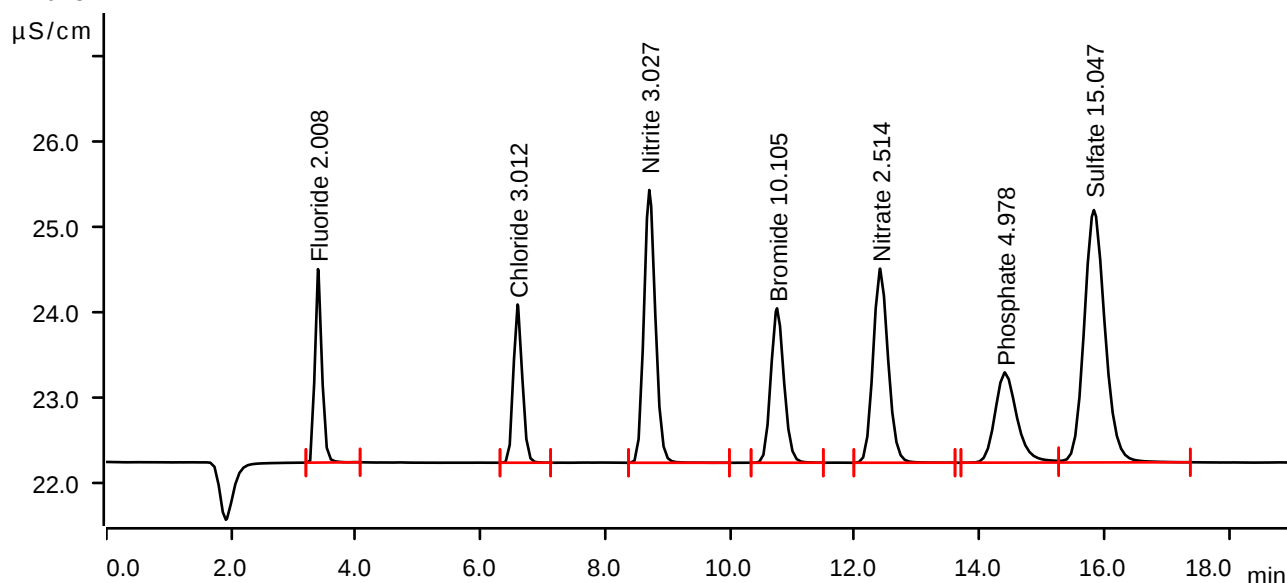

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.393	0.2933	2.266	2.008	Fluoride
2	6.593	0.3075	1.854	3.012	Chloride
3	8.705	0.6805	3.195	3.027	Nitrite
4	10.753	0.4432	1.809	10.105	Bromide
5	12.407	0.6363	2.273	2.514	Nitrate
6	14.405	0.4310	1.057	4.978	Phosphate
7	15.833	1.1470	2.956	15.047	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-09-09 13:58:07 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

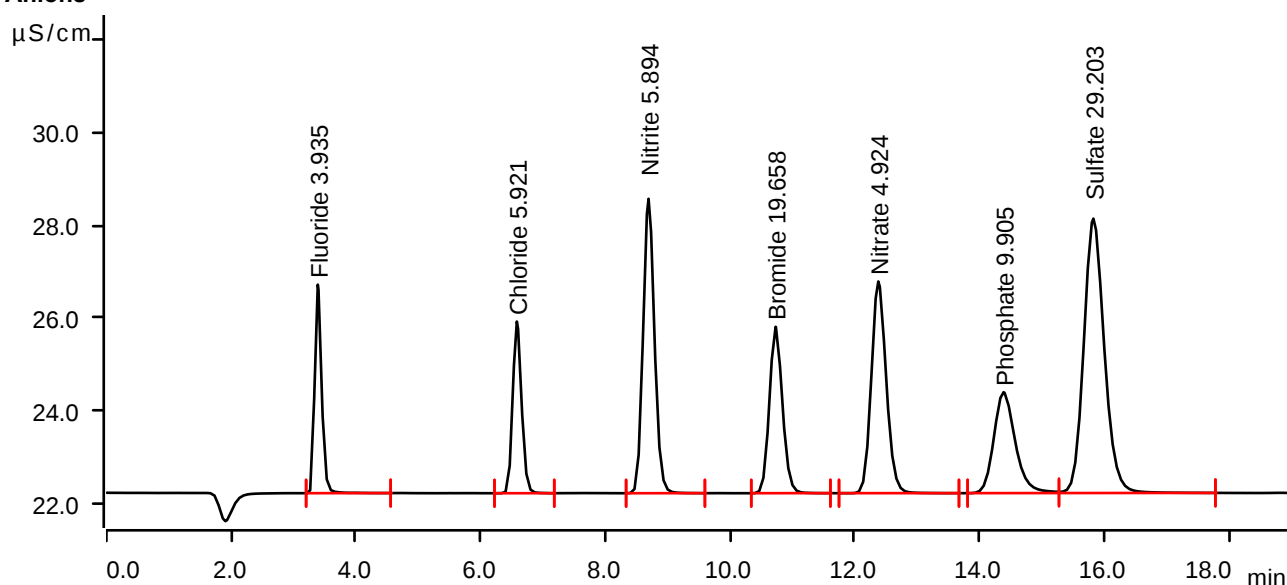

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.390	0.5787	4.477	3.935	Fluoride
2	6.582	0.6073	3.687	5.921	Chloride
3	8.693	1.3385	6.323	5.894	Nitrite
4	10.730	0.8677	3.574	19.658	Bromide
5	12.377	1.2581	4.546	4.924	Nitrate
6	14.385	0.8642	2.167	9.905	Phosphate
7	15.825	2.2540	5.893	29.203	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-09-09 14:41:06 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

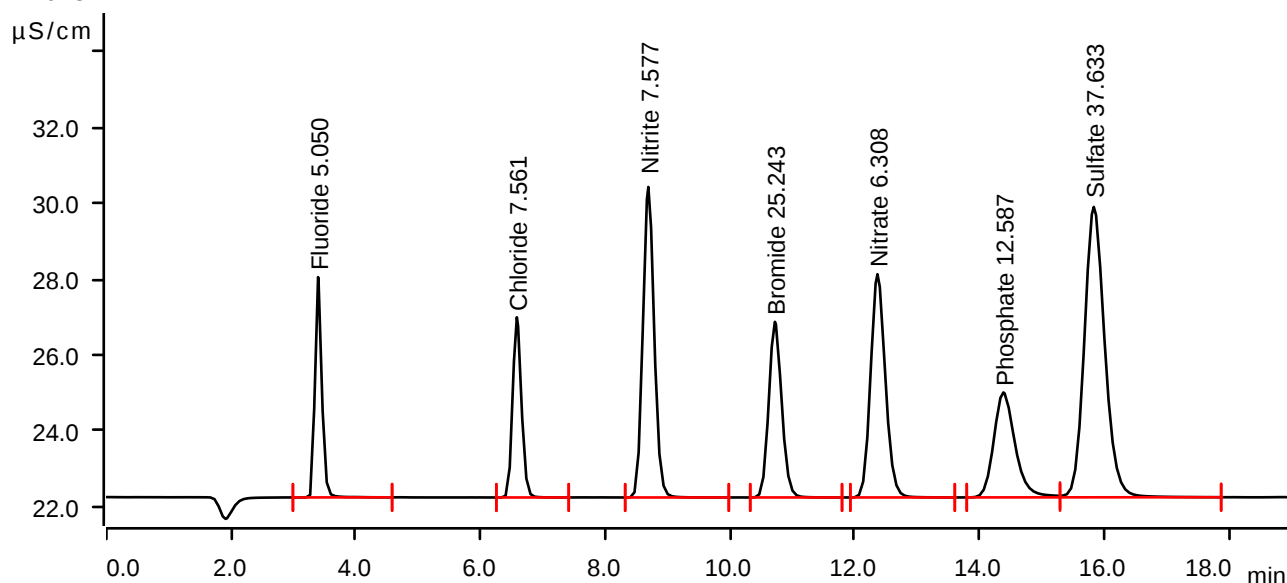

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.395	0.7438	5.806	5.050	Fluoride
2	6.582	0.7764	4.748	7.561	Chloride
3	8.690	1.7250	8.184	7.577	Nitrite
4	10.718	1.1158	4.629	25.243	Bromide
5	12.363	1.6152	5.884	6.308	Nitrate
6	14.382	1.1001	2.766	12.587	Phosphate
7	15.832	2.9131	7.654	37.633	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-09-09 15:02:34 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.50 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

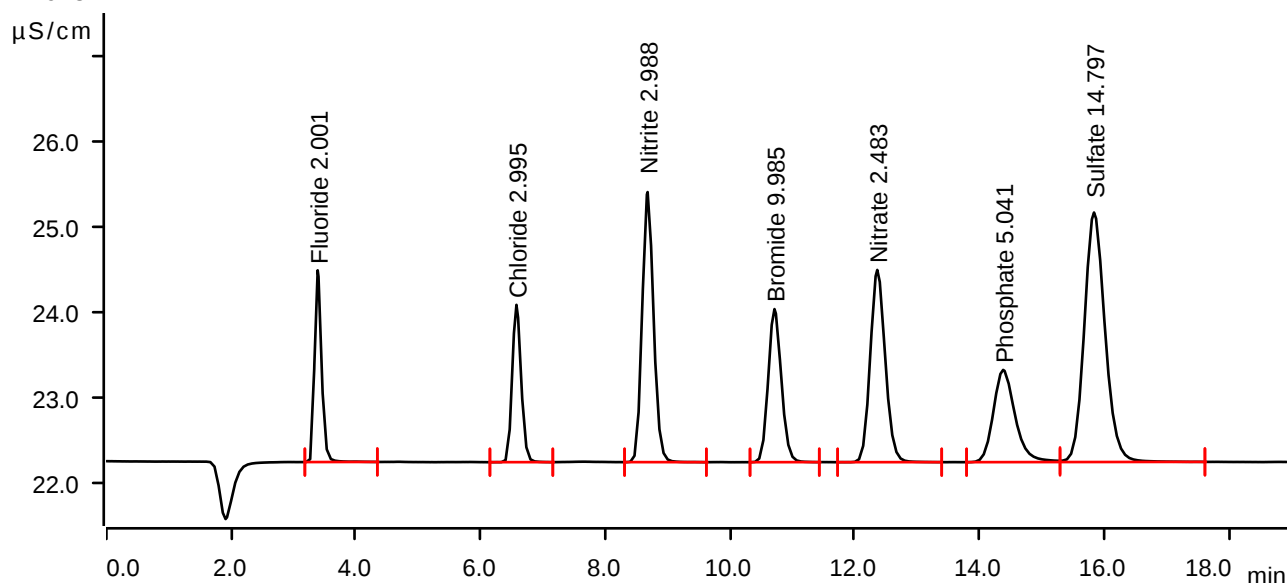

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.388	0.2923	2.246	2.001	Fluoride
2	6.575	0.3057	1.843	2.995	Chloride
3	8.678	0.6715	3.164	2.988	Nitrite
4	10.712	0.4379	1.793	9.985	Bromide
5	12.360	0.6282	2.252	2.483	Nitrate
6	14.378	0.4365	1.080	5.041	Phosphate
7	15.835	1.1275	2.923	14.797	Sulfate


Sample data

Ident ICB
Sample type Sample
Determination start 2025-09-09 15:45:30 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

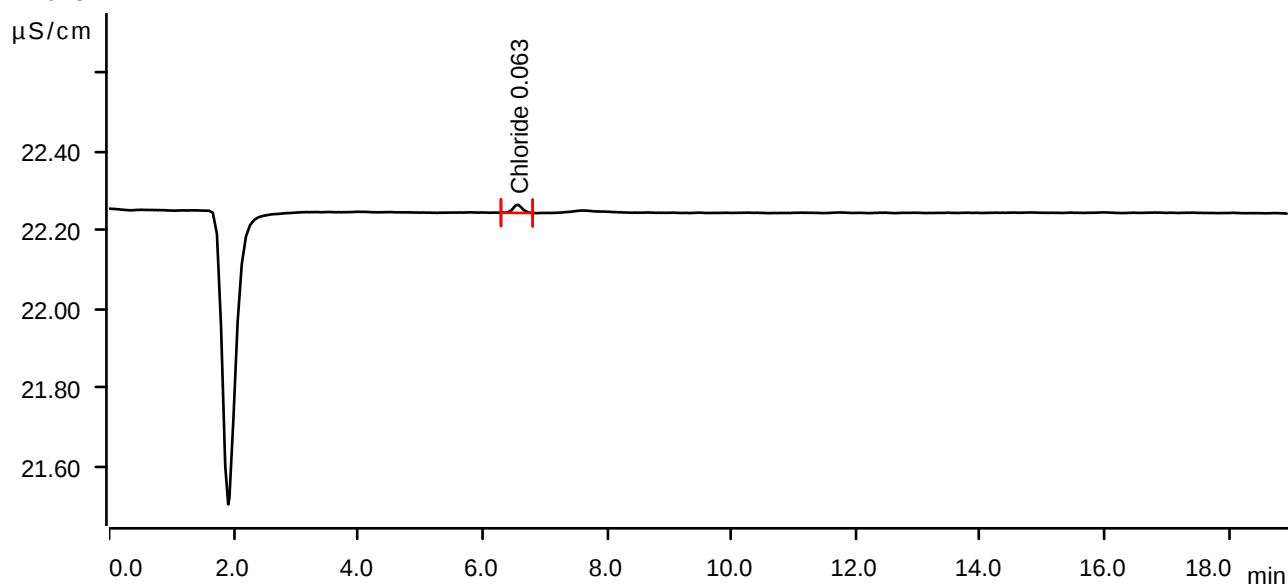

Peak number	Retention time	Area	Height	Concentration	Component name
	min	(µS/cm) x min	µS/cm	ppm	
1	6.568	0.0036	0.021	0.063	Chloride


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-09-24 09:20:39 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.05 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

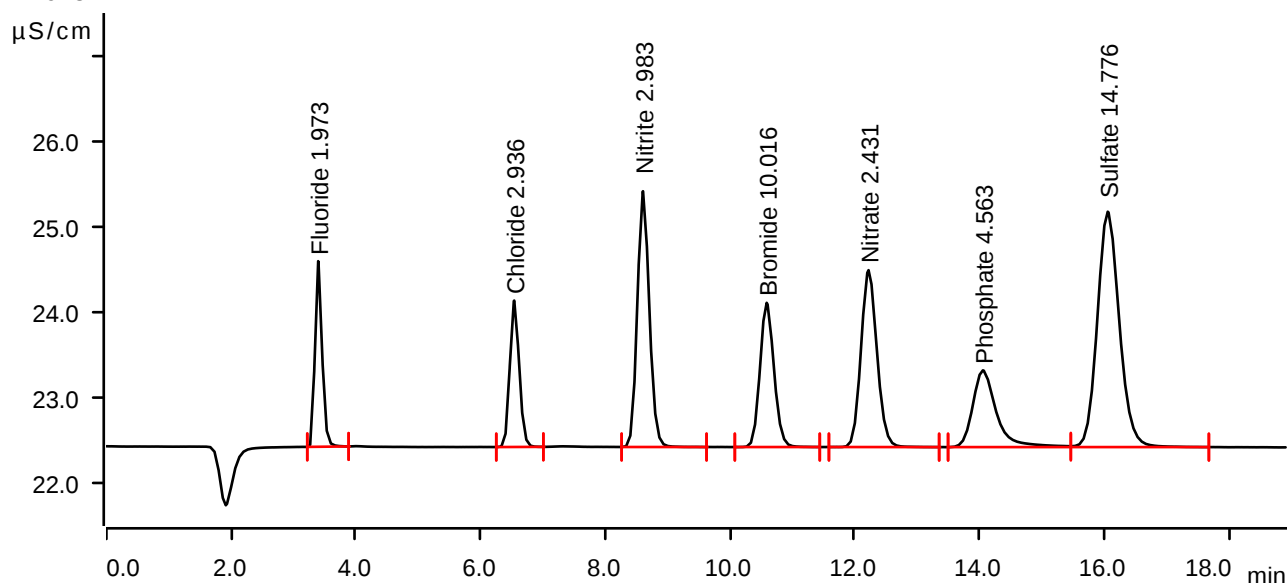


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.397	0.2883	2.174	1.973	Fluoride
2	6.540	0.2997	1.715	2.936	Chloride
3	8.605	0.6703	2.996	2.983	Nitrite
4	10.587	0.4393	1.689	10.016	Bromide
5	12.220	0.6148	2.072	2.431	Nitrate
6	14.053	0.3945	0.899	4.563	Phosphate
7	16.055	1.1259	2.757	14.776	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-09-24 09:42:10 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.05 MPa
Maximum pressure monitored yes
Temperature ---- °C

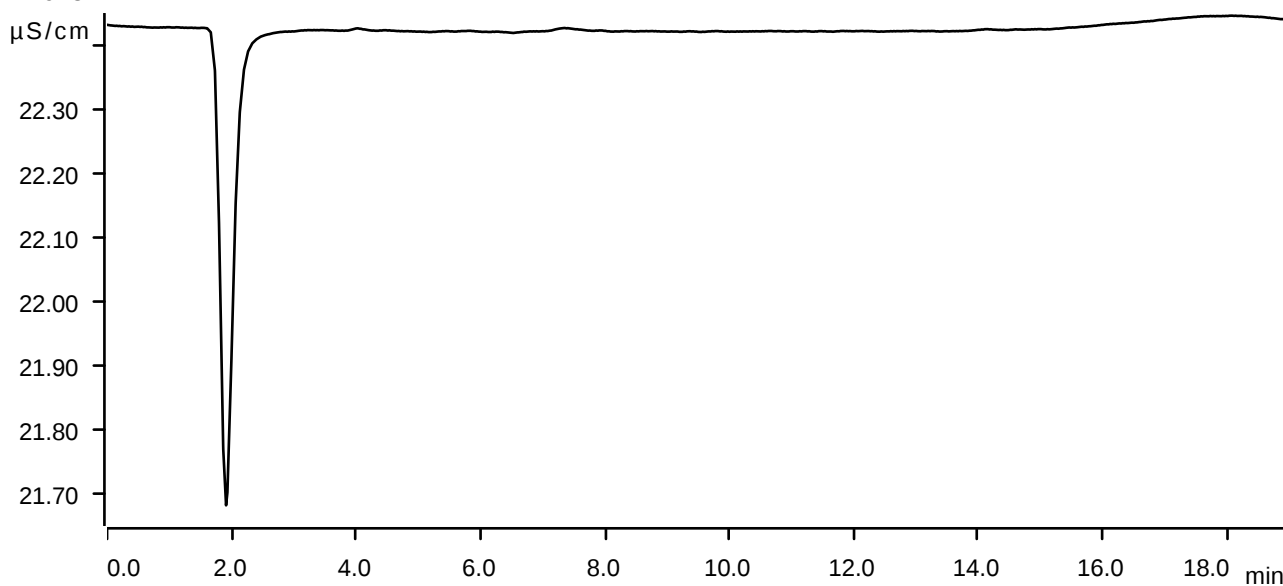
Anions

Sample data

Ident LB137286BLW
Sample type Sample
Determination start 2025-09-24 10:03:41 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

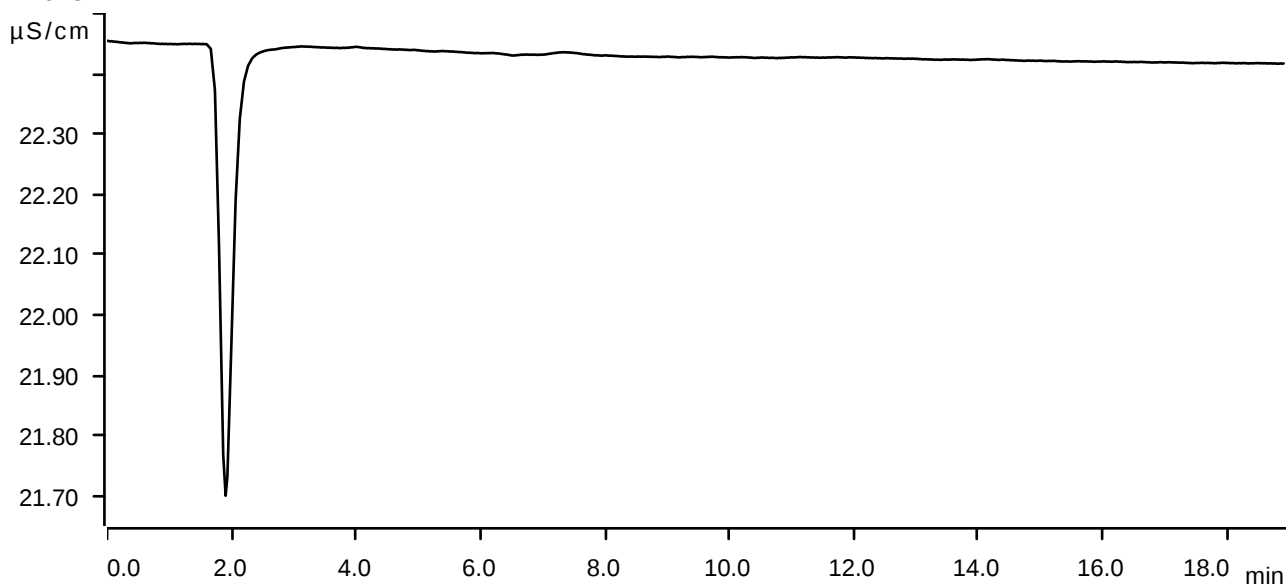Anions


Sample data

Ident LB137286BSW
Sample type Check standard 1
Determination start 2025-09-24 10:25:12 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

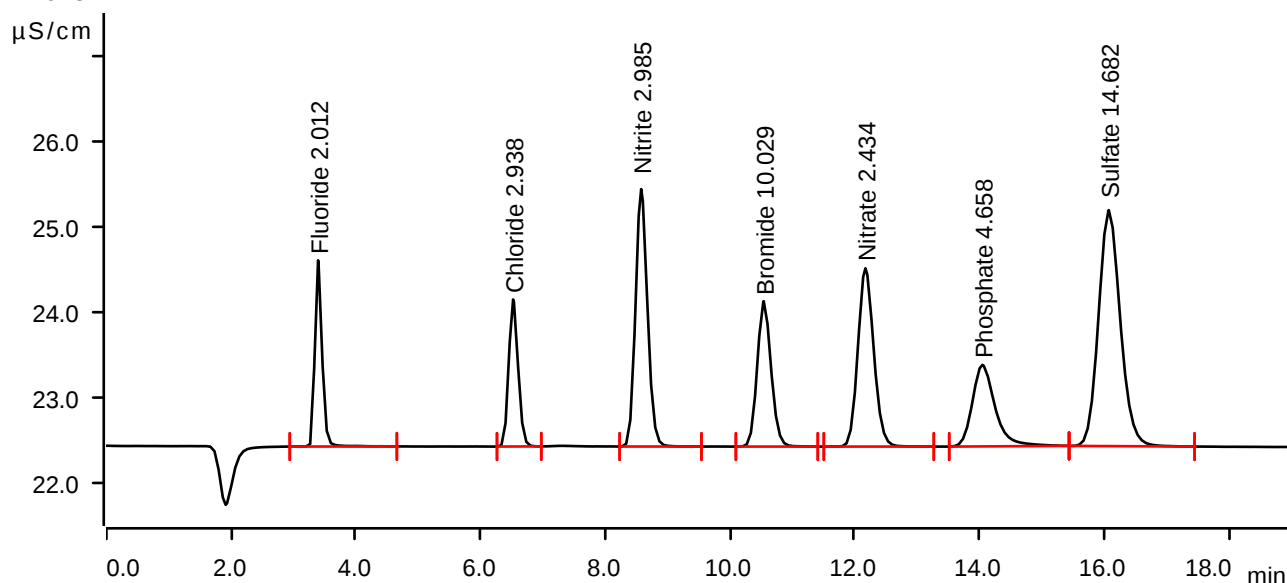

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.395	0.2939	2.181	2.012	Fluoride
2	6.522	0.2998	1.722	2.938	Chloride
3	8.575	0.6709	3.015	2.985	Nitrite
4	10.540	0.4399	1.702	10.029	Bromide
5	12.170	0.6156	2.088	2.434	Nitrate
6	14.045	0.4029	0.955	4.658	Phosphate
7	16.072	1.1185	2.764	14.682	Sulfate


Sample data

Ident Q3172-01
Sample type Sample
Determination start 2025-09-24 10:46:45 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

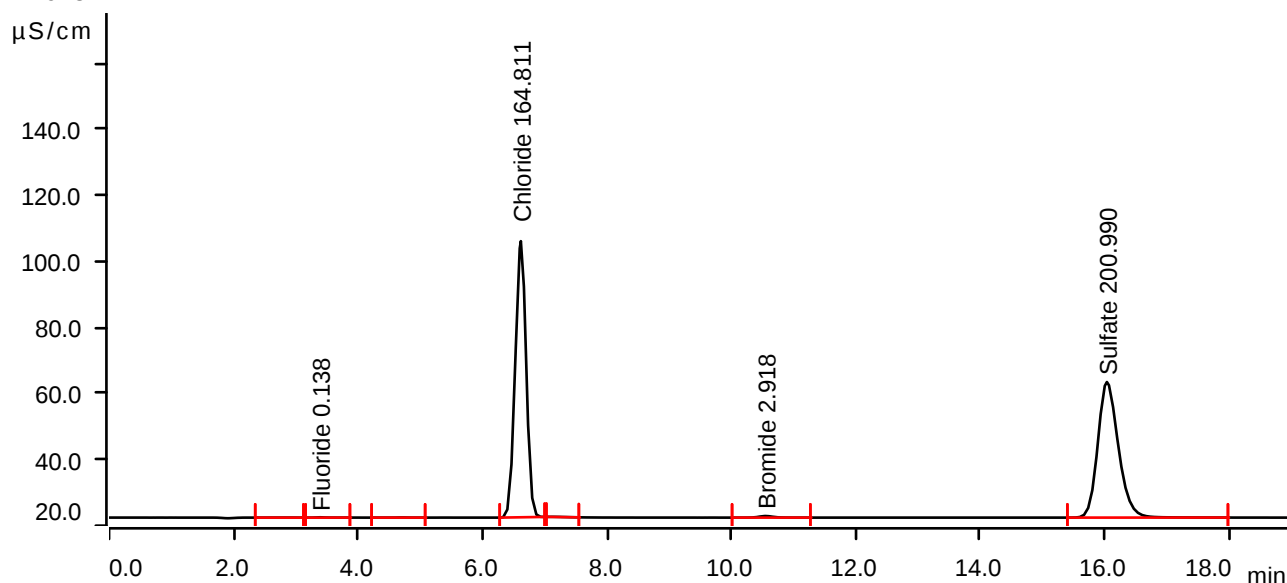

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	2.777	0.0072	0.014	invalid	
2	3.390	0.0166	0.105	0.138	Fluoride
3	4.697	0.0075	0.044	invalid	
4	6.618	16.9837	83.553	164.811	Chloride
5	7.115	0.0132	0.042	invalid	
6	10.548	0.1240	0.483	2.918	Bromide
7	16.035	15.6869	41.034	200.990	Sulfate


Sample data

Ident Q3168-05
Sample type Sample
Determination start 2025-09-24 11:08:20 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

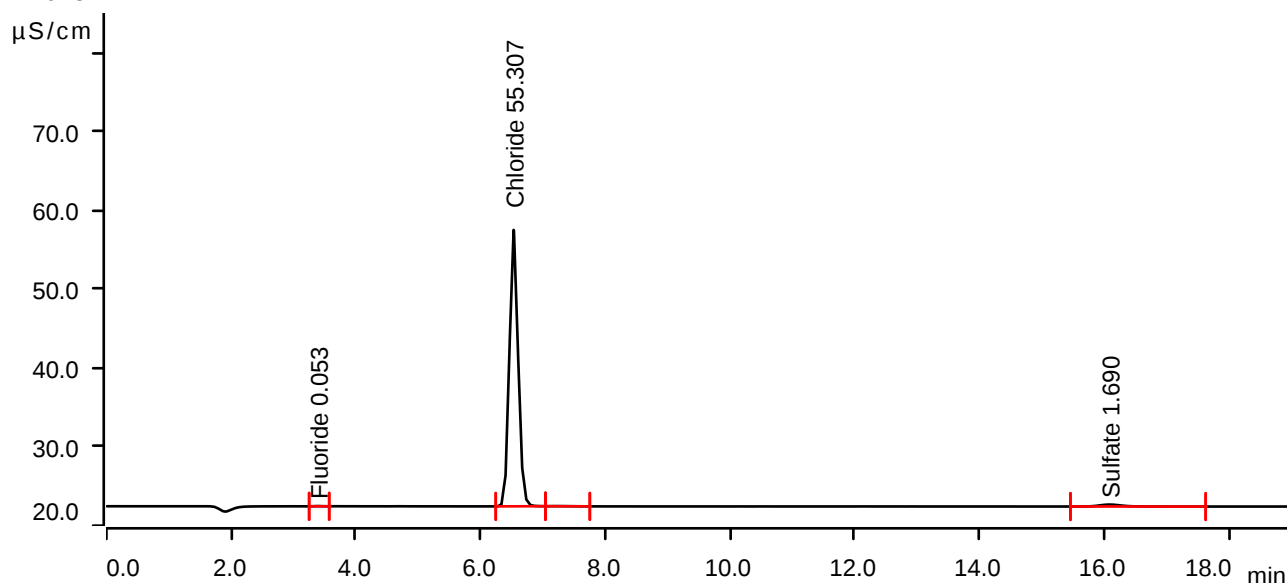

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.390	0.0040	0.031	0.053	Fluoride
2	6.530	5.6974	35.076	55.307	Chloride
3	7.235	0.0054	0.015	invalid	
4	16.083	0.1026	0.249	1.690	Sulfate


Sample data

Ident Q3168-05MS
Sample type Sample
Determination start 2025-09-24 11:29:53 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

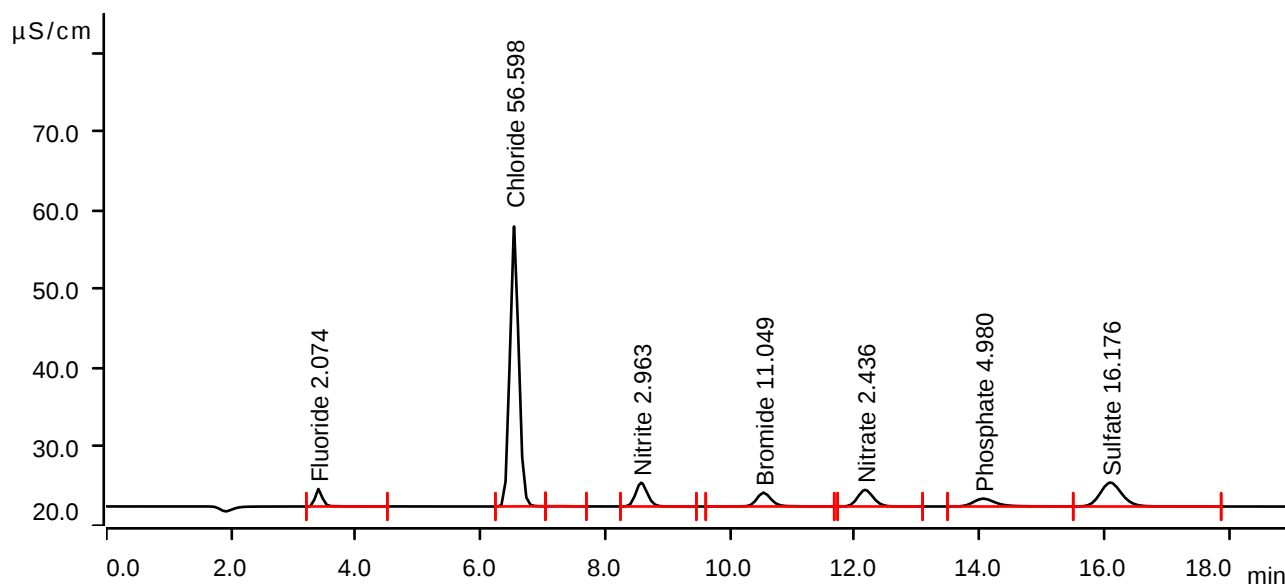

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.398	0.3032	2.217	2.074	Fluoride
2	6.538	5.8305	35.528	56.598	Chloride
3	7.257	0.0056	0.017	invalid	
4	8.575	0.6658	3.010	2.963	Nitrite
5	10.535	0.4852	1.766	11.049	Bromide
6	12.165	0.6163	2.104	2.436	Nitrate
7	14.058	0.4312	0.999	4.980	Phosphate
8	16.097	1.2353	3.041	16.176	Sulfate


Sample data

Ident Q3168-05MSD
Sample type Sample
Determination start 2025-09-24 11:51:27 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

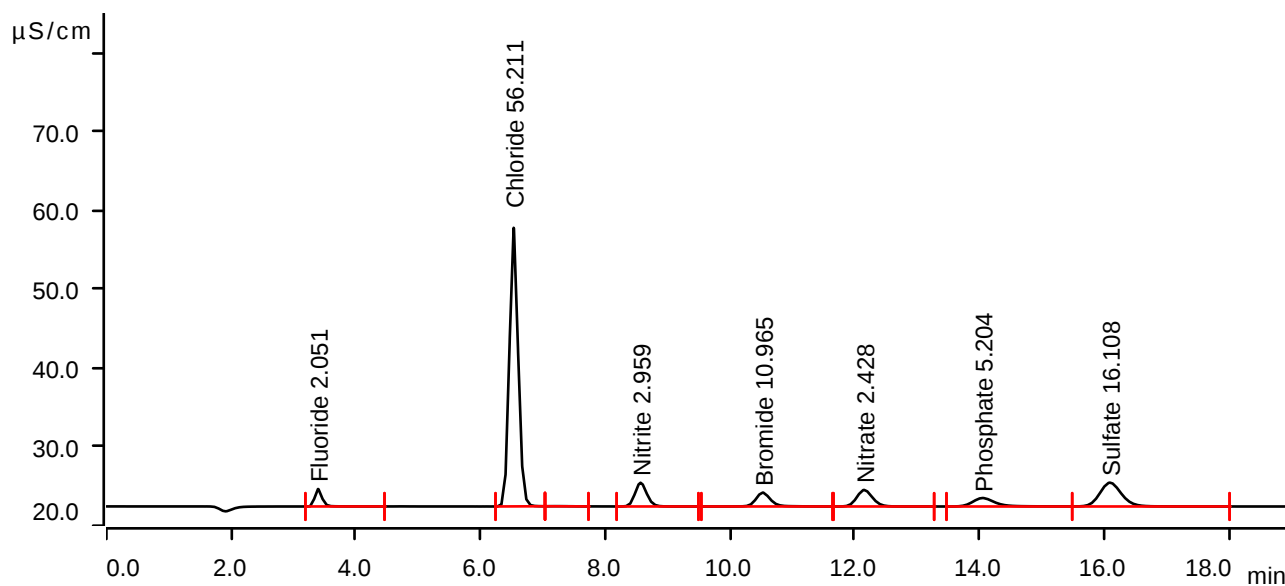

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.393	0.2997	2.214	2.051	Fluoride
2	6.530	5.7906	35.354	56.211	Chloride
3	7.245	0.0057	0.017	invalid	
4	8.565	0.6649	3.009	2.959	Nitrite
5	10.523	0.4815	1.763	10.965	Bromide
6	12.150	0.6140	2.098	2.428	Nitrate
7	14.048	0.4509	1.074	5.204	Phosphate
8	16.090	1.2300	3.026	16.108	Sulfate


Sample data

Ident Q3168-06
Sample type Sample
Determination start 2025-09-24 12:13:02 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

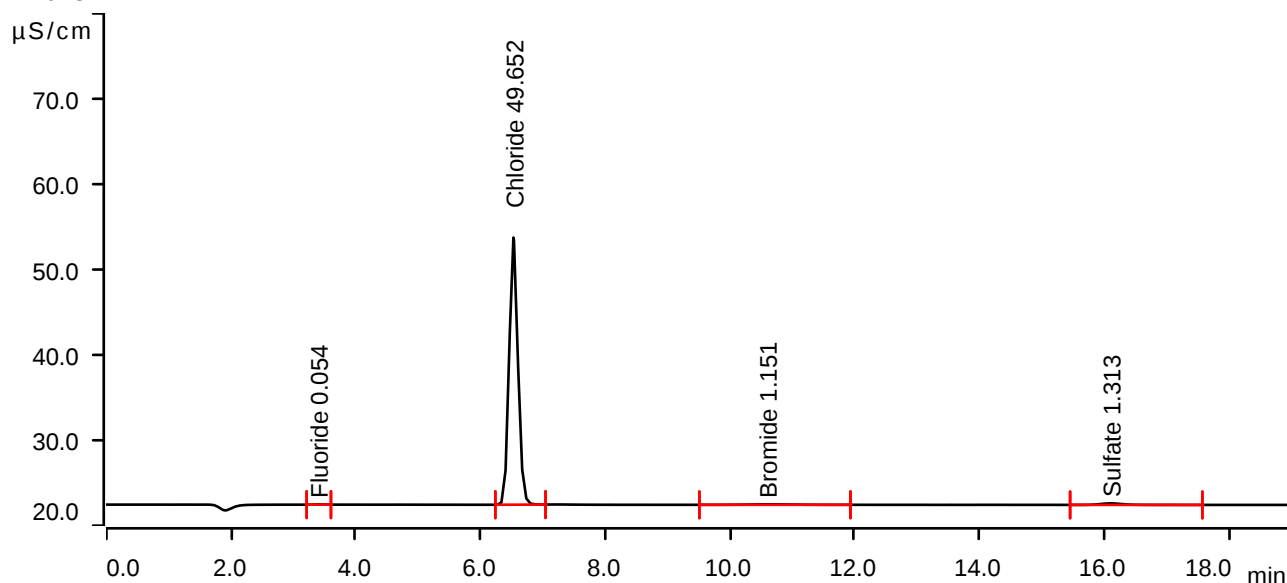

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.390	0.0041	0.031	0.054	Fluoride
2	6.527	5.1145	31.280	49.652	Chloride
3	10.588	0.0454	0.055	1.151	Bromide
4	16.098	0.0731	0.177	1.313	Sulfate


Sample data

Ident Q3172-01DLX10
Sample type Sample
Determination start 2025-09-24 12:34:37 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

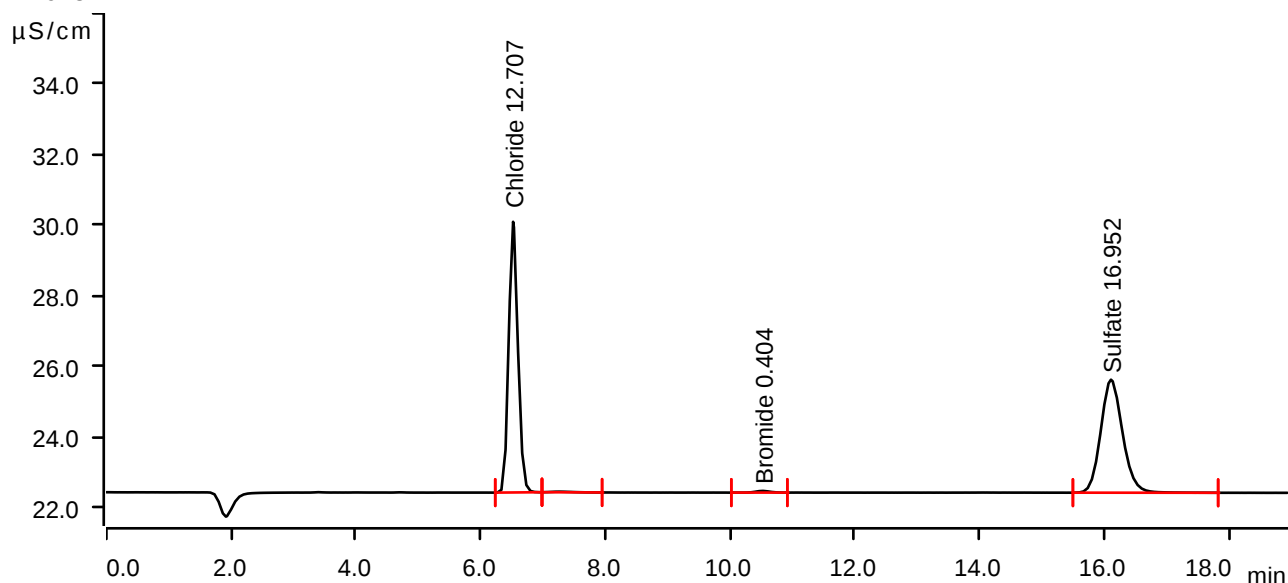

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.522	1.3067	7.662	12.707	Chloride
2	7.262	0.0069	0.018	invalid	
3	10.525	0.0123	0.047	0.404	Bromide
4	16.107	1.2960	3.200	16.952	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-09-24 12:56:11 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

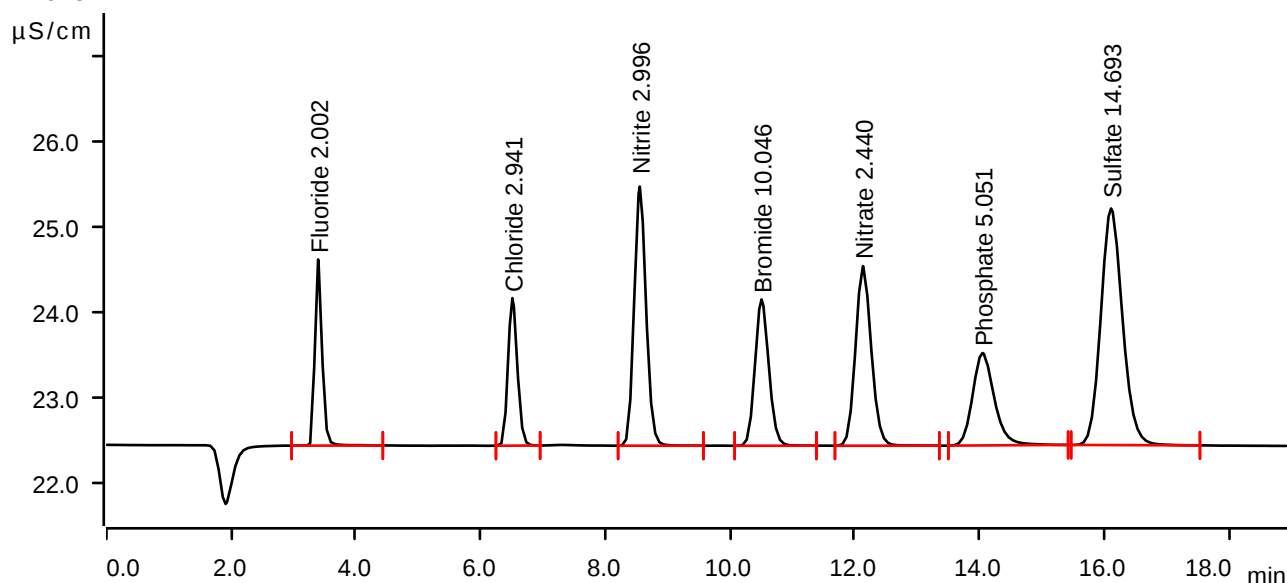


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.395	0.2924	2.181	2.002	Fluoride
2	6.510	0.3002	1.728	2.941	Chloride
3	8.553	0.6733	3.035	2.996	Nitrite
4	10.505	0.4407	1.714	10.046	Bromide
5	12.130	0.6171	2.104	2.440	Nitrate
6	14.047	0.4374	1.083	5.051	Phosphate
7	16.108	1.1193	2.772	14.693	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-09-24 13:17:42 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

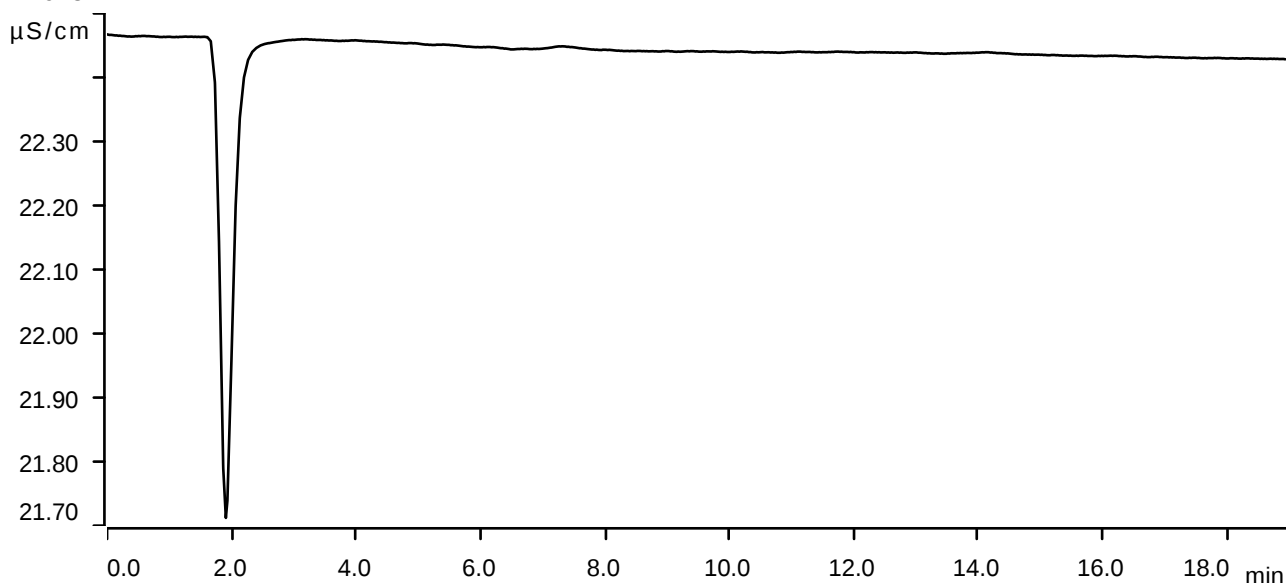Anions

WORKLIST(Hardcopy Internal Chain)

6137286

WorkList Name : anion-3168

WorkList ID : 192035

Department : Wet-Chemistry

Date : 09-24-2025 08:12:05

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q3168-05	TOTES COMP#1	Water	Anions Group1	Cool 4 deg C	PSEG03	J11	09/23/2025	300.0
Q3168-06	TOTES COMP#2	Water	Anions Group1	Cool 4 deg C	PSEG03	J11	09/23/2025	300.0
Q3172-01	FW7D	Water	Anions Group1	Cool 4 deg C	GENV01	J43	09/22/2025	300.0

Date/Time 09/24/25 10:05
Raw Sample Received by: 12 (WC)
Raw Sample Relinquished by: 28 (WC)

Date/Time 09/24/25 12:35
Raw Sample Received by: 28 (WC)
Raw Sample Relinquished by: 12 (WC)