
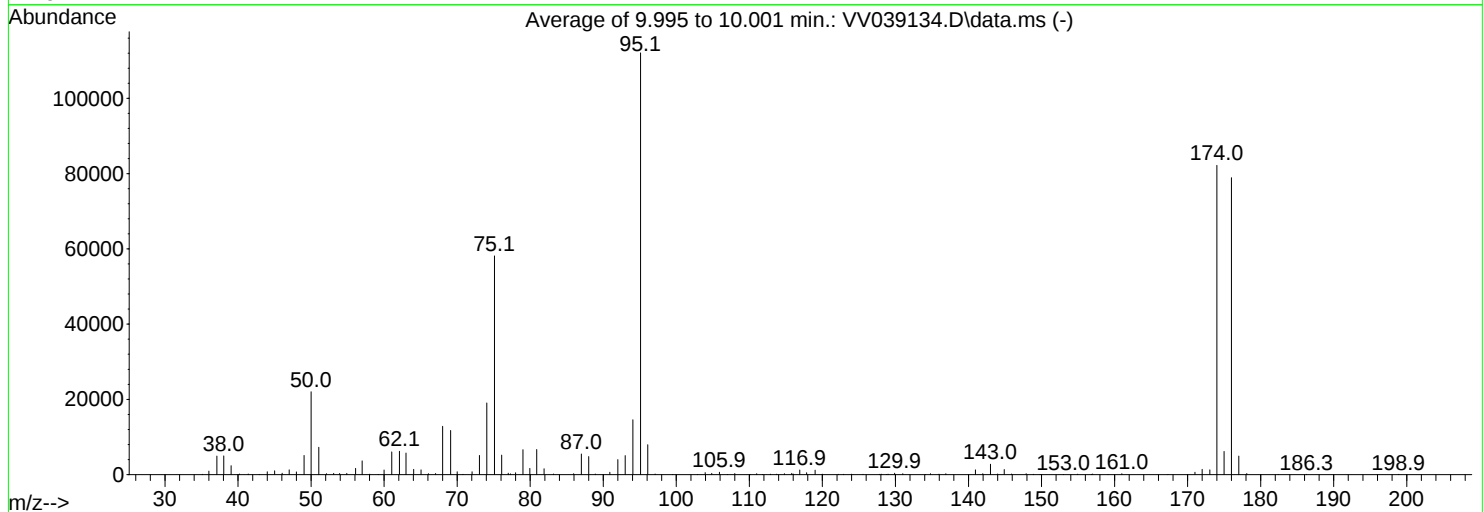


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092225\
Data File : VV039134.D
Acq On : 22 Sep 2025 10:15
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M
Title : SW846 8260
Last Update : Wed Sep 24 08:08:08 2025

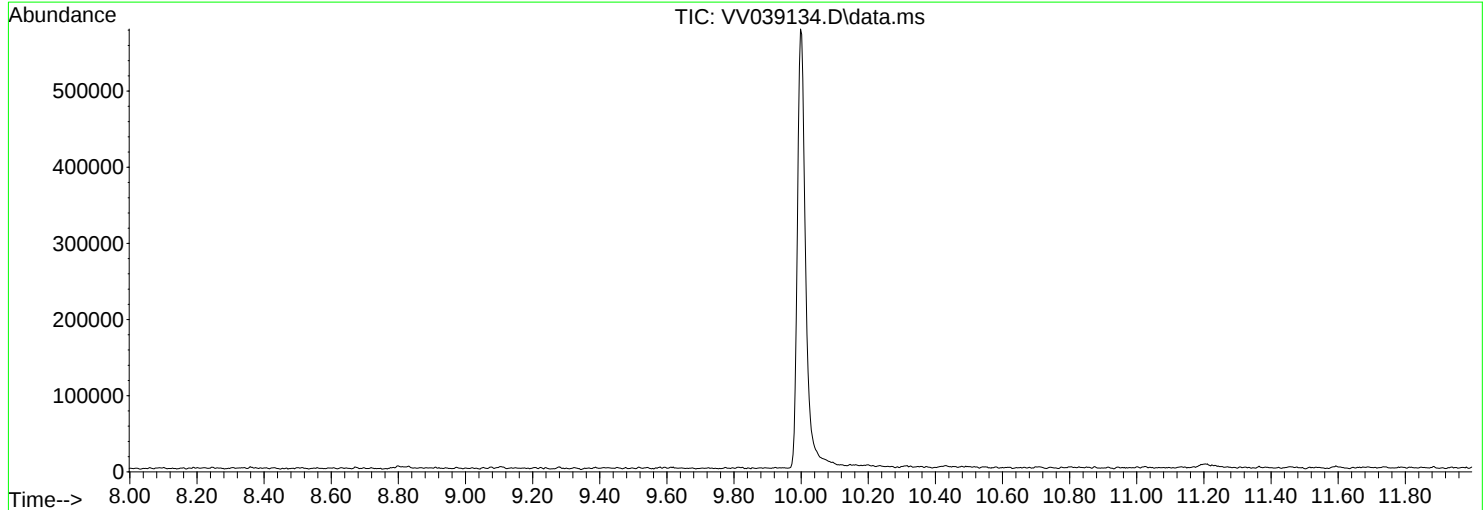

AutoFind: Scans 2785, 2786, 2787; Background Corrected with Scan 2774

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	22014	PASS
75	95	30	60	51.9	58147	PASS
95	95	100	100	100.0	112096	PASS
96	95	5	9	7.1	7955	PASS
173	174	0.00	2	1.6	1275	PASS
174	95	50	100	73.3	82200	PASS
175	174	5	9	7.5	6152	PASS
176	174	95	101	96.0	78917	PASS
177	176	5	9	6.3	4933	PASS