


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092525\
Data File : VV039167.D
Acq On : 25 Sep 2025 09:14
Operator : SY/MD
Sample : BFB
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M
Title : SW846 8260
Last Update : Wed Sep 24 08:08:08 2025

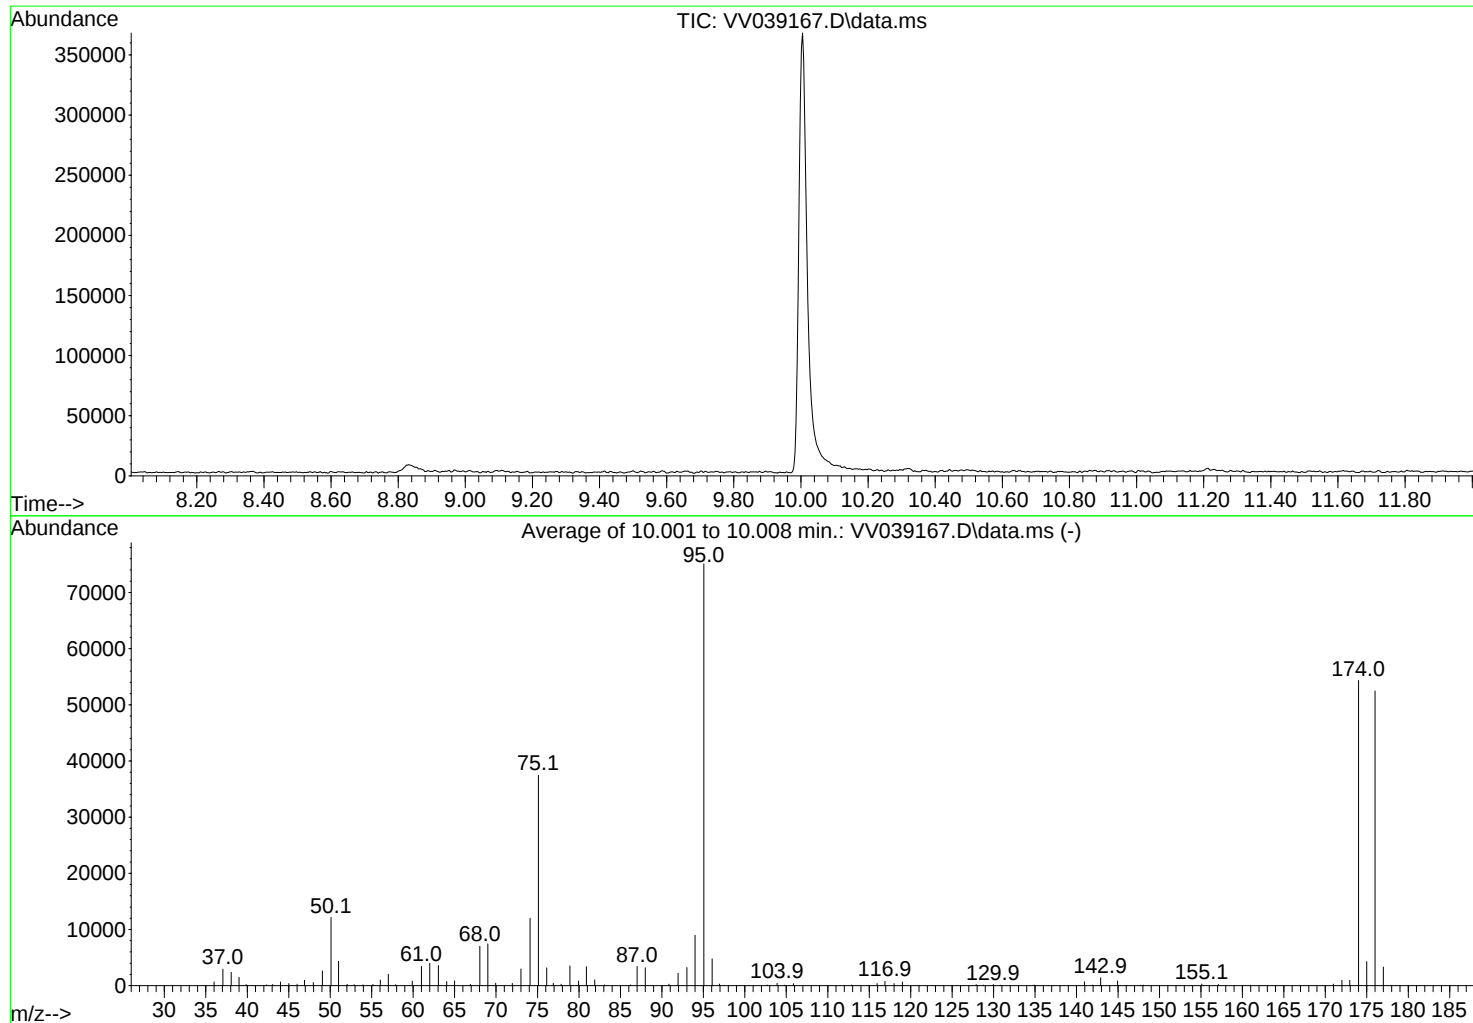

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	12139	PASS
75	95	30	60	49.9	37445	PASS
95	95	100	100	100.0	75093	PASS
96	95	5	9	6.3	4756	PASS
173	174	0.00	2	1.7	944	PASS
174	95	50	100	72.3	54320	PASS
175	174	5	9	7.9	4279	PASS
176	174	95	101	96.6	52461	PASS
177	176	5	9	6.3	3317	PASS