

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092025\
 Data File : PL097287.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2025 20:44
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL092025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 05:35:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:34:42 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.528	2.823	184.1E6	356.3E6	49.817	50.659
28)	SA Decachlor...	9.000	7.983	130.8E6	237.4E6	48.853	49.226
Target Compounds							
23)	Chlordane-1	4.680	3.833	104.6E6	128.6E6	493.606	505.910
24)	Chlordane-2	5.204	4.411	110.5E6	145.2E6	498.009	494.288
25)	Chlordane-3	5.906	5.044	415.0E6	447.5E6	508.848	500.451
26)	Chlordane-4	5.990	5.108	504.8E6	386.8E6	504.683	507.972
27)	Chlordane-5	6.828	6.001	82793302	150.0E6	493.895	503.231



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092025\
Data File : PL097287.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2025 20:44
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL092025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 05:35:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:34:42 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

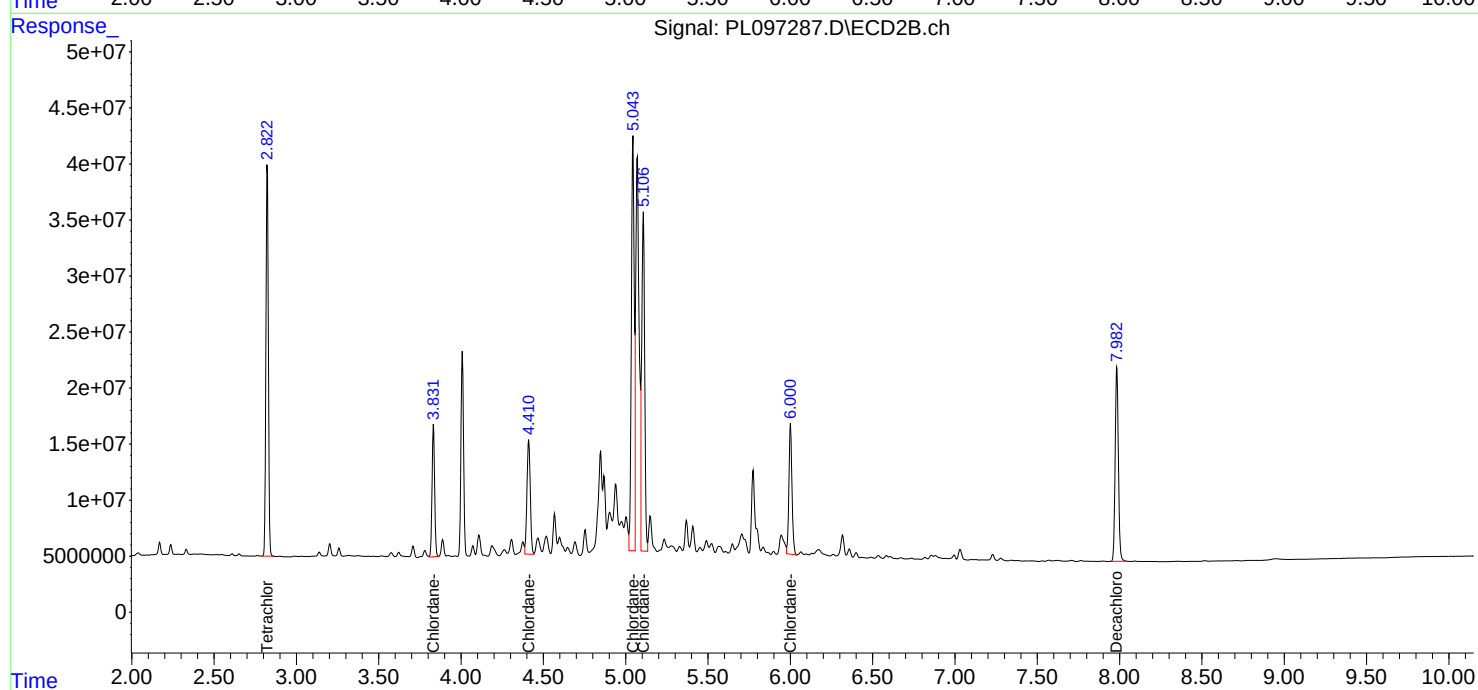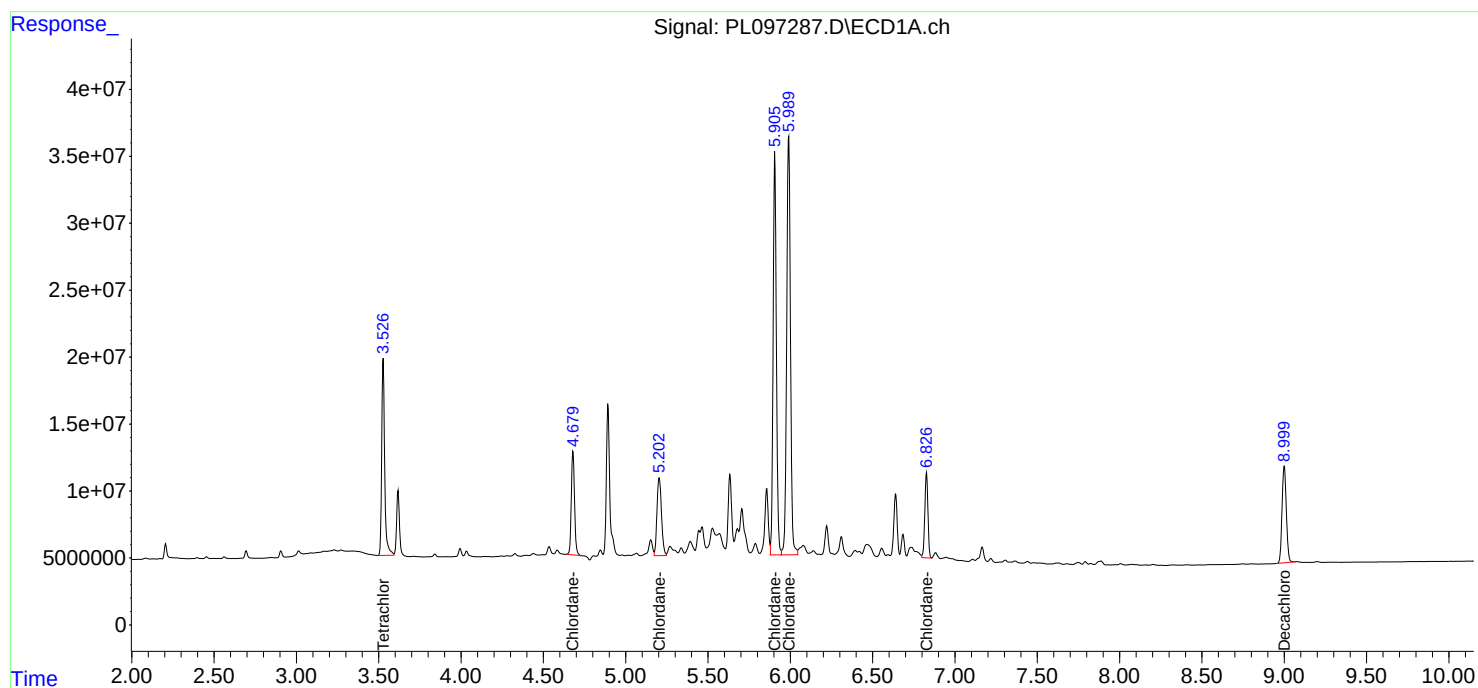


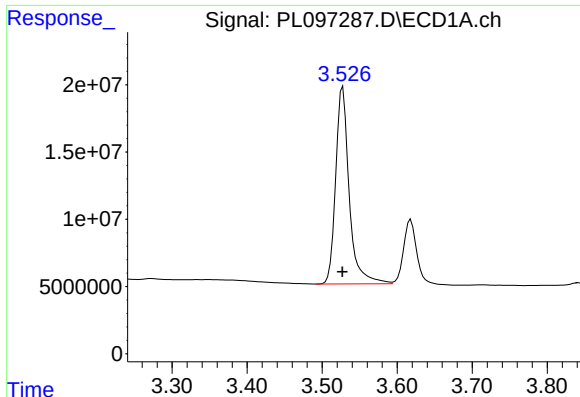

#1 Tetrachloro-m-xylene


R.T.: 3.528 min
Delta R.T.: 0.000 min
Response: 184140628
Conc: 49.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL092025

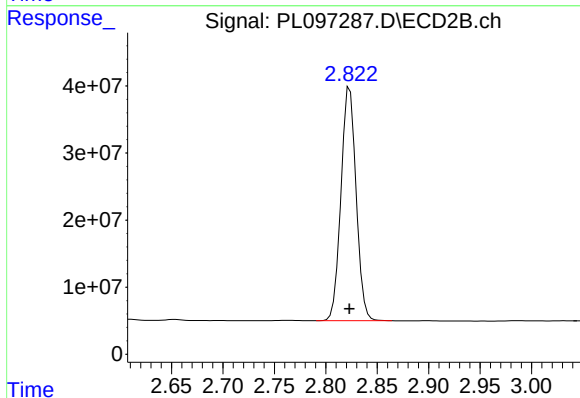


#1 Tetrachloro-m-xylene

R.T.: 2.823 min
Delta R.T.: 0.000 min
Response: 356326657
Conc: 50.66 ng/ml

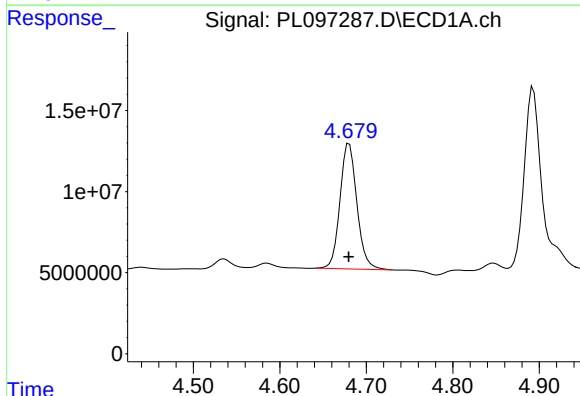


#23 Chlordane-1

R.T.: 4.680 min
Delta R.T.: 0.000 min
Response: 104612447
Conc: 493.61 ng/ml

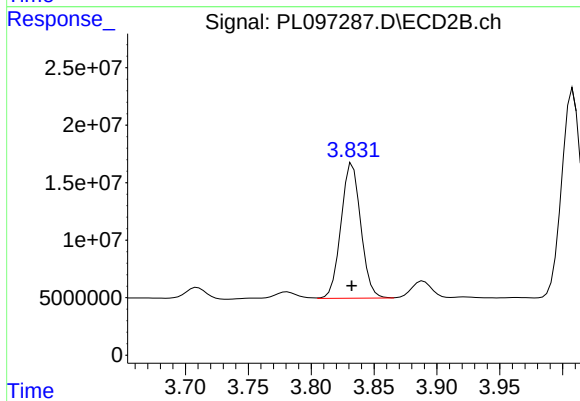

#23 Chlordane-1


R.T.: 3.833 min
Delta R.T.: 0.000 min
Response: 128579498
Conc: 505.91 ng/ml

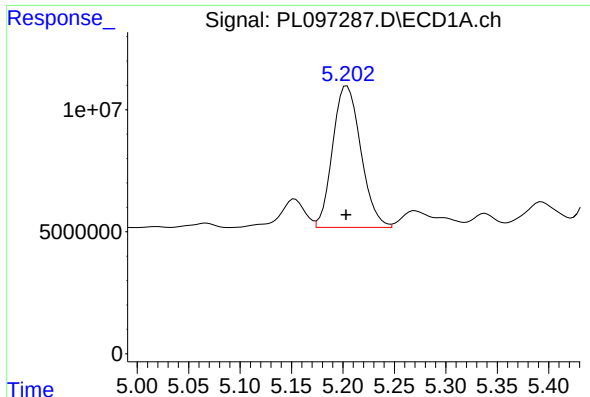

#24 Chlordane-2


R.T.: 5.204 min
Delta R.T.: 0.000 min
Response: 110544817
Conc: 498.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL092025

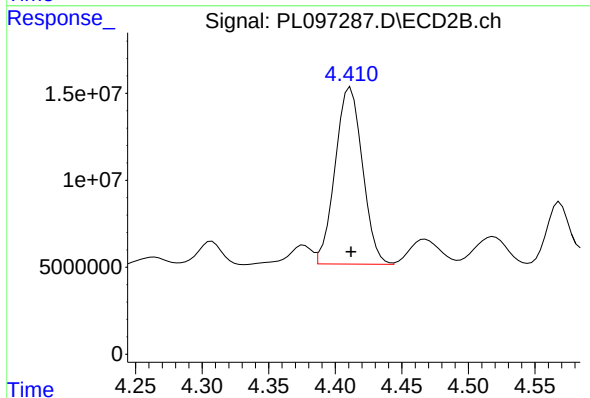


#24 Chlordane-2

R.T.: 4.411 min
Delta R.T.: 0.000 min
Response: 145179087
Conc: 494.29 ng/ml

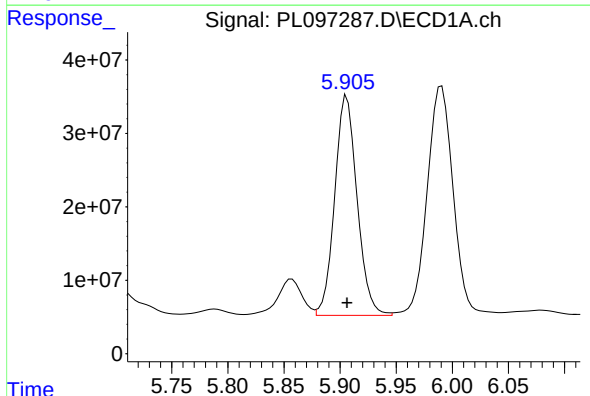


#25 Chlordane-3

R.T.: 5.906 min
Delta R.T.: 0.000 min
Response: 415036714
Conc: 508.85 ng/ml

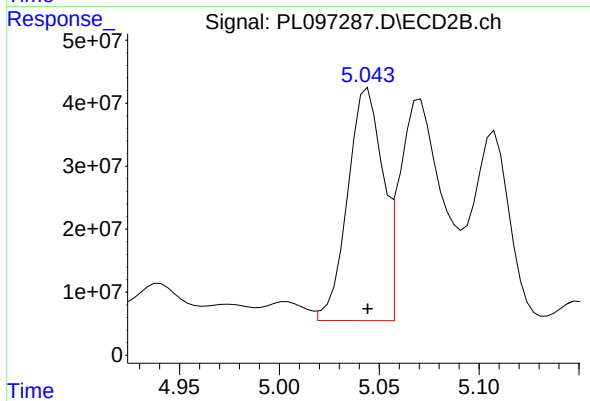

#25 Chlordane-3


R.T.: 5.044 min
Delta R.T.: 0.000 min
Response: 447511749
Conc: 500.45 ng/ml

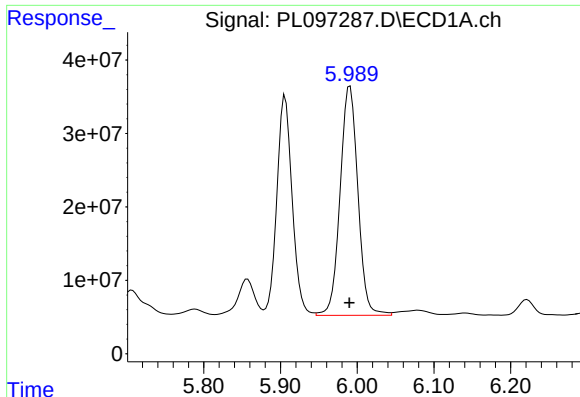

#26 Chlordane-4


R.T.: 5.990 min
Delta R.T.: 0.000 min
Response: 504796787
Conc: 504.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL092025

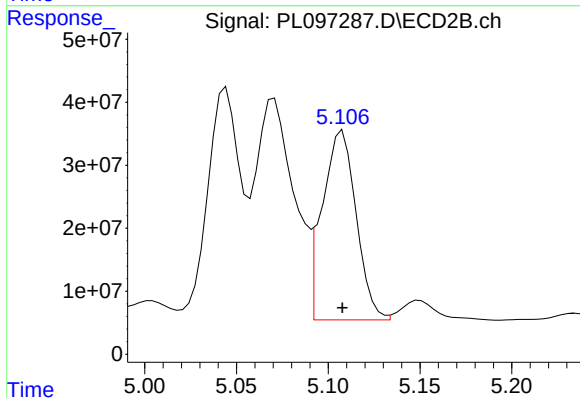


#26 Chlordane-4

R.T.: 5.108 min
Delta R.T.: 0.000 min
Response: 386843517
Conc: 507.97 ng/ml

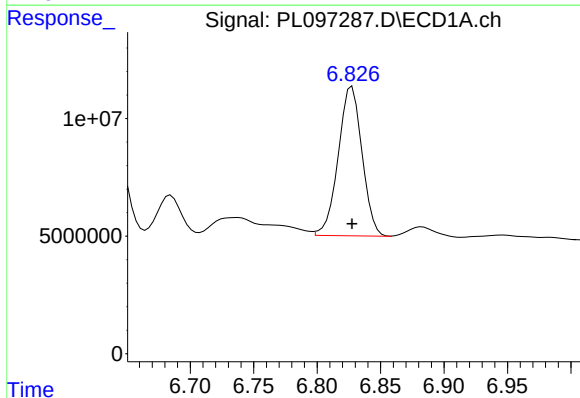


#27 Chlordane-5

R.T.: 6.828 min
Delta R.T.: 0.000 min
Response: 82793302
Conc: 493.89 ng/ml

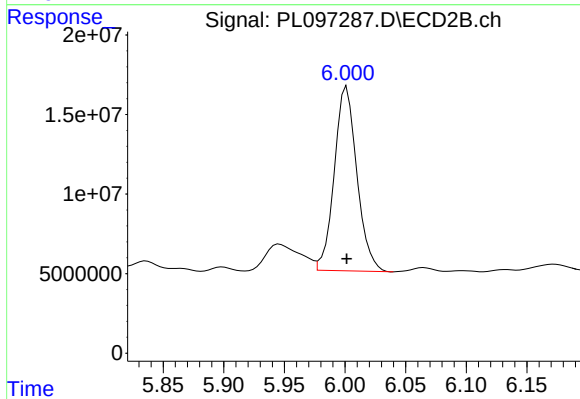

#27 Chlordane-5


R.T.: 6.001 min
Delta R.T.: 0.000 min
Response: 150034770
Conc: 503.23 ng/ml

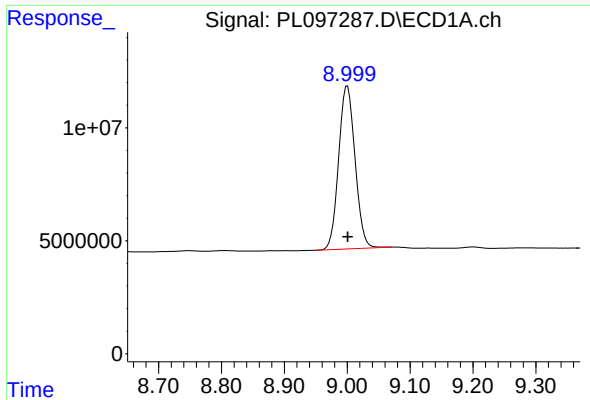

#28 Decachlorobiphenyl

R.T.: 9.000 min
Delta R.T.: 0.000 min
Response: 130848141
Conc: 48.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL092025

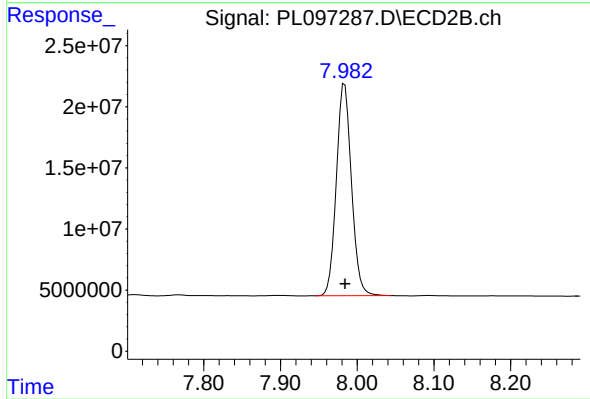

#28 Decachlorobiphenyl

R.T.: 7.983 min
Delta R.T.: 0.000 min
Response: 237448221
Conc: 49.23 ng/ml