


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092525\
Data File : VN087947.D
Acq On : 25 Sep 2025 10:47
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N092325W.M
Title : SW846 8260
Last Update : Wed Sep 24 05:05:30 2025

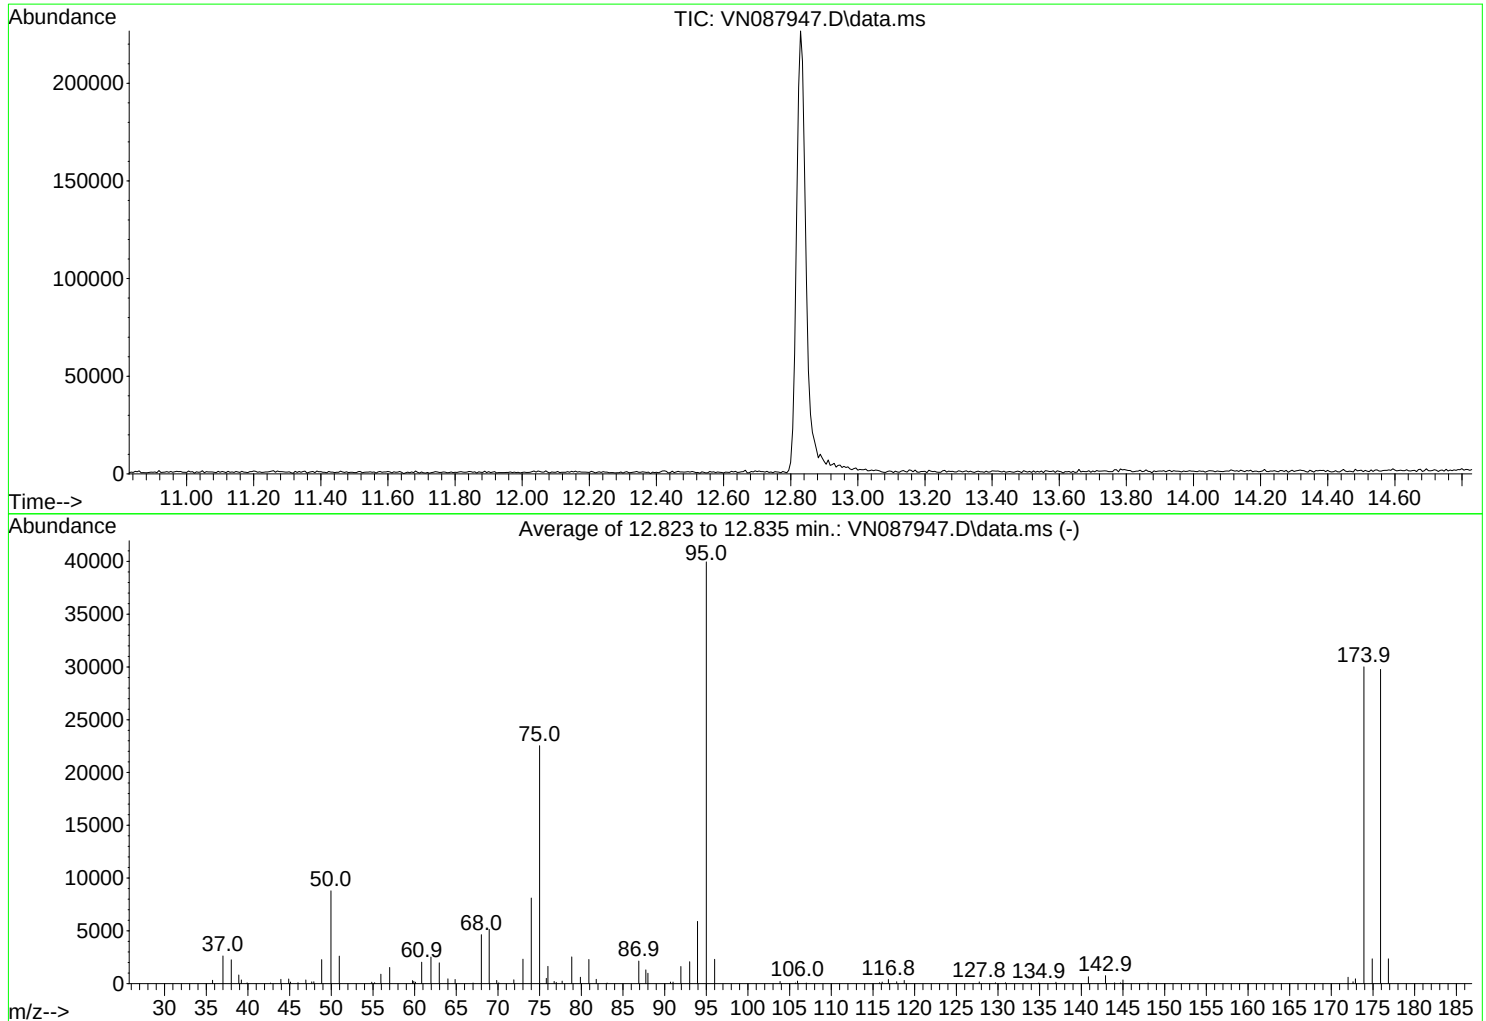

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1840

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	8793	PASS
75	95	30	60	56.4	22541	PASS
95	95	100	100	100.0	39955	PASS
96	95	5	9	5.8	2310	PASS
173	174	0.00	2	1.5	450	PASS
174	95	50	100	75.1	30013	PASS
175	174	5	9	7.8	2352	PASS
176	174	95	101	99.2	29768	PASS
177	176	5	9	7.9	2353	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.75	321	46.95	351	59.90	209	70.10	71
37.00	2621	47.65	165	60.10	133	71.90	36
38.00	2253	47.90	176	60.85	2033	73.00	231
38.90	819	48.85	2274	61.95	2518	74.00	810
39.20	354	49.95	8793	62.95	1964	75.00	22541
39.90	70	50.95	2608	64.00	461	75.80	501
42.70	61	54.85	136	64.85	403	76.00	1637
43.95	409	55.20	84	67.00	64	76.75	213
44.90	439	55.95	891	68.00	4641	77.00	122
45.10	155	57.00	1532	68.95	5145	77.70	236
46.00	91	59.75	294	69.85	304	78.85	2531

Average of 12.823 to 12.835 min.: VN087947.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.90	613	93.95	5897	118.75	302	148.00	56
80.90	2290	95.00	39955	127.75	167	172.00	614
81.80	417	96.00	2310	129.70	86	172.60	180
83.10	54	103.85	215	130.90	85	172.90	450
86.90	2137	105.70	58	134.90	56	173.90	30013
87.75	1310	105.95	246	136.95	144	174.90	2352
88.00	986	107.00	67	140.85	654	175.90	29768
90.70	146	115.80	85	142.90	752	176.85	2353
91.00	153	116.10	158	144.00	77		
91.95	1621	116.85	401	144.70	73		
93.00	2076	117.85	185	145.00	351		

Instrument :

MSVOA_N

ClientSampleId :

BFB