

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092025\
 Data File : PL097278.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2025 18:41
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 05:25:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:24:11 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.528	2.823	181.2E6	350.3E6	50.000	50.000
28)	SA Decachlor...	9.002	7.984	130.8E6	233.3E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.680	3.832	103.4E6	126.1E6	500.000	500.000
24)	Chlordane-2	5.204	4.412	108.0E6	142.2E6	500.000	500.000
25)	Chlordane-3	5.907	5.044	406.9E6	438.8E6	500.000	500.000
26)	Chlordane-4	5.991	5.108	496.0E6	383.2E6	500.000	500.000
27)	Chlordane-5	6.828	6.002	81439283	146.3E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092025\
Data File : PL097278.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2025 18:41
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 05:25:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:24:11 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

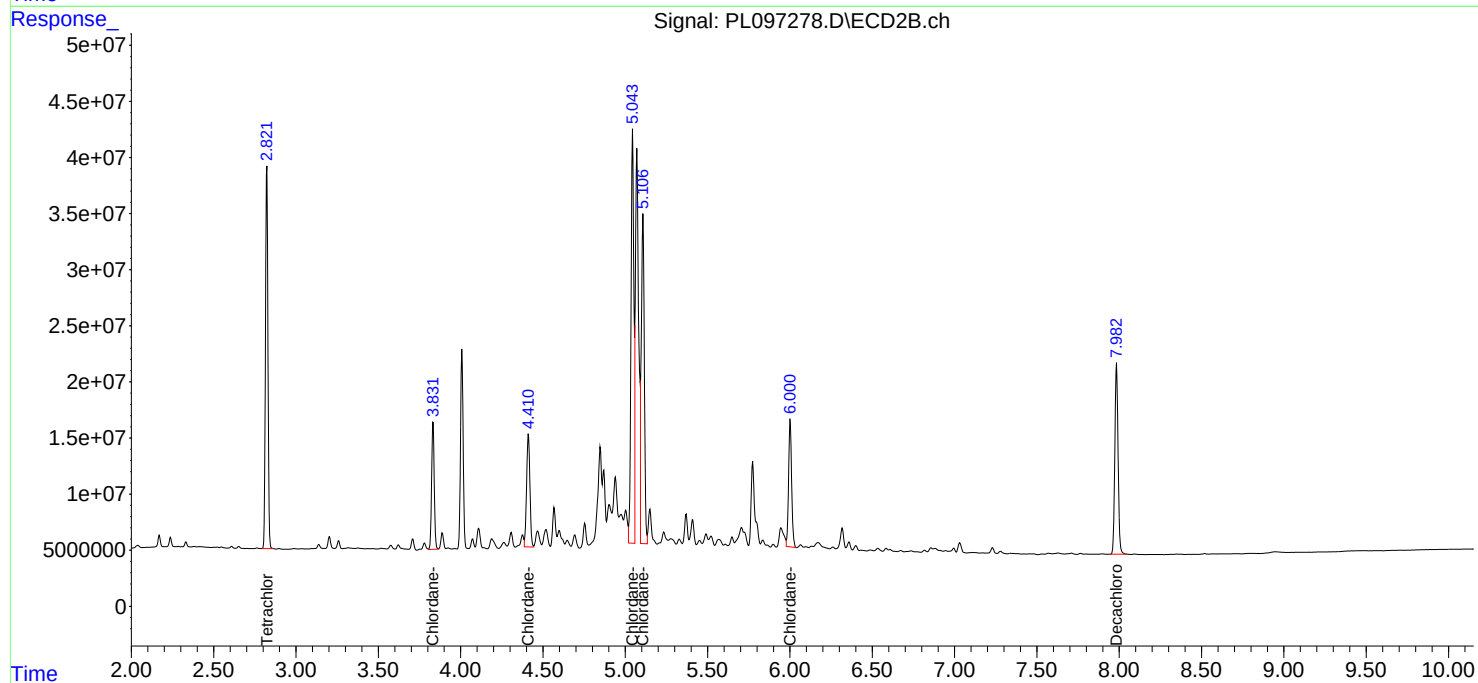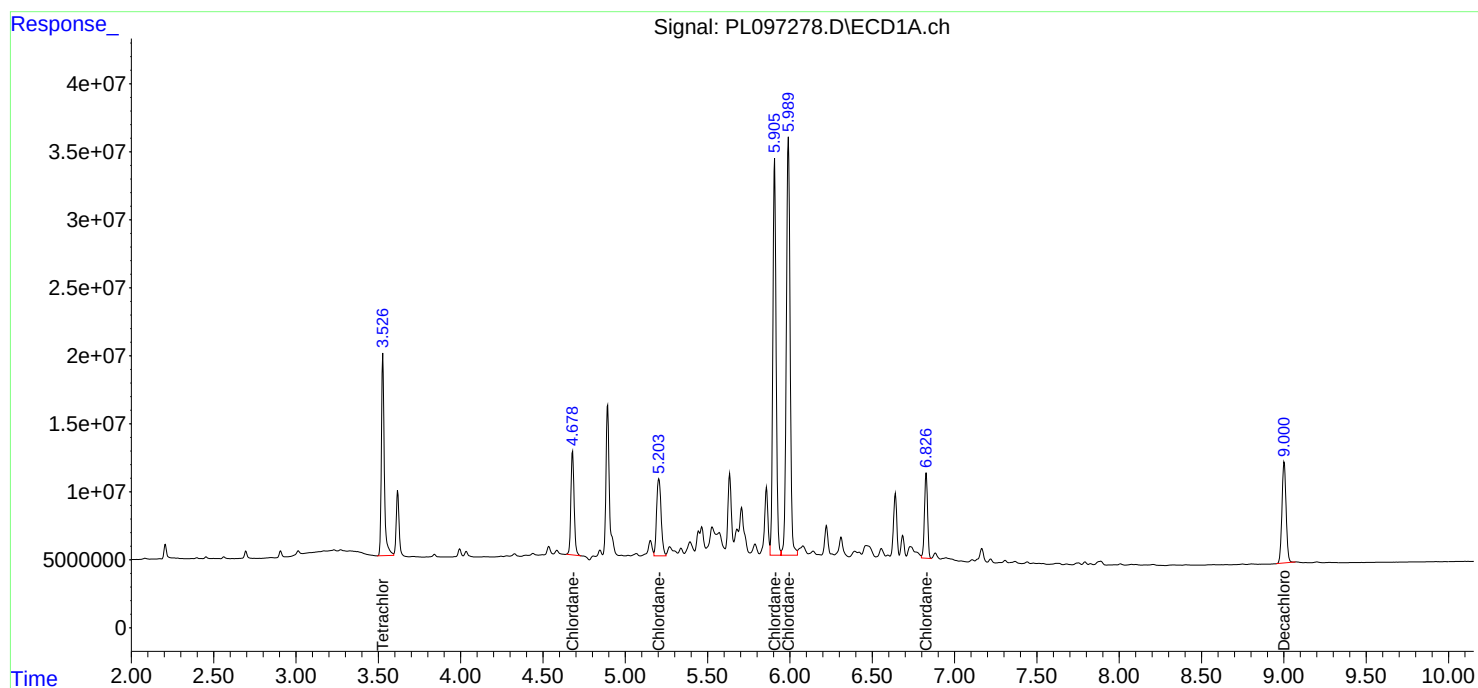


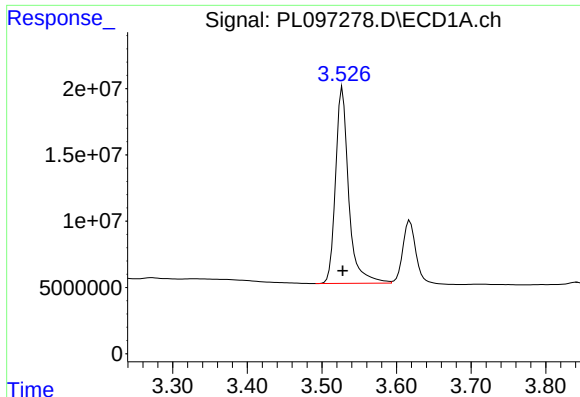

#1 Tetrachloro-m-xylene


R.T.: 3.528 min
Delta R.T.: 0.000 min
Response: 181210972
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

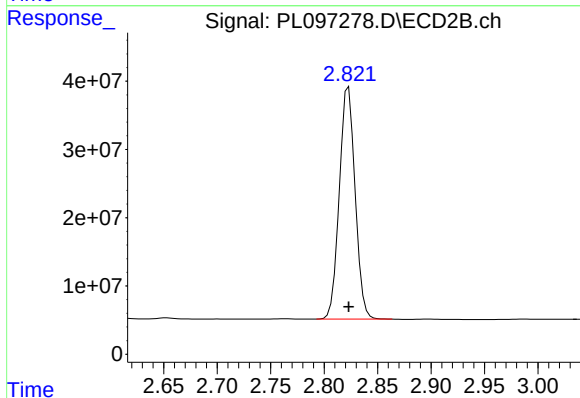


#1 Tetrachloro-m-xylene

R.T.: 2.823 min
Delta R.T.: 0.000 min
Response: 350295281
Conc: 50.00 ng/ml

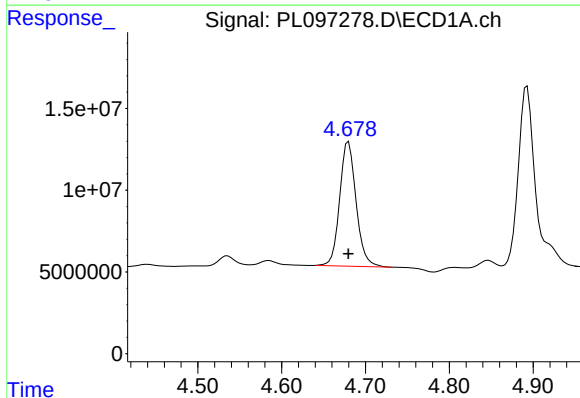


#23 Chlordane-1

R.T.: 4.680 min
Delta R.T.: 0.000 min
Response: 103425253
Conc: 500.00 ng/ml

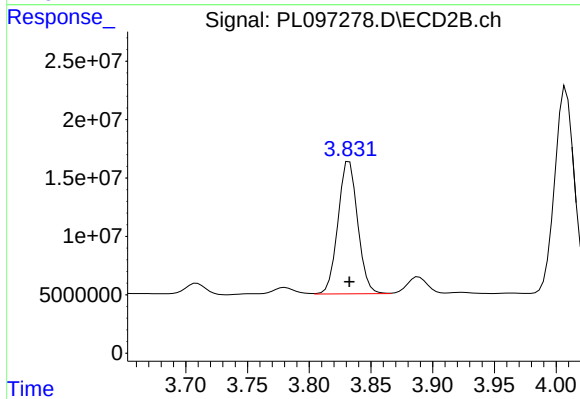

#23 Chlordane-1


R.T.: 3.832 min
Delta R.T.: 0.000 min
Response: 126078711
Conc: 500.00 ng/ml

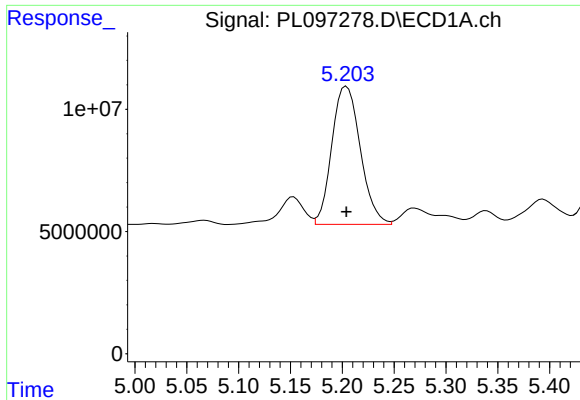

#24 Chlordane-2


R.T.: 5.204 min
Delta R.T.: 0.000 min
Response: 108047949
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

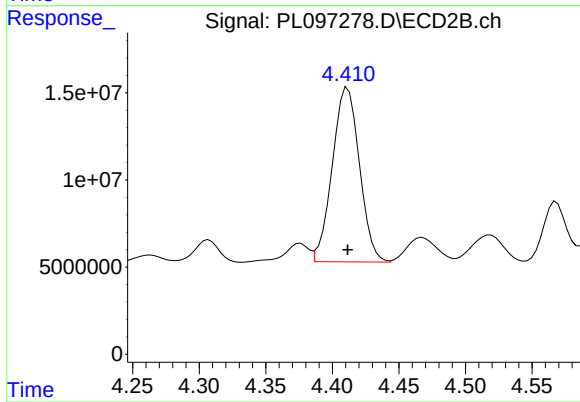


#24 Chlordane-2

R.T.: 4.412 min
Delta R.T.: 0.000 min
Response: 142152665
Conc: 500.00 ng/ml

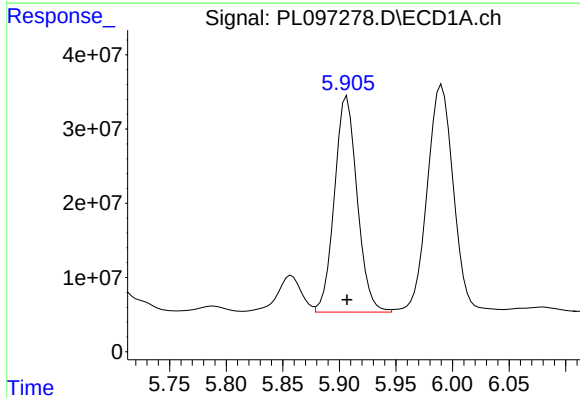


#25 Chlordane-3

R.T.: 5.907 min
Delta R.T.: 0.000 min
Response: 406877107
Conc: 500.00 ng/ml

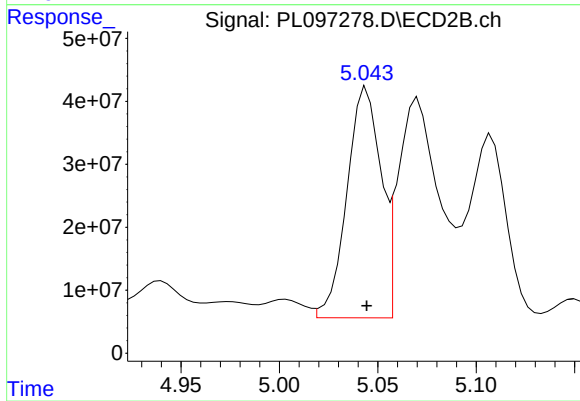

#25 Chlordane-3


R.T.: 5.044 min
Delta R.T.: 0.000 min
Response: 438817615
Conc: 500.00 ng/ml

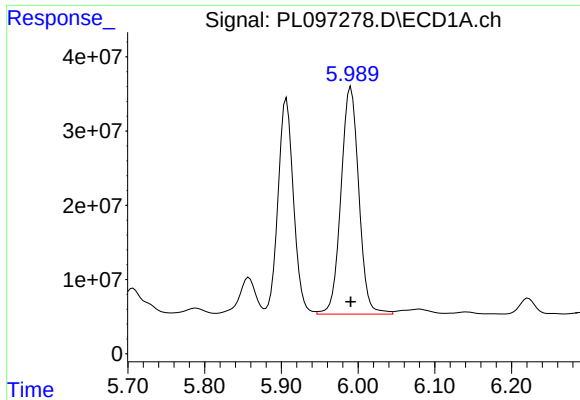

#26 Chlordane-4


R.T.: 5.991 min
Delta R.T.: 0.000 min
Response: 496022448
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

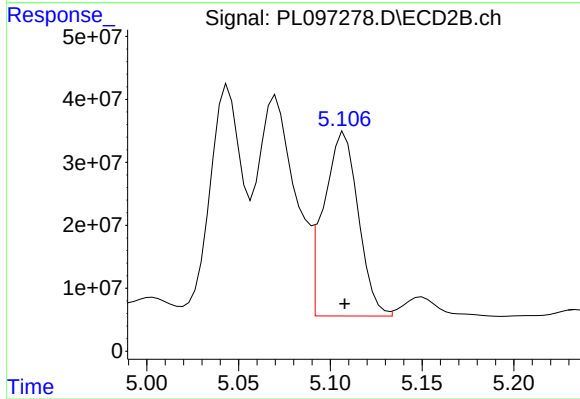


#26 Chlordane-4

R.T.: 5.108 min
Delta R.T.: 0.000 min
Response: 383235793
Conc: 500.00 ng/ml

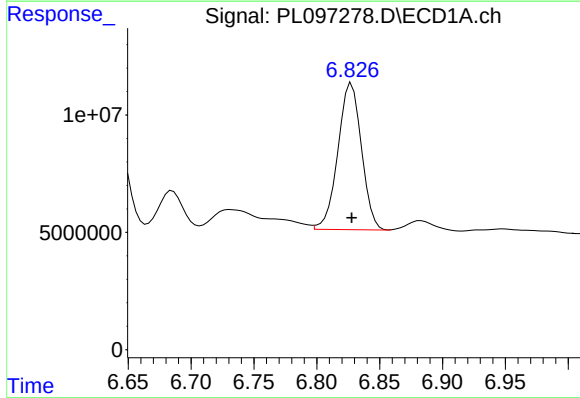


#27 Chlordane-5

R.T.: 6.828 min
Delta R.T.: 0.000 min
Response: 81439283
Conc: 500.00 ng/ml

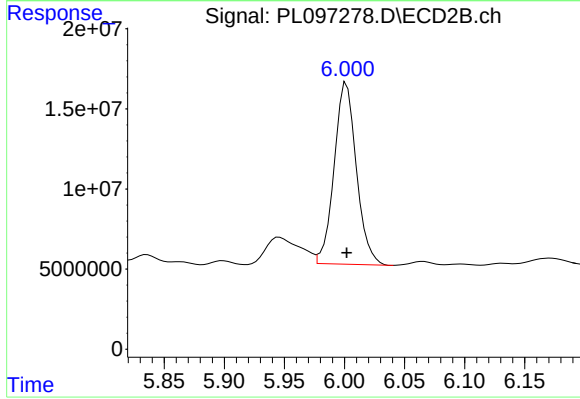

#27 Chlordane-5


R.T.: 6.002 min
Delta R.T.: 0.000 min
Response: 146266920
Conc: 500.00 ng/ml

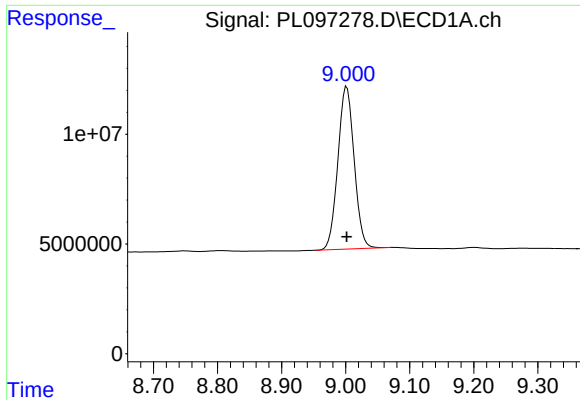

#28 Decachlorobiphenyl

R.T.: 9.002 min
Delta R.T.: 0.000 min
Response: 130810747
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

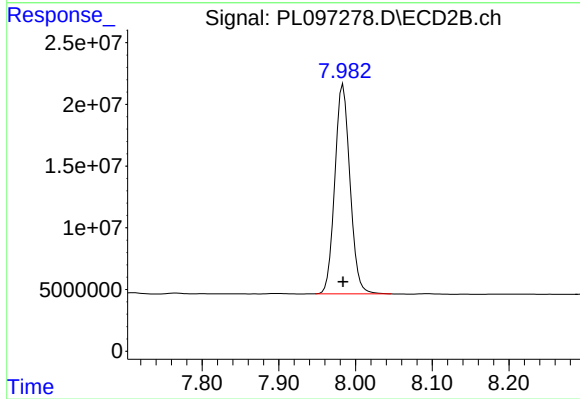

#28 Decachlorobiphenyl

R.T.: 7.984 min
Delta R.T.: 0.000 min
Response: 233255429
Conc: 50.00 ng/ml