


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092325\
Data File : BF143790.D
Acq On : 23 Sep 2025 09:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF092325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 24 05:00:00 2025

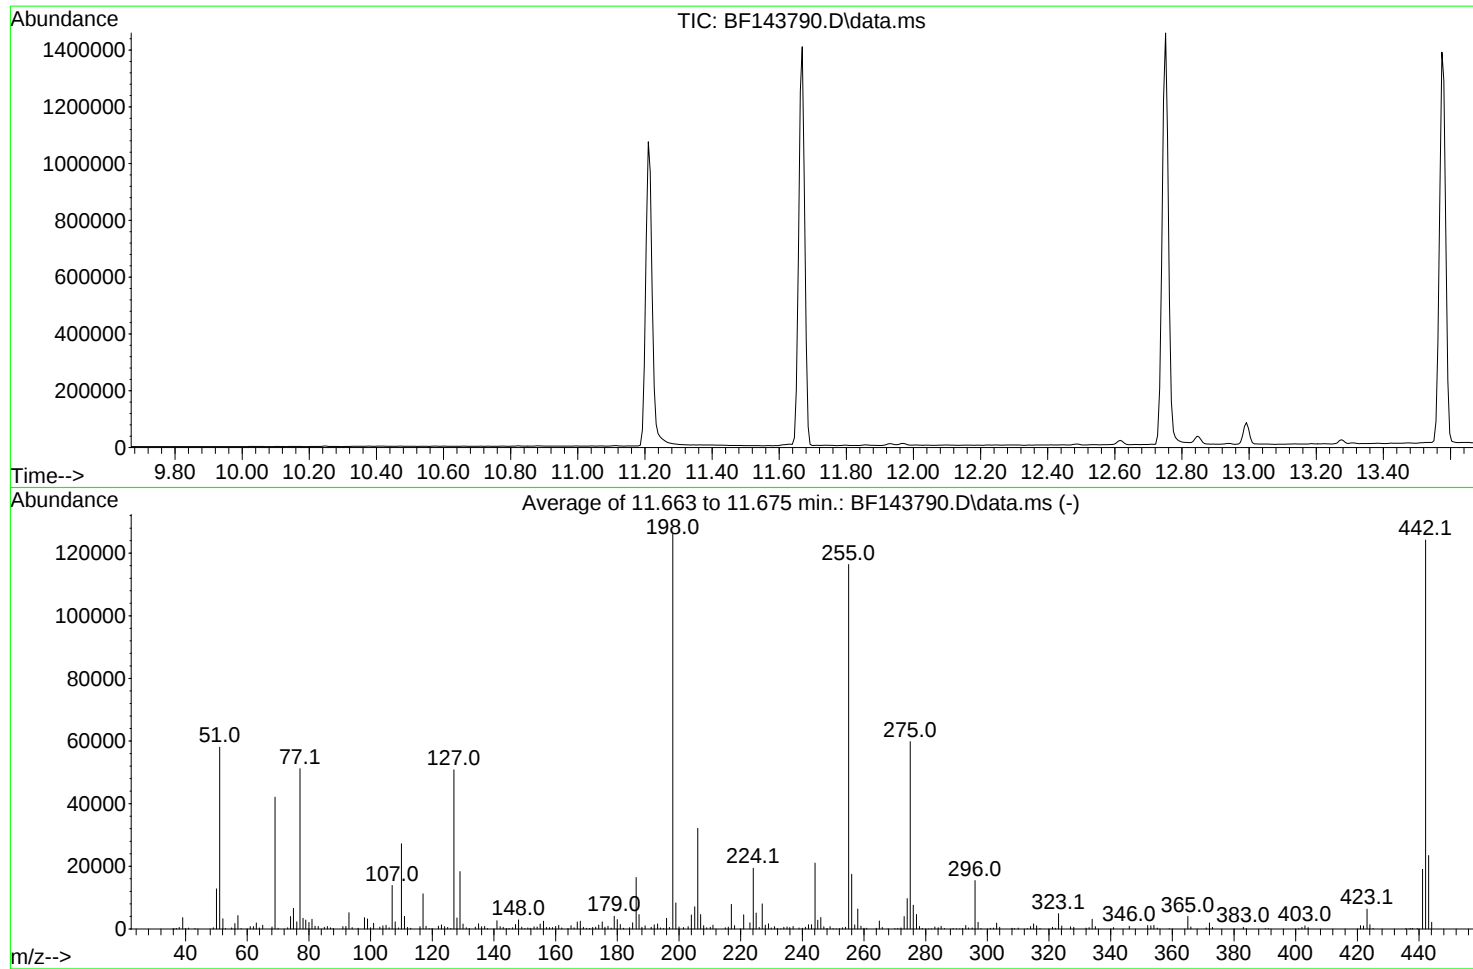




AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1604

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	670	PASS
69	69	100	100	100.0	42104	PASS
70	69	0.00	2	0.6	252	PASS
197	198	0.00	2	0.4	514	PASS
198	198	100	100	100.0	126099	PASS
199	198	5	9	6.6	8311	PASS
365	198	1	100	3.2	4006	PASS
441	443	0.01	150	81.4	19061	PASS
442	442	100	100	100.0	124205	PASS
443	442	15	24	18.9	23416	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092325\
Data File : BF143790.D
Acq On : 23 Sep 2025 09:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 23 14:37:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF092325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 23 14:30:38 2025
Response via : Initial Calibration

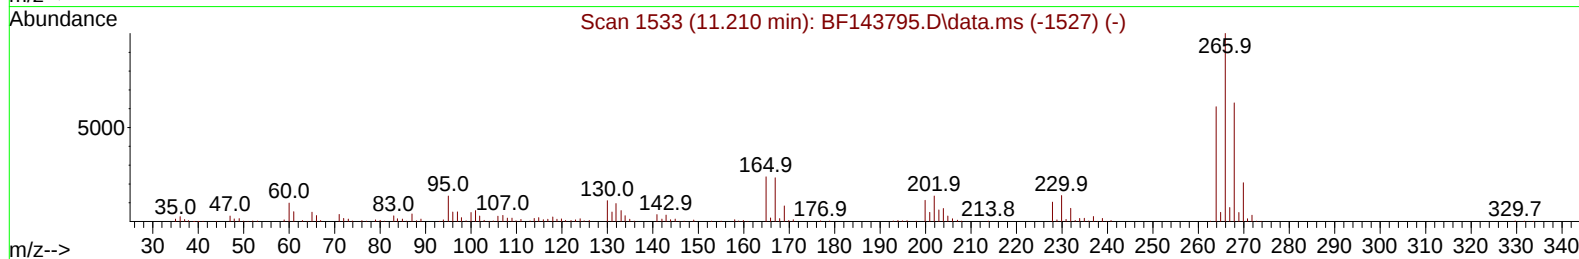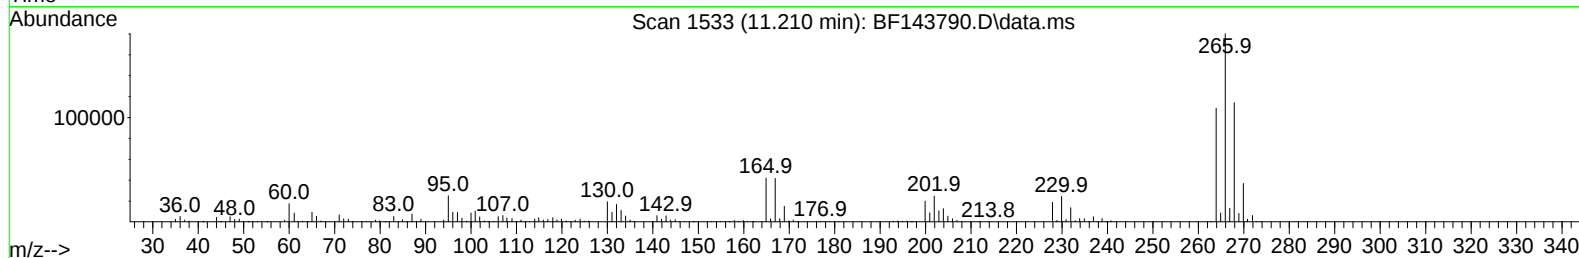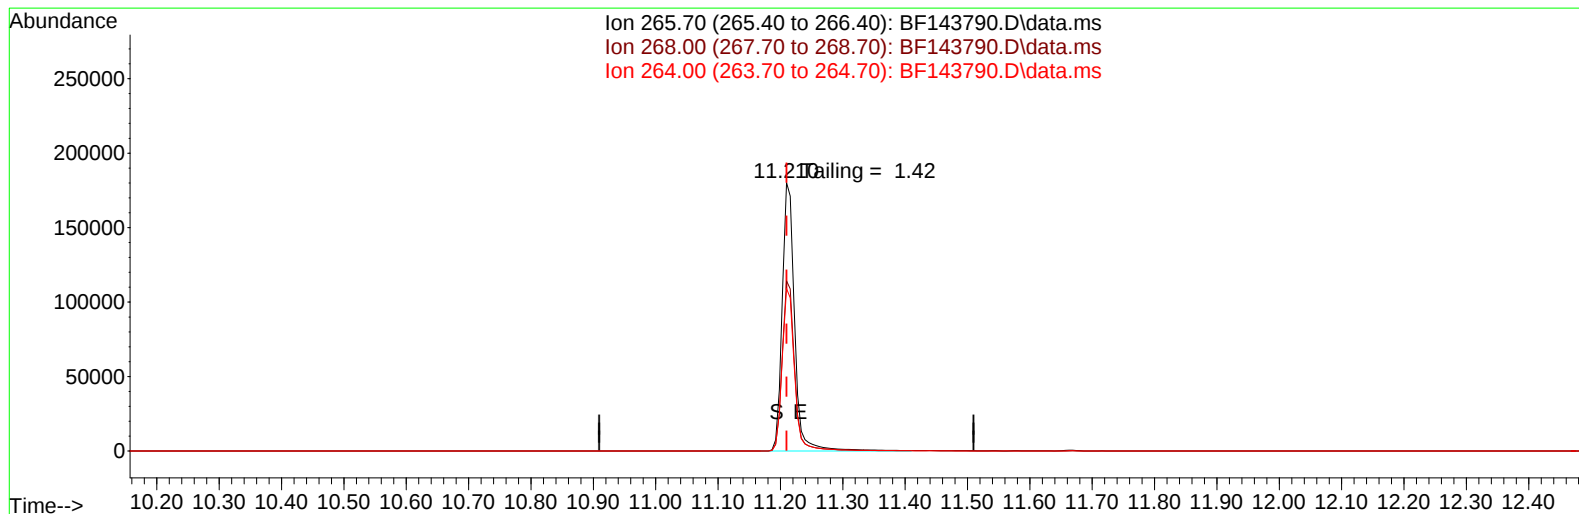

TIC: BF143790.D\data.ms

(70) Pentachlorophenol (C)

11.210min (+ 0.000) 32047.58 ng




response 252838

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.36
264.00	61.00	60.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092325\
Data File : BF143790.D
Acq On : 23 Sep 2025 09:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 23 14:37:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF092325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 23 14:30:38 2025
Response via : Initial Calibration

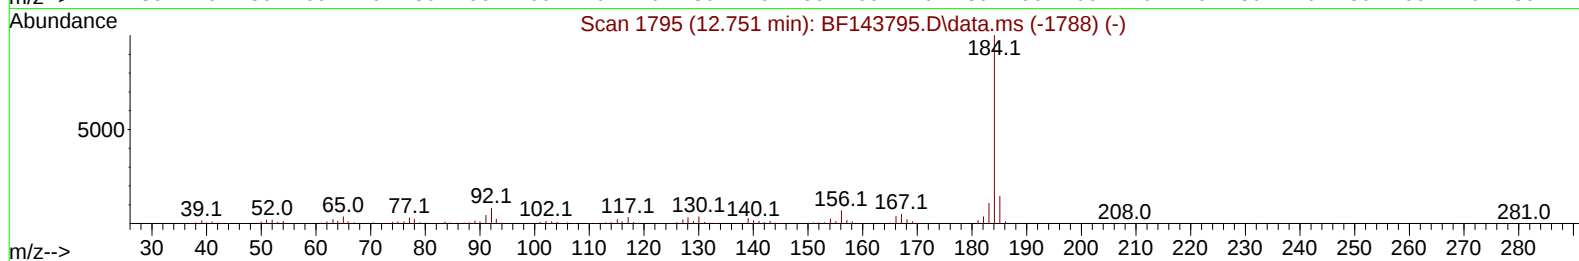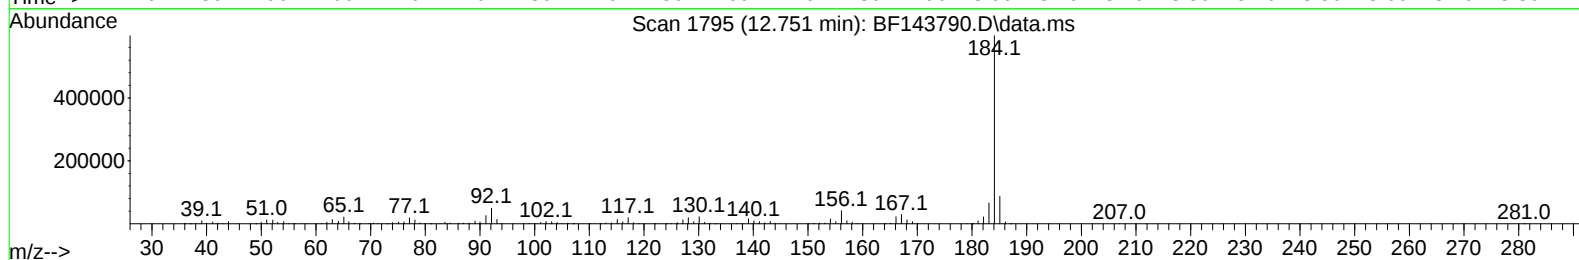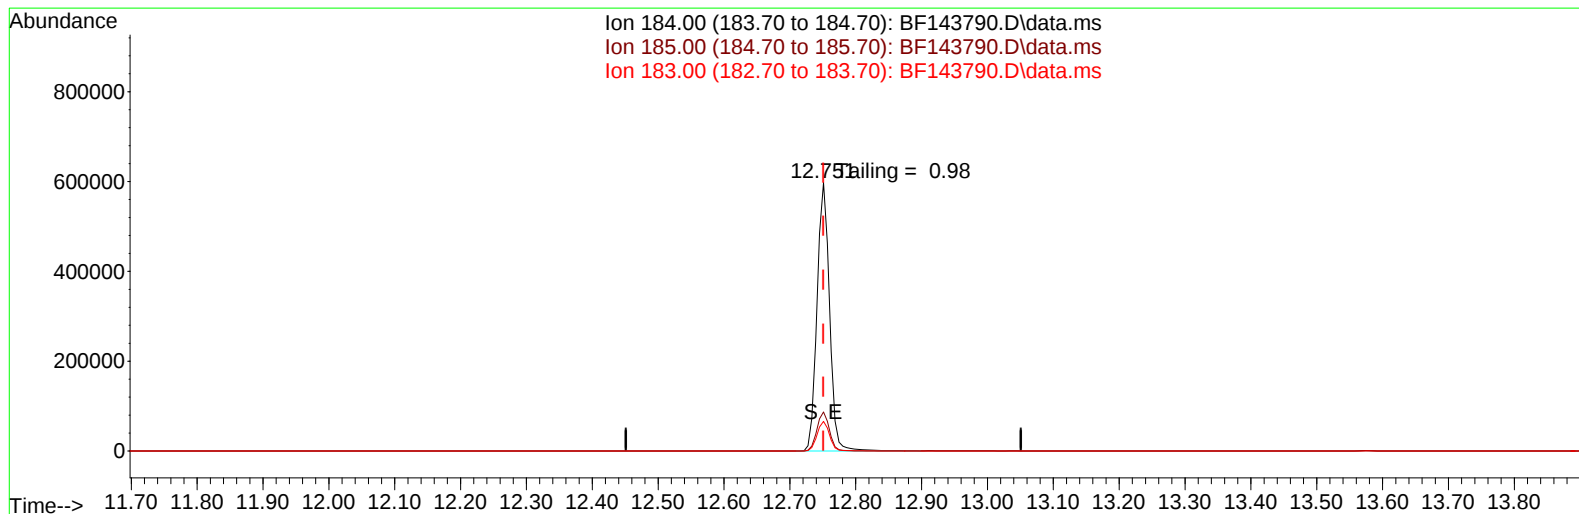

TIC: BF143790.D\data.ms

(77) Benzidine

12.751min (+ 0.000) 22811.55 ng

response 789331

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.56
183.00	10.80	11.07
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/23/2025	BNA_F	<u>BF143790.D</u>
Compound Name	Response	Retention Time
DDT	356414	13.574
DDD	5539	13.274
DDE	649	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6188	362602	1.71

Instrument :
BNA_F
ClientSampleId :
DFTPP