
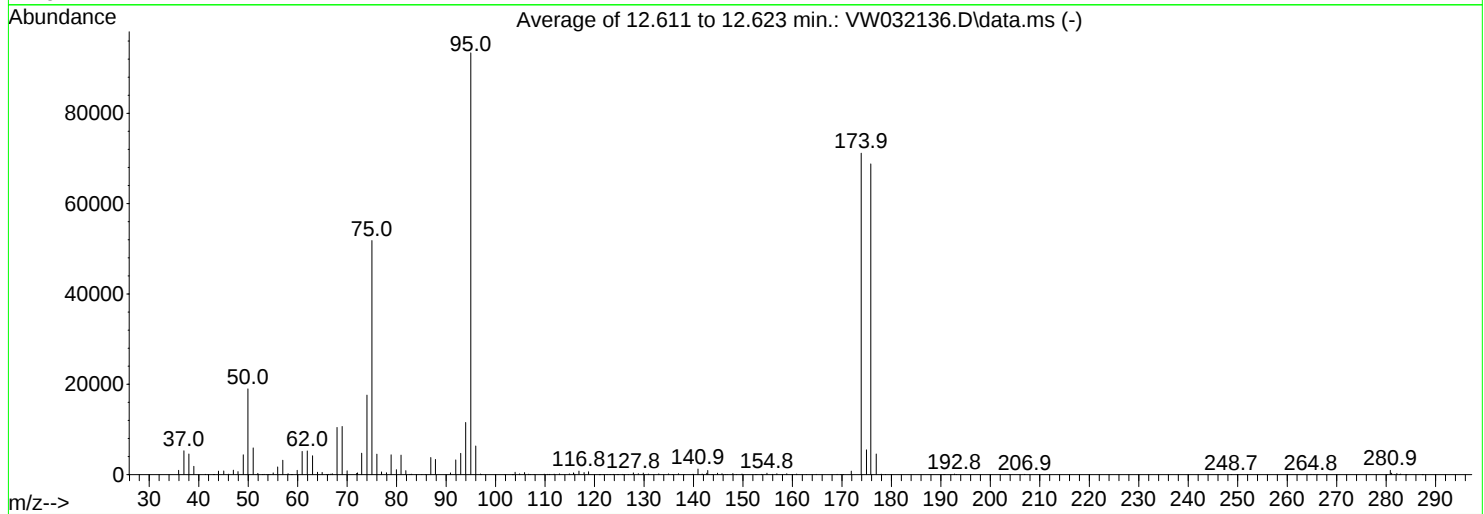


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082625\
Data File : VW032136.D
Acq On : 26 Aug 2025 08:38
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W082625S.M
Title : SW846 8260
Last Update : Wed Aug 27 04:13:40 2025

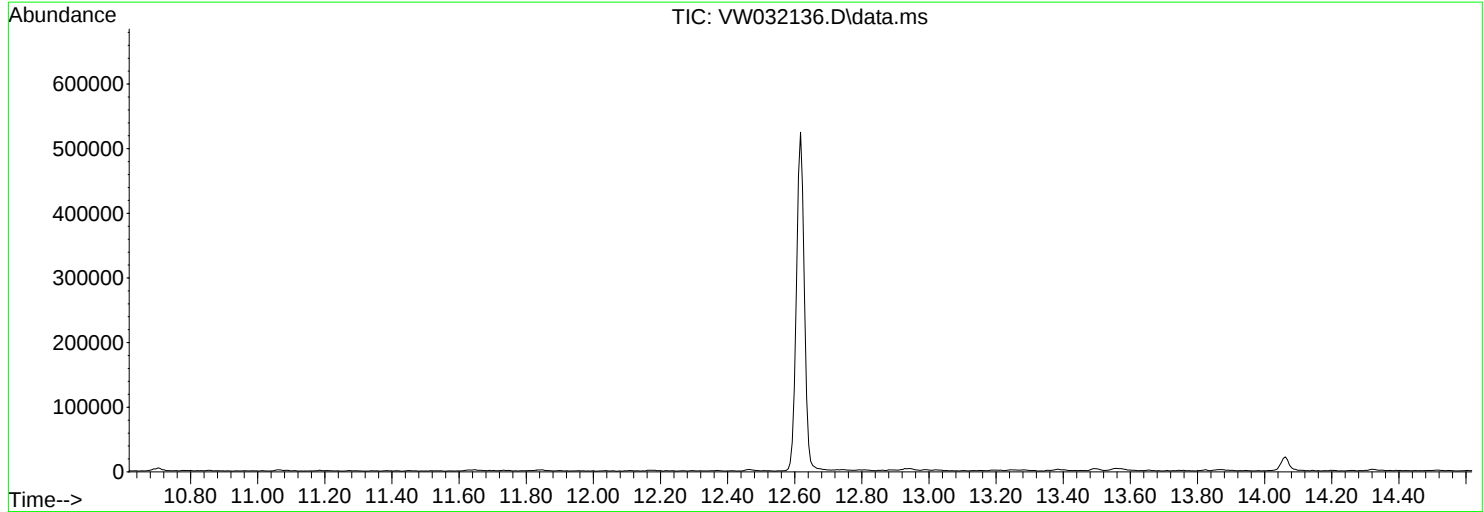

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.3	18996	PASS
75	95	30	60	55.5	51824	PASS
95	95	100	100	100.0	93381	PASS
96	95	5	9	6.8	6324	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	76.2	71157	PASS
175	174	5	9	7.7	5501	PASS
176	174	95	101	96.7	68787	PASS
177	176	5	9	6.6	4557	PASS