


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092325\
Data File : VN087922.D
Acq On : 23 Sep 2025 08:31
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N092325W.M
Title : SW846 8260
Last Update : Wed Sep 24 05:05:30 2025

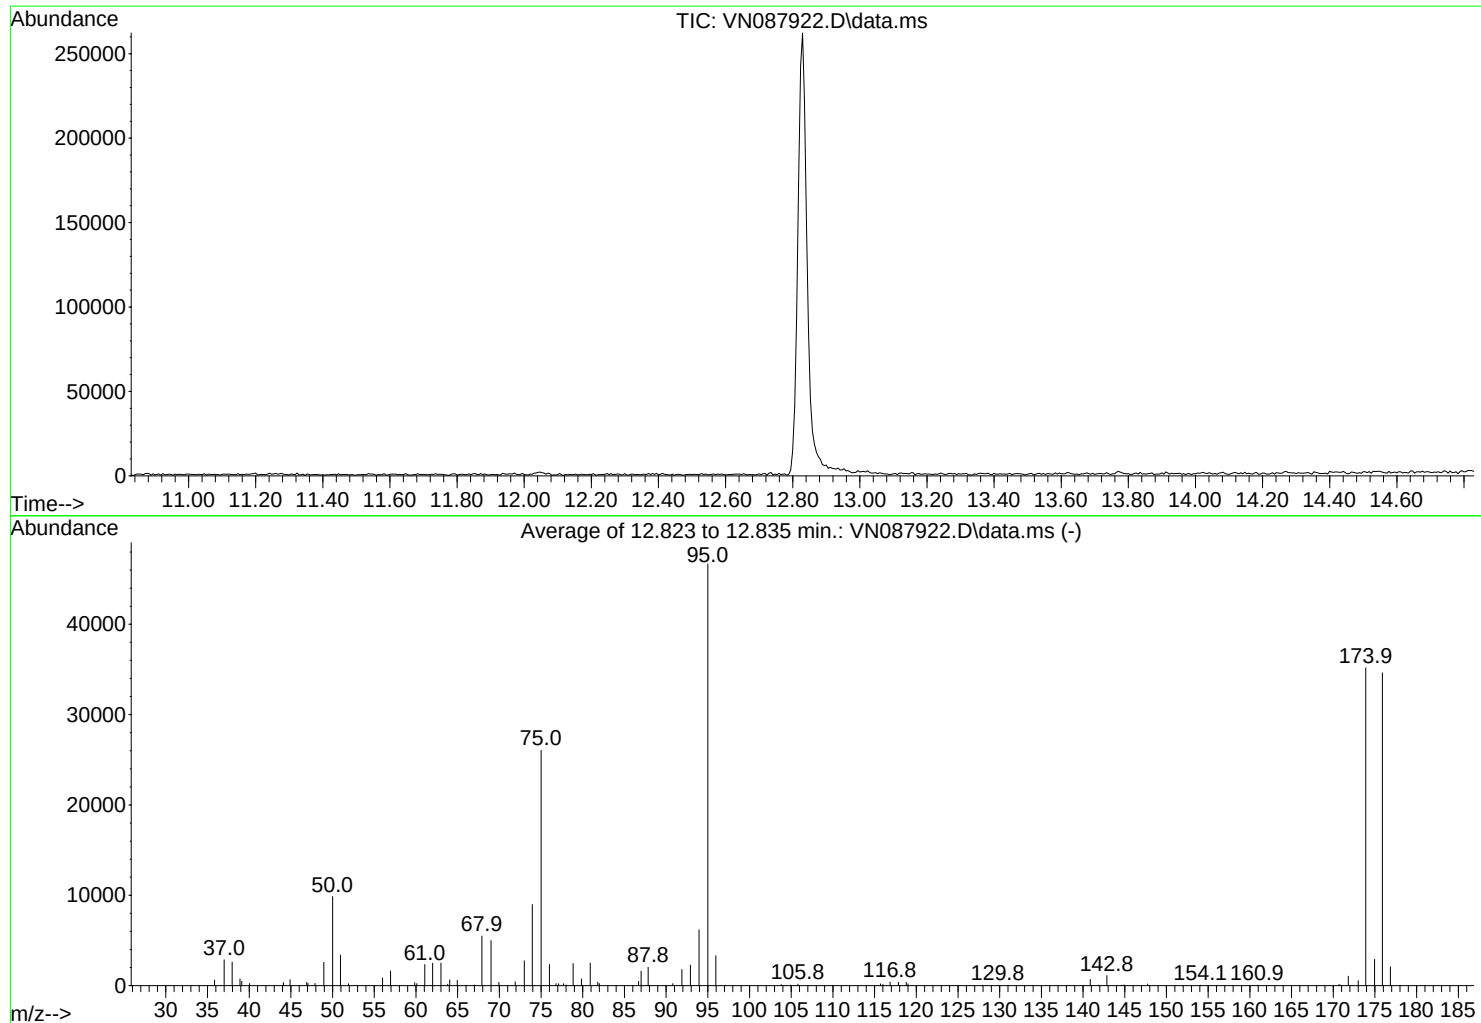

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1840

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	9874	PASS
75	95	30	60	55.8	26056	PASS
95	95	100	100	100.0	46688	PASS
96	95	5	9	7.1	3306	PASS
173	174	0.00	2	1.6	554	PASS
174	95	50	100	75.3	35176	PASS
175	174	5	9	8.3	2908	PASS
176	174	95	101	98.4	34627	PASS
177	176	5	9	6.0	2077	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	625	48.95	2588	63.80	152	75.00	2605
37.00	2871	50.00	9874	64.05	645	76.00	2331
37.95	2605	50.95	3389	64.95	588	76.80	2205
38.90	742	51.90	213	66.00	61	77.10	209
39.10	485	56.00	853	67.00	79	77.70	218
40.05	250	56.95	1606	67.90	5482	78.00	70
44.10	330	59.85	316	69.00	5001	78.85	2440
44.90	658	60.10	236	69.95	346	79.85	751
46.90	367	61.05	2344	71.90	433	80.90	2498
47.05	246	62.00	2480	73.00	2738	81.80	389
47.90	253	63.00	2501	73.95	8981	82.00	222

Average of 12.823 to 12.835 min.: VN087922.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.70	487	104.90	74	141.90	65	173.90	35176
87.00	1618	105.80	183	142.85	1122	174.95	2908
87.85	2037	115.70	188	144.60	61	175.90	34627
90.80	228	116.00	127	144.90	85	176.85	2077
91.90	1791	116.85	389	147.75	172		
92.90	2267	117.85	359	154.10	52		
93.95	6190	118.80	369	160.90	59		
95.00	46688	119.00	193	170.70	137		
95.95	3306	127.90	51	170.90	58		
97.10	61	129.80	57	171.80	1053		
103.80	124	140.85	699	173.00	554		

Instrument :

MSVOA_N

ClientSampleId :

BFB