

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092625\
 Data File : PP075357.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2025 12:52
 Operator : YP\AJ
 Sample : PB169856BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB169856BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/29/2025
 Supervised By :mohammad ahmed 09/30/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 02:03:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 24 10:55:35 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.666	3.798	29943091	96914462	22.884	15.885 #
2) SA Decachlor...	10.455	8.810	23593154	150.5E6	23.651m	24.951

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092625\
Data File : PP075357.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2025 12:52
Operator : YP\AJ
Sample : PB169856BL
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PB169856BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/29/2025
Supervised By :mohammad ahmed 09/30/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 02:03:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 24 10:55:35 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

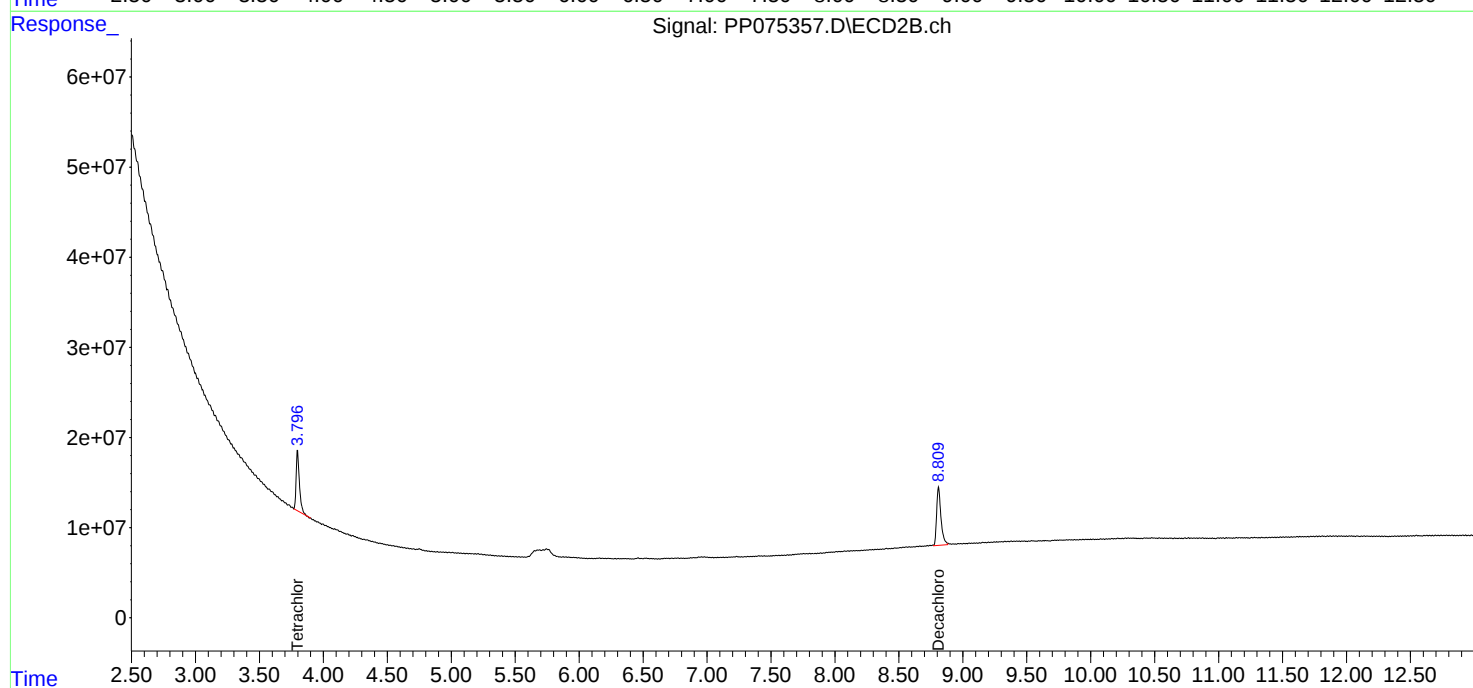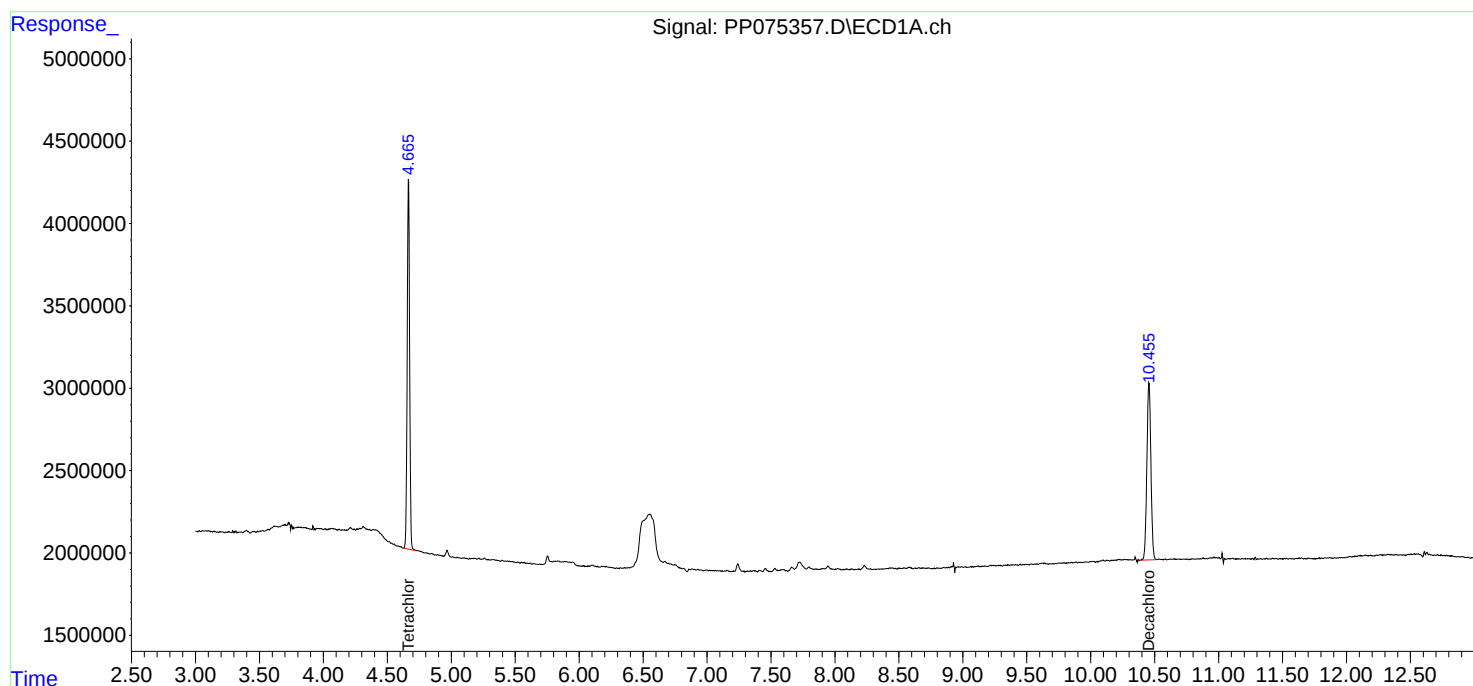

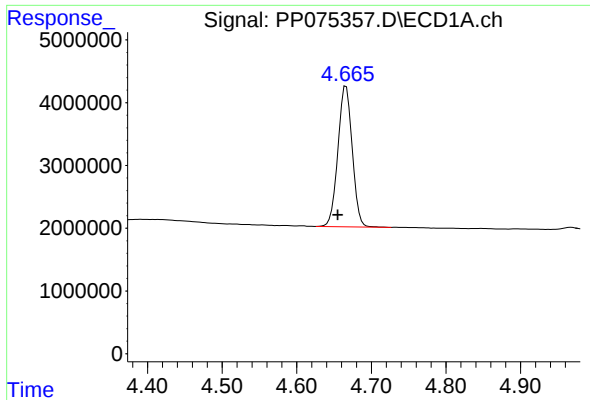


#1 Tetrachloro-m-xylene

R.T.: 4.666 min
Delta R.T.: 0.011 min
Response: 29943091
Conc: 22.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB169856BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/29/2025
Supervised By :mohammad ahmed 09/30/2025

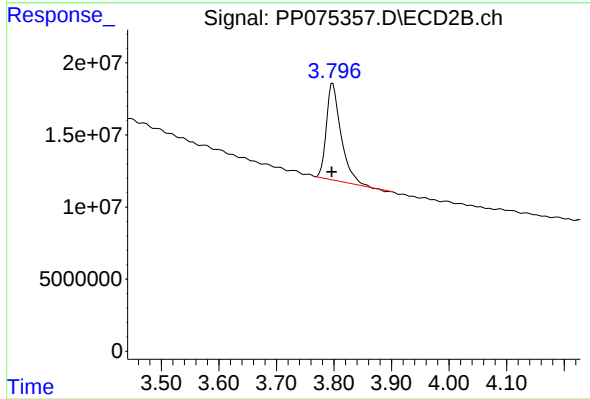


#1 Tetrachloro-m-xylene

R.T.: 3.798 min
Delta R.T.: 0.002 min
Response: 96914462
Conc: 15.89 ng/ml

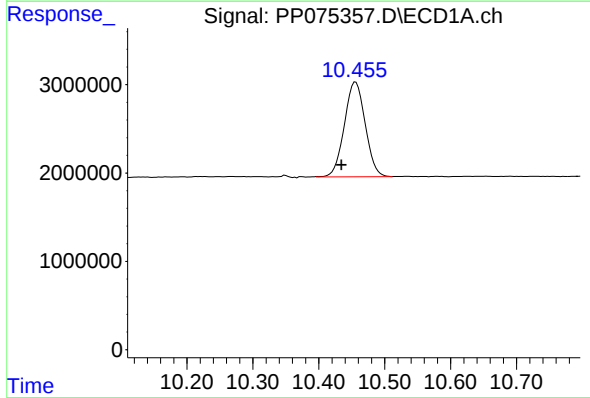

#2 Decachlorobiphenyl

R.T.: 10.455 min
Delta R.T.: 0.020 min
Response: 23593154
Conc: 23.65 ng/ml m

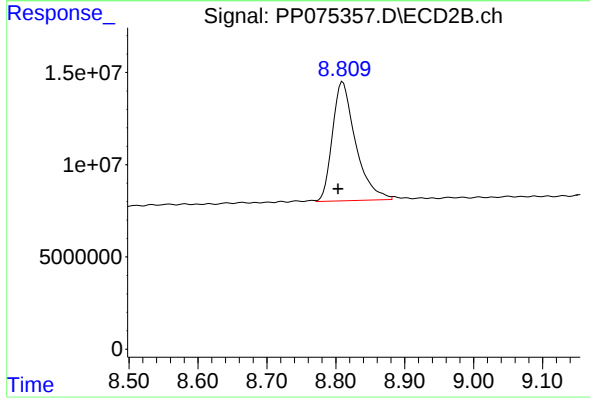

#2 Decachlorobiphenyl

R.T.: 8.810 min
Delta R.T.: 0.007 min
Response: 150516772
Conc: 24.95 ng/ml