
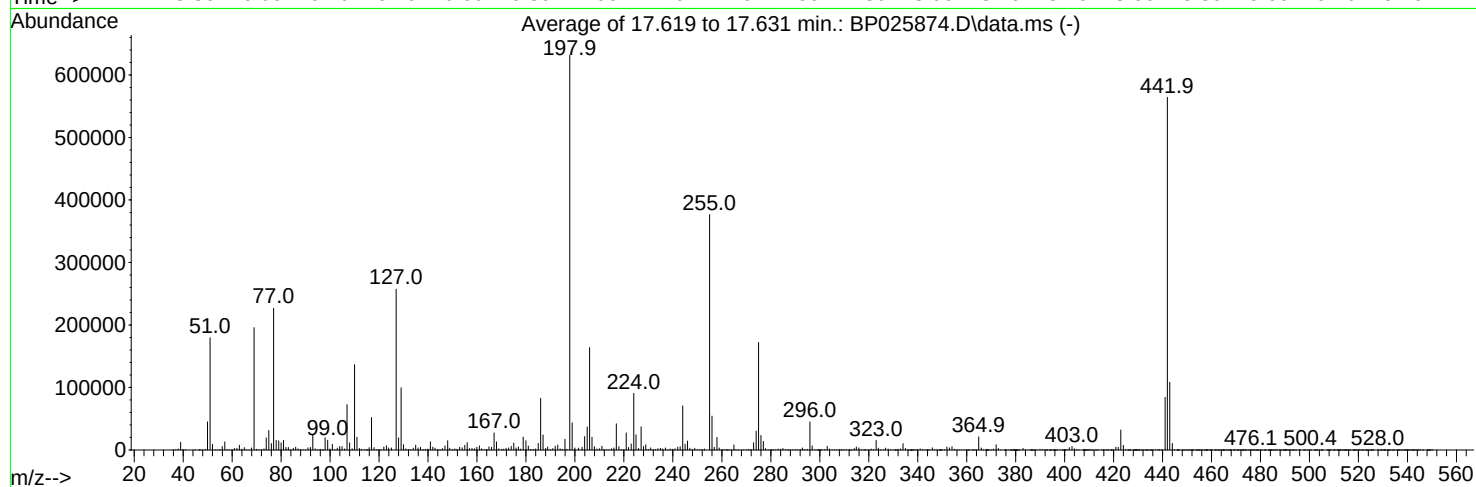


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092925\
Data File : BP025874.D
Acq On : 29 Sep 2025 10:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 11 16:45:04 2025

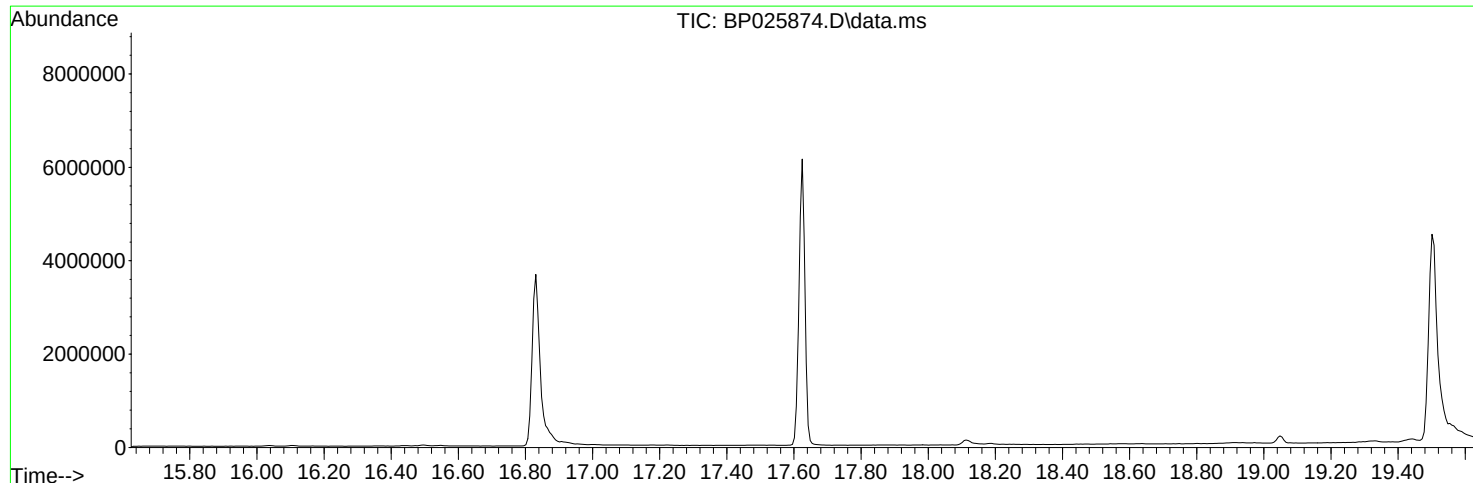




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2485

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	3224	PASS
69	69	100	100	100.0	195709	PASS
70	69	0.00	2	0.5	913	PASS
197	198	0.00	2	0.2	1038	PASS
198	198	100	100	100.0	631900	PASS
199	198	5	9	6.9	43343	PASS
365	198	1	100	3.3	20885	PASS
441	443	0.01	150	77.6	84245	PASS
442	442	100	100	100.0	564169	PASS
443	442	15	24	19.2	108585	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092925\
Data File : BP025874.D
Acq On : 29 Sep 2025 10:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 29 12:06:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

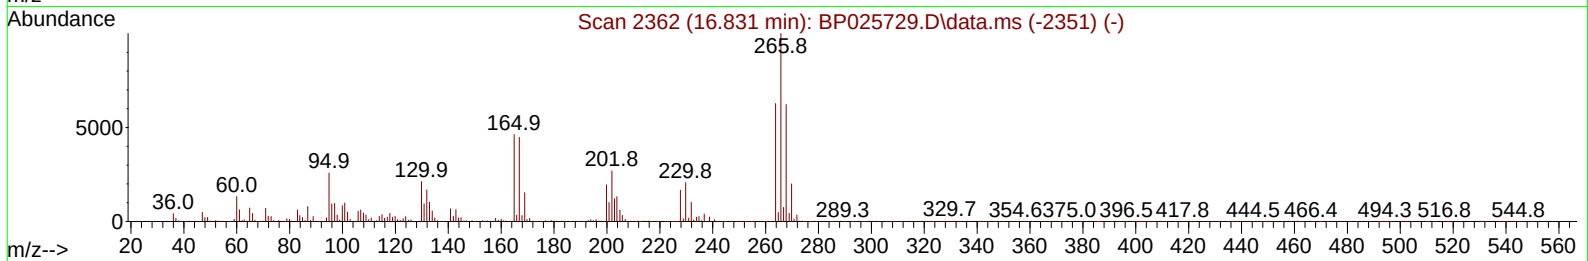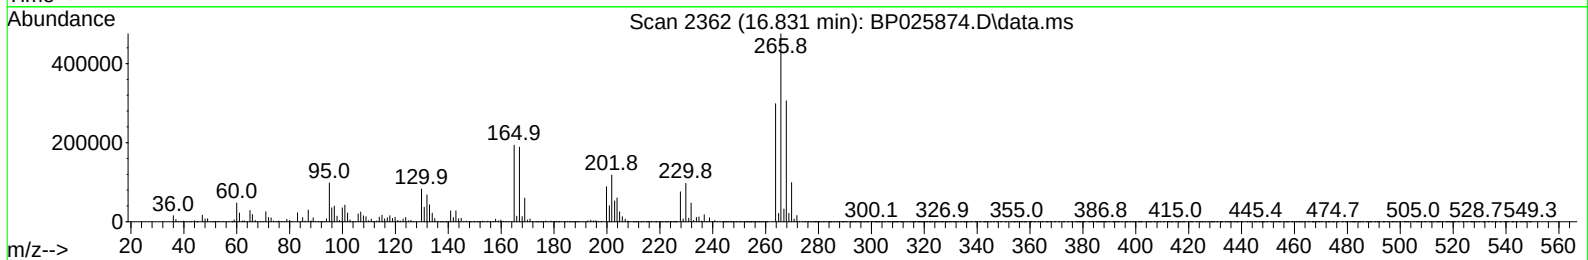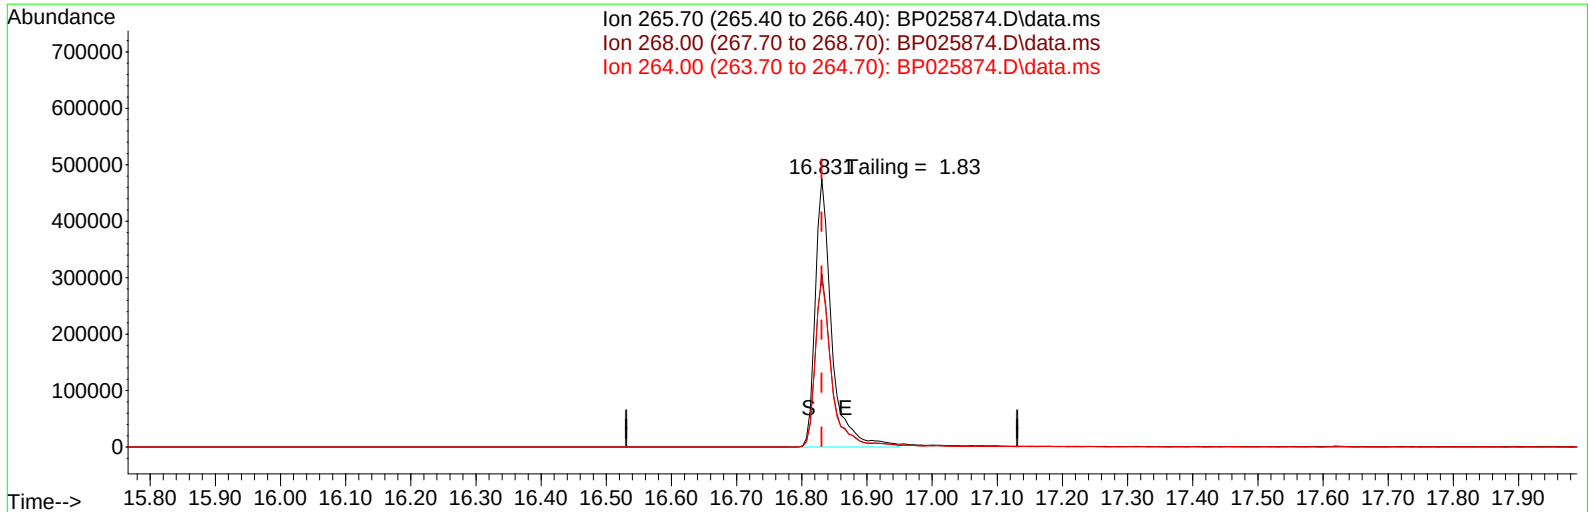

TIC: BP025874.D\data.ms

(70) Pentachlorophenol (C)

16.831min (+ 0.000) 45846.44 ng




response 845567

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.31
264.00	62.70	62.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092925\
Data File : BP025874.D
Acq On : 29 Sep 2025 10:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 29 12:06:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

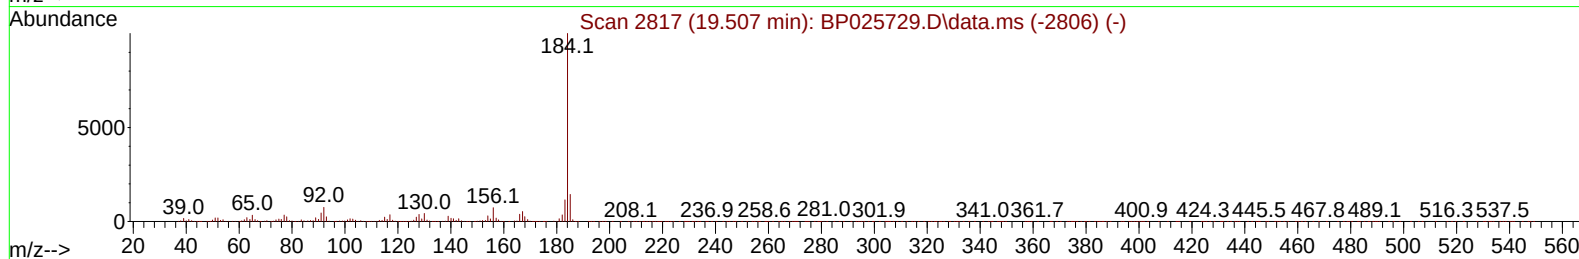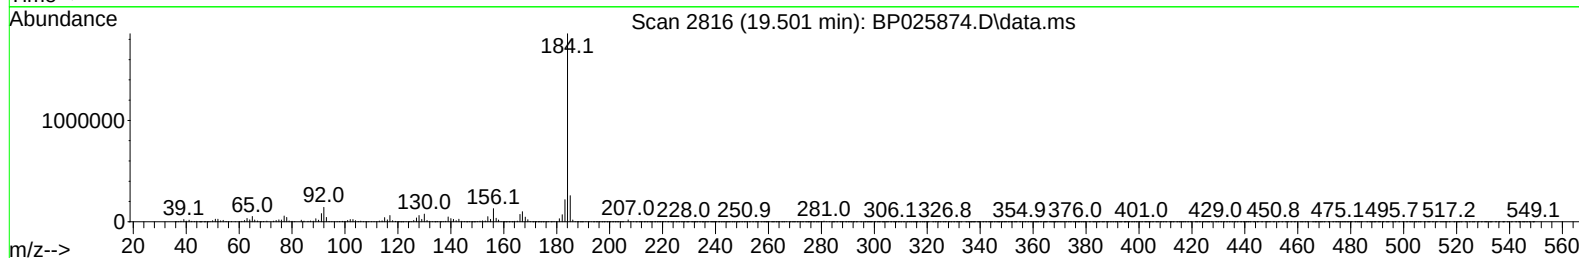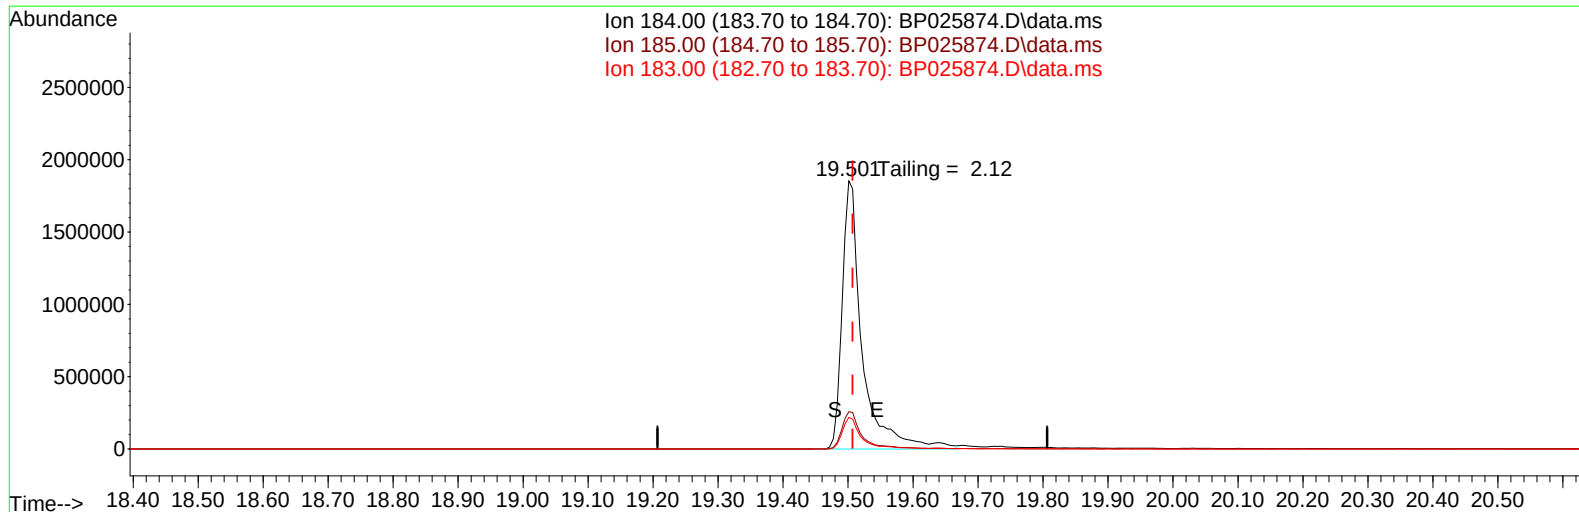

TIC: BP025874.D\data.ms

(77) Benzidine

19.501min (-0.006) 31908.41 ng

response 3894366

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.90
183.00	11.50	11.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/29/2025	BNA_P	<u>BP025874.D</u>
Compound Name	Response	Retention Time
DDT	2183238	20.783
DDD	44359	20.33
DDE	8549	19.795
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
52908	2236146	2.37

Instrument :
BNA_P
ClientSampleId :
DFTPP