
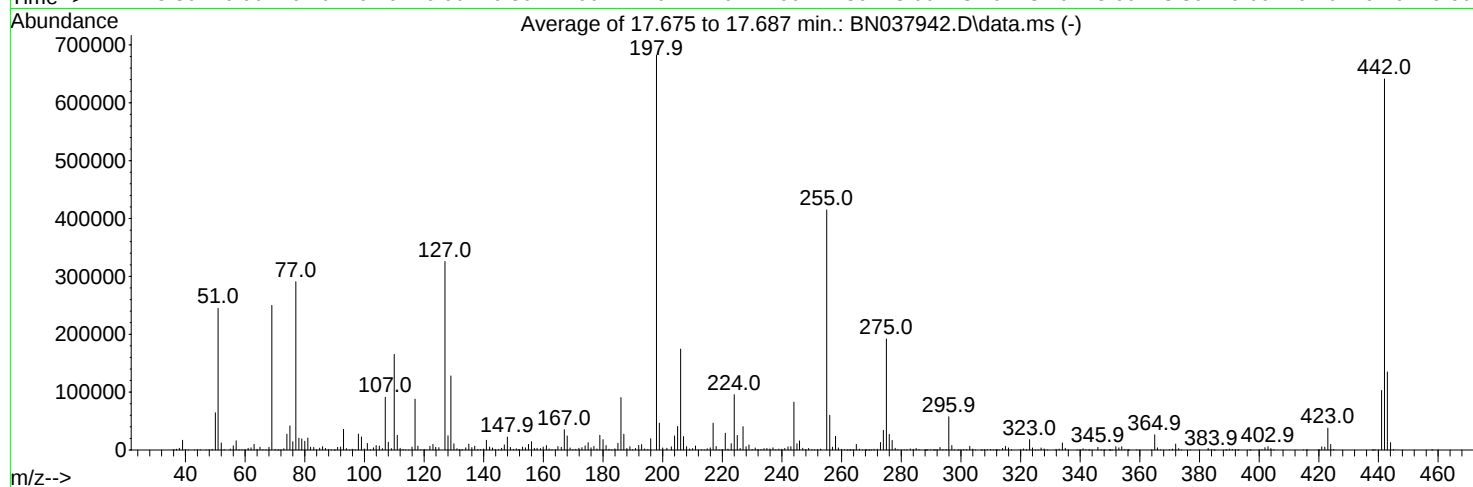


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093025\
Data File : BN037942.D
Acq On : 30 Sep 2025 11:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 24 11:00:01 2025

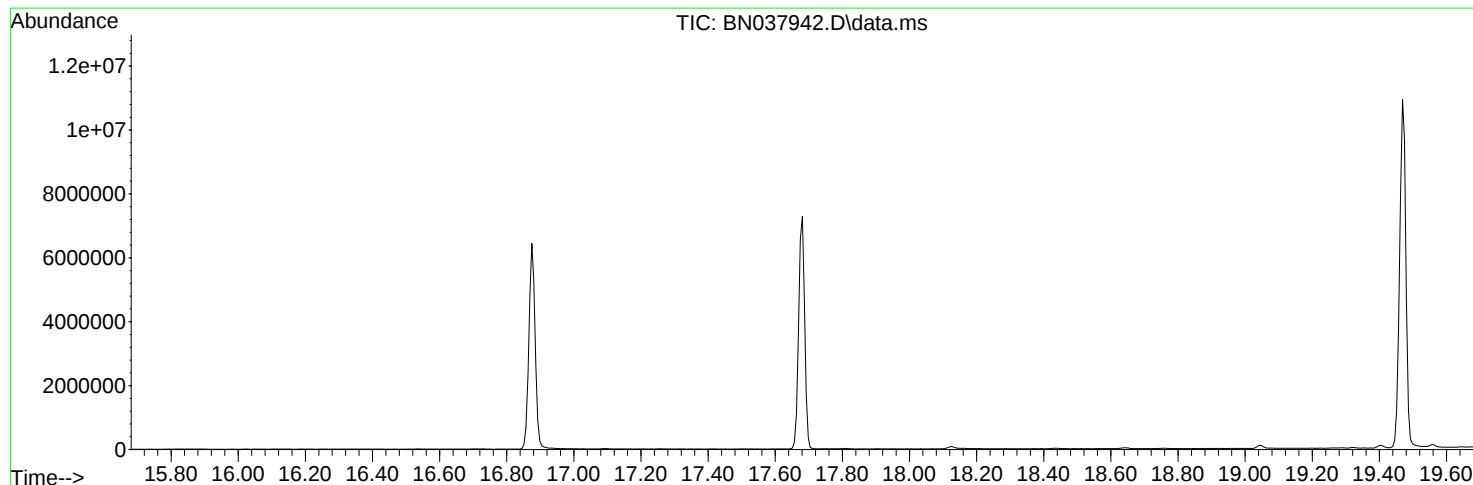




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2472

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.9	4633	PASS
69	69	100	100	100.0	249877	PASS
70	69	0.00	2	0.5	1311	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	682325	PASS
199	198	5	9	6.8	46557	PASS
365	198	1	100	3.8	26251	PASS
441	443	0.01	150	76.2	102832	PASS
442	442	100	100	100.0	641173	PASS
443	442	15	24	21.0	134901	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093025\
Data File : BN037942.D
Acq On : 30 Sep 2025 11:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 30 13:14:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

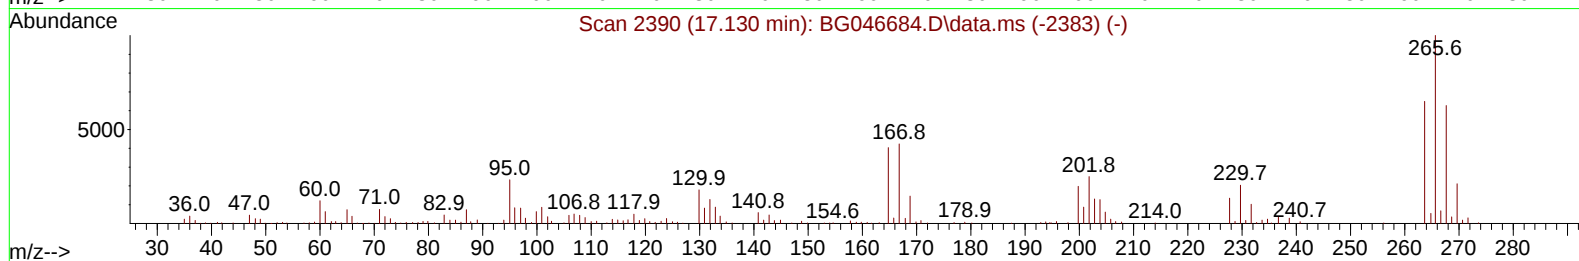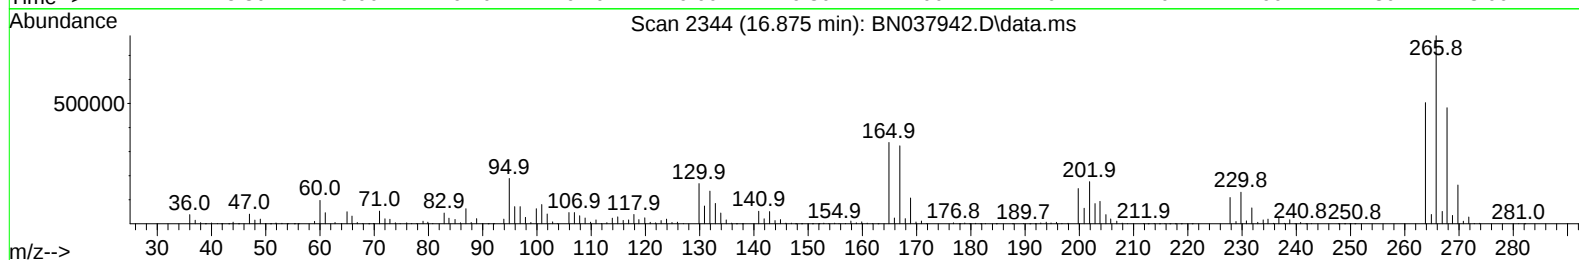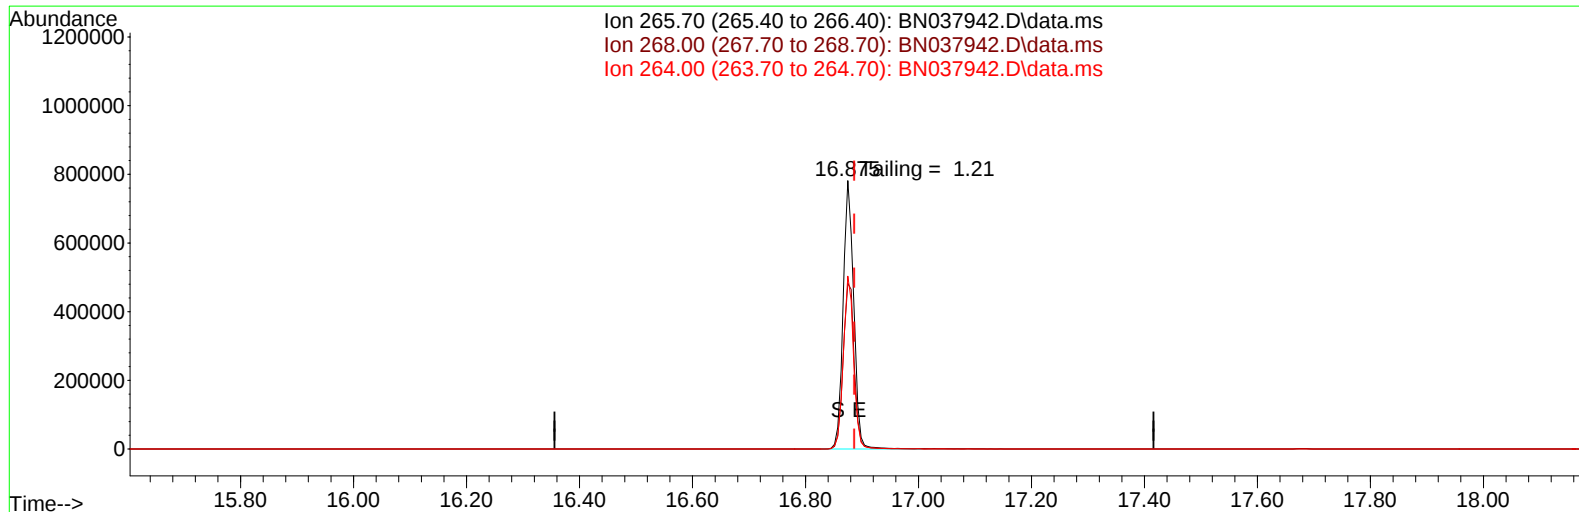

TIC: BN037942.D\data.ms

(70) Pentachlorophenol (C)

16.875min (-0.011) 31430.20 ng




response 1011044

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.70
264.00	61.60	64.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093025\
Data File : BN037942.D
Acq On : 30 Sep 2025 11:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 30 13:14:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

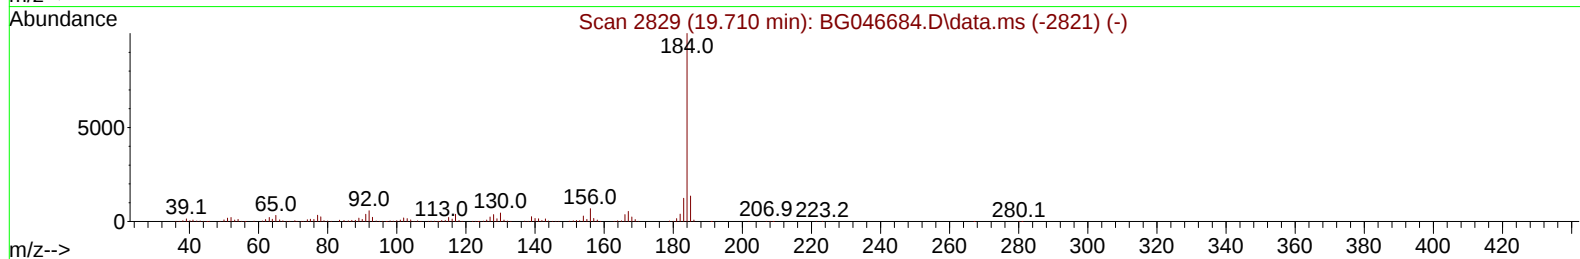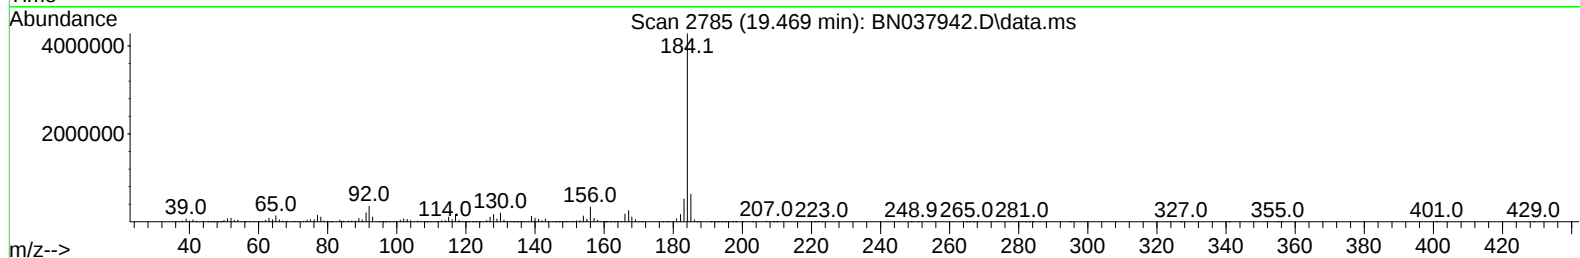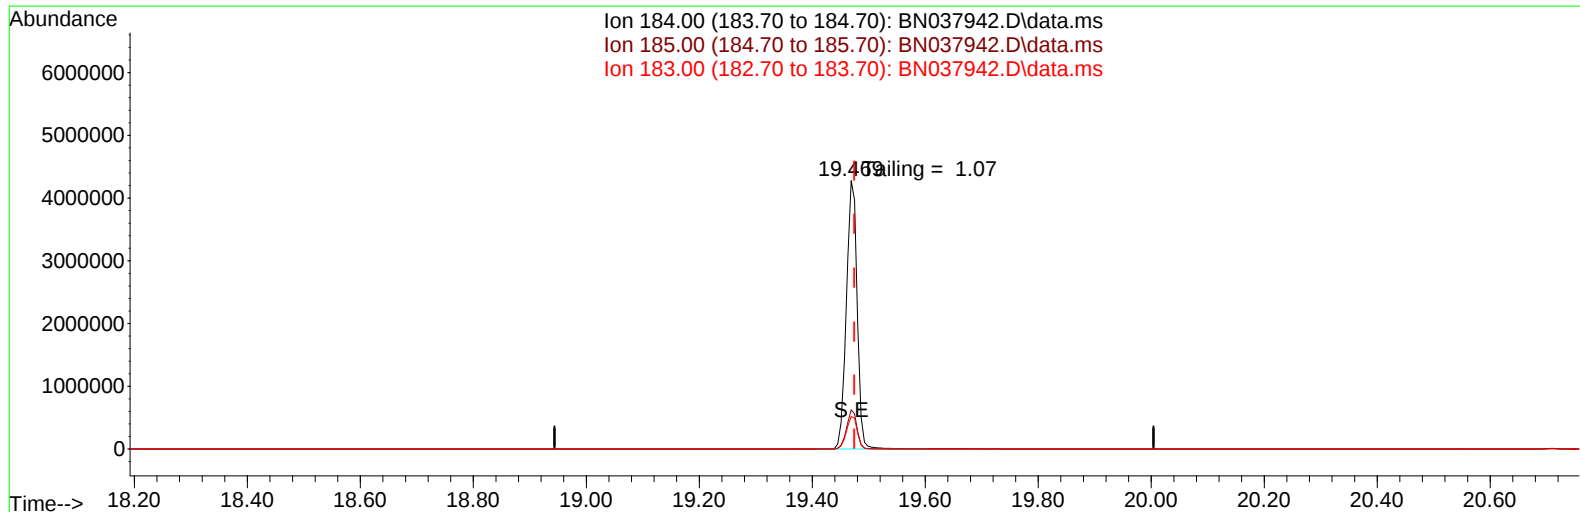

TIC: BN037942.D\data.ms

(77) Benzidine

19.469min (-0.005) 0.00 ng

response 5670270

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.62
183.00	13.20	12.12
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/30/2025	BNA_N	<u>BN037942.D</u>
Compound Name	Response	Retention Time
DDT	2784316	20.71
DDD	23255	20.263
DDE	189	19.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23444	2807760	0.83

Instrument :
BNA_N
ClientSampleId :
DFTPP