


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093025\
Data File : BN037960.D
Acq On : 01 Oct 2025 00:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 24 11:00:01 2025

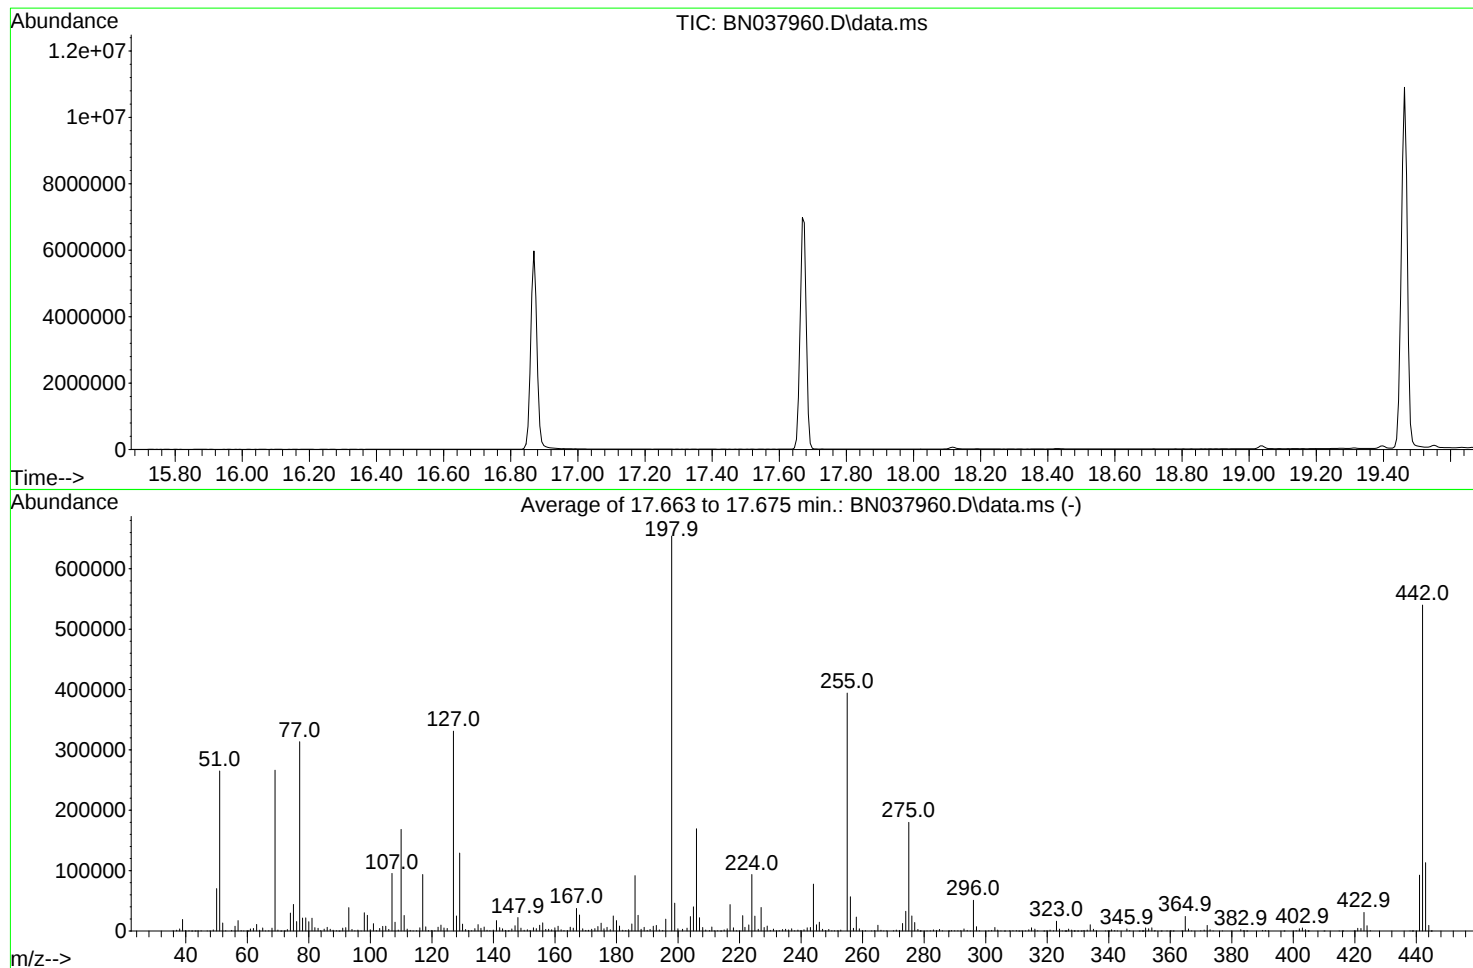




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	4757	PASS
69	69	100	100	100.0	266453	PASS
70	69	0.00	2	0.6	1630	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	654037	PASS
199	198	5	9	7.1	46264	PASS
365	198	1	100	3.7	24233	PASS
441	443	0.01	150	81.9	92611	PASS
442	442	100	100	100.0	540011	PASS
443	442	15	24	20.9	113085	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093025\
Data File : BN037960.D
Acq On : 01 Oct 2025 00:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 01 01:44:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

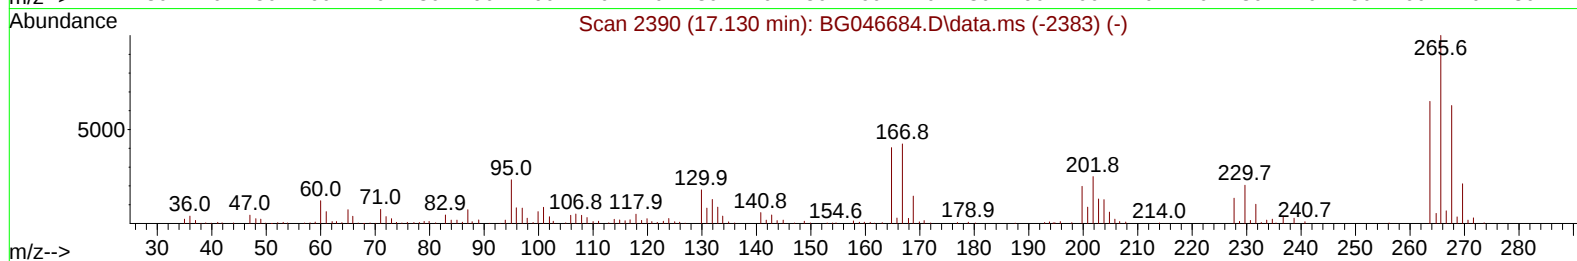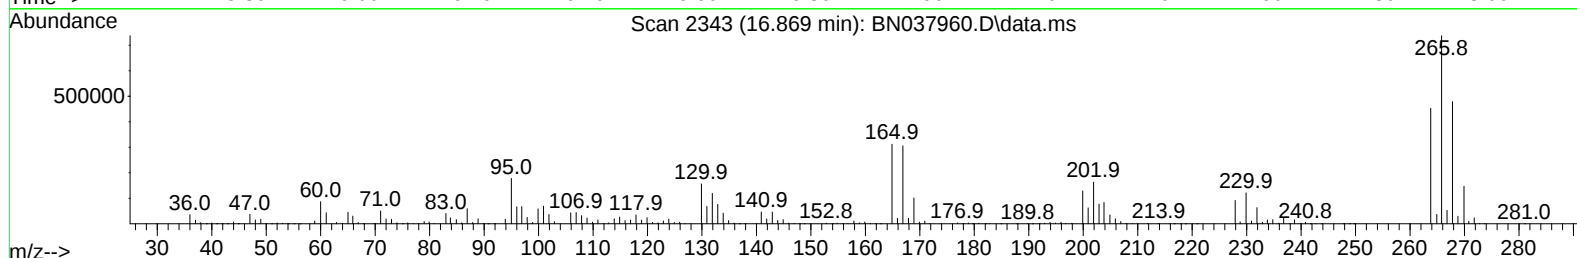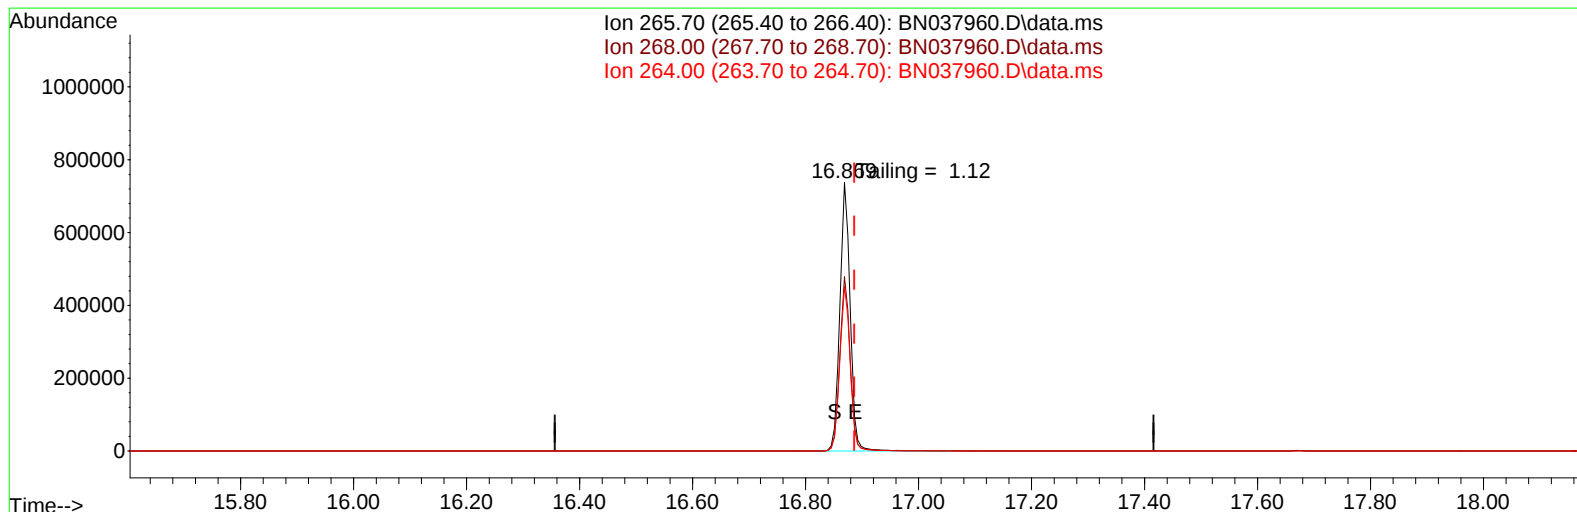

TIC: BN037960.D\data.ms

(70) Pentachlorophenol (C)

16.869min (-0.017) 27797.15 ng




response 931043

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.93
264.00	61.60	61.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093025\
Data File : BN037960.D
Acq On : 01 Oct 2025 00:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 01 01:44:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

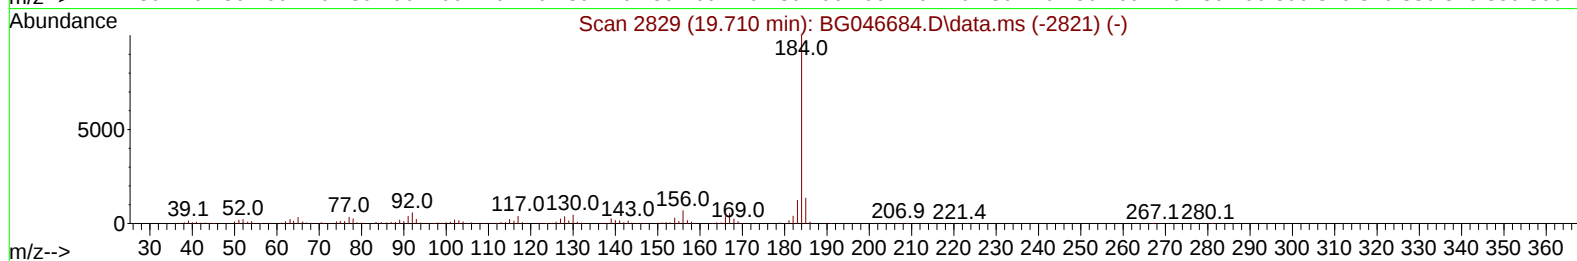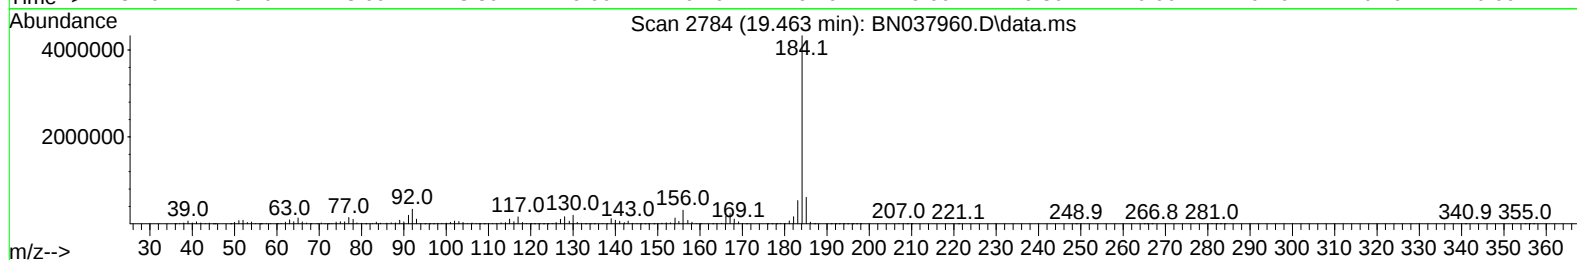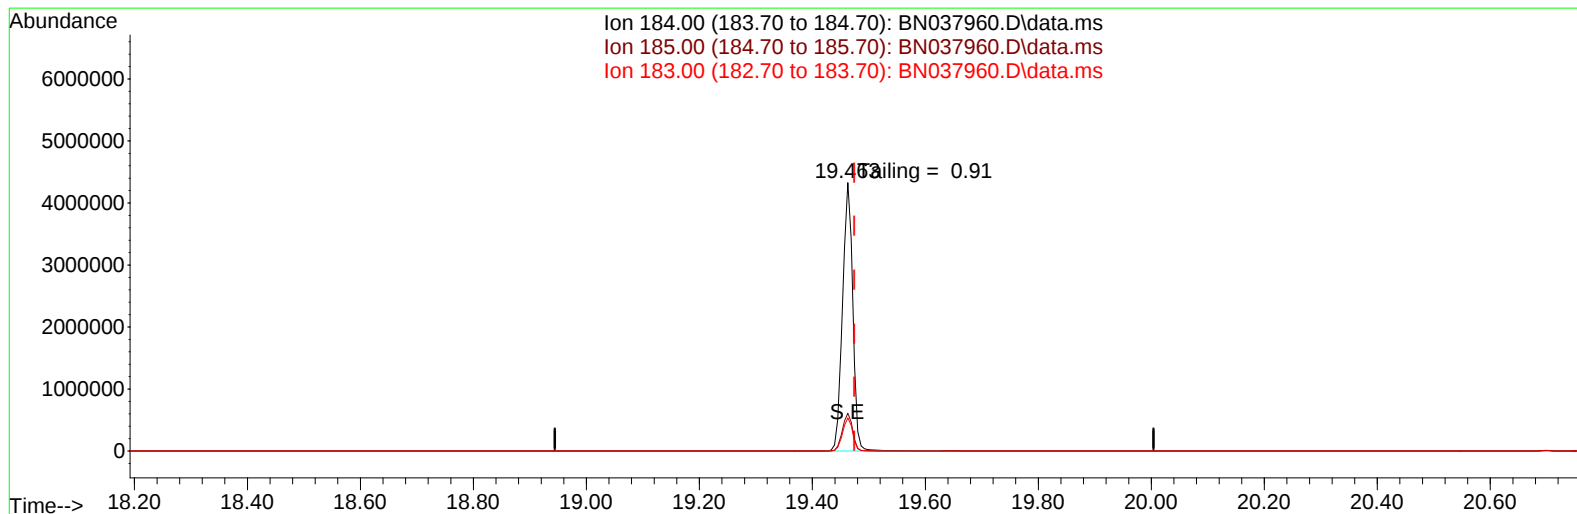

TIC: BN037960.D\data.ms

(77) Benzidine

19.463min (-0.011) 0.00 ng

response 5415438

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.08
183.00	13.20	12.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/30/2025	BNA_N	<u>BN037960.D</u>
Compound Name	Response	Retention Time
DDT	2668483	20.698
DDD	21470	20.257
DDE	699	19.757
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22169	2690652	0.82

Instrument :
BNA_N
ClientSampleId :
DFTPP