

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100325\
 Data File : VX047988.D
 Acq On : 03 Oct 2025 13:09
 Operator : JC/MD
 Sample : Q3193-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EB04-20250923

Quant Time: Oct 03 23:46:53 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 17 06:39:58 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	129971	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.751	114	263211	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	269714	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	138755	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	104463	50.494	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 100.980%	
35) Dibromofluoromethane	5.373	113	85003	48.154	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 96.300%	
50) Toluene-d8	8.635	98	292943	47.960	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 95.920%	
62) 4-Bromofluorobenzene	11.061	95	126344	54.503	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 109.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100325\
Data File : VX047988.D
Acq On : 03 Oct 2025 13:09
Operator : JC/MD
Sample : Q3193-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB04-20250923


Quant Time: Oct 03 23:46:53 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 17 06:39:58 2025
Response via : Initial Calibration

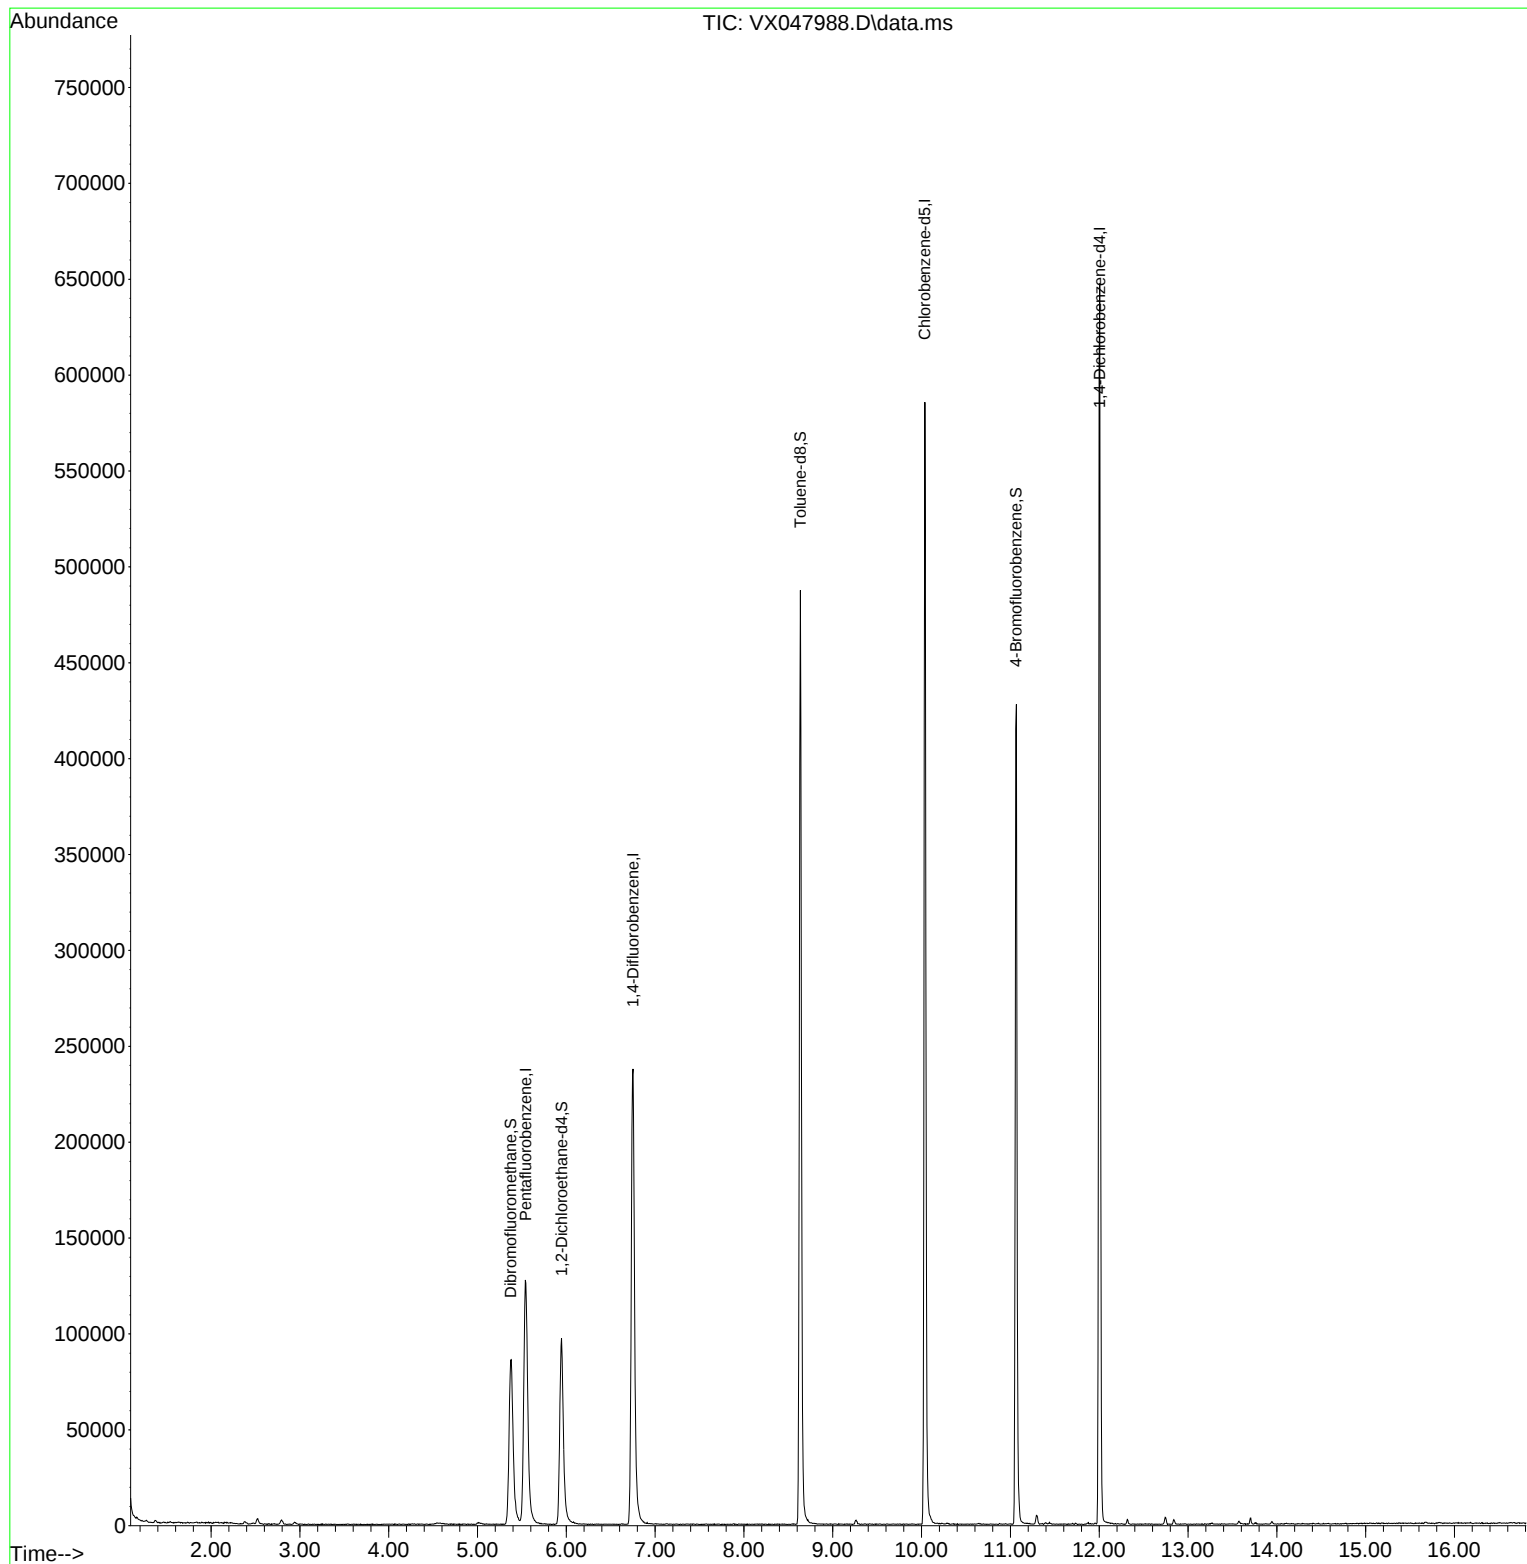


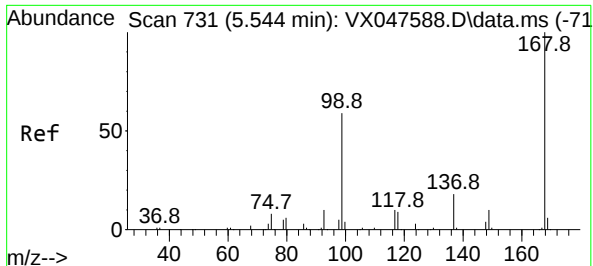


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX047988.D
Acq: 03 Oct 2025 13:09

Instrument :
MSVOA_X
ClientSampleId :
EB04-20250923



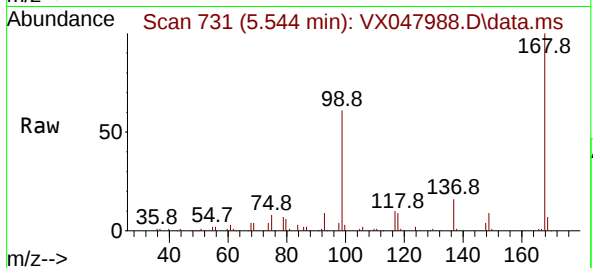


Tgt Ion:168 Resp: 129971
Ion Ratio Lower Upper
168 100
99 61.5 48.8 73.2

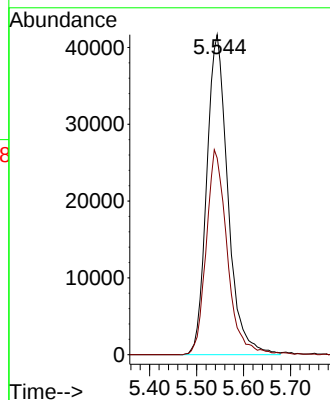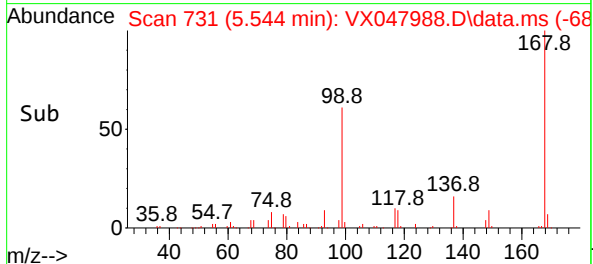

#33
1,2-Dichloroethane-d4
Concen: 50.494 ug/l
RT: 5.946 min Scan# 797
Delta R.T. 0.006 min
Lab File: VX047988.D
Acq: 03 Oct 2025 13:09

Tgt Ion: 65 Resp: 104463
Ion Ratio Lower Upper
65 100
67 51.2 0.0 103.0

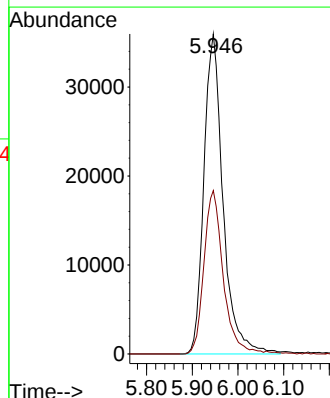
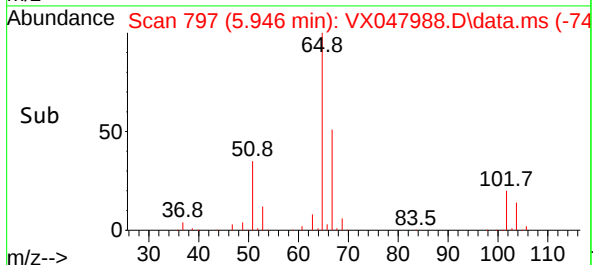
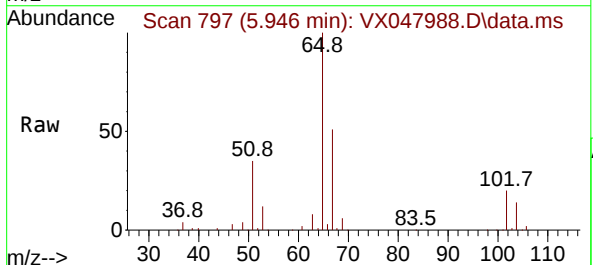




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.751 min Scan# 91
Delta R.T. 0.006 min
Lab File: VX047988.D
Acq: 03 Oct 2025 13:09




Instrument :
MSVOA_X
ClientSampleId :
EB04-20250923

Tgt Ion:114 Resp: 263211
Ion Ratio Lower Upper
114 100
63 20.9 0.0 44.0
88 15.6 0.0 34.2

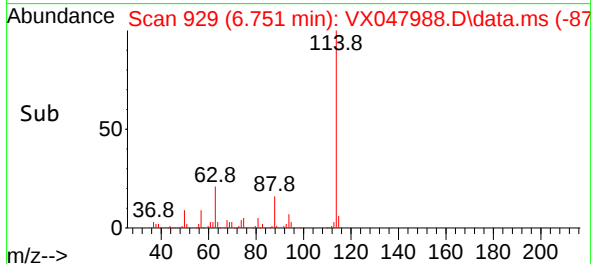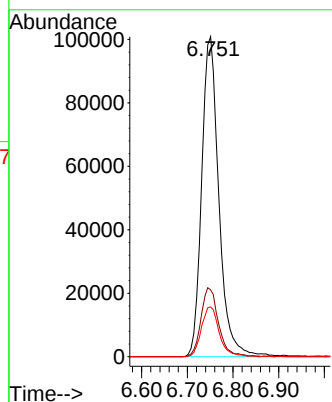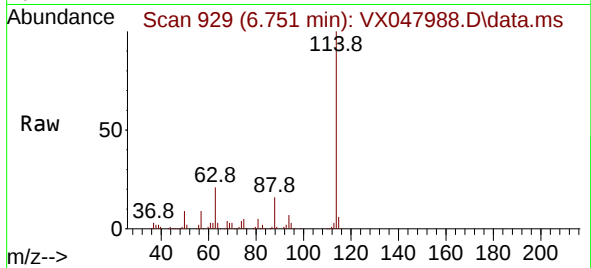

#35
Dibromofluoromethane
Concen: 48.154 ug/l
RT: 5.373 min Scan# 703
Delta R.T. -0.000 min
Lab File: VX047988.D
Acq: 03 Oct 2025 13:09

Tgt Ion:113 Resp: 85003
Ion Ratio Lower Upper
113 100
111 103.3 80.9 121.3
192 17.4 14.2 21.4

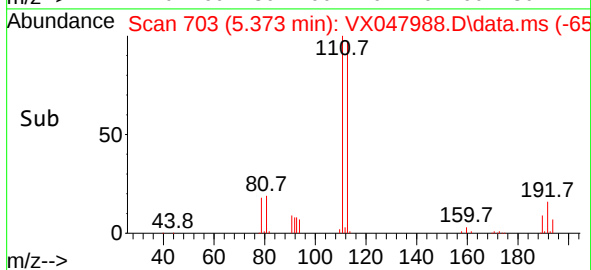
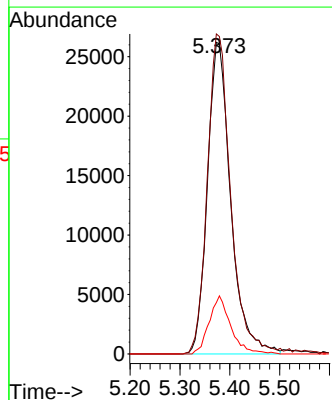
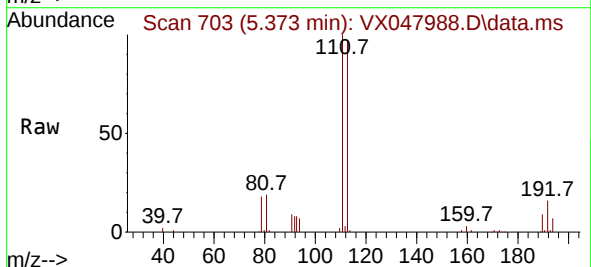




#50
Toluene-d8
Concen: 47.960 ug/l
RT: 8.635 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX047988.D
Acq: 03 Oct 2025 13:09




Instrument :
MSVOA_X
ClientSampleId :
EB04-20250923


Tgt Ion: 98 Resp: 292943
Ion Ratio Lower Upper
98 100
100 66.9 53.0 79.4

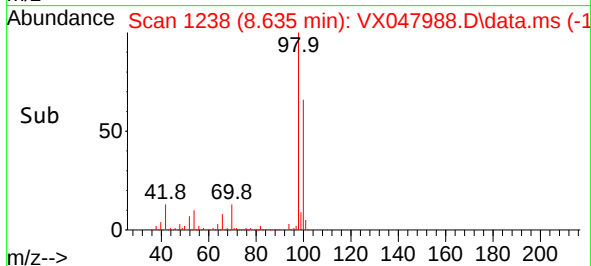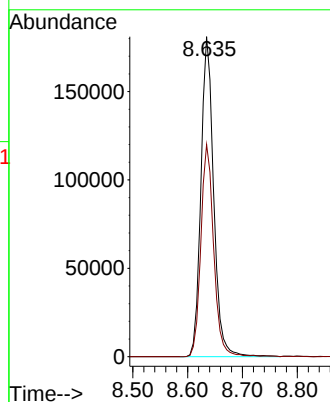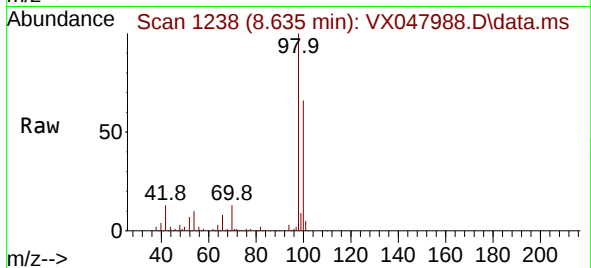

#62
4-Bromofluorobenzene
Concen: 54.503 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. -0.000 min
Lab File: VX047988.D
Acq: 03 Oct 2025 13:09

Tgt Ion: 95 Resp: 126344
Ion Ratio Lower Upper
95 100
174 72.2 0.0 141.6
176 70.0 0.0 138.4


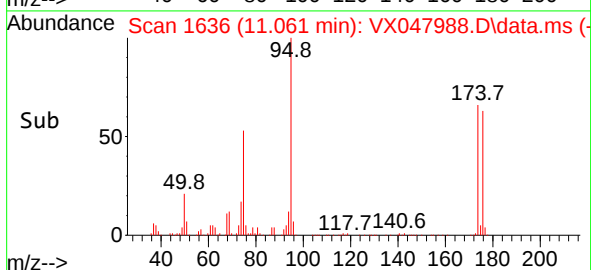
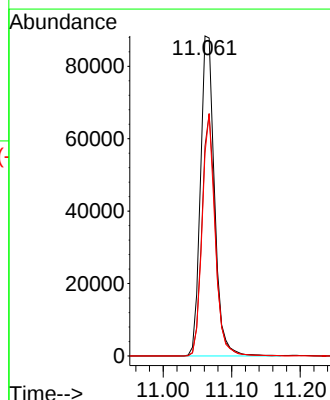
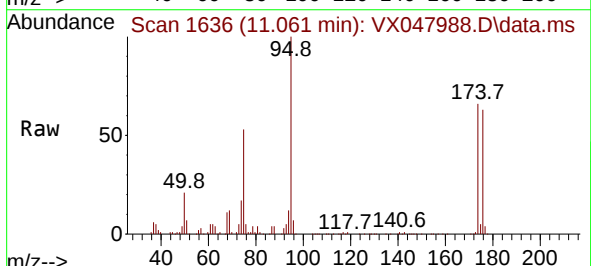


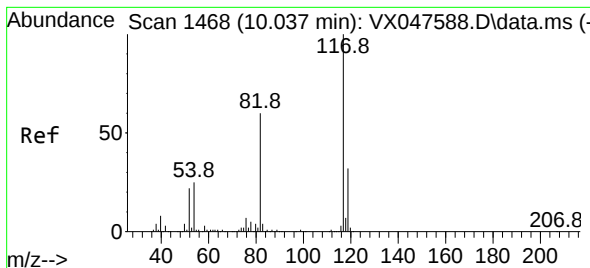

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.037 min Scan# 1468
Delta R.T. -0.000 min
Lab File: VX047988.D
Acq: 03 Oct 2025 13:09

Instrument :
MSVOA_X
ClientSampleId :
EB04-20250923

Tgt Ion:117 Resp: 269714
Ion Ratio Lower Upper
117 100
82 58.3 47.8 71.6
119 33.1 25.2 37.8

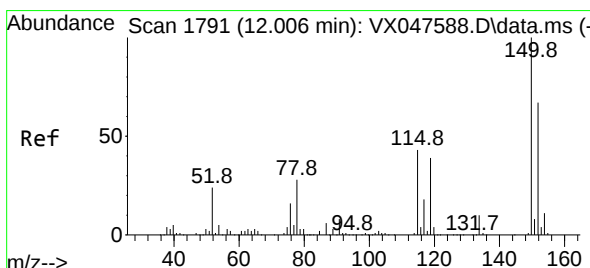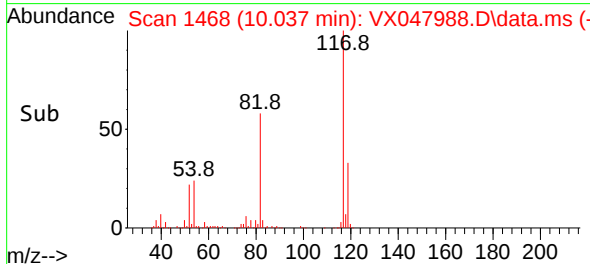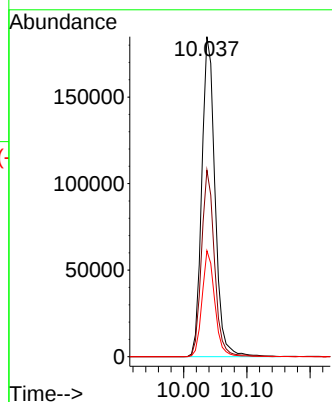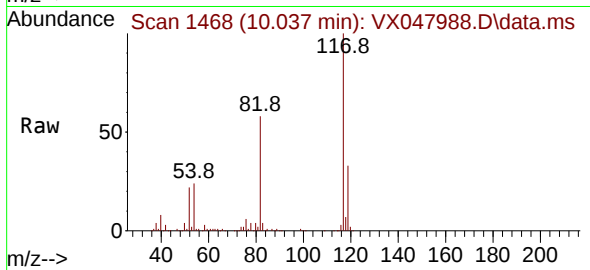

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. -0.000 min
Lab File: VX047988.D
Acq: 03 Oct 2025 13:09

Tgt Ion:152 Resp: 138755
Ion Ratio Lower Upper
152 100
115 60.4 44.9 134.5
150 155.8 0.0 352.0

