


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100625\
Data File : BN038003.D
Acq On : 06 Oct 2025 10:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 24 11:00:01 2025

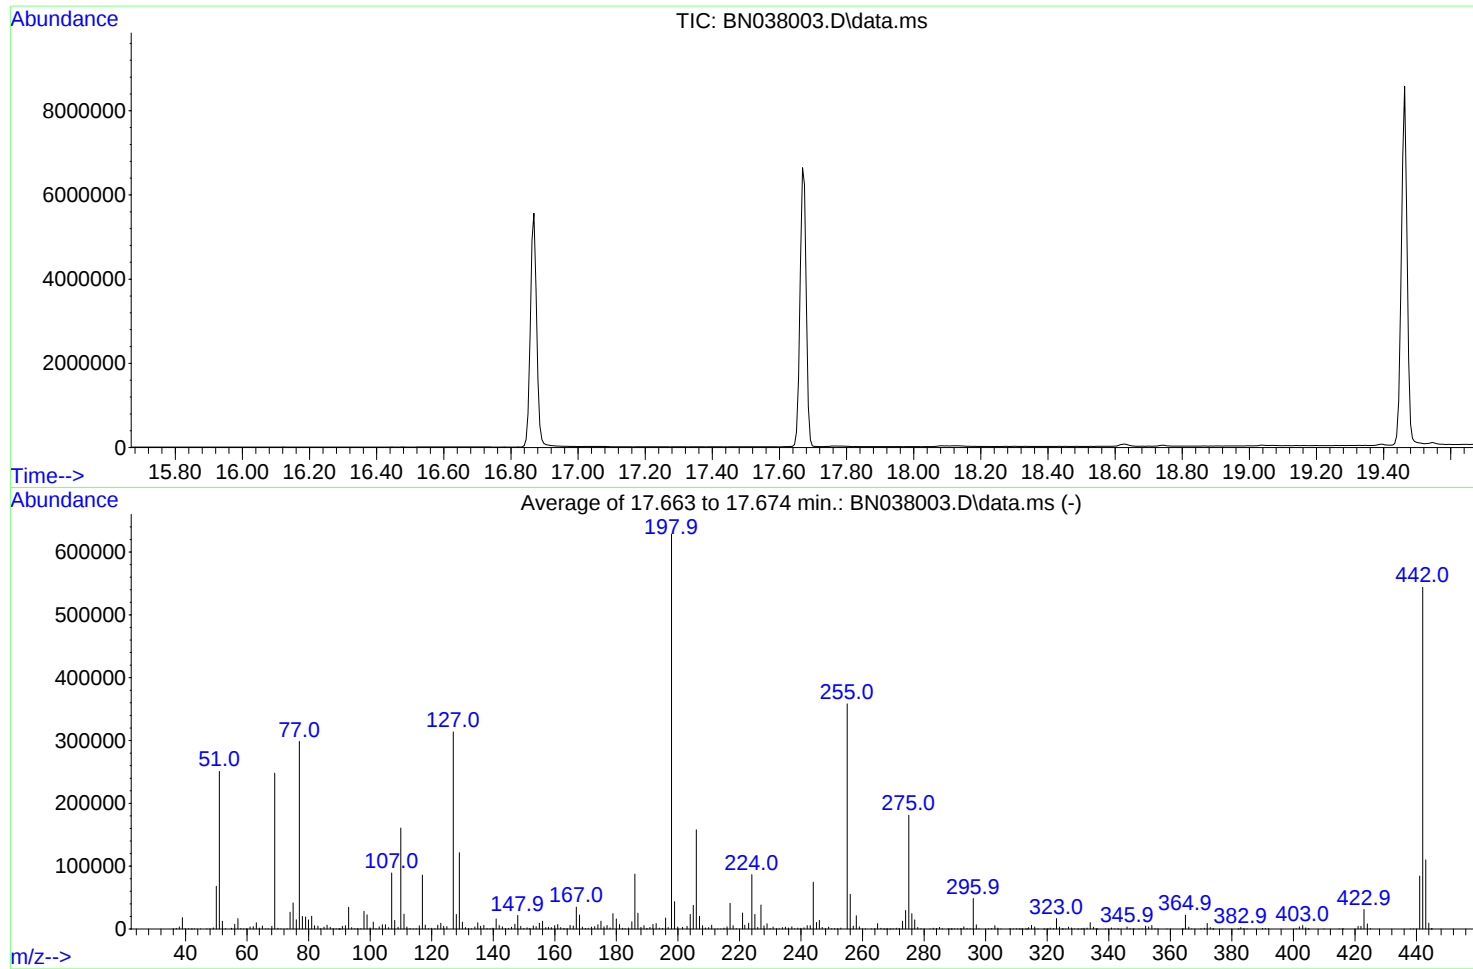

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	4386	PASS
69	69	100	100	100.0	248192	PASS
70	69	0.00	2	0.5	1328	PASS
197	198	0.00	2	0.4	2346	PASS
198	198	100	100	100.0	628459	PASS
199	198	5	9	6.9	43651	PASS
365	198	1	100	3.5	21859	PASS
441	443	0.01	150	76.6	84267	PASS
442	442	100	100	100.0	543808	PASS
443	442	15	24	20.2	109976	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/6/2025	BNA_N	<u>BN038003.D</u>
Compound Name	Response	Retention Time
DDT	2162356	20.698
DDD	10094	20.315
DDE	758	19.757
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10852	2173208	0.50

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100625\
Data File : BN038003.D
Acq On : 06 Oct 2025 10:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 06 11:09:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

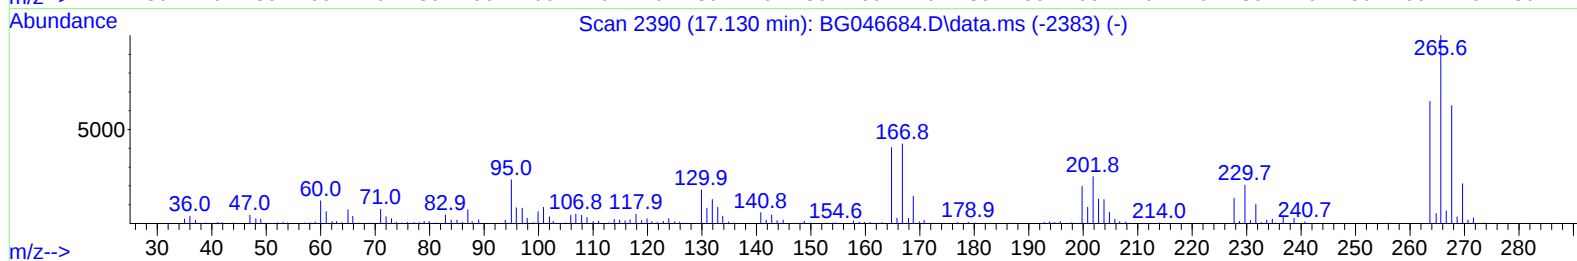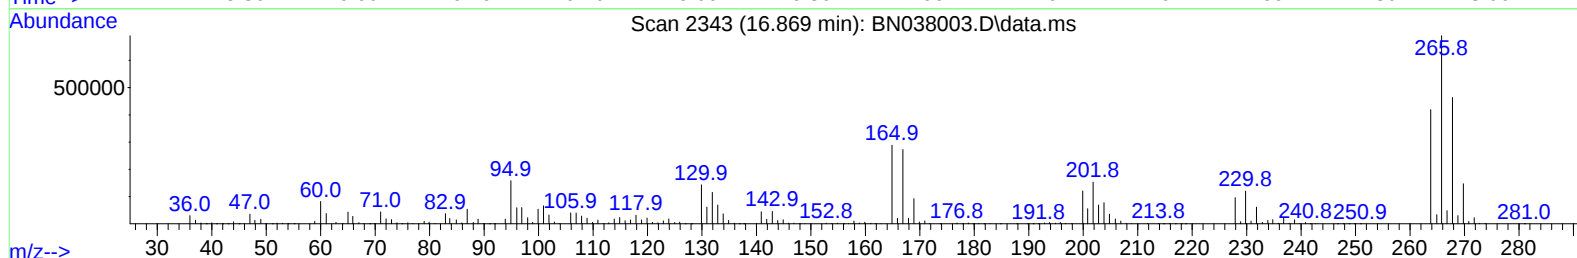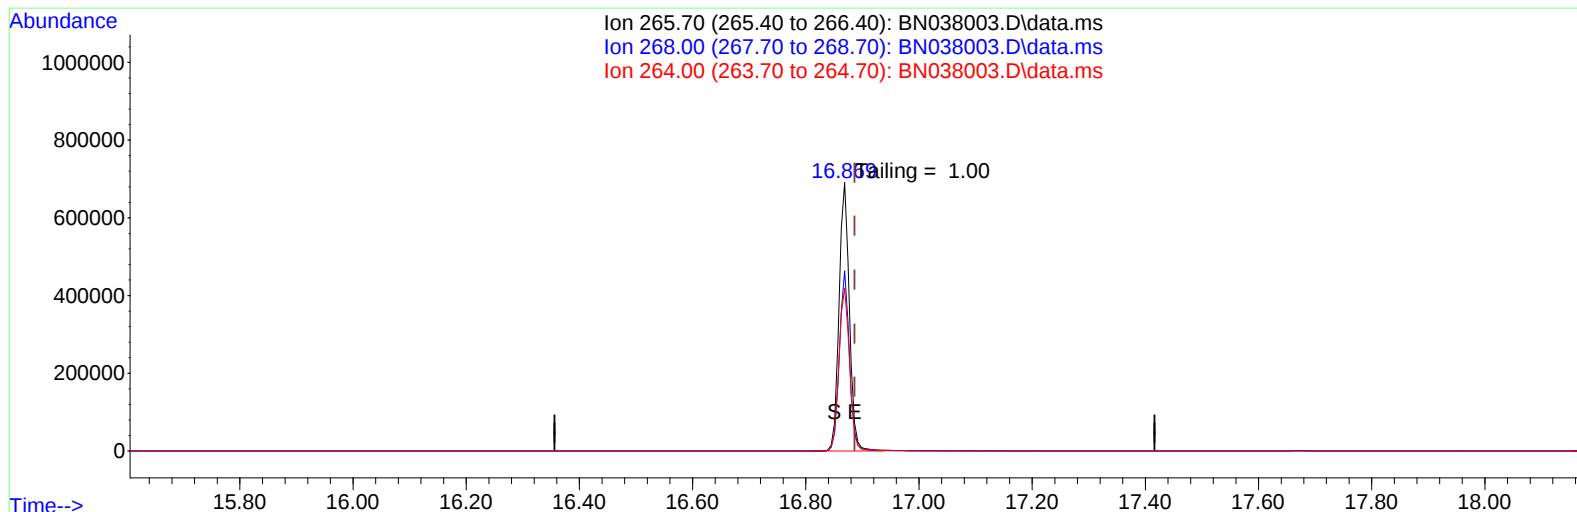

TIC: BN038003.D\data.ms

(70) Pentachlorophenol (C)

16.869min (-0.017) 28237.23 ng




response 876201

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.14
264.00	61.60	60.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100625\
Data File : BN038003.D
Acq On : 06 Oct 2025 10:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 06 11:09:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

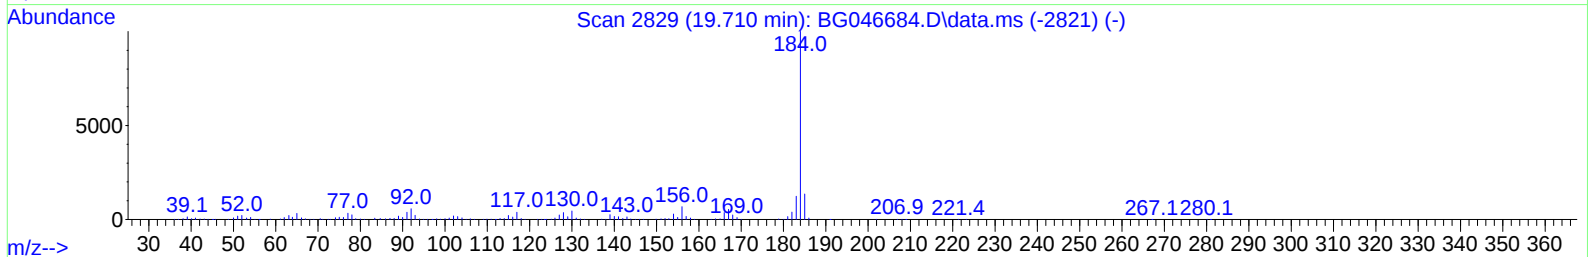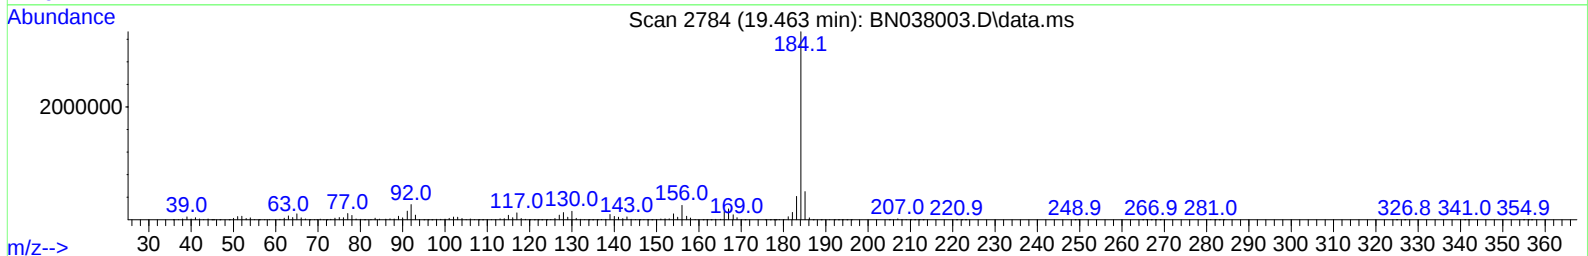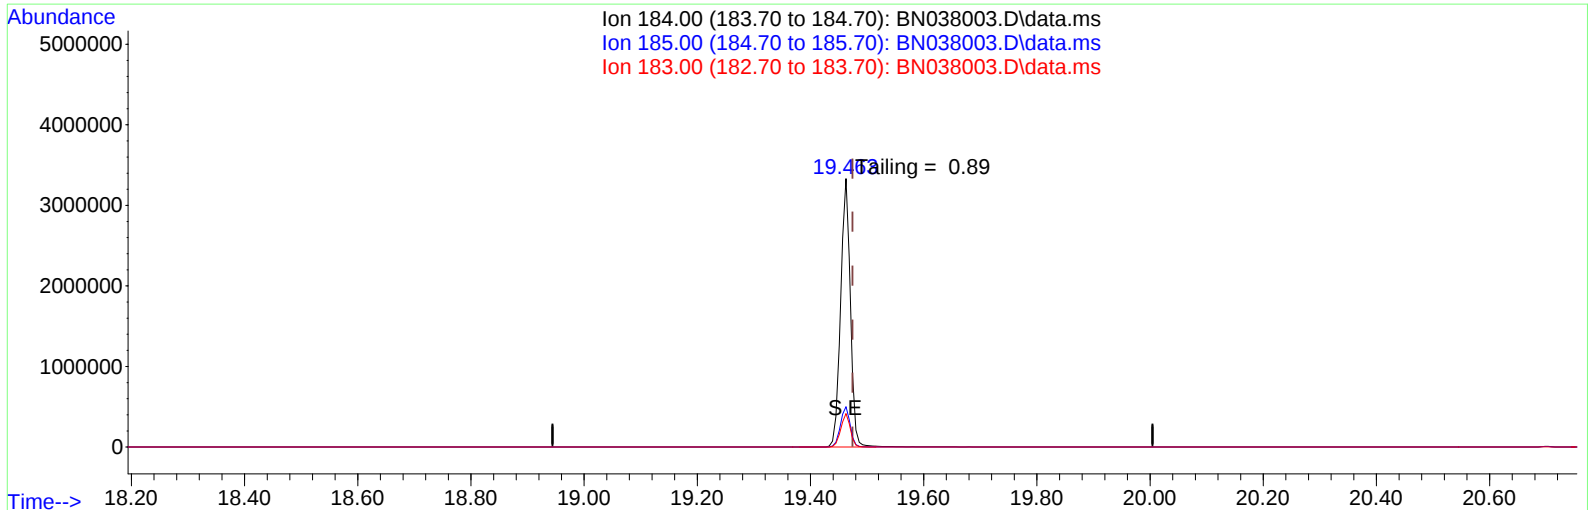

TIC: BN038003.D\data.ms

(77) Benzidine

19.463min (-0.012) 0.00 ng

response 4005964

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.03
183.00	13.20	12.47
0.00	0.00	0.00