

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100625\
 Data File : BN038026.D
 Acq On : 07 Oct 2025 01:57
 Operator : RC/JU
 Sample : Q3194-16
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EB06-20250924

Quant Time: Oct 07 04:16:33 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092325.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 24 11:00:01 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.804	152	7814	0.400	ng	-0.02
7) Naphthalene-d8	10.605	136	22108	0.400	ng	-0.02
13) Acenaphthene-d10	14.462	164	10302	0.400	ng	-0.01
19) Phenanthrene-d10	17.211	188	18362	0.400	ng	-0.01
29) Chrysene-d12	21.384	240	13636	0.400	ng	#-0.02
35) Perylene-d12	23.706	264	11958	0.400	ng	#-0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.377	112	2337	0.131	ng	0.00
5) Phenol-d6	6.959	99	1758	0.075	ng	-0.01
8) Nitrobenzene-d5	8.950	82	6053	0.359	ng	-0.02
11) 2-Methylnaphthalene-d10	12.197	152	9534	0.310	ng	-0.02
14) 2,4,6-Tribromophenol	15.945	330	1131	0.290	ng	-0.02
15) 2-Fluorobiphenyl	13.083	172	16674	0.395	ng	-0.01
27) Fluoranthene-d10	19.239	212	16216	0.351	ng	-0.01
31) Terphenyl-d14	19.838	244	12770	0.470	ng	-0.01
Target Compounds						Qvalue
2) 1,4-Dioxane	3.290	88	878	0.111	ng	# 39
34) Bis(2-ethylhexyl)phtha...	21.304	149	1809	0.096	ng	# 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100625\
Data File : BN038026.D
Acq On : 07 Oct 2025 01:57
Operator : RC/JU
Sample : Q3194-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EB06-20250924


Quant Time: Oct 07 04:16:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 24 11:00:01 2025
Response via : Initial Calibration

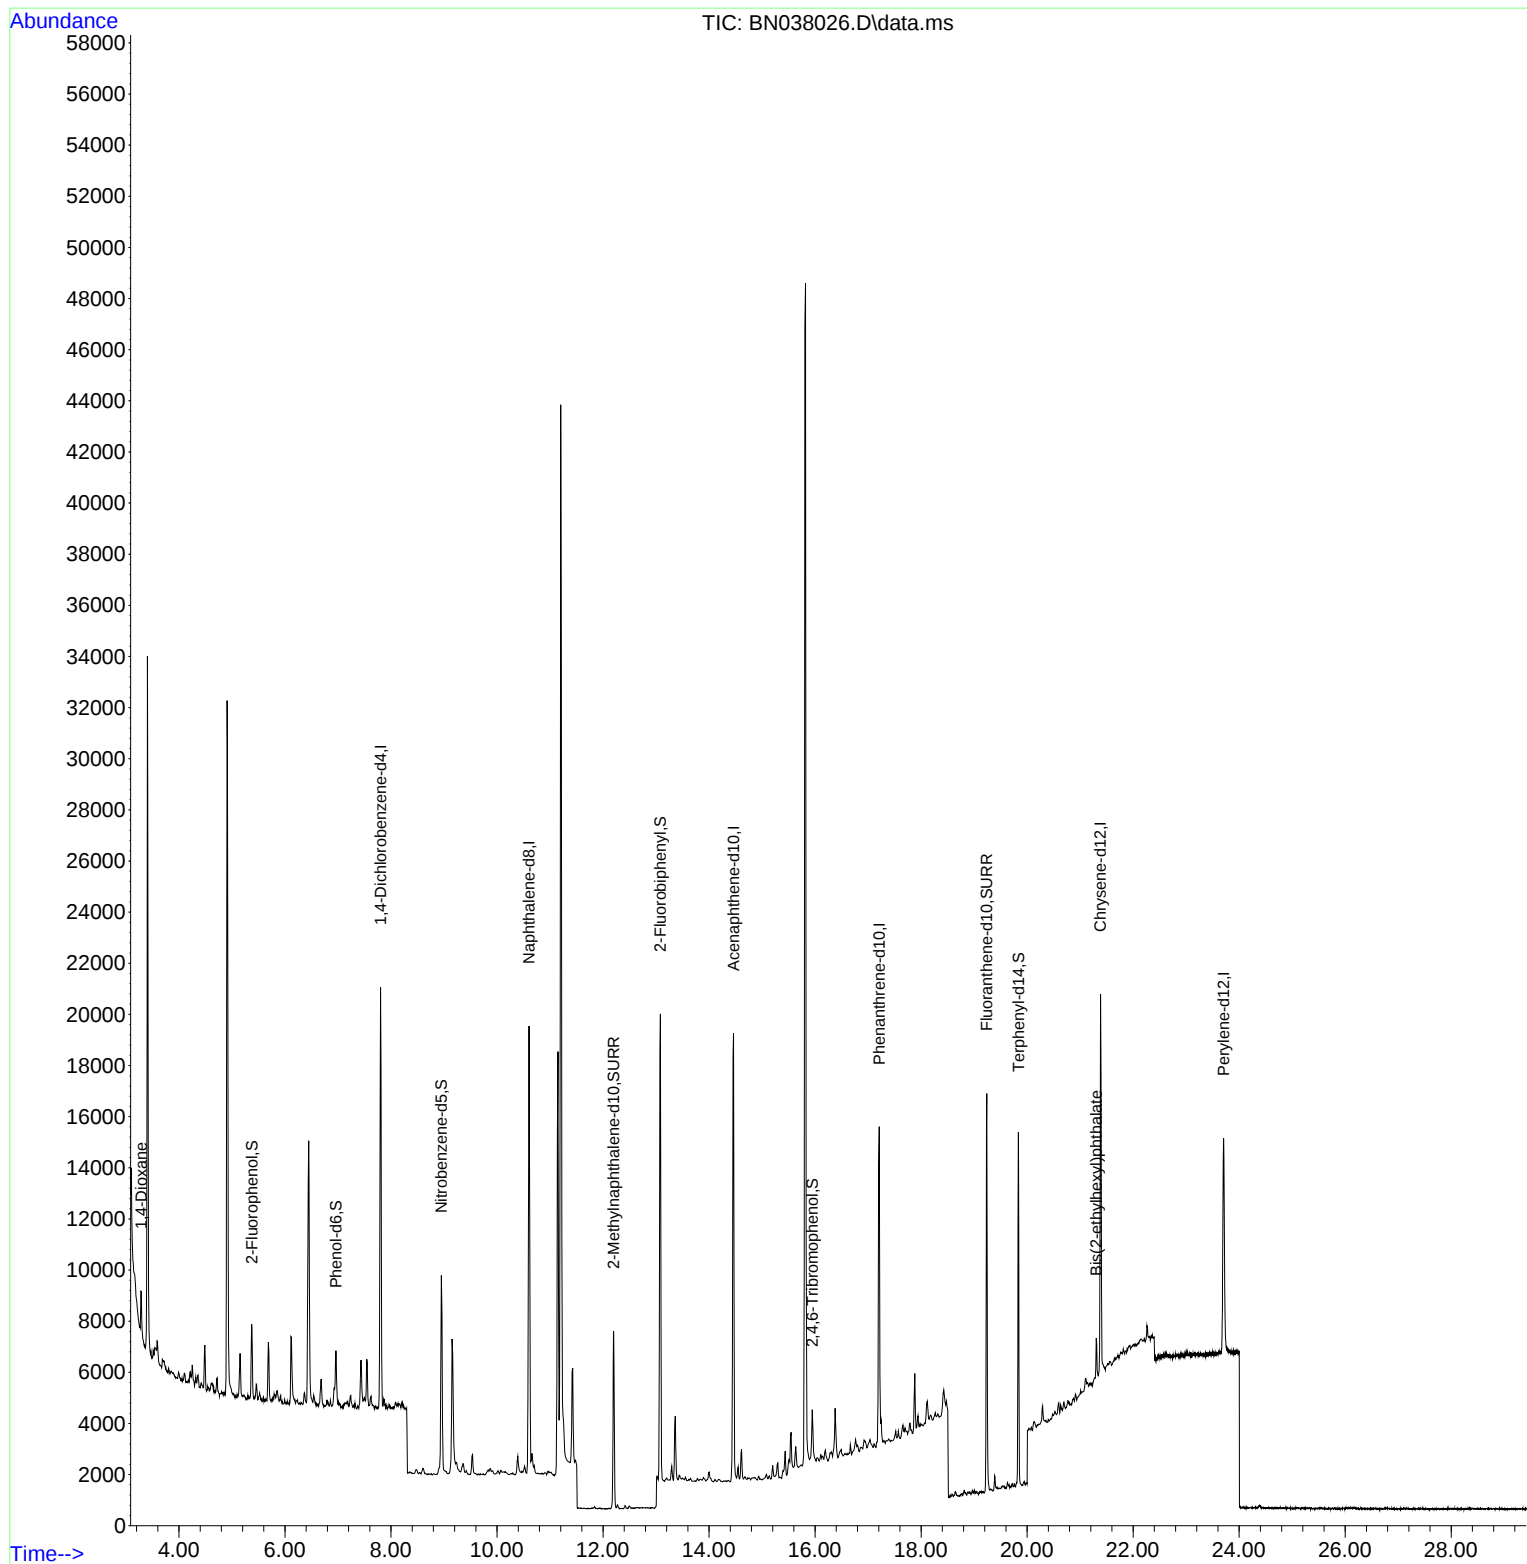





#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.804 min Scan# 61
Delta R.T. -0.021 min
Lab File: BN038026.D
Acq: 07 Oct 2025 01:57

Instrument :
BNA_N
ClientSampleId :
EB06-20250924



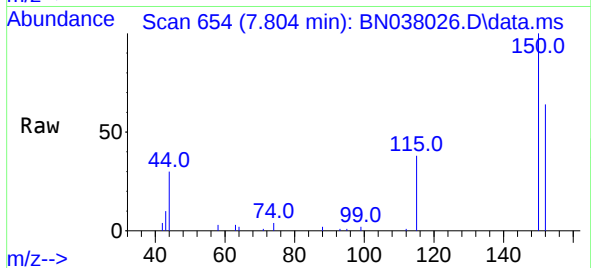



Tgt Ion:152 Resp: 7814
Ion Ratio Lower Upper
152 100
150 157.0 121.0 181.4
115 60.4 47.4 71.0

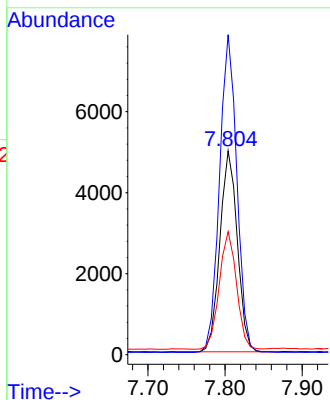

#2
1,4-Dioxane
Concen: 0.111 ng
RT: 3.290 min Scan# 29
Delta R.T. -0.007 min
Lab File: BN038026.D
Acq: 07 Oct 2025 01:57

Tgt Ion: 88 Resp: 878
Ion Ratio Lower Upper
88 100
43 136.2 26.6 39.8#
58 78.7 58.9 88.3


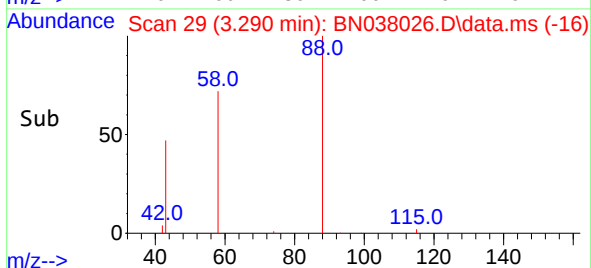
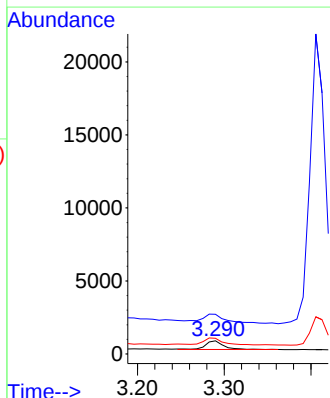



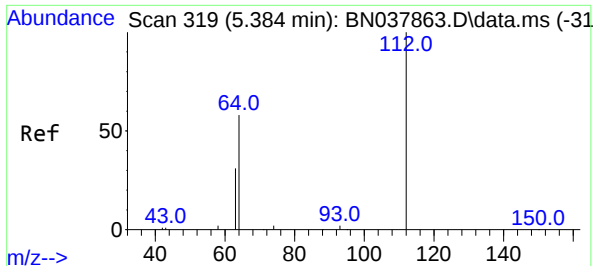

#4
2-Fluorophenol
Concen: 0.131 ng
RT: 5.377 min Scan# 31
Delta R.T. -0.007 min
Lab File: BN038026.D
Acq: 07 Oct 2025 01:57




Instrument :
BNA_N
ClientSampleId :
EB06-20250924


Tgt Ion:112 Resp: 2337
Ion Ratio Lower Upper
112 100
64 55.6 44.6 66.8
63 31.8 24.9 37.3

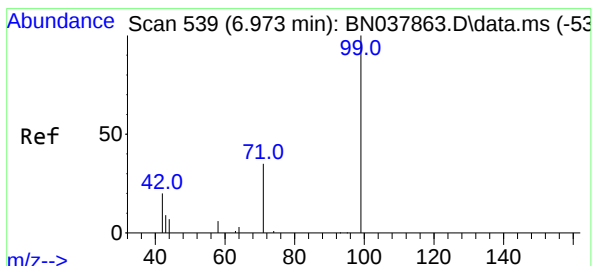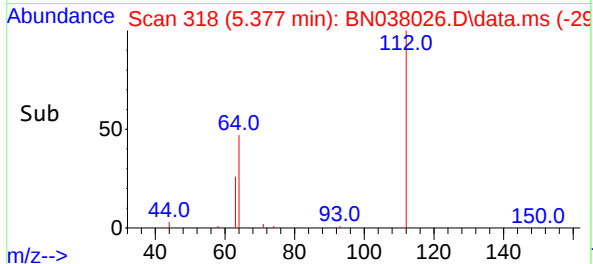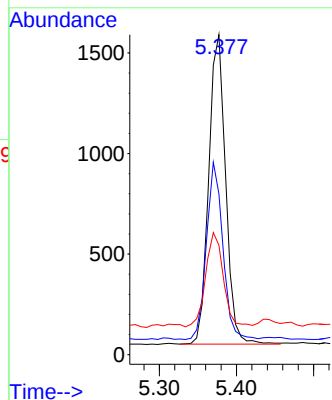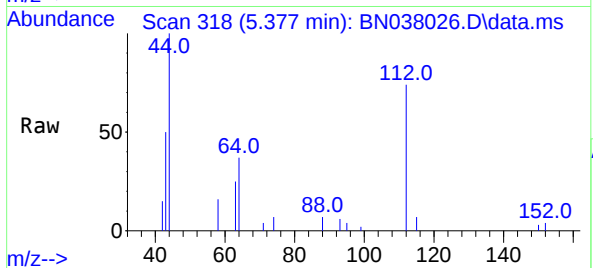

#5
Phenol-d6
Concen: 0.075 ng
RT: 6.959 min Scan# 537
Delta R.T. -0.014 min
Lab File: BN038026.D
Acq: 07 Oct 2025 01:57

Tgt Ion: 99 Resp: 1758
Ion Ratio Lower Upper
99 100
42 27.9 17.2 25.8#
71 42.4 27.3 40.9#

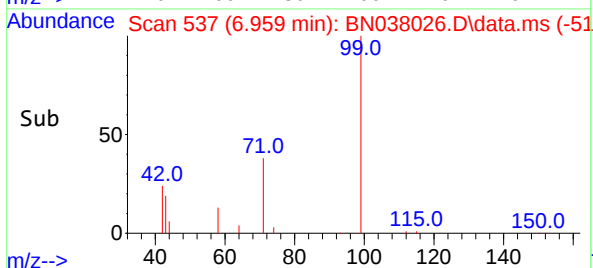
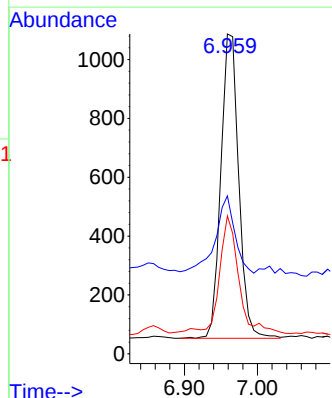
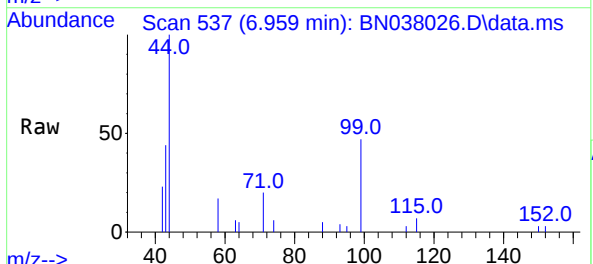


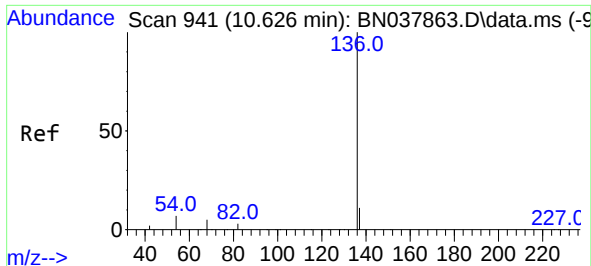

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.605 min Scan# 91
Delta R.T. -0.021 min
Lab File: BN038026.D
Acq: 07 Oct 2025 01:57




Instrument :
BNA_N
ClientSampleId :
EB06-20250924

Tgt Ion:136	Resp:	22108
Ion Ratio	Lower	Upper
136	100	
137	11.2	9.0 13.4
54	7.8	5.8 8.8
68	6.1	4.3 6.5

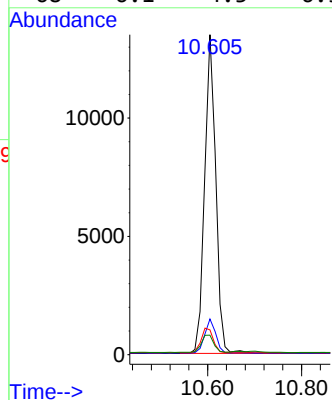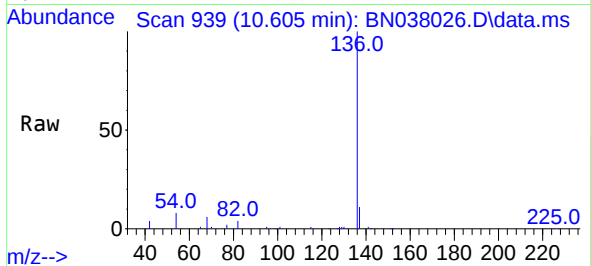

#8
Nitrobenzene-d5
Concen: 0.359 ng
RT: 8.950 min Scan# 784
Delta R.T. -0.021 min
Lab File: BN038026.D
Acq: 07 Oct 2025 01:57

Tgt Ion: 82	Resp:	6053
Ion Ratio	Lower	Upper
82	100	
128	39.1	34.8 52.2
54	57.7	42.2 63.2


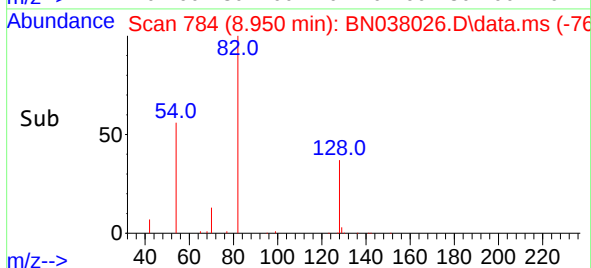
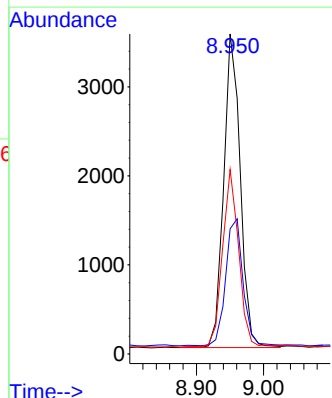





#11
2-Methylnaphthalene-d10
Concen: 0.310 ng
RT: 12.197 min Scan# 11
Delta R.T. -0.020 min
Lab File: BN038026.D
Acq: 07 Oct 2025 01:57




Instrument :
BNA_N
ClientSampleId :
EB06-20250924

Tgt Ion:152 Resp: 9534
Ion Ratio Lower Upper
152 100
151 22.0 17.4 26.2

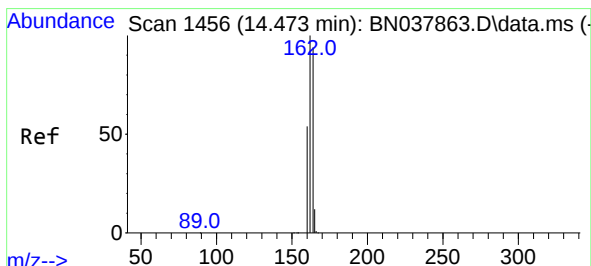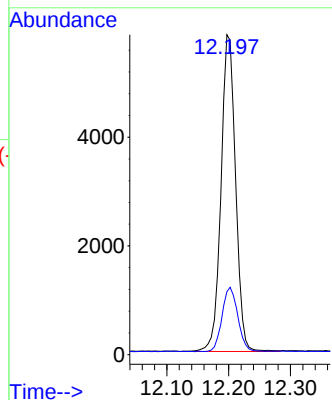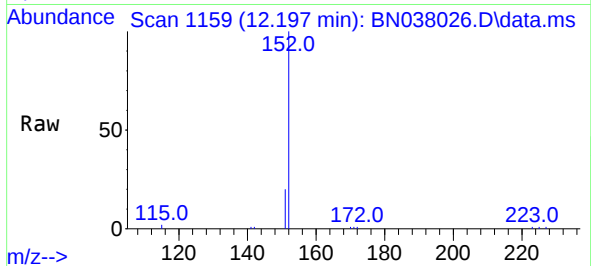

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.462 min Scan# 1455
Delta R.T. -0.011 min
Lab File: BN038026.D
Acq: 07 Oct 2025 01:57


Tgt Ion:164 Resp: 10302
Ion Ratio Lower Upper
164 100
162 101.9 84.8 127.2
160 53.3 46.1 69.1

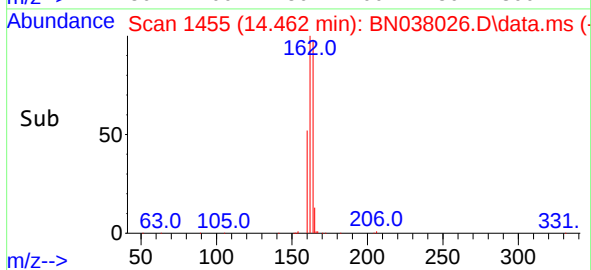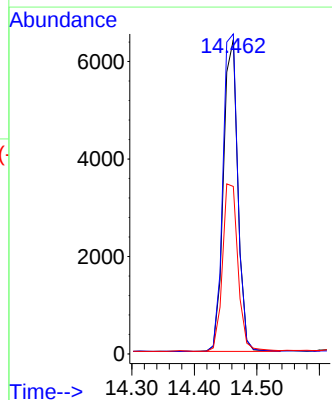





#14
2,4,6-Tribromophenol
Concen: 0.290 ng
RT: 15.945 min Scan# 11
Delta R.T. -0.024 min
Lab File: BN038026.D
Acq: 07 Oct 2025 01:57

Instrument :
BNA_N
ClientSampleId :
EB06-20250924



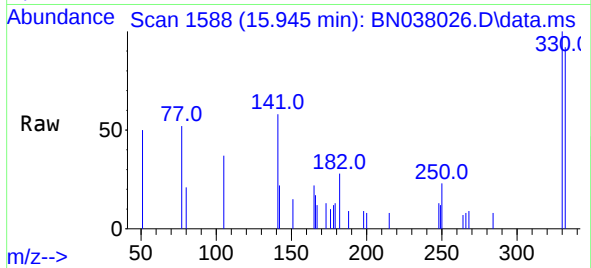


Tgt Ion:330 Resp: 1131
Ion Ratio Lower Upper
330 100
332 93.3 77.2 115.8
141 43.3 37.2 55.8

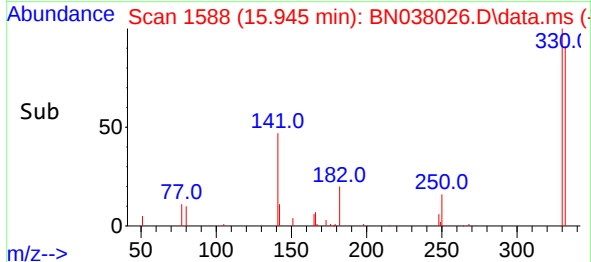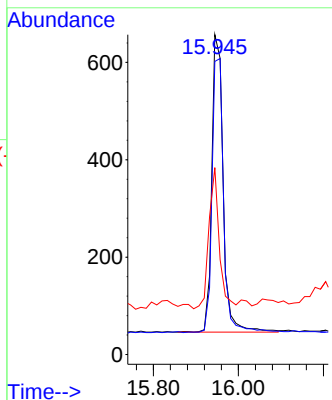

#15
2-Fluorobiphenyl
Concen: 0.395 ng
RT: 13.083 min Scan# 1326
Delta R.T. -0.011 min
Lab File: BN038026.D
Acq: 07 Oct 2025 01:57


Tgt Ion:172 Resp: 16674
Ion Ratio Lower Upper
172 100
171 34.1 28.6 43.0
170 23.4 19.7 29.5

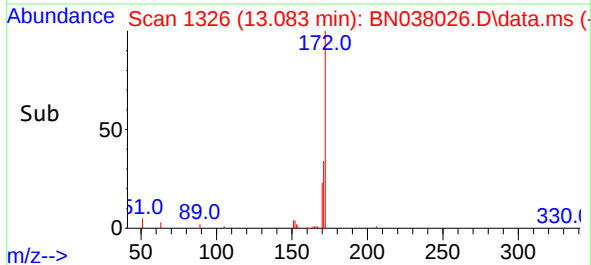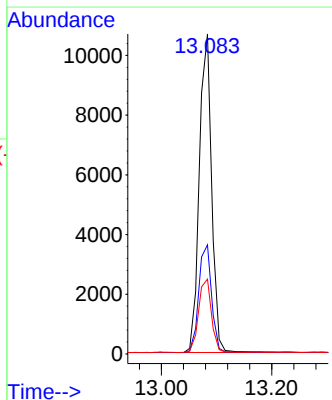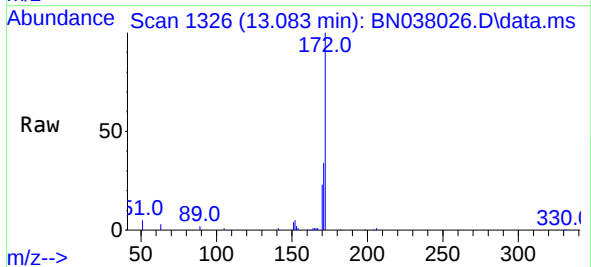






#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.211 min Scan# 1690
Delta R.T. -0.012 min
Lab File: BN038026.D
Acq: 07 Oct 2025 01:57

Instrument :
BNA_N
ClientSampleId :
EB06-20250924



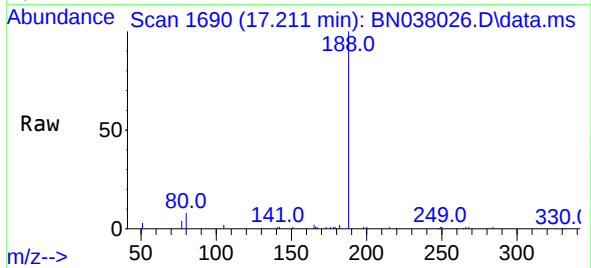


Tgt Ion:188 Resp: 18362
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.1 7.6 11.4

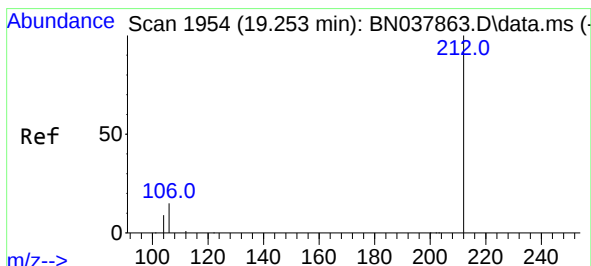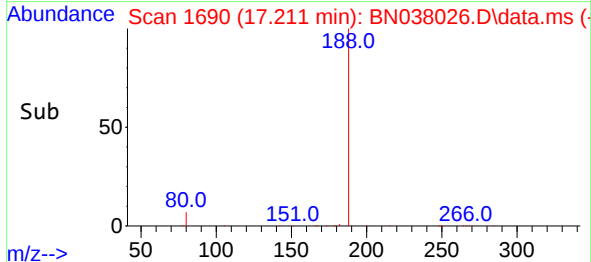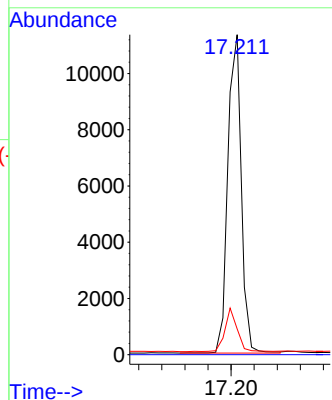

#27
Fluoranthene-d10
Concen: 0.351 ng
RT: 19.239 min Scan# 1951
Delta R.T. -0.014 min
Lab File: BN038026.D
Acq: 07 Oct 2025 01:57


Tgt Ion:212 Resp: 16216
Ion Ratio Lower Upper
212 100
106 16.8 12.6 19.0
104 9.6 7.4 11.0

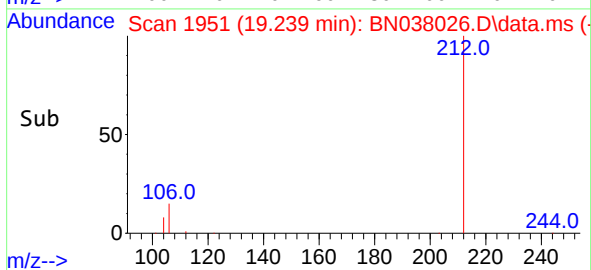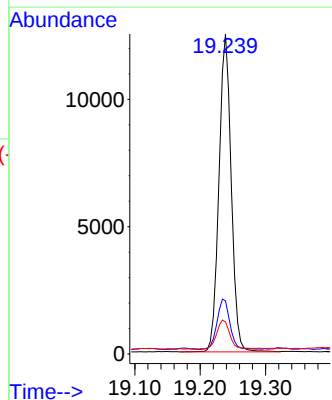





#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.384 min Scan# 21
Delta R.T. -0.018 min
Lab File: BN038026.D
Acq: 07 Oct 2025 01:57

Instrument :
BNA_N
ClientSampleId :
EB06-20250924



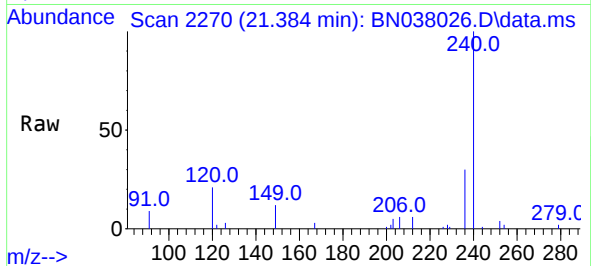



Tgt Ion:240 Resp: 13636
Ion Ratio Lower Upper
240 100
120 20.9 11.4 17.2#
236 29.9 23.0 34.6

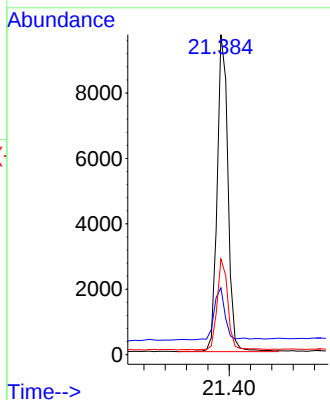

#31
Terphenyl-d14
Concen: 0.470 ng
RT: 19.838 min Scan# 2080
Delta R.T. -0.014 min
Lab File: BN038026.D
Acq: 07 Oct 2025 01:57

Tgt Ion:244 Resp: 12770
Ion Ratio Lower Upper
244 100
212 9.6 7.6 11.4
122 17.1 13.9 20.9


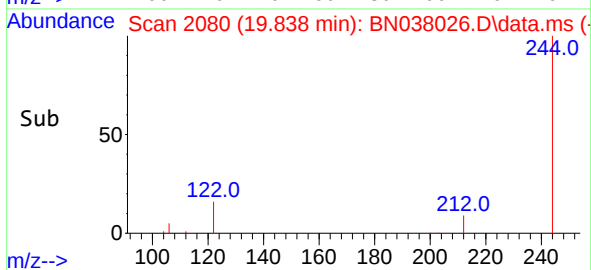
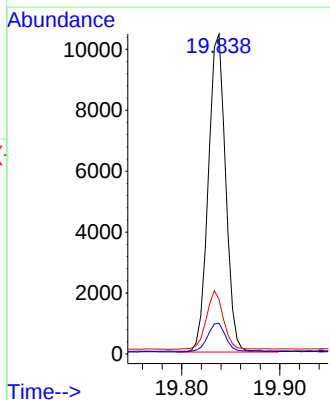



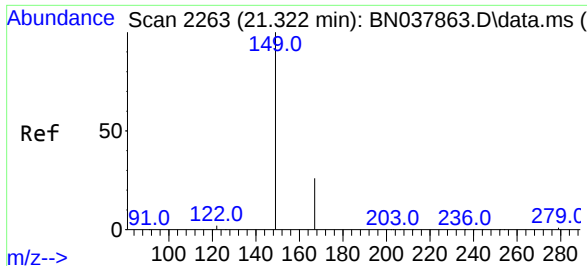

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.096 ng
RT: 21.304 min Scan# 21
Delta R.T. -0.018 min
Lab File: BN038026.D
Acq: 07 Oct 2025 01:57

Instrument :
BNA_N
ClientSampleId :
EB06-20250924

Tgt Ion:149 Resp: 1809
Ion Ratio Lower Upper
149 100
167 24.2 20.4 30.6
279 5.5 2.4 3.6#

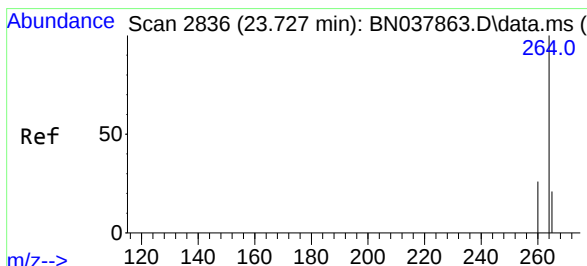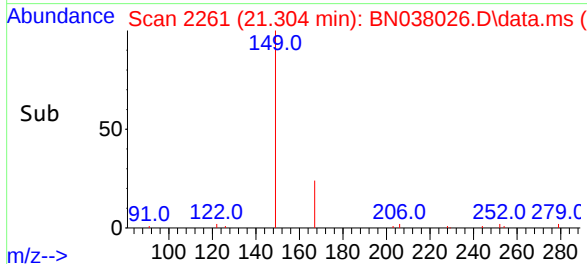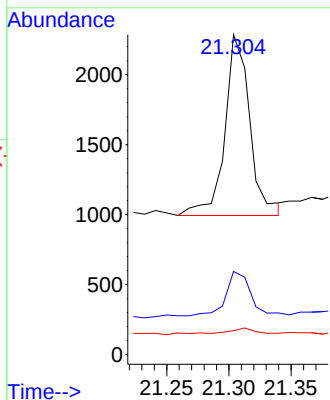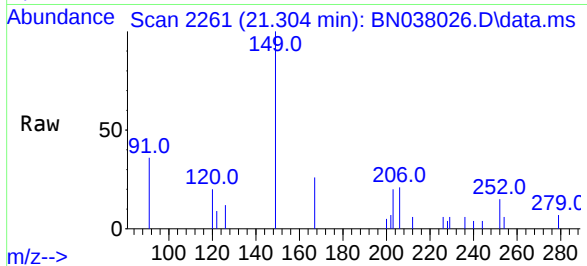

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.706 min Scan# 2829
Delta R.T. -0.020 min
Lab File: BN038026.D
Acq: 07 Oct 2025 01:57

Tgt Ion:264 Resp: 11958
Ion Ratio Lower Upper
264 100
260 27.6 21.5 32.3
265 96.4 53.8 80.6#

