
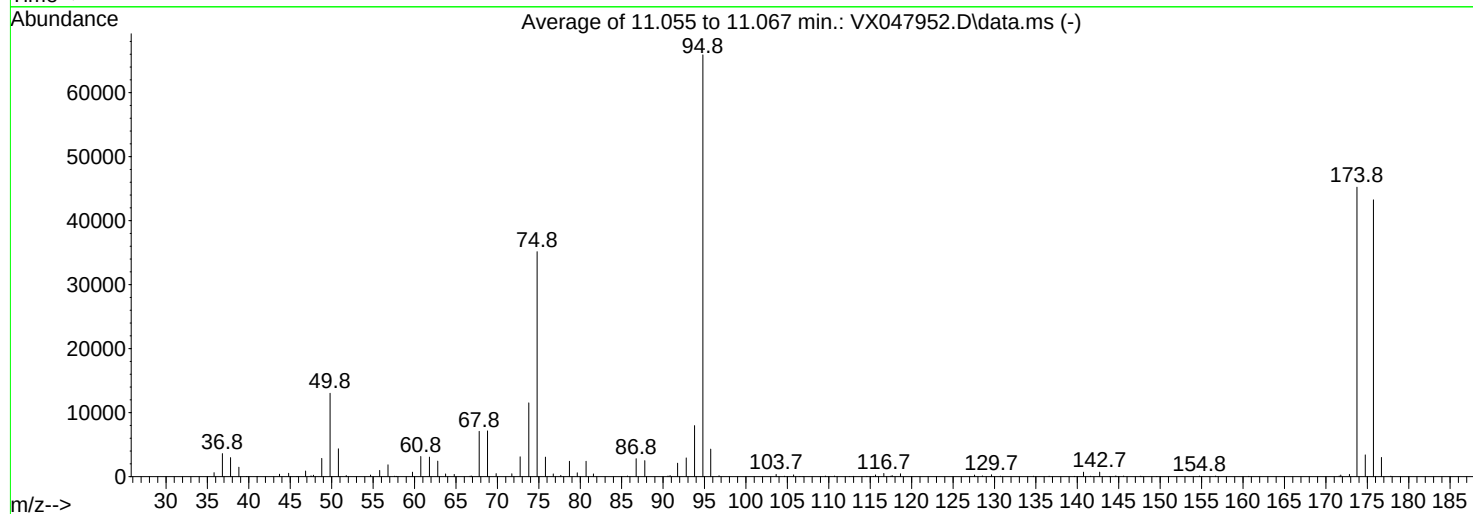


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX100225\  
Data File : VX047952.D  
Acq On : 02 Oct 2025 08:18  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091625W.M  
Title : SW846 8260  
Last Update : Wed Sep 17 06:39:58 2025

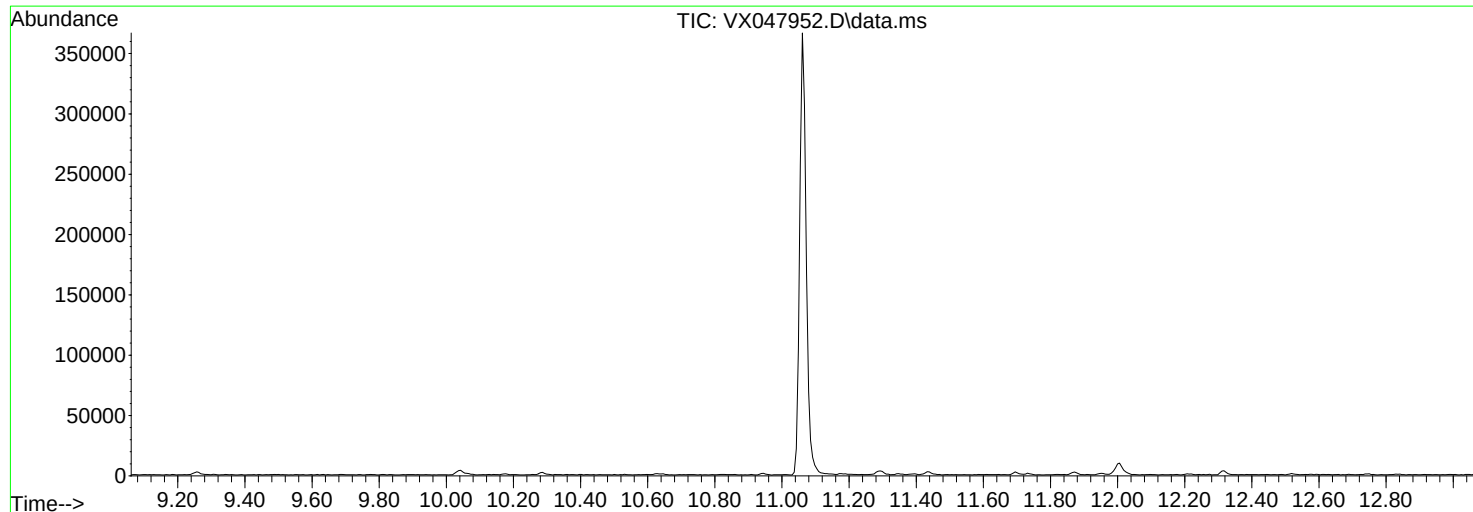

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1629

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 19.8  | 13014 | PASS      |
| 75     | 95      | 30     | 60     | 53.3  | 35144 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 65893 | PASS      |
| 96     | 95      | 5      | 9      | 6.5   | 4293  | PASS      |
| 173    | 174     | 0.00   | 2      | 0.8   | 357   | PASS      |
| 174    | 95      | 50     | 100    | 68.6  | 45208 | PASS      |
| 175    | 174     | 5      | 9      | 7.5   | 3409  | PASS      |
| 176    | 174     | 95     | 101    | 95.7  | 43251 | PASS      |
| 177    | 176     | 5      | 9      | 7.0   | 3006  | PASS      |