

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100125\
 Data File : VX047927.D
 Acq On : 01 Oct 2025 10:03
 Operator : JC/MD
 Sample : VX1001WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1001WBL01

Quant Time: Oct 03 01:15:46 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 17 06:39:58 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.537	168	138593	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.745	114	281738	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	294028	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	149007	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.940	65	119484	54.162	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	108.320%
35) Dibromofluoromethane	5.373	113	96410	51.024	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	102.040%
50) Toluene-d8	8.634	98	321714	49.207	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.420%
62) 4-Bromofluorobenzene	11.061	95	138483	55.811	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	111.620%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100125\
Data File : VX047927.D
Acq On : 01 Oct 2025 10:03
Operator : JC/MD
Sample : VX1001WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1001WBL01

Quant Time: Oct 03 01:15:46 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 17 06:39:58 2025
Response via : Initial Calibration




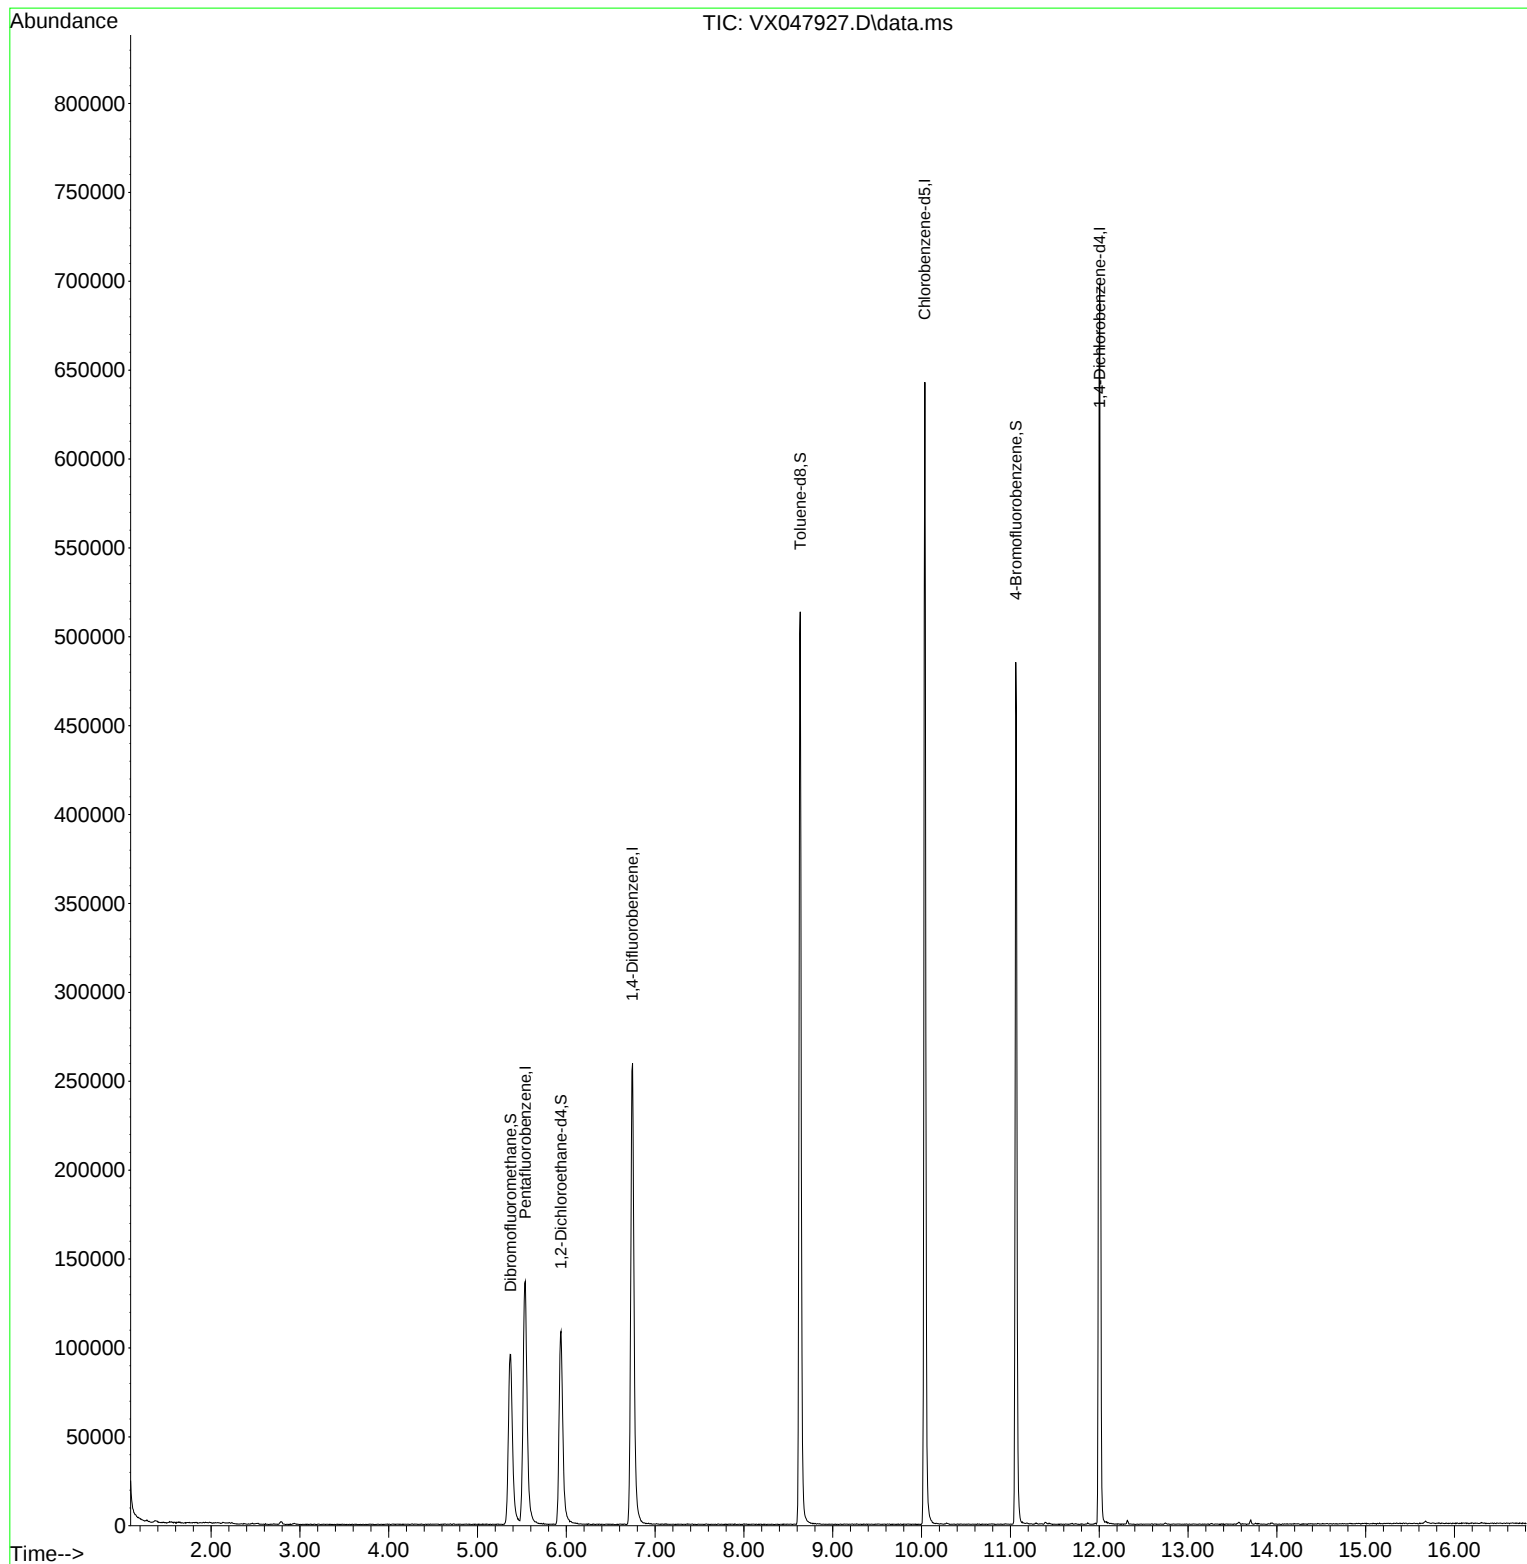


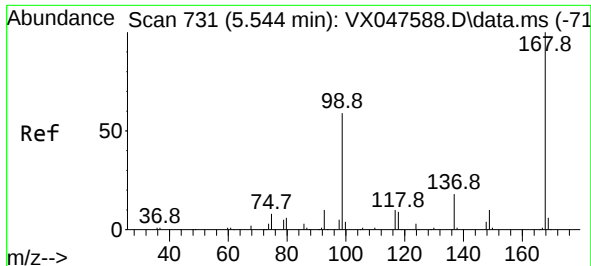

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.537 min Scan# 730
Delta R.T. -0.007 min
Lab File: VX047927.D
Acq: 01 Oct 2025 10:03




Instrument :
MSVOA_X
ClientSampleId :
VX1001WBL01

Tgt Ion:168 Resp: 138593
Ion Ratio Lower Upper
168 100
99 63.9 48.8 73.2

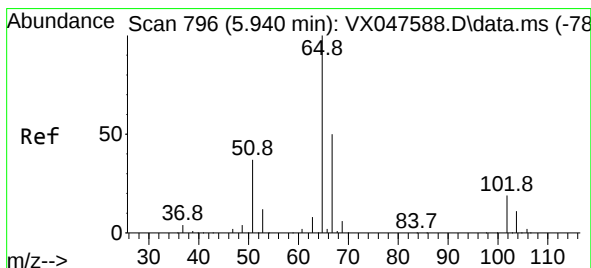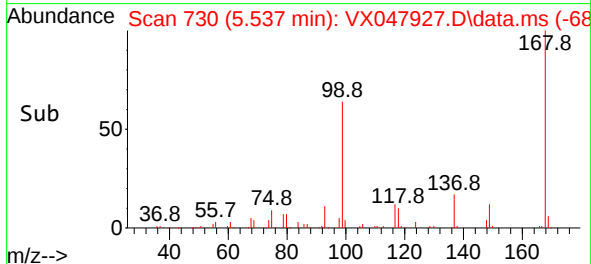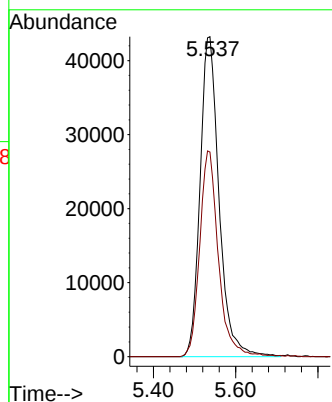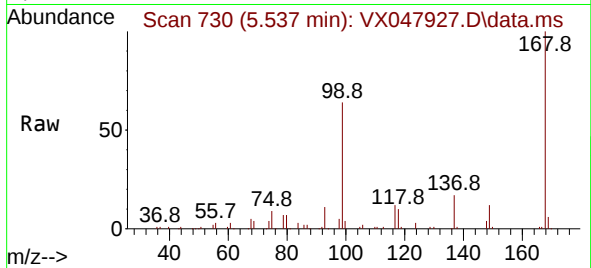

#33
1,2-Dichloroethane-d4
Concen: 54.162 ug/l
RT: 5.940 min Scan# 796
Delta R.T. -0.000 min
Lab File: VX047927.D
Acq: 01 Oct 2025 10:03

Tgt Ion: 65 Resp: 119484
Ion Ratio Lower Upper
65 100
67 50.9 0.0 103.0


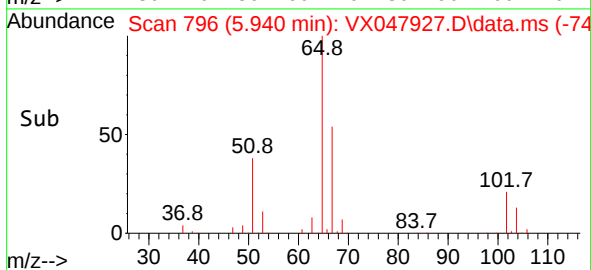
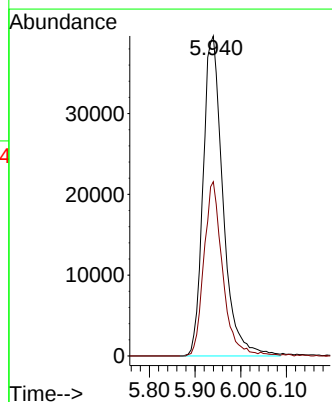
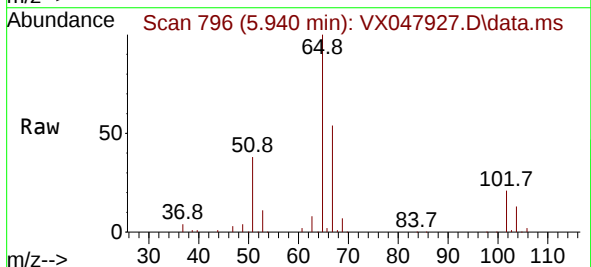




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.745 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX047927.D
Acq: 01 Oct 2025 10:03




Instrument :
MSVOA_X
ClientSampleId :
VX1001WBL01

Tgt Ion:114 Resp: 281738
Ion Ratio Lower Upper
114 100
63 22.2 0.0 44.0
88 17.1 0.0 34.2

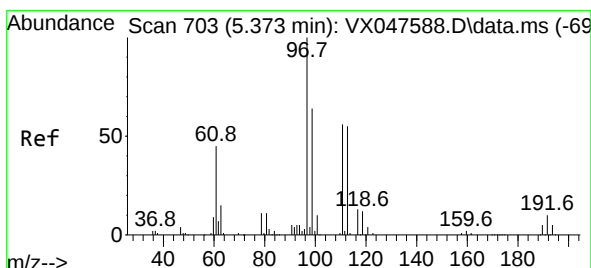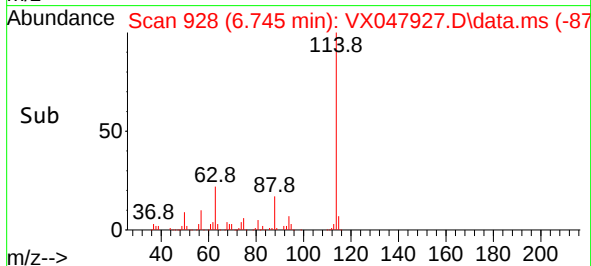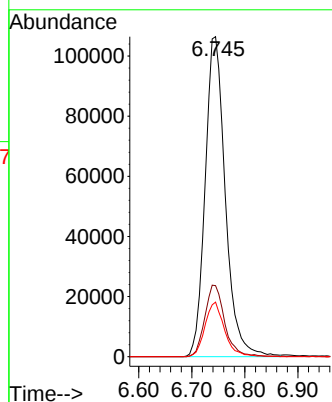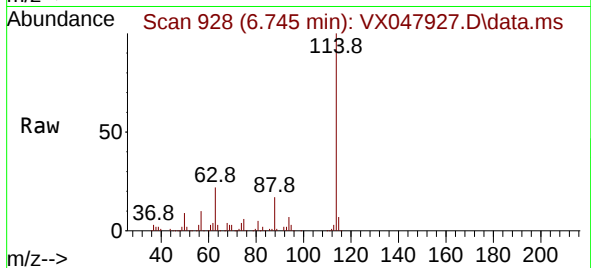

#35
Dibromofluoromethane
Concen: 51.024 ug/l
RT: 5.373 min Scan# 703
Delta R.T. -0.000 min
Lab File: VX047927.D
Acq: 01 Oct 2025 10:03

Tgt Ion:113 Resp: 96410
Ion Ratio Lower Upper
113 100
111 101.6 80.9 121.3
192 17.3 14.2 21.4

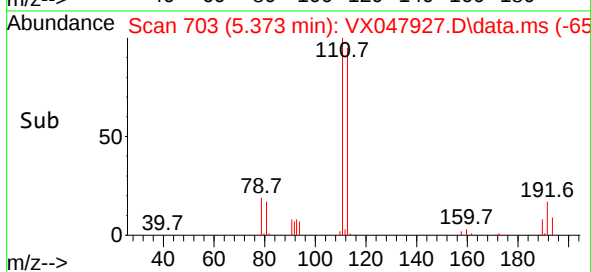
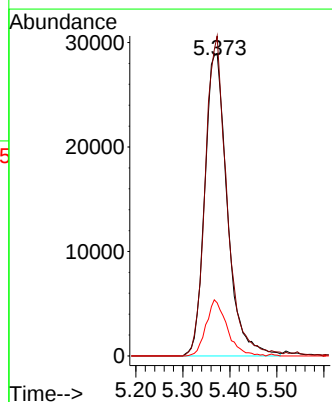
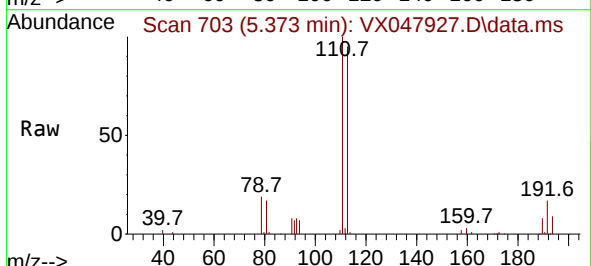




#50
Toluene-d8
Concen: 49.207 ug/l
RT: 8.634 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX047927.D
Acq: 01 Oct 2025 10:03




Instrument :
MSVOA_X
ClientSampleId :
VX1001WBL01


Tgt Ion: 98 Resp: 321714
Ion Ratio Lower Upper
98 100
100 65.9 53.0 79.4

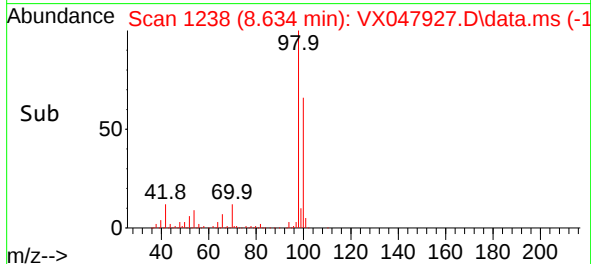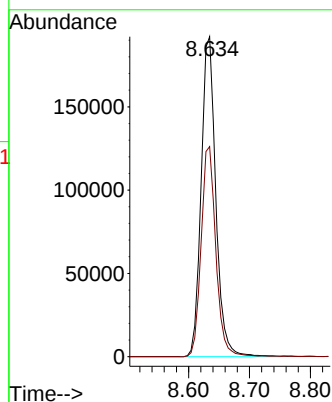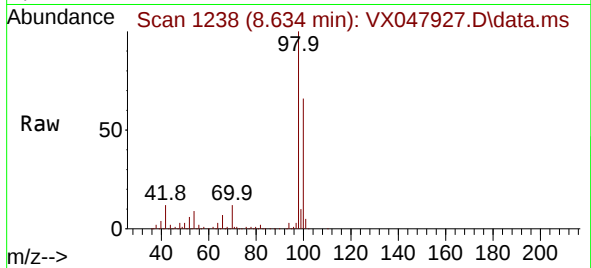

#62
4-Bromofluorobenzene
Concen: 55.811 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. -0.000 min
Lab File: VX047927.D
Acq: 01 Oct 2025 10:03

Tgt Ion: 95 Resp: 138483
Ion Ratio Lower Upper
95 100
174 73.2 0.0 141.6
176 69.6 0.0 138.4


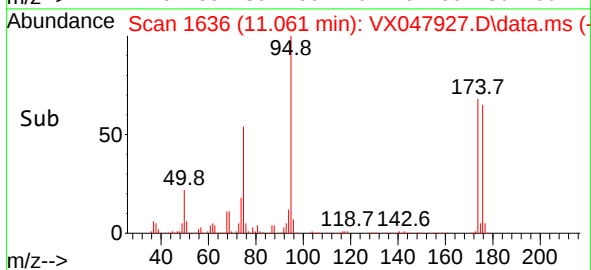
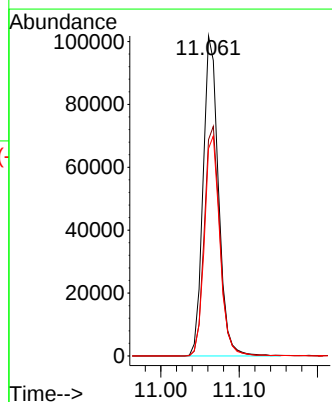
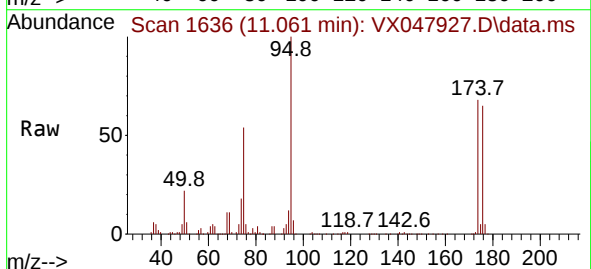


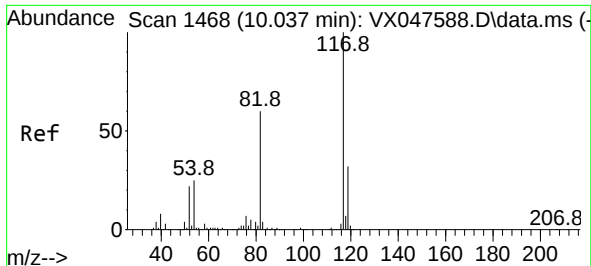

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.037 min Scan# 1468
Delta R.T. -0.000 min
Lab File: VX047927.D
Acq: 01 Oct 2025 10:03

Instrument :
MSVOA_X
ClientSampleId :
VX1001WBL01

Tgt Ion:117 Resp: 294028
Ion Ratio Lower Upper
117 100
82 57.5 47.8 71.6
119 32.6 25.2 37.8

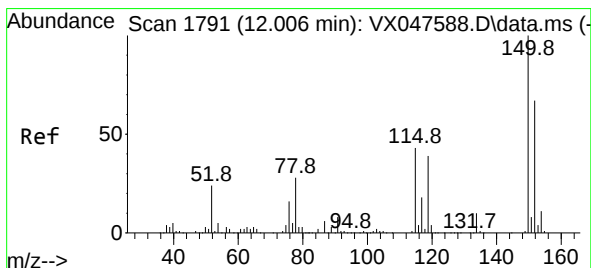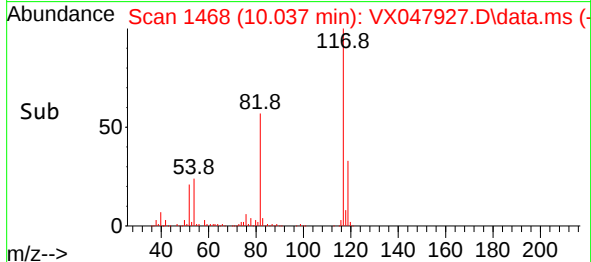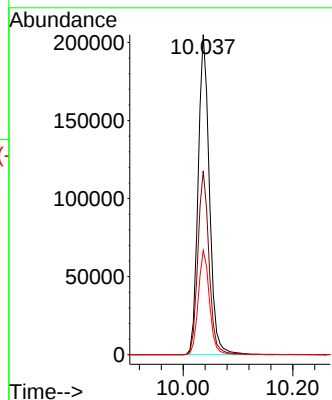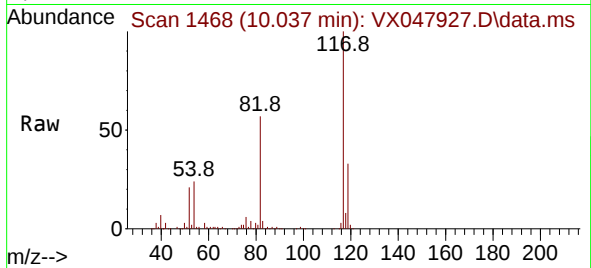

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. -0.000 min
Lab File: VX047927.D
Acq: 01 Oct 2025 10:03

Tgt Ion:152 Resp: 149007
Ion Ratio Lower Upper
152 100
115 63.9 44.9 134.5
150 158.9 0.0 352.0

