
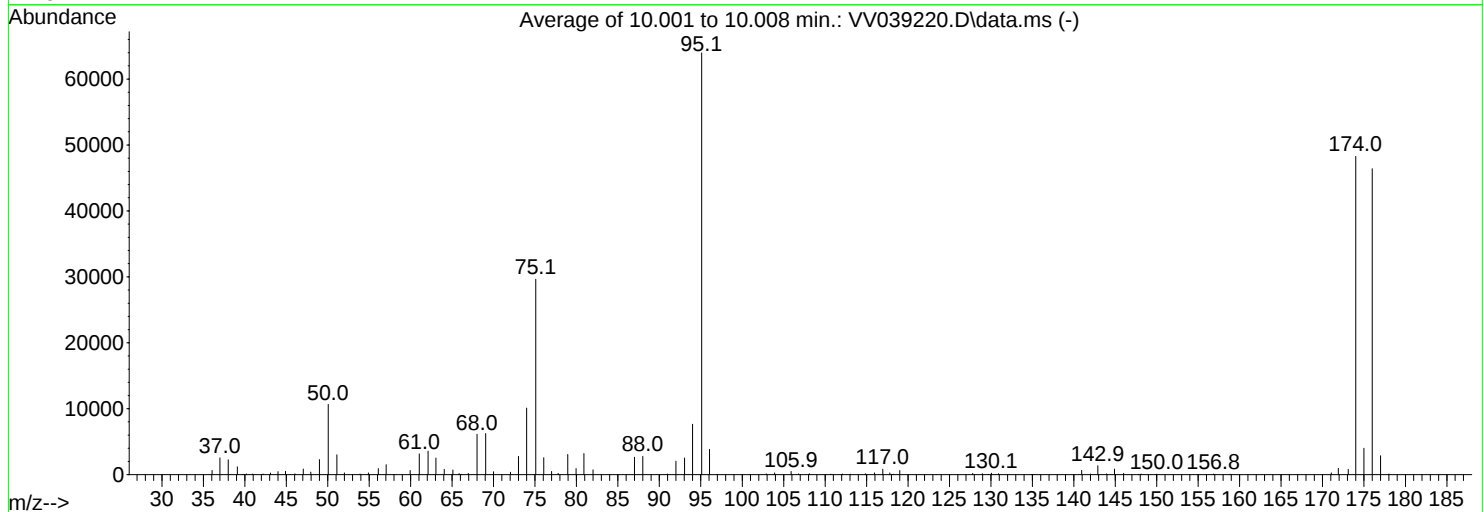


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092925\
Data File : VV039220.D
Acq On : 29 Sep 2025 09:48
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M
Title : SW846 8260
Last Update : Wed Sep 24 08:08:08 2025

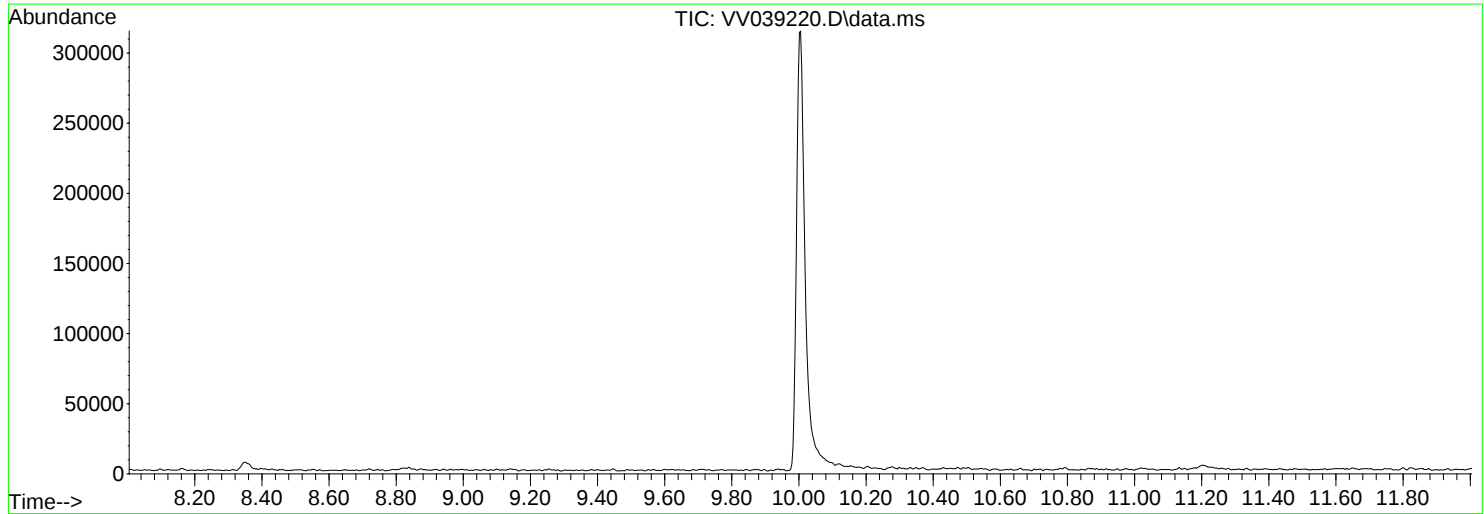

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	10649	PASS
75	95	30	60	46.3	29627	PASS
95	95	100	100	100.0	63979	PASS
96	95	5	9	6.0	3829	PASS
173	174	0.00	2	1.7	809	PASS
174	95	50	100	75.5	48283	PASS
175	174	5	9	8.3	4007	PASS
176	174	95	101	96.1	46392	PASS
177	176	5	9	6.2	2861	PASS