

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100325\
 Data File : VV039249.D
 Acq On : 03 Oct 2025 15:04
 Operator : SY/MD
 Sample : Q3201-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 FIELD-BLANK

Quant Time: Oct 04 01:11:35 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 24 08:08:08 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	4.603	168	349814	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	5.535	114	588713	50.000	ug/l	0.00
63) Chlorobenzene-d5	8.776	117	608055	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.175	152	300076	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	4.944	65	283815	56.058	ug/l	0.00
Spiked Amount	50.000	Range	81 - 118	Recovery	=	112.120%
35) Dibromofluoromethane	4.503	113	269374	56.917	ug/l	0.00
Spiked Amount	50.000	Range	80 - 119	Recovery	=	113.840%
50) Toluene-d8	7.236	98	625684	45.013	ug/l	0.00
Spiked Amount	50.000	Range	89 - 112	Recovery	=	90.020%
62) 4-Bromofluorobenzene	10.001	95	253724	44.339	ug/l	0.00
Spiked Amount	50.000	Range	85 - 114	Recovery	=	88.680%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100325\
Data File : VV039249.D
Acq On : 03 Oct 2025 15:04
Operator : SY/MD
Sample : Q3201-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
FIELD-BLANK

Quant Time: Oct 04 01:11:35 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 24 08:08:08 2025
Response via : Initial Calibration




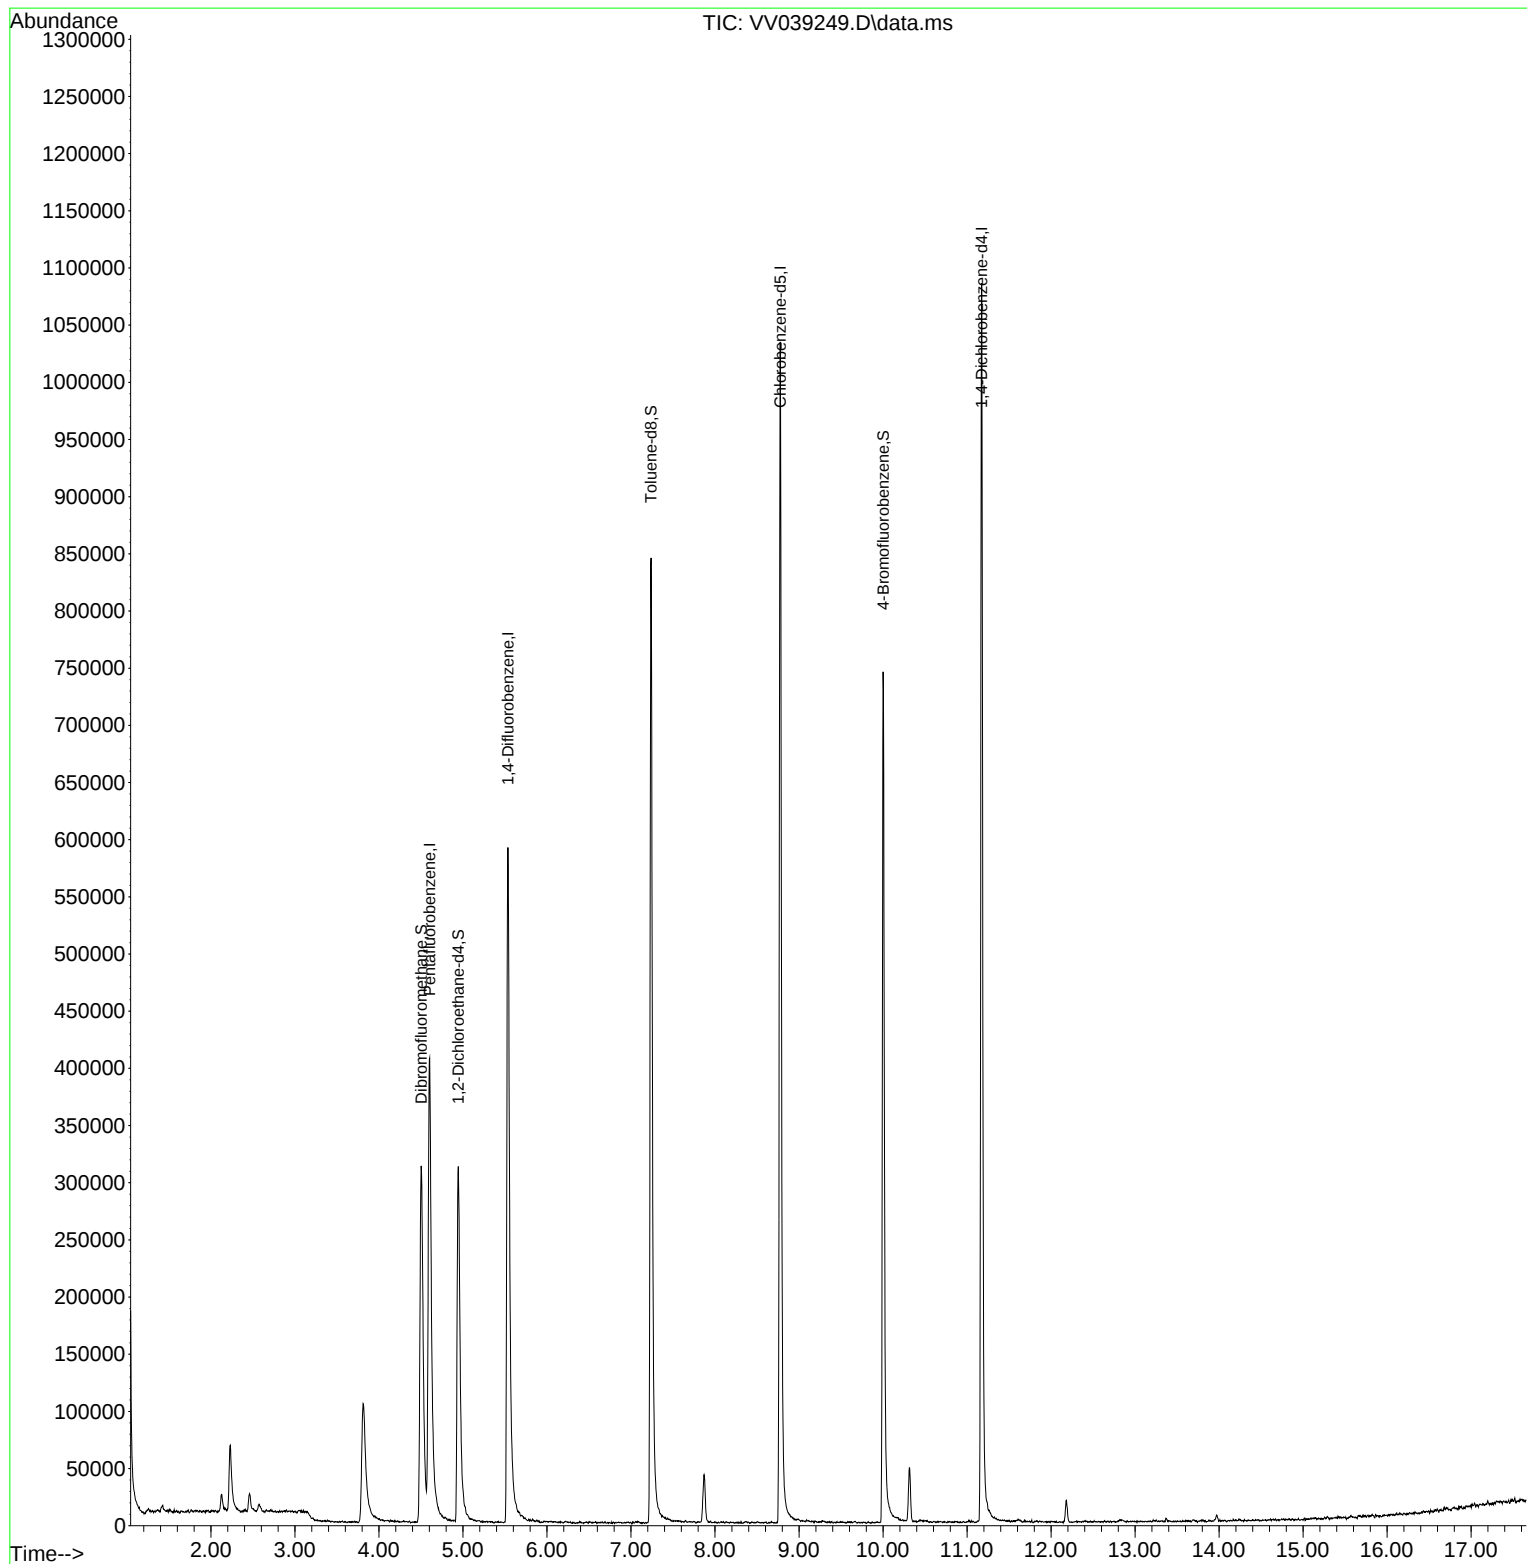


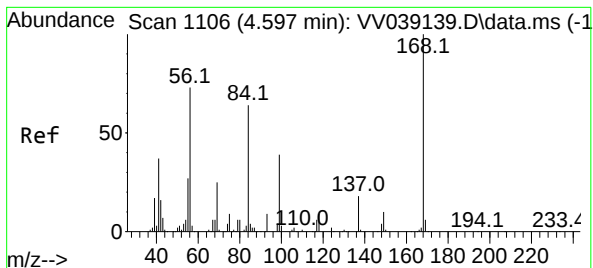

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 4.603 min Scan# 1108
Delta R.T. 0.006 min
Lab File: VV039249.D
Acq: 03 Oct 2025 15:04




Instrument :
MSVOA_V
ClientSampleId :
FIELD-BLANK


Tgt Ion:168 Resp: 349814
Ion Ratio Lower Upper
168 100
99 62.5 49.6 74.4

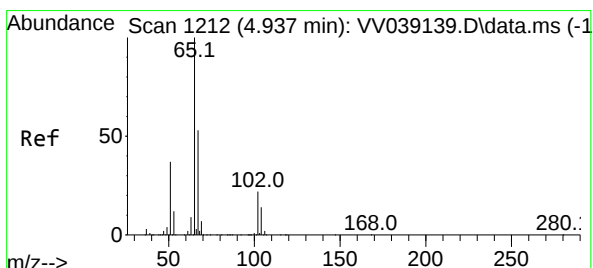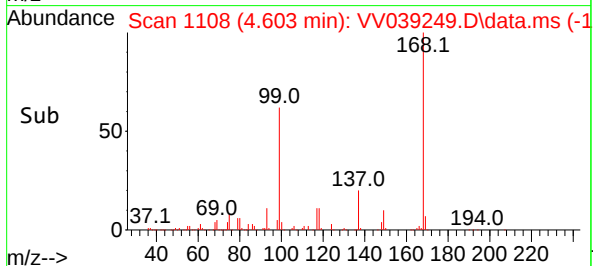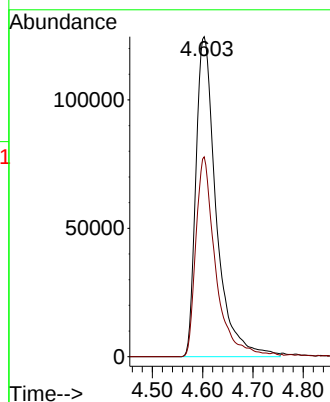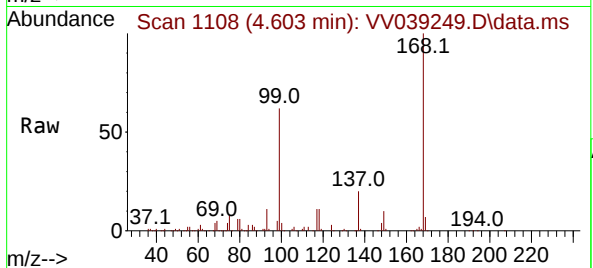

#33
1,2-Dichloroethane-d4
Concen: 56.058 ug/l
RT: 4.944 min Scan# 1214
Delta R.T. 0.006 min
Lab File: VV039249.D
Acq: 03 Oct 2025 15:04

Tgt Ion: 65 Resp: 283815
Ion Ratio Lower Upper
65 100
67 52.9 0.0 107.0

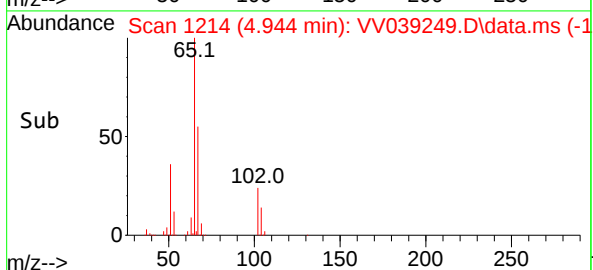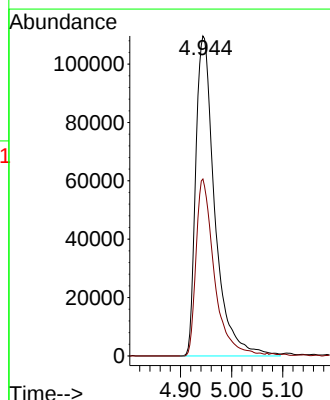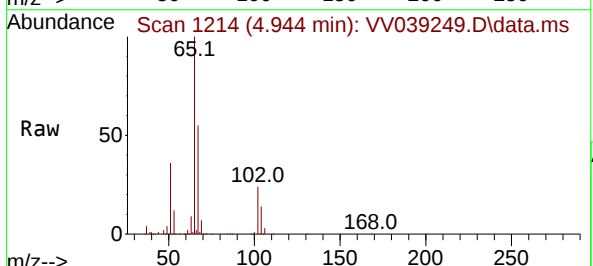

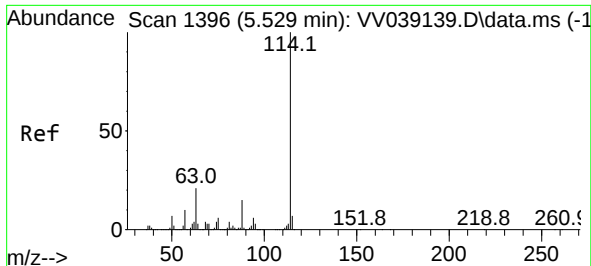

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 5.535 min Scan# 11

Delta R.T. 0.006 min

Lab File: VV039249.D

Acq: 03 Oct 2025 15:04

Instrument :

MSVOA_V

ClientSampleId :

FIELD-BLANK





Tgt Ion:114 Resp: 588713

Ion Ratio Lower Upper

114 100

63 19.7 0.0 42.6

88 15.6 0.0 30.8

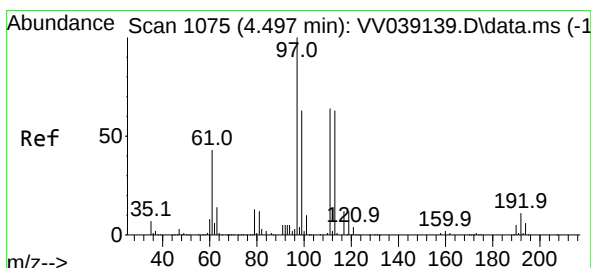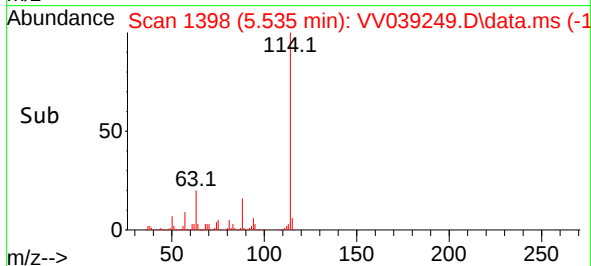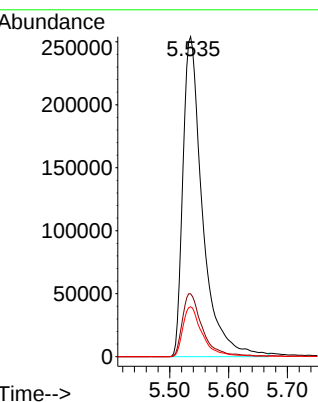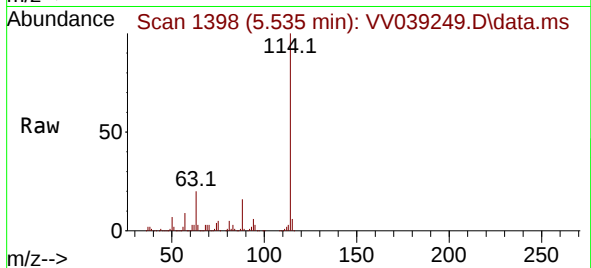

#35

Dibromofluoromethane

Concen: 56.917 ug/l

RT: 4.503 min Scan# 1077

Delta R.T. 0.006 min

Lab File: VV039249.D

Acq: 03 Oct 2025 15:04




Tgt Ion:113 Resp: 269374


Ion Ratio Lower Upper

113 100

111 102.3 82.4 123.6

192 18.2 13.8 20.8


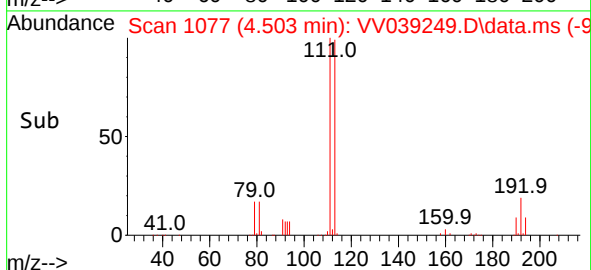
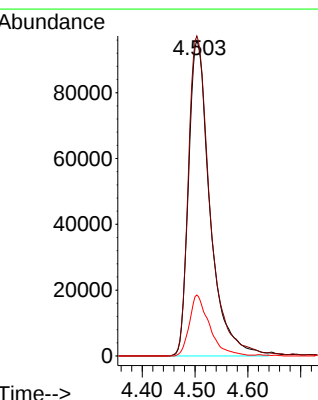
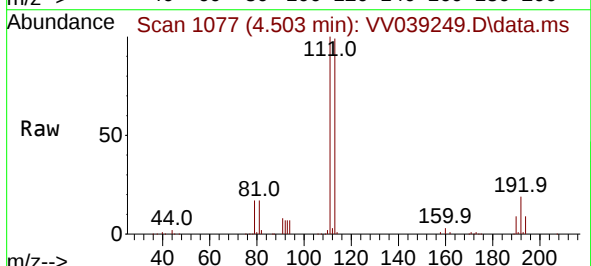


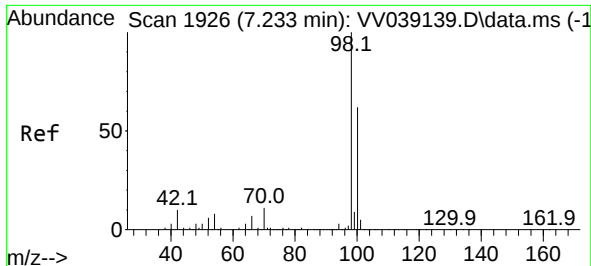

#50
Toluene-d8
Concen: 45.013 ug/l
RT: 7.236 min Scan# 1926
Delta R.T. 0.003 min
Lab File: VV039249.D
Acq: 03 Oct 2025 15:04




Instrument :
MSVOA_V
ClientSampleId :
FIELD-BLANK


Tgt Ion: 98 Resp: 625684
Ion Ratio Lower Upper
98 100
100 63.9 52.2 78.2

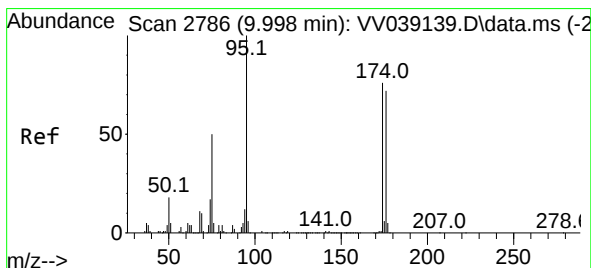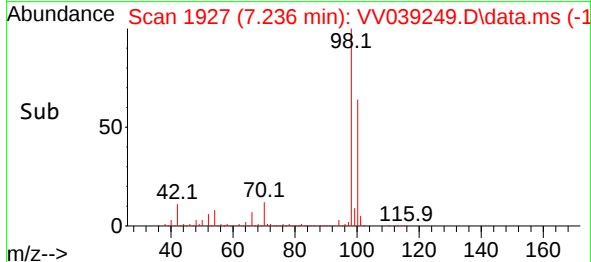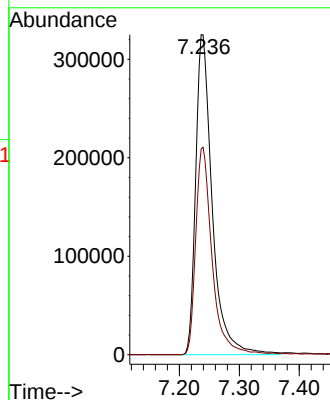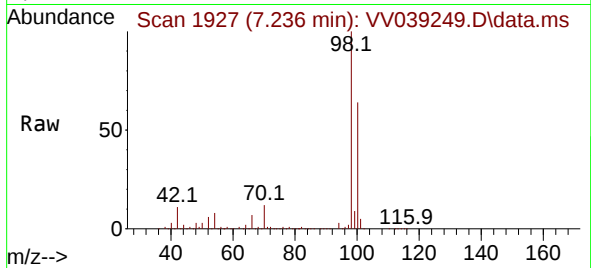

#62
4-Bromofluorobenzene
Concen: 44.339 ug/l
RT: 10.001 min Scan# 2787
Delta R.T. 0.003 min
Lab File: VV039249.D
Acq: 03 Oct 2025 15:04

Tgt Ion: 95 Resp: 253724
Ion Ratio Lower Upper
95 100
174 79.9 0.0 150.4
176 74.1 0.0 144.2


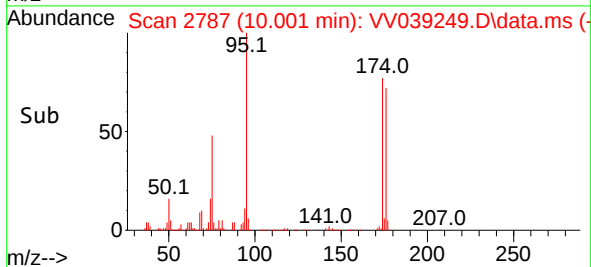
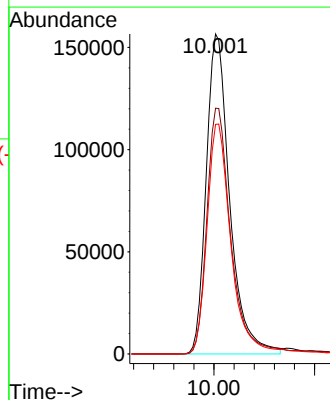
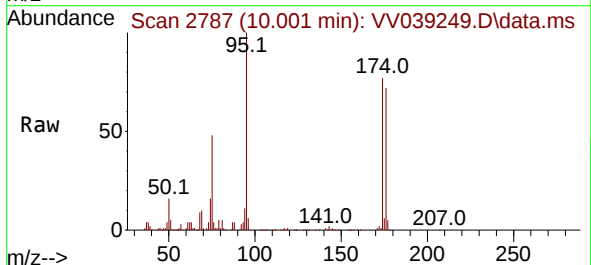


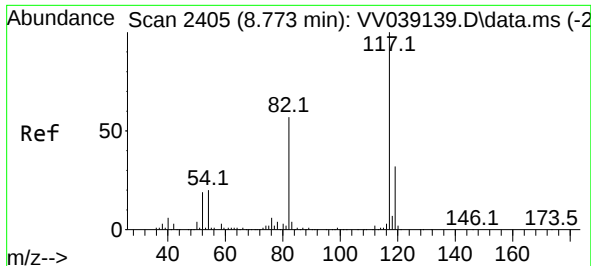

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 8.776 min Scan# 2406
Delta R.T. 0.003 min
Lab File: VV039249.D
Acq: 03 Oct 2025 15:04

Instrument :
MSVOA_V
ClientSampleId :
FIELD-BLANK

Tgt Ion:117 Resp: 608055
Ion Ratio Lower Upper
117 100
82 54.7 45.4 68.2
119 31.2 25.6 38.4

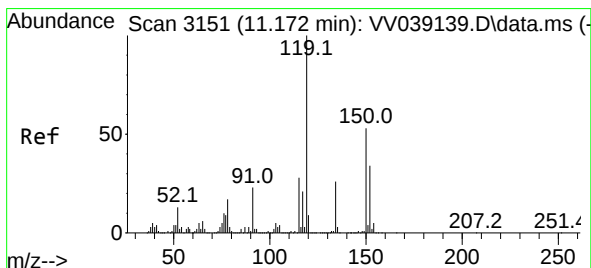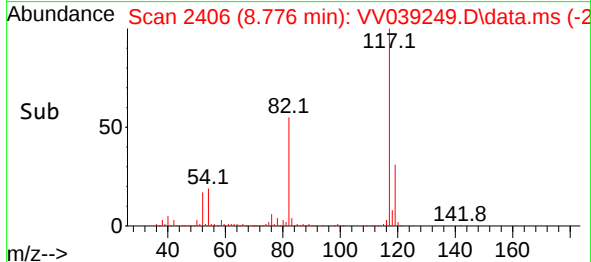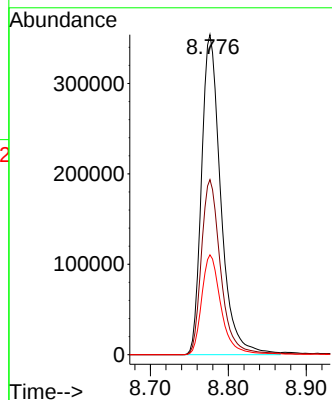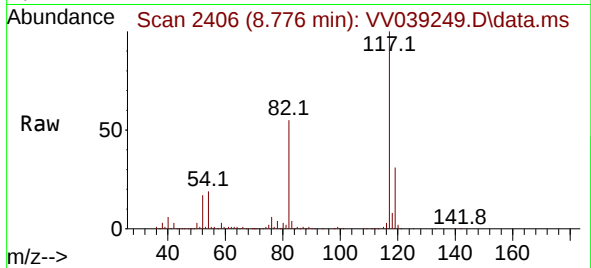

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.175 min Scan# 3152
Delta R.T. 0.003 min
Lab File: VV039249.D
Acq: 03 Oct 2025 15:04

Tgt Ion:152 Resp: 300076
Ion Ratio Lower Upper
152 100
115 59.0 44.8 134.4
150 154.0 0.0 353.8

