


Instrument IC-1				Analyst: RM	Method: 300.0 / 9056A					
Ident	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4	Method name	date time	Initial v Analyst
STD1	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-090925	9/9/2025 10:21	10 RM/IZ
STD2	0.423	0.641	0.632	2.091	0.529	1.063	3.237	IC1-090925	9/9/2025 10:42	10 RM/IZ
STD3	0.794	1.189	1.197	3.984	0.997	2.006	6.010	IC1-090925	9/9/2025 11:25	10 RM/IZ
STD4	0.990	1.475	1.473	4.920	1.228	2.461	7.371	IC1-090925	9/9/2025 11:47	10 RM/IZ
STD5	2.008	3.012	3.027	10.105	2.514	4.978	15.047	IC1-090925	9/9/2025 13:36	10 RM/IZ
STD6	3.935	5.921	5.894	19.658	4.924	9.905	29.203	IC1-090925	9/9/2025 13:58	10 RM/IZ
STD7	5.050	7.561	7.577	25.243	6.308	12.587	37.633	IC1-090925	9/9/2025 14:41	10 RM/IZ
ICV	2.001	2.995	2.988	9.985	2.483	5.041	14.797	IC1-090925	9/9/2025 15:02	10 RM/IZ
ICB	0.000	0.063	0.000	0.000	0.000	0.000	0.000	IC1-090925	9/9/2025 15:45	10 RM/IZ
CCV	1.976	2.943	2.981	10.039	2.435	4.674	14.687	IC1-090925	9/25/2025 9:29	10 RM/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-090925	9/25/2025 9:51	10 RM/IZ
Q3202-01	0.038	6.943	0.000	0.229	1.502	0.000	26.241	IC1-090925	9/25/2025 10:12	10 RM/IZ
Q3202-03	0.132	388.453	0.000	0.000	3.029	0.000	21.967	IC1-090925	9/25/2025 10:34	10 RM/IZ
Q3202-05	0.086	300.476	0.000	0.000	2.963	0.000	13.237	IC1-090925	9/25/2025 10:55	10 RM/IZ
Q3202-07	0.083	298.727	0.000	0.000	2.993	0.000	13.377	IC1-090925	9/25/2025 11:17	10 RM/IZ
Q3202-09	0.053	4.908	0.000	0.000	0.085	0.000	0.823	IC1-090925	9/25/2025 11:38	10 RM/IZ
Q3202-11	0.259	967.298	0.000	0.348	0.000	0.000	39.913	IC1-090925	9/25/2025 12:00	10 RM/IZ
Q3202-13MS	2.215	921.362	2.960	10.244	2.438	3.365	53.804	IC1-090925	9/25/2025 12:22	10 RM/IZ
Q3202-15MSD	2.195	924.995	2.893	10.018	2.375	2.739	53.573	IC1-090925	9/25/2025 12:43	10 RM/IZ
Q3202-17	0.107	397.261	0.000	0.303	0.100	0.000	21.579	IC1-090925	9/25/2025 13:05	10 RM/IZ
LB137321BLW	0.000	0.000	0.000	0.000	0.000	0.164	0.000	IC1-090925	9/25/2025 13:26	10 RM/IZ
CCV	2.009	2.952	2.998	10.076	2.441	5.195	14.901	IC1-090925	9/25/2025 13:48	10 RM/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-090925	9/25/2025 14:09	10 RM/IZ
LB137321BSW	1.982	2.960	3.001	10.087	2.449	5.125	14.820	IC1-090925	9/25/2025 14:31	10 RM/IZ
Q3202-03DLX100	0.000	2.609	0.000	0.000	0.067	0.000	0.602	IC1-090925	9/25/2025 14:55	10 RM/IZ
Q3202-05DLX100	0.000	2.078	0.000	0.000	0.070	0.000	0.553	IC1-090925	9/25/2025 15:18	10 RM/IZ
Q3202-07DLX100	0.000	2.033	0.000	0.000	0.071	0.000	0.530	IC1-090925	9/25/2025 15:39	10 RM/IZ
Q3202-11DLX2	0.147	471.543	0.000	0.231	0.000	0.000	19.598	IC1-090925	9/25/2025 16:01	10 RM/IZ
Q3202-11DL2X200	0.000	3.158	0.000	0.000	0.000	0.000	0.601	IC1-090925	9/25/2025 16:22	10 RM/IZ
Q3202-17DLX100	0.000	2.708	0.000	0.000	0.000	0.000	0.616	IC1-090925	9/25/2025 16:44	10 RM/IZ
CCV	2.029	2.954	2.997	10.074	2.437	5.173	14.867	IC1-090925	9/25/2025 17:05	10 RM/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-090925	9/25/2025 17:27	10 RM/IZ

Clear table

Instrument ID: IC-2 Analyst: IZ Method: 300.0 / 9056A									
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentratio n HPO4	concentrati on SO4	file name	Initial wt/ Final
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-090925	10 RM/IZ
STD2	0.4230	0.6410	0.6320	2.0910	0.5290	1.0630	3.2370	IC1-090925	10 RM/IZ
STD3	0.7940	1.1890	1.1970	3.9840	0.9970	2.0060	6.0100	IC1-090925	10 RM/IZ
STD4	0.9900	1.4750	1.4730	4.9200	1.2280	2.4610	7.3710	IC1-090925	10 RM/IZ
STD5	2.0080	3.0120	3.0270	10.1050	2.5140	4.9780	15.0470	IC1-090925	10 RM/IZ
STD6	3.9350	5.9210	5.8940	19.6580	4.9240	9.9050	29.2030	IC1-090925	10 RM/IZ
STD7	5.0500	7.5610	7.5770	25.2430	6.3080	12.5870	37.6330	IC1-090925	10 RM/IZ
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000		
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000		
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000		
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000		
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000		
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000		
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000		
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4		
STD1									
STD2	5.7500	6.8333	5.3333	4.5500	5.8000	6.3000	7.9000		
STD3	-0.7500	-0.9167	-0.2500	-0.4000	-0.3000	0.3000	0.1667		
STD4	-1.0000	-1.6667	-1.8000	-1.6000	-1.7600	-1.5600	-1.7200		
STD5	0.4000	0.4000	0.9000	1.0500	0.5600	-0.4400	0.3133		
STD6	-1.6250	-1.3167	-1.7667	-1.7100	-1.5200	-0.9500	-2.6567		
STD7	1.0000	0.8133	1.0267	0.9720	0.9280	0.6960	1.7108		

Fluoride (Anions)

($\mu\text{S}/\text{cm}$) x min

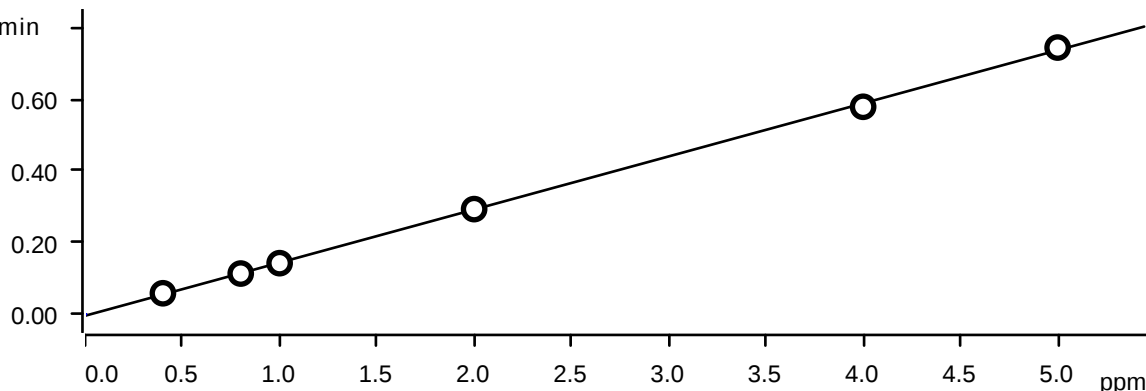

Function: $A = -3.91674E-3 + 0.0148053 \times Q$


Relative standard deviation 1.985504 %

Correlation coefficient 0.999790

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.059	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.114	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.143	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.293	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.579	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.744	STD7	2025-09-09 14:41:06 UTC-4	used

Chloride (Anions)

($\mu\text{S}/\text{cm}$) x min

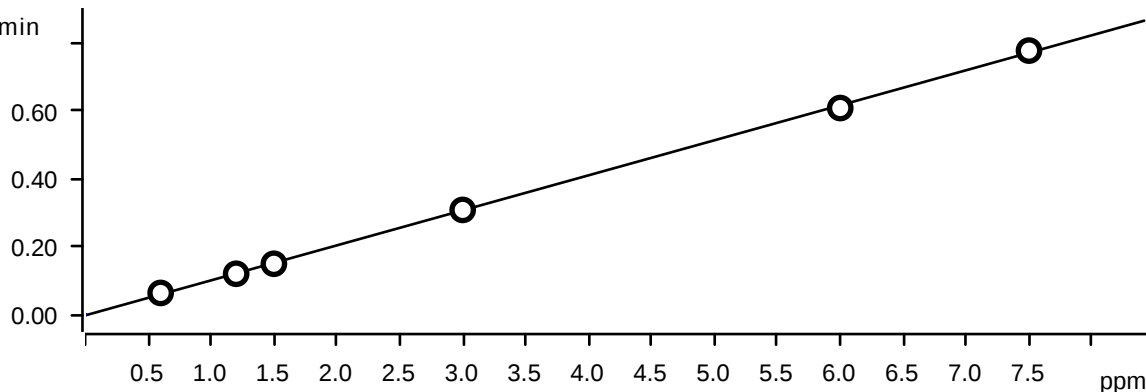


Function: $A = -2.97735E-3 + 0.0103068 \times Q$

Relative standard deviation 1.712968 %

Correlation coefficient 0.999843

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.063	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.120	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.149	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.307	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.607	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.776	STD7	2025-09-09 14:41:06 UTC-4	used

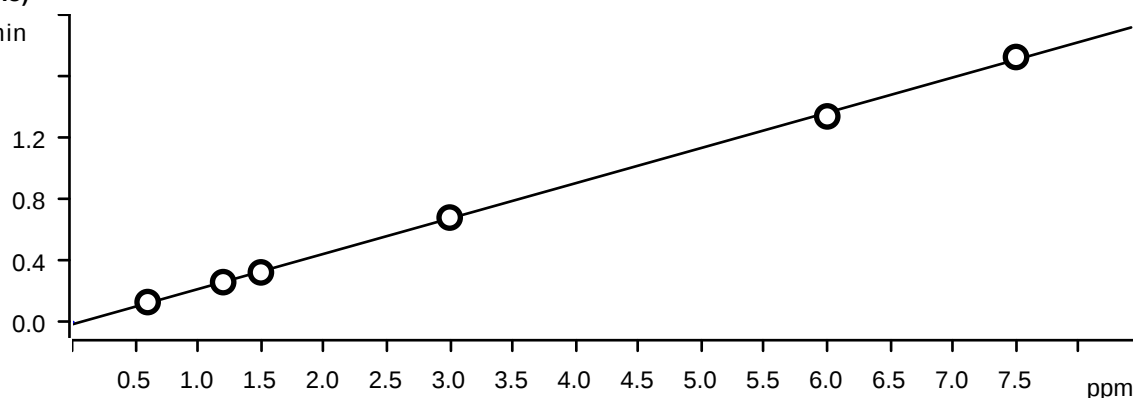
Nitrite (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0143669 + 0.0229543 \times Q$

Relative standard deviation 2.170764 %

Correlation coefficient 0.999753

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.131	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.260	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.324	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.681	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.339	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.725	STD7	2025-09-09 14:41:06 UTC-4	used

Bromide (Anions)

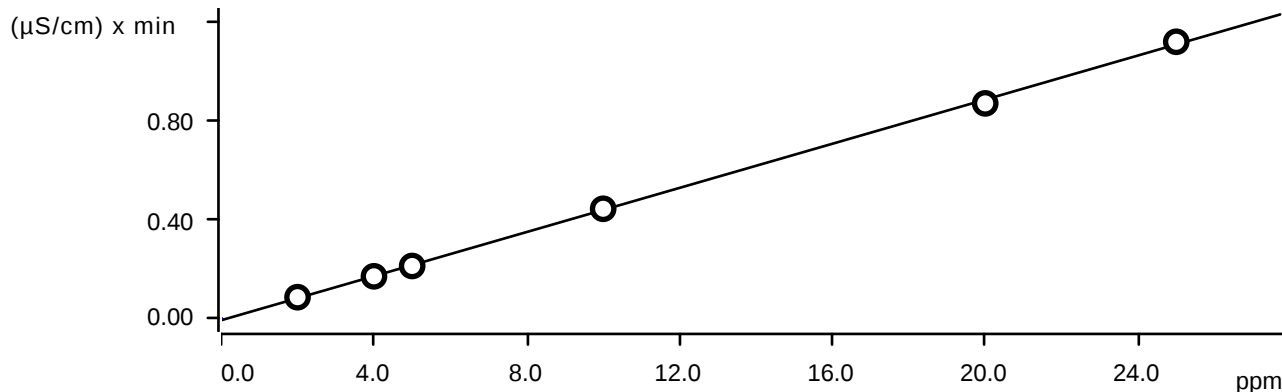


Function: $A = -5.68247E-3 + 4.44287E-3 \times Q$

Relative standard deviation: 2.066849 %

Correlation coefficient: 0.999773

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.087	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.171	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.213	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.443	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.868	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.116	STD7	2025-09-09 14:41:06 UTC-4	used

Nitrate (Anions)

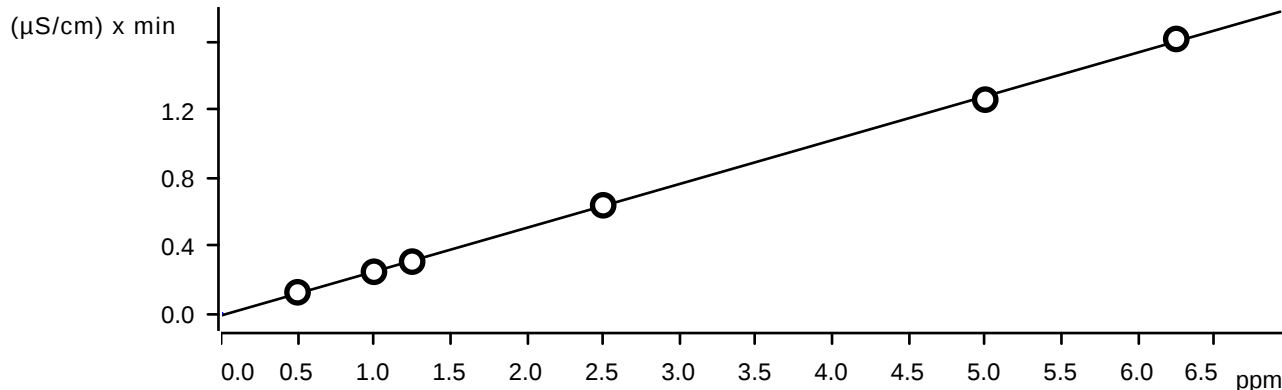


Function: $A = -0.0122982 + 0.0258010 \times Q$

Relative standard deviation: 1.914251 %

Correlation coefficient 0.999807

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.124	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.245	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.305	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.636	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.258	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.615	STD7	2025-09-09 14:41:06 UTC-4	used

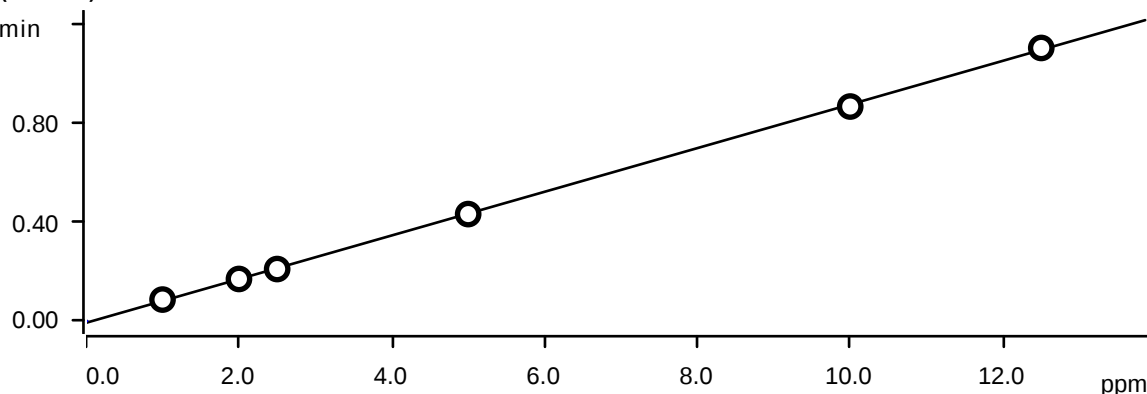
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -6.72192E-3 + 8.79335E-3 \times Q$

Relative standard deviation 1.384046 %

Correlation coefficient 0.999898

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.087	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.170	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.210	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.431	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.864	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.100	STD7	2025-09-09 14:41:06 UTC-4	used

Sulfate (Anions)

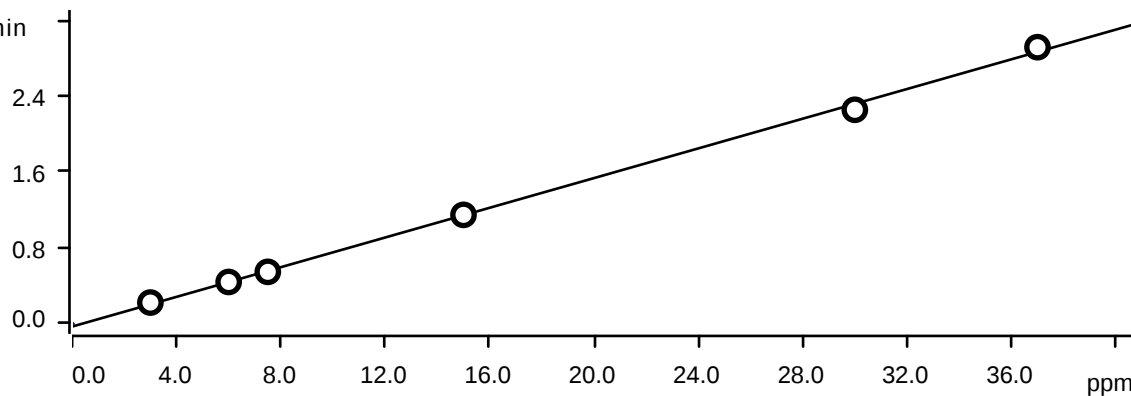 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0295615 + 7.81954E-3 \times Q$

Relative standard deviation 3.285067 %

Correlation coefficient 0.999433


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.224	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.440	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.547	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.147	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.254	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.913	STD7	2025-09-09 14:41:06 UTC-4	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-09-09 10:21:26 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 13.06 MPa
Maximum pressure monitored yes
Temperature ---- °C

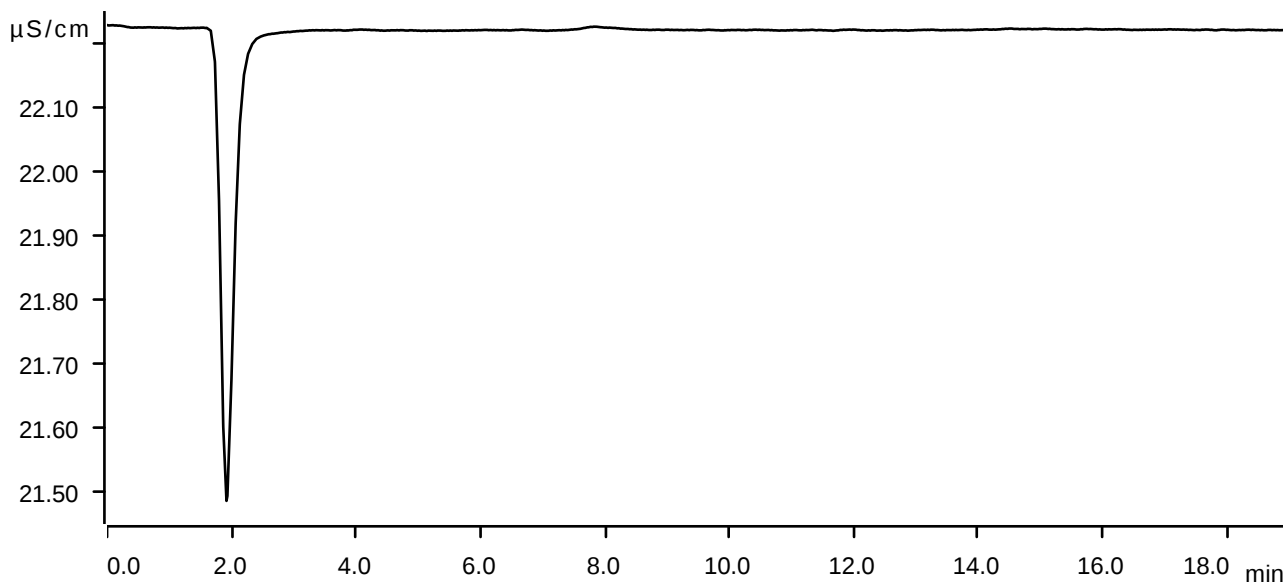Anions


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-09-09 10:42:49 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.84 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

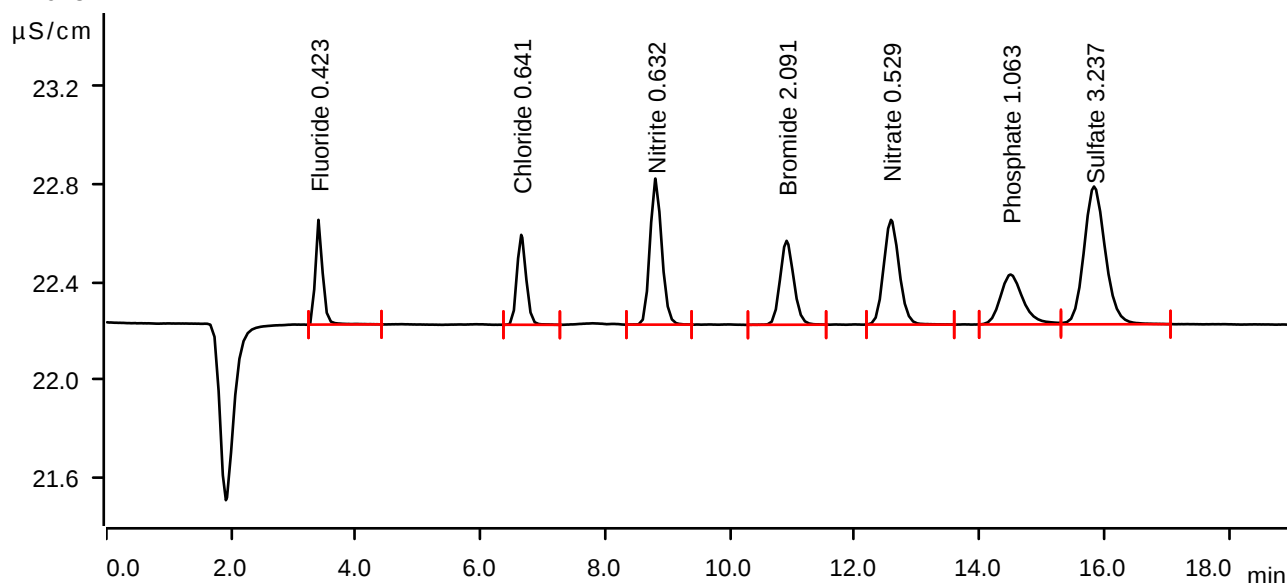

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.400	0.0587	0.429	0.423	Fluoride
2	6.652	0.0631	0.369	0.641	Chloride
3	8.803	0.1306	0.599	0.632	Nitrite
4	10.907	0.0872	0.344	2.091	Bromide
5	12.580	0.1242	0.430	0.529	Nitrate
6	14.497	0.0867	0.205	1.063	Phosphate
7	15.835	0.2236	0.565	3.237	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-09-09 11:25:44 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.67 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

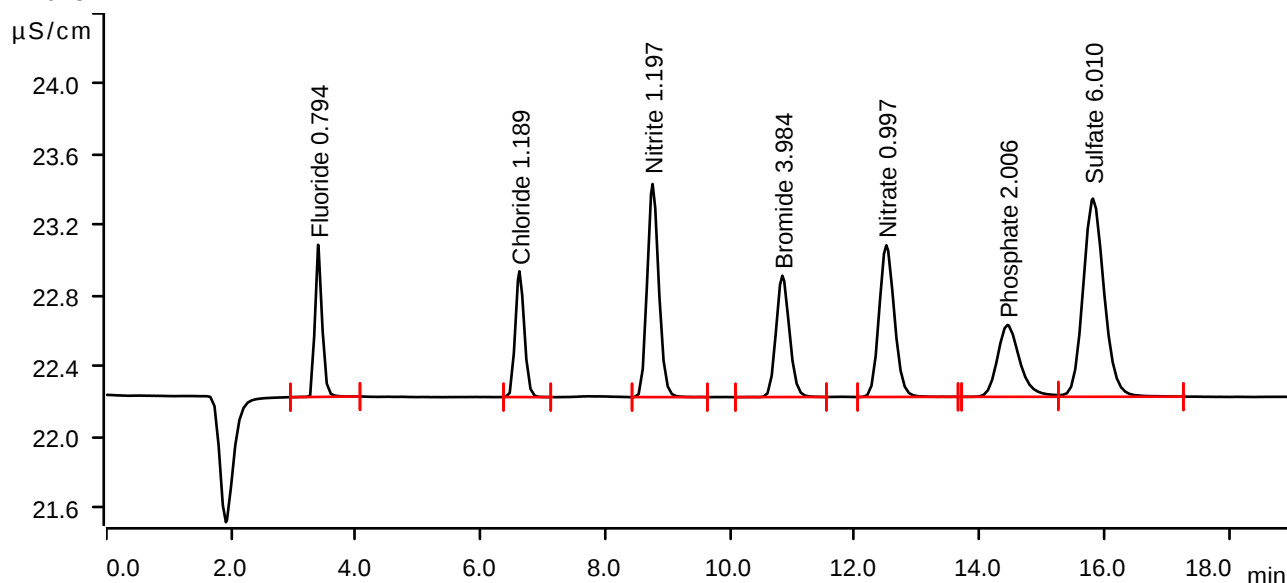

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.395	0.1137	0.861	0.794	Fluoride
2	6.623	0.1196	0.712	1.189	Chloride
3	8.758	0.2603	1.206	1.197	Nitrite
4	10.838	0.1713	0.687	3.984	Bromide
5	12.505	0.2450	0.859	0.997	Nitrate
6	14.448	0.1697	0.407	2.006	Phosphate
7	15.818	0.4404	1.122	6.010	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-09-09 11:47:10 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.61 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

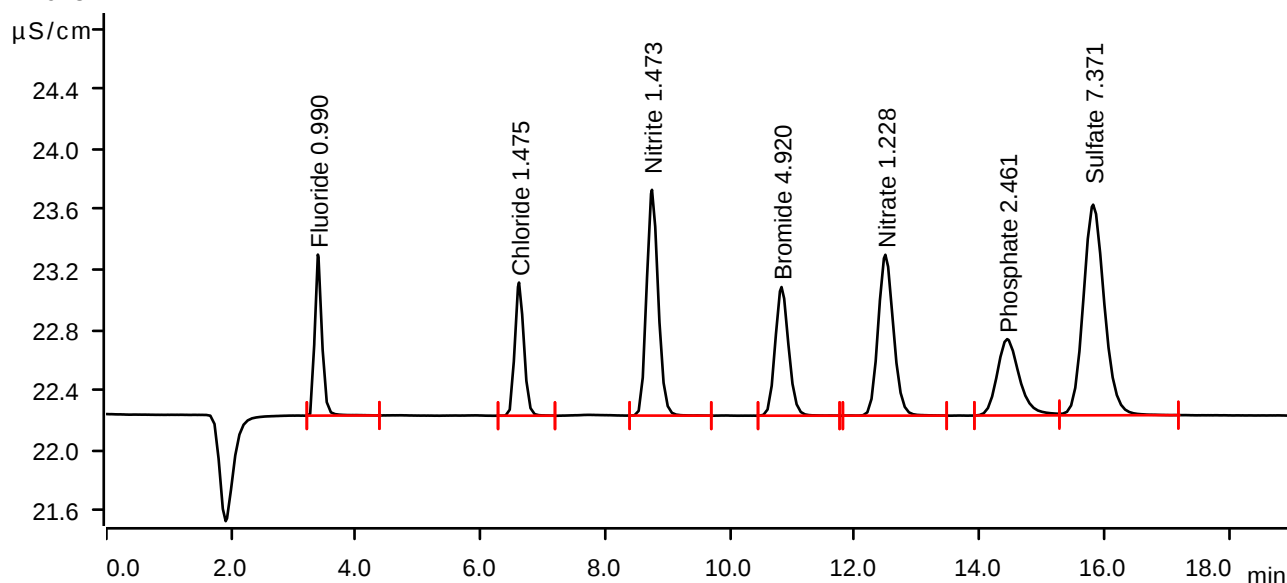

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.392	0.1426	1.068	0.990	Fluoride
2	6.617	0.1490	0.884	1.475	Chloride
3	8.748	0.3238	1.499	1.473	Nitrite
4	10.825	0.2129	0.854	4.920	Bromide
5	12.490	0.3046	1.068	1.228	Nitrate
6	14.443	0.2097	0.507	2.461	Phosphate
7	15.822	0.5468	1.398	7.371	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2025-09-09 13:36:36 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.50 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

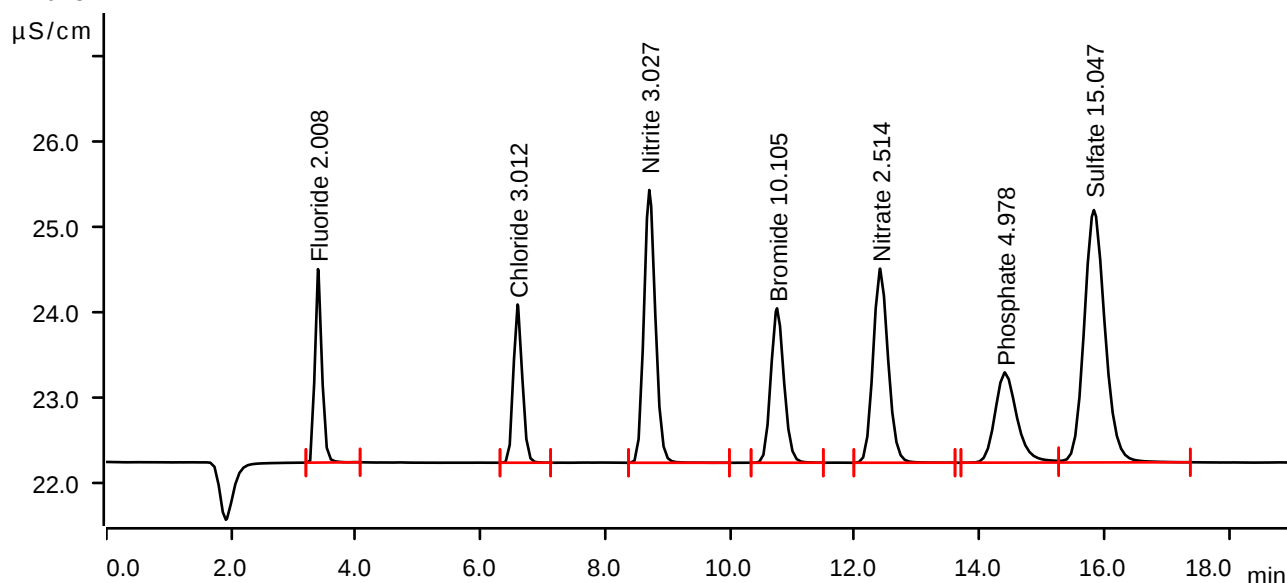

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.393	0.2933	2.266	2.008	Fluoride
2	6.593	0.3075	1.854	3.012	Chloride
3	8.705	0.6805	3.195	3.027	Nitrite
4	10.753	0.4432	1.809	10.105	Bromide
5	12.407	0.6363	2.273	2.514	Nitrate
6	14.405	0.4310	1.057	4.978	Phosphate
7	15.833	1.1470	2.956	15.047	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-09-09 13:58:07 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

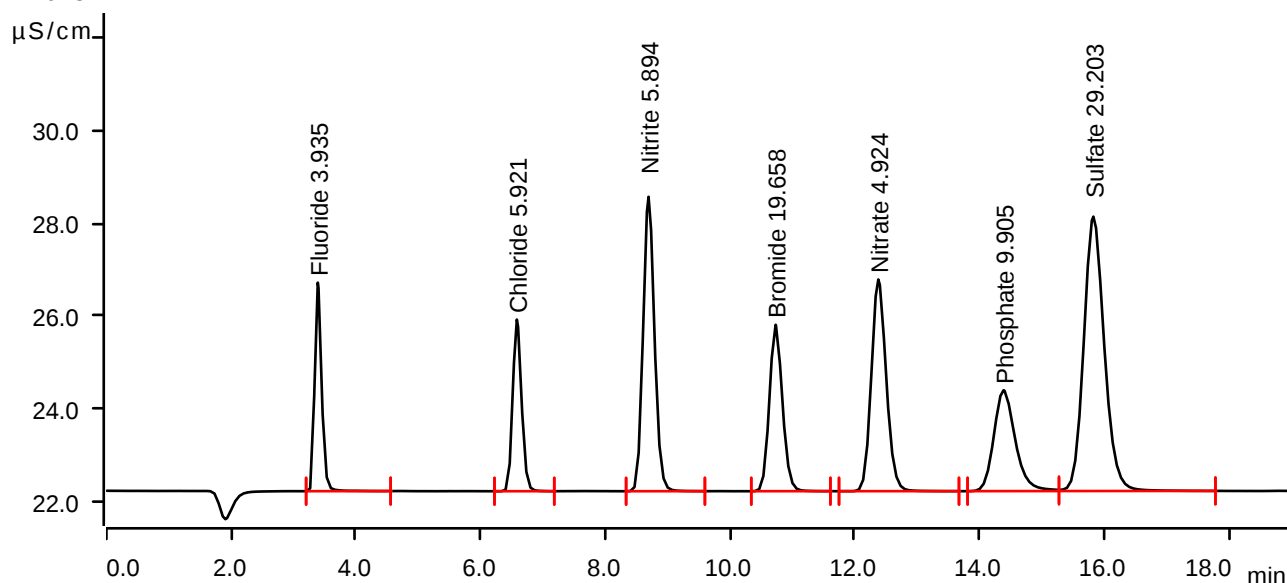

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.390	0.5787	4.477	3.935	Fluoride
2	6.582	0.6073	3.687	5.921	Chloride
3	8.693	1.3385	6.323	5.894	Nitrite
4	10.730	0.8677	3.574	19.658	Bromide
5	12.377	1.2581	4.546	4.924	Nitrate
6	14.385	0.8642	2.167	9.905	Phosphate
7	15.825	2.2540	5.893	29.203	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-09-09 14:41:06 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

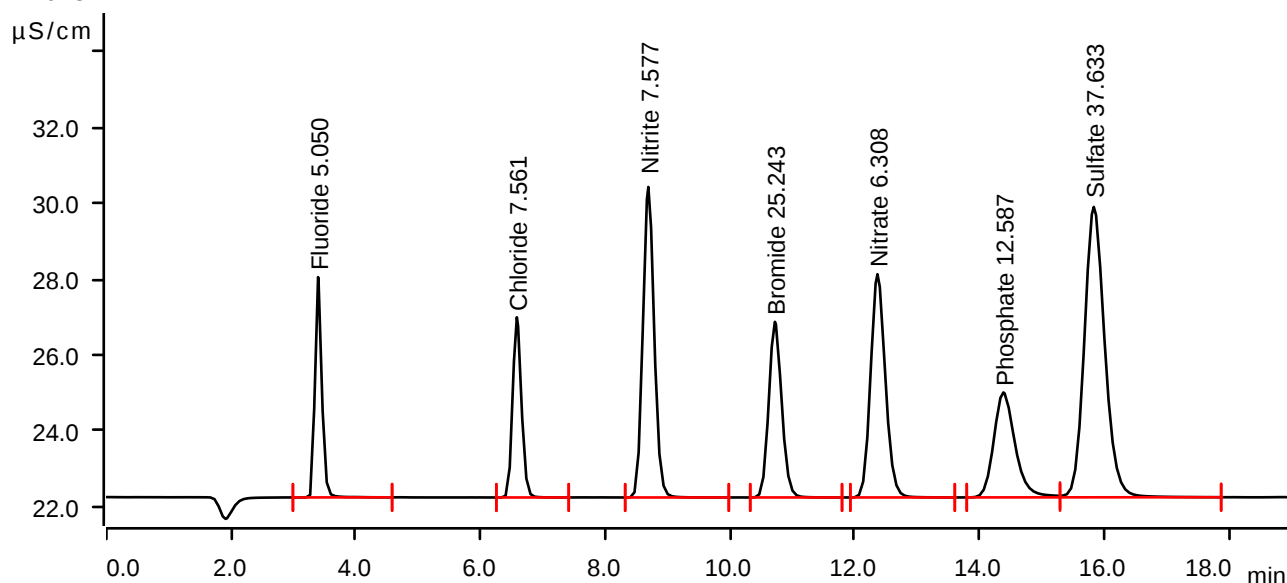

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.395	0.7438	5.806	5.050	Fluoride
2	6.582	0.7764	4.748	7.561	Chloride
3	8.690	1.7250	8.184	7.577	Nitrite
4	10.718	1.1158	4.629	25.243	Bromide
5	12.363	1.6152	5.884	6.308	Nitrate
6	14.382	1.1001	2.766	12.587	Phosphate
7	15.832	2.9131	7.654	37.633	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-09-09 15:02:34 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.50 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

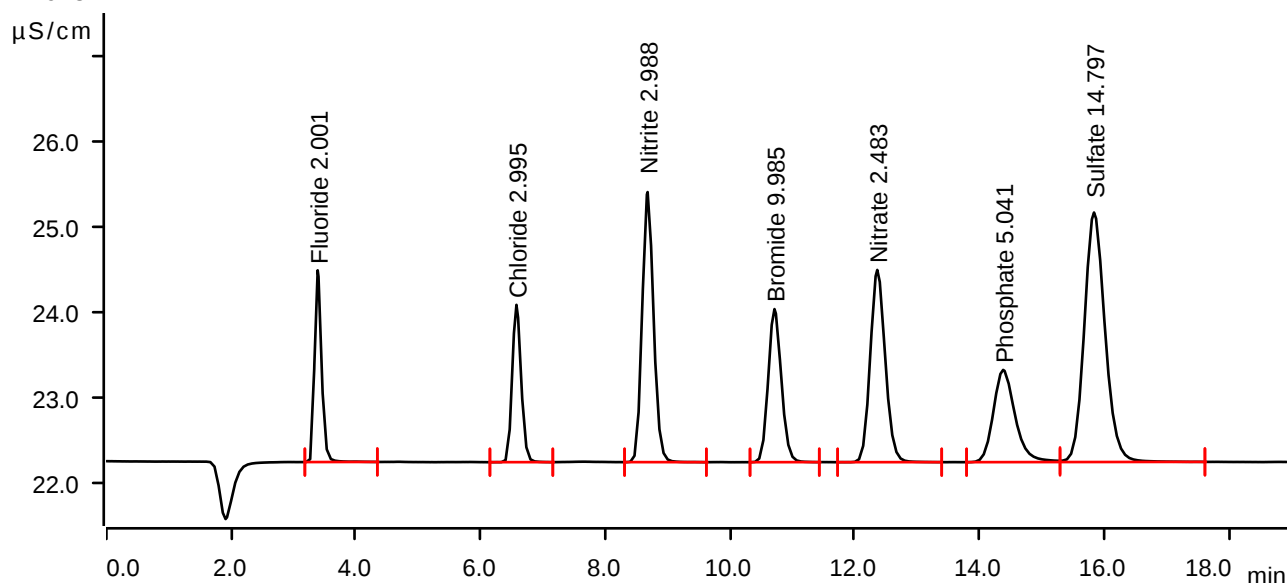

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.388	0.2923	2.246	2.001	Fluoride
2	6.575	0.3057	1.843	2.995	Chloride
3	8.678	0.6715	3.164	2.988	Nitrite
4	10.712	0.4379	1.793	9.985	Bromide
5	12.360	0.6282	2.252	2.483	Nitrate
6	14.378	0.4365	1.080	5.041	Phosphate
7	15.835	1.1275	2.923	14.797	Sulfate


Sample data

Ident ICB
Sample type Sample
Determination start 2025-09-09 15:45:30 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

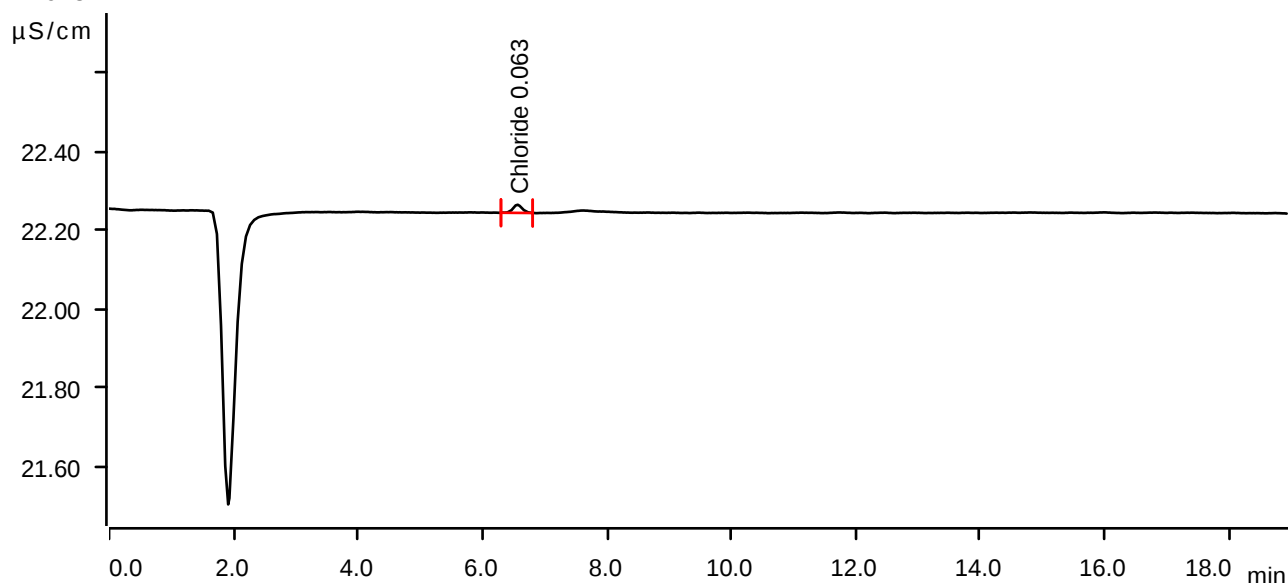

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.568	0.0036	0.021	0.063	Chloride


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-09-25 09:29:37 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

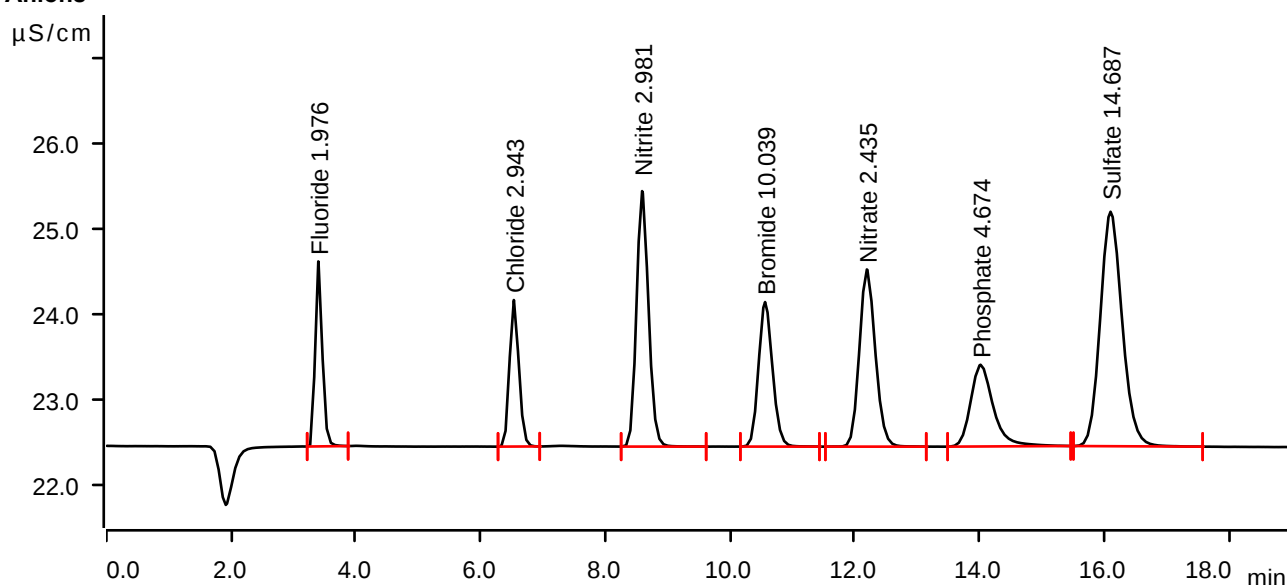


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.398	0.2886	2.166	1.976	Fluoride
2	6.533	0.3003	1.716	2.943	Chloride
3	8.590	0.6698	2.993	2.981	Nitrite
4	10.562	0.4403	1.693	10.039	Bromide
5	12.193	0.6161	2.075	2.435	Nitrate
6	14.017	0.4043	0.957	4.674	Phosphate
7	16.100	1.1189	2.746	14.687	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-09-25 09:51:08 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

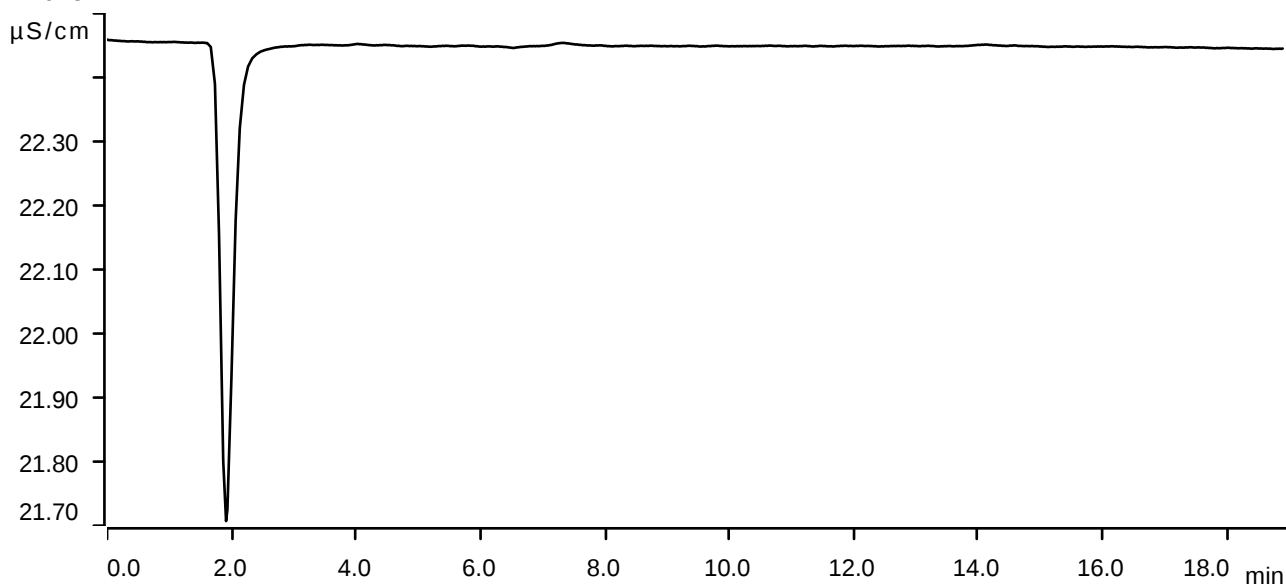Anions


Sample data

Ident Q3202-01
Sample type Sample
Determination start 2025-09-25 10:12:40 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

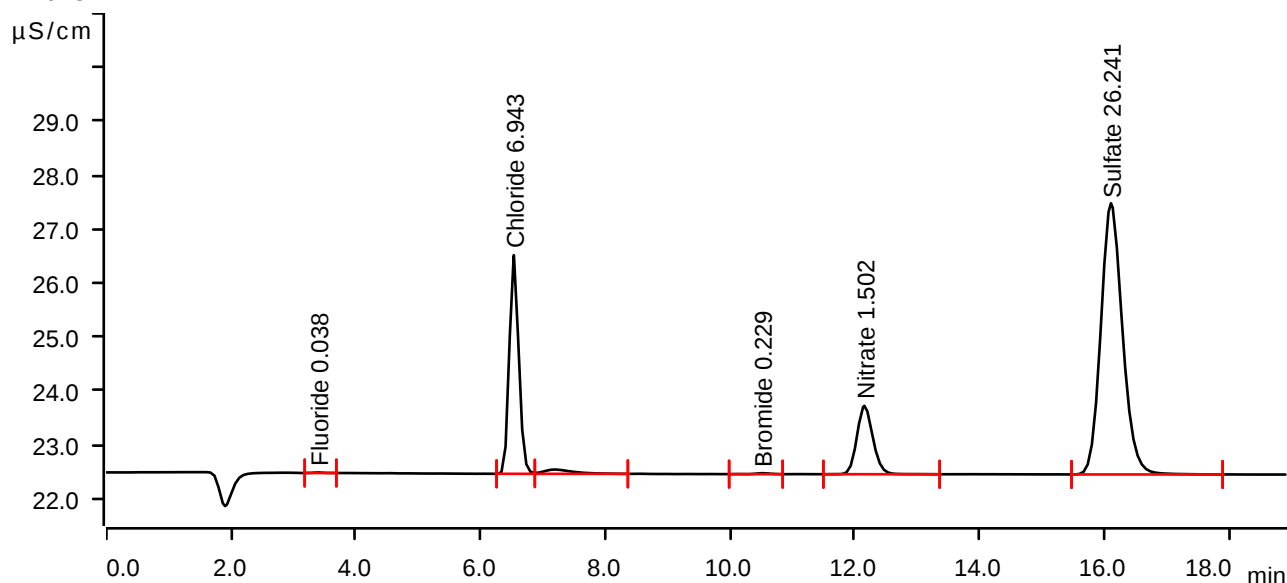

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.398	0.0017	0.011	0.038	Fluoride
2	6.532	0.7126	4.056	6.943	Chloride
3	7.185	0.0431	0.079	invalid	
4	10.512	0.0045	0.018	0.229	Bromide
5	12.153	0.3751	1.269	1.502	Nitrate
6	16.107	2.0223	5.030	26.241	Sulfate


Sample data

Ident Q3202-03
Sample type Sample
Determination start 2025-09-25 10:34:14 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

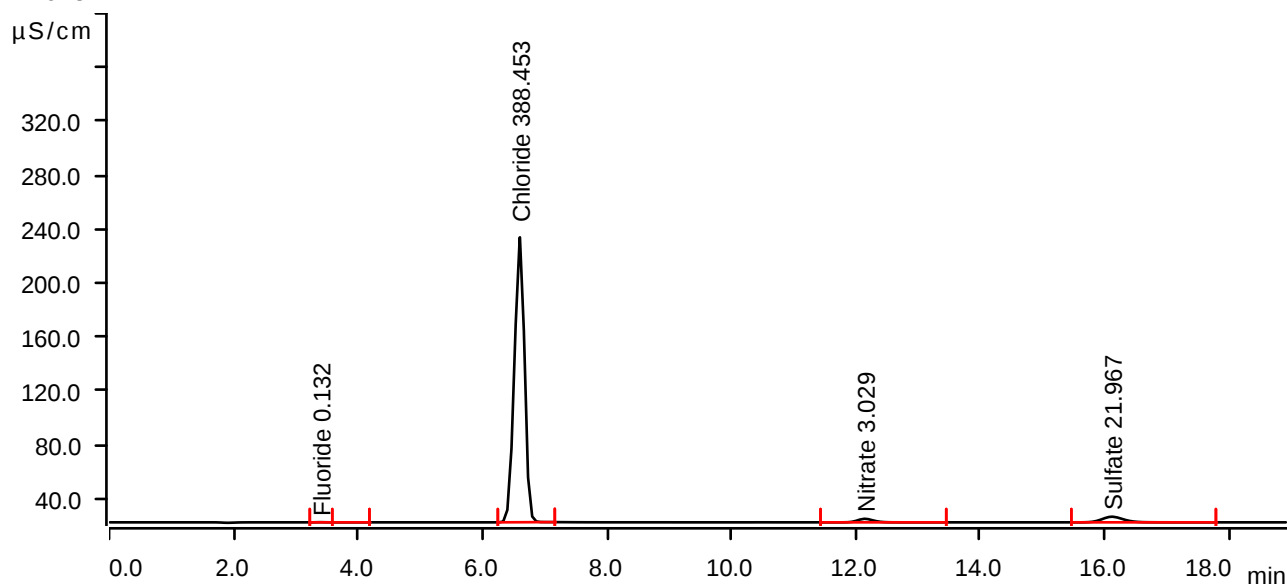

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.397	0.0156	0.114	0.132	Fluoride
2	3.660	0.0019	0.008	invalid	
3	6.603	40.0340	211.397	388.453	Chloride
4	12.145	0.7691	2.622	3.029	Nitrate
5	16.115	1.6882	4.177	21.967	Sulfate


Sample data

Ident Q3202-05
Sample type Sample
Determination start 2025-09-25 10:55:48 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

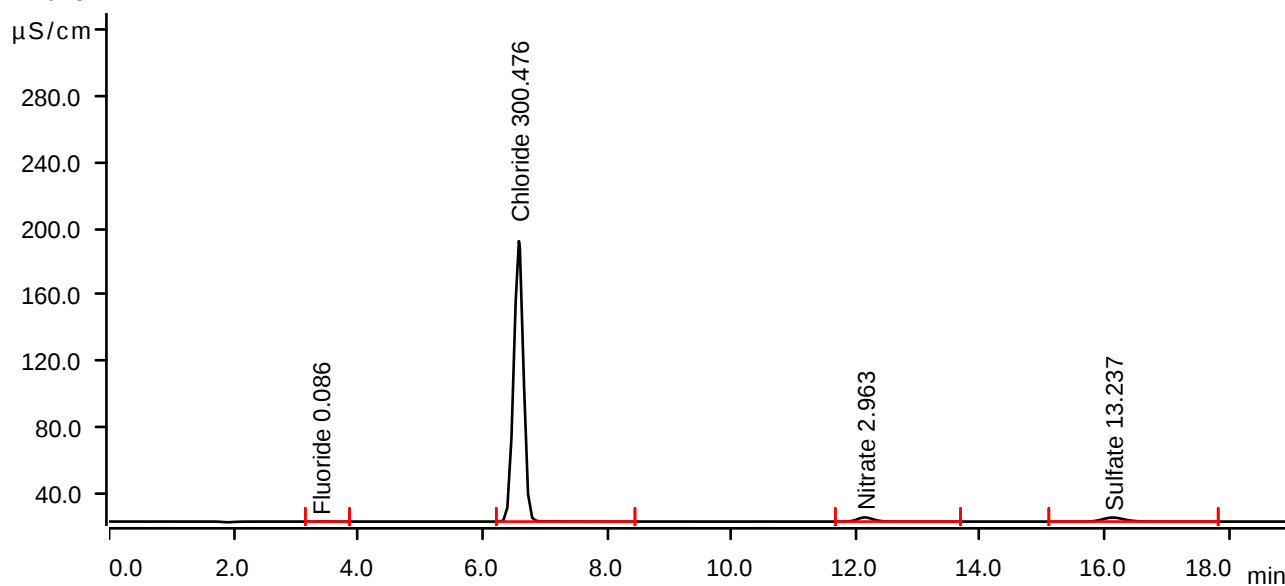

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.393	0.0088	0.061	0.086	Fluoride
2	6.587	30.9665	169.691	300.476	Chloride
3	12.143	0.7522	2.556	2.963	Nitrate
4	16.128	1.0055	2.462	13.237	Sulfate


Sample data

Ident Q3202-07
Sample type Sample
Determination start 2025-09-25 11:17:23 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

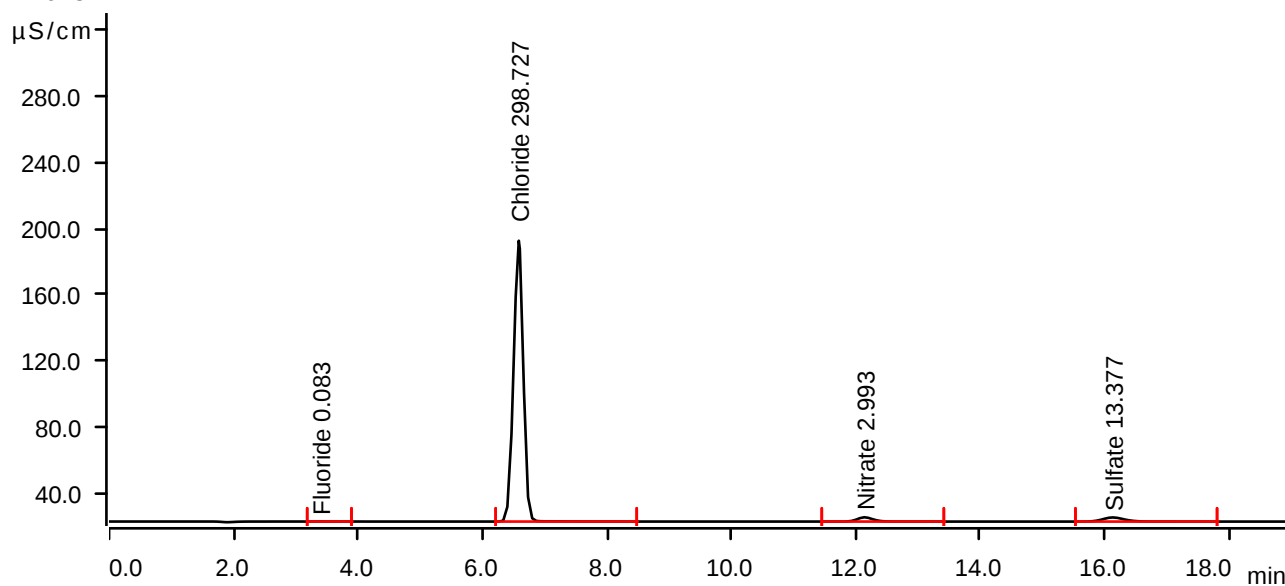

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.395	0.0084	0.057	0.083	Fluoride
2	6.585	30.7862	169.947	298.727	Chloride
3	12.140	0.7598	2.591	2.993	Nitrate
4	16.128	1.0164	2.507	13.377	Sulfate


Sample data

Ident Q3202-09
Sample type Sample
Determination start 2025-09-25 11:38:58 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

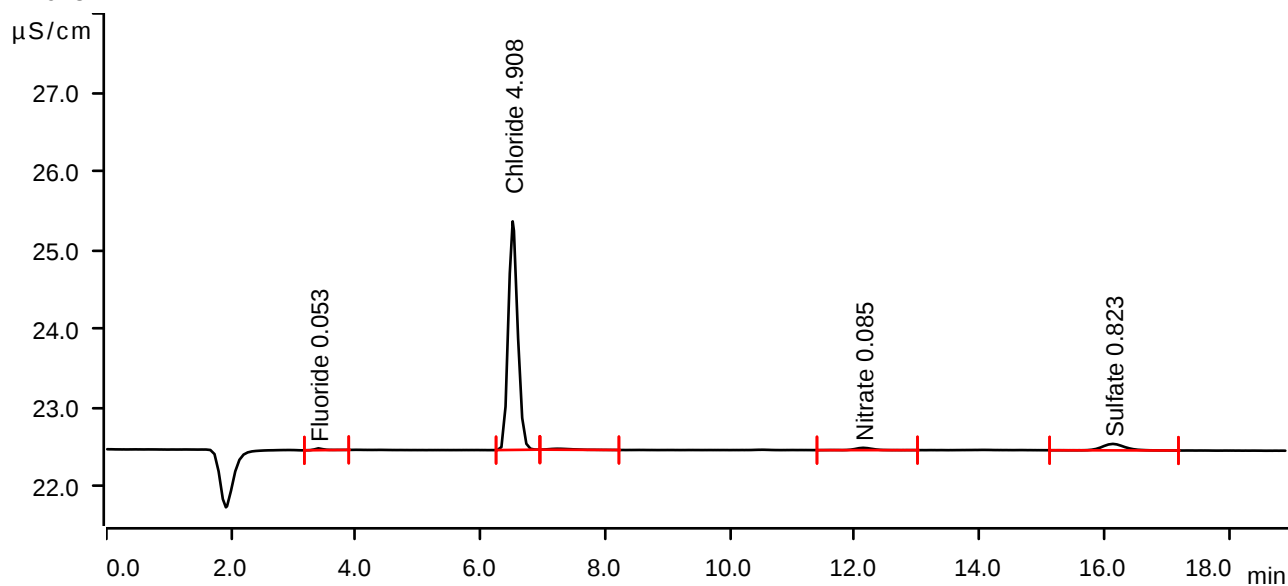

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.398	0.0039	0.023	0.053	Fluoride
2	6.515	0.5028	2.900	4.908	Chloride
3	7.232	0.0054	0.013	invalid	
4	12.135	0.0096	0.029	0.085	Nitrate
5	16.142	0.0348	0.082	0.823	Sulfate


Sample data

Ident Q3202-11
Sample type Sample
Determination start 2025-09-25 12:00:33 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

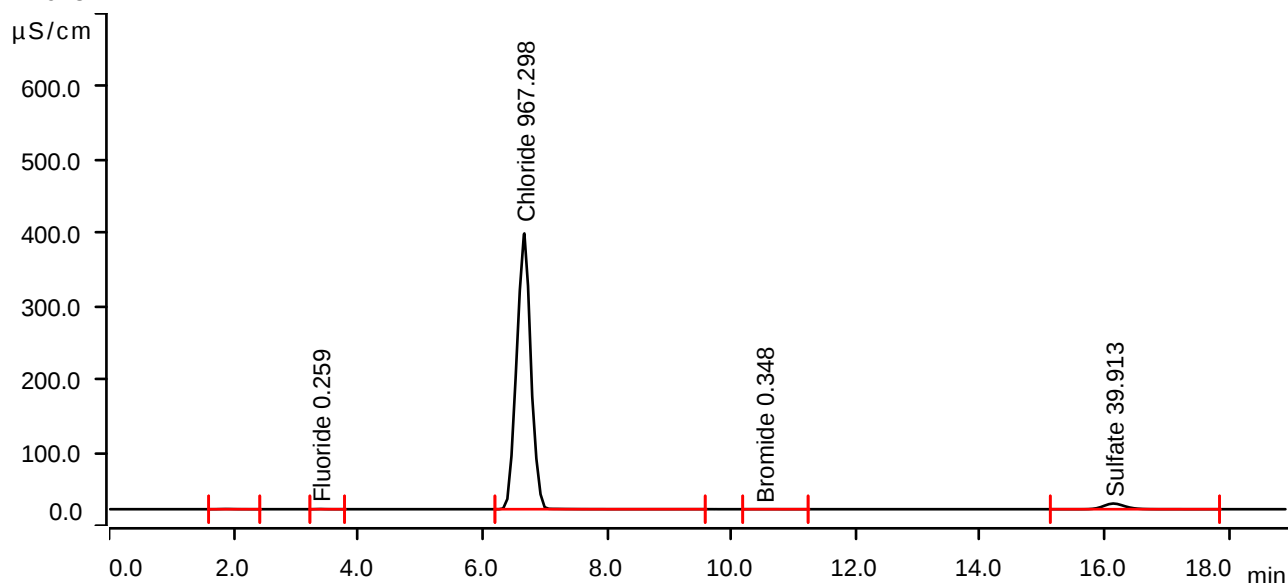

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.882	0.0714	0.283	invalid	
2	3.393	0.0344	0.254	0.259	Fluoride
3	6.675	99.6942	376.905	967.298	Chloride
4	10.522	0.0098	0.038	0.348	Bromide
5	16.138	3.0915	7.767	39.913	Sulfate


Sample data

Ident Q3202-13MS
Sample type Sample
Determination start 2025-09-25 12:22:07 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

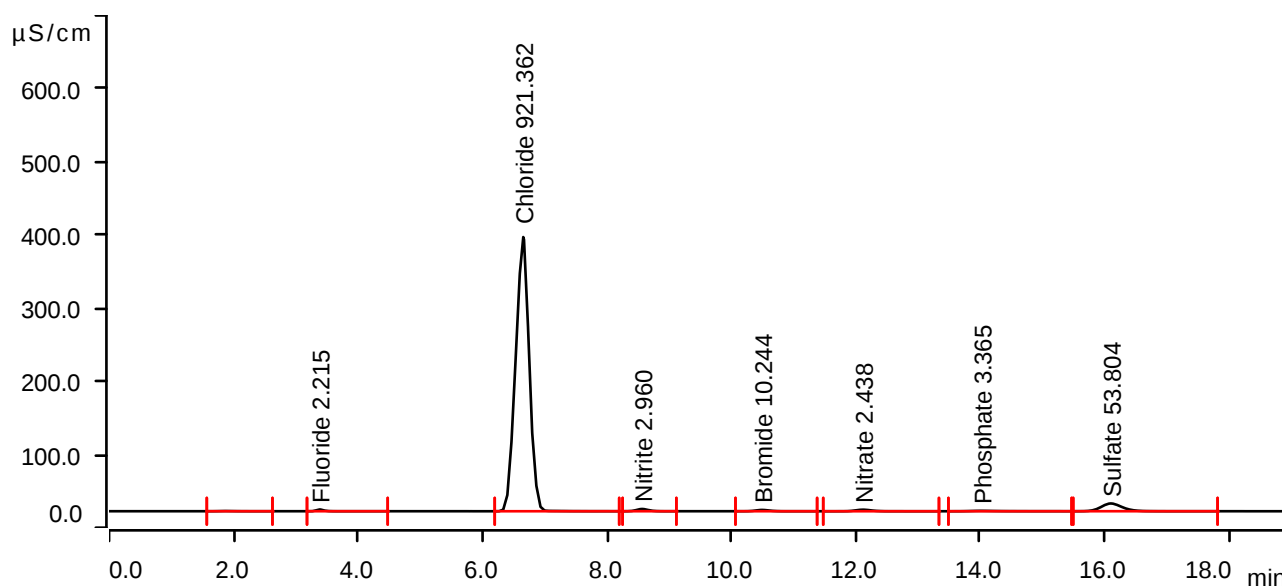

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.872	0.0713	0.284	invalid	
2	3.385	0.3240	2.359	2.215	Fluoride
3	6.657	94.9597	374.696	921.362	Chloride
4	8.567	0.6650	3.068	2.960	Nitrite
5	10.495	0.4494	1.759	10.244	Bromide
6	12.115	0.6168	2.106	2.438	Nitrate
7	14.018	0.2892	0.554	3.365	Phosphate
8	16.098	4.1777	10.594	53.804	Sulfate


Sample data

Ident Q3202-15MSD
Sample type Sample
Determination start 2025-09-25 12:43:41 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

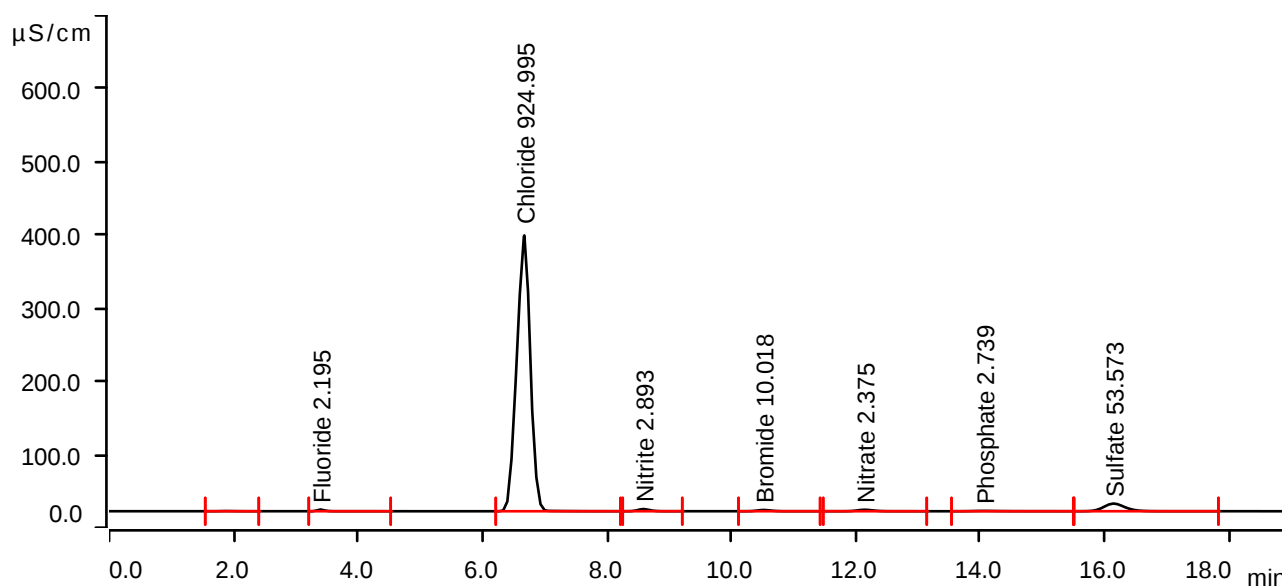

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.885	0.0717	0.284	invalid	
2	3.398	0.3210	2.340	2.195	Fluoride
3	6.675	95.3342	376.955	924.995	Chloride
4	8.587	0.6498	2.966	2.893	Nitrite
5	10.518	0.4394	1.700	10.018	Bromide
6	12.142	0.6004	2.032	2.375	Nitrate
7	14.060	0.2341	0.448	2.739	Phosphate
8	16.142	4.1596	10.445	53.573	Sulfate


Sample data

Ident Q3202-17
Sample type Sample
Determination start 2025-09-25 13:05:14 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

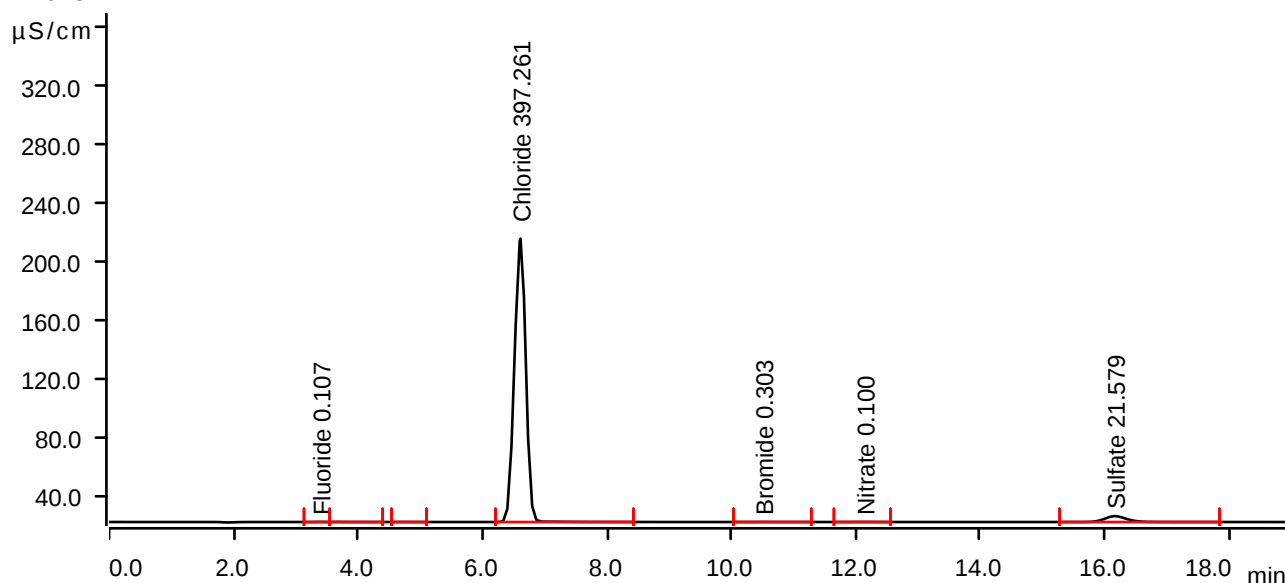

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.398	0.0120	0.083	0.107	Fluoride
2	3.680	0.0127	0.061	invalid	
3	4.723	0.0046	0.023	invalid	
4	6.612	40.9419	193.653	397.261	Chloride
5	10.512	0.0078	0.028	0.303	Bromide
6	12.140	0.0135	0.045	0.100	Nitrate
7	16.163	1.6578	4.039	21.579	Sulfate


Sample data

Ident LB137321BLW
Sample type Sample
Determination start 2025-09-25 13:26:46 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.05 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

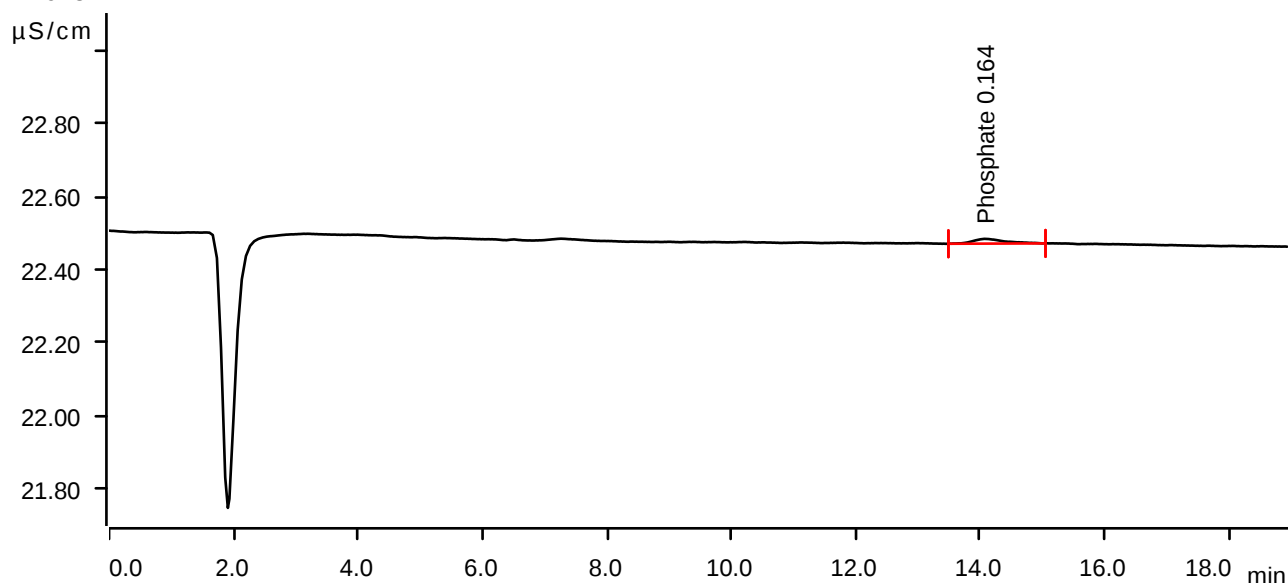

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	14.065	0.0077	0.013	0.164	Phosphate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-09-25 13:48:18 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

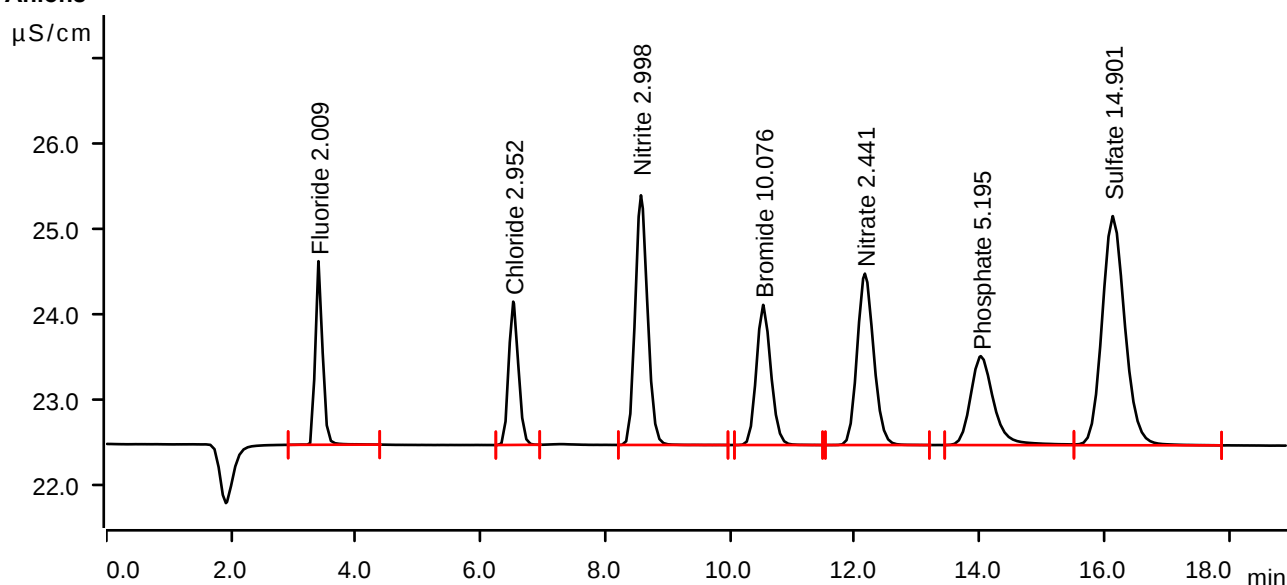


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.402	0.2935	2.150	2.009	Fluoride
2	6.523	0.3013	1.678	2.952	Chloride
3	8.572	0.6739	2.925	2.998	Nitrite
4	10.530	0.4420	1.642	10.076	Bromide
5	12.162	0.6174	2.008	2.441	Nitrate
6	14.020	0.4501	1.042	5.195	Phosphate
7	16.137	1.1356	2.684	14.901	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-09-25 14:09:50 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

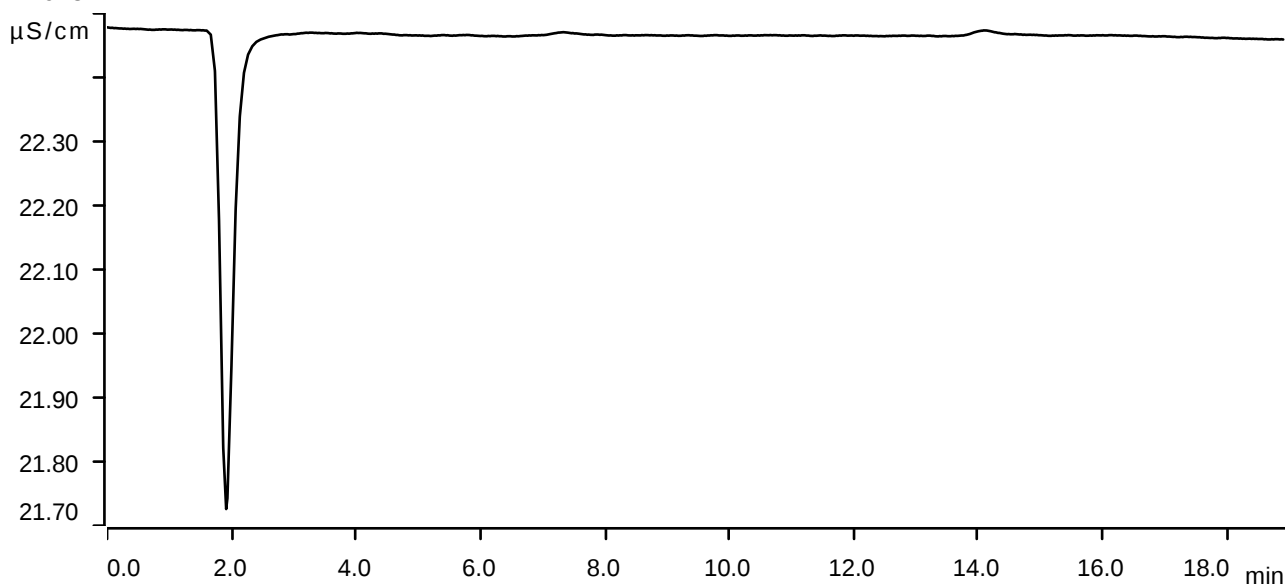Anions


Sample data

Ident LB137321BSW
Sample type Check standard 1
Determination start 2025-09-25 14:31:21 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.05 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

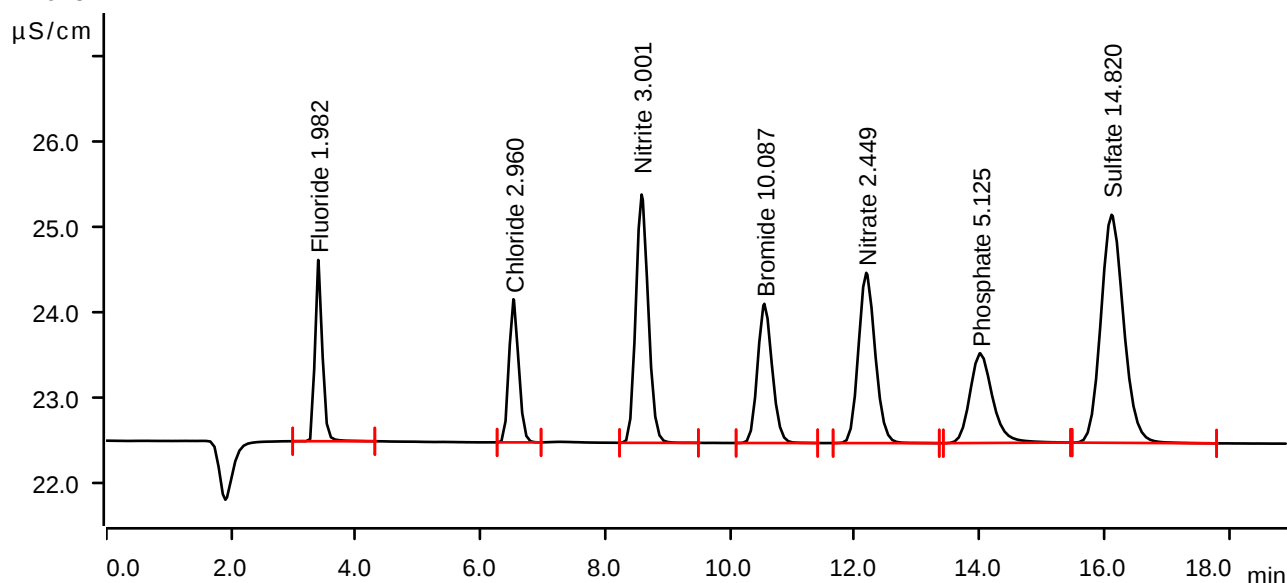

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.397	0.2896	2.123	1.982	Fluoride
2	6.527	0.3021	1.677	2.960	Chloride
3	8.582	0.6745	2.909	3.001	Nitrite
4	10.550	0.4425	1.630	10.087	Bromide
5	12.183	0.6197	1.995	2.449	Nitrate
6	14.010	0.4439	1.051	5.125	Phosphate
7	16.117	1.1293	2.671	14.820	Sulfate


Sample data

Ident Q3202-03DLX100
Sample type Sample
Determination start 2025-09-25 14:55:05 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.16 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

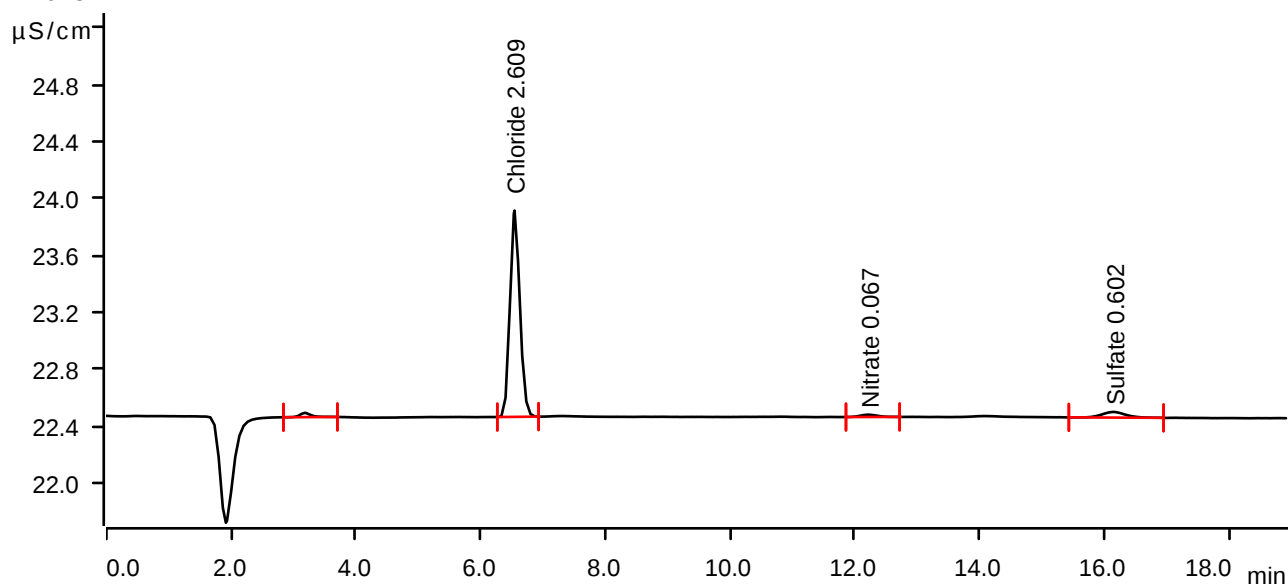

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.183	0.0062	0.030	invalid	
2	6.545	0.2659	1.450	2.609	Chloride
3	12.227	0.0051	0.016	0.067	Nitrate
4	16.157	0.0175	0.040	0.602	Sulfate


Sample data

Ident Q3202-05DLX100
Sample type Sample
Determination start 2025-09-25 15:18:27 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.05 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

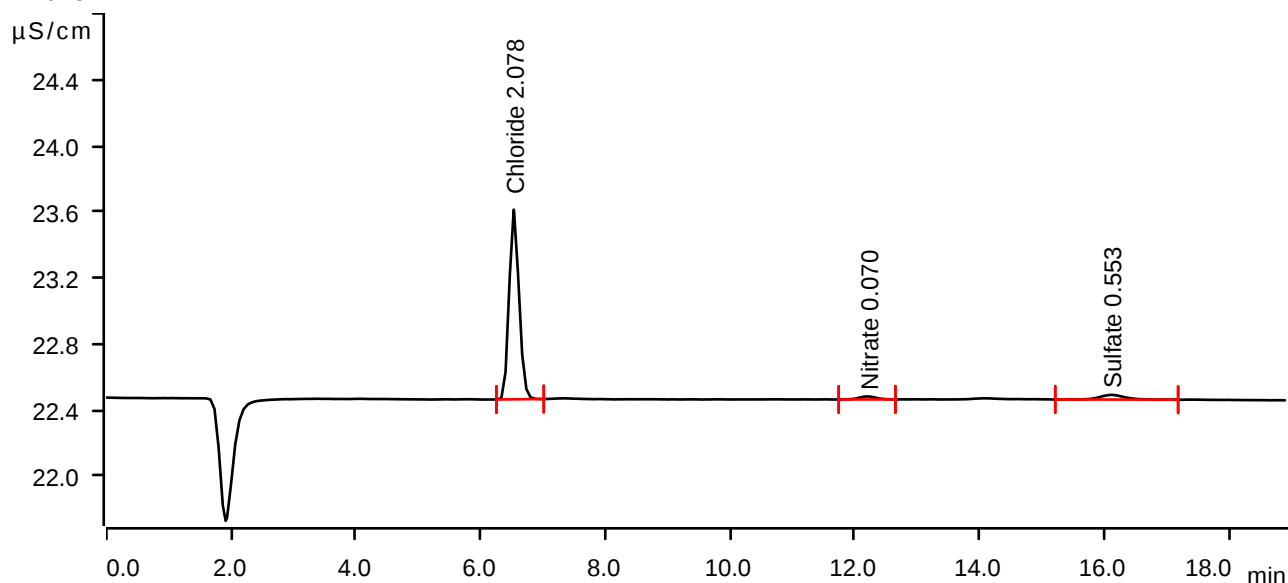

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.532	0.2112	1.148	2.078	Chloride
2	12.215	0.0058	0.018	0.070	Nitrate
3	16.112	0.0137	0.028	0.553	Sulfate


Sample data

Ident Q3202-07DLX100
Sample type Sample
Determination start 2025-09-25 15:39:57 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

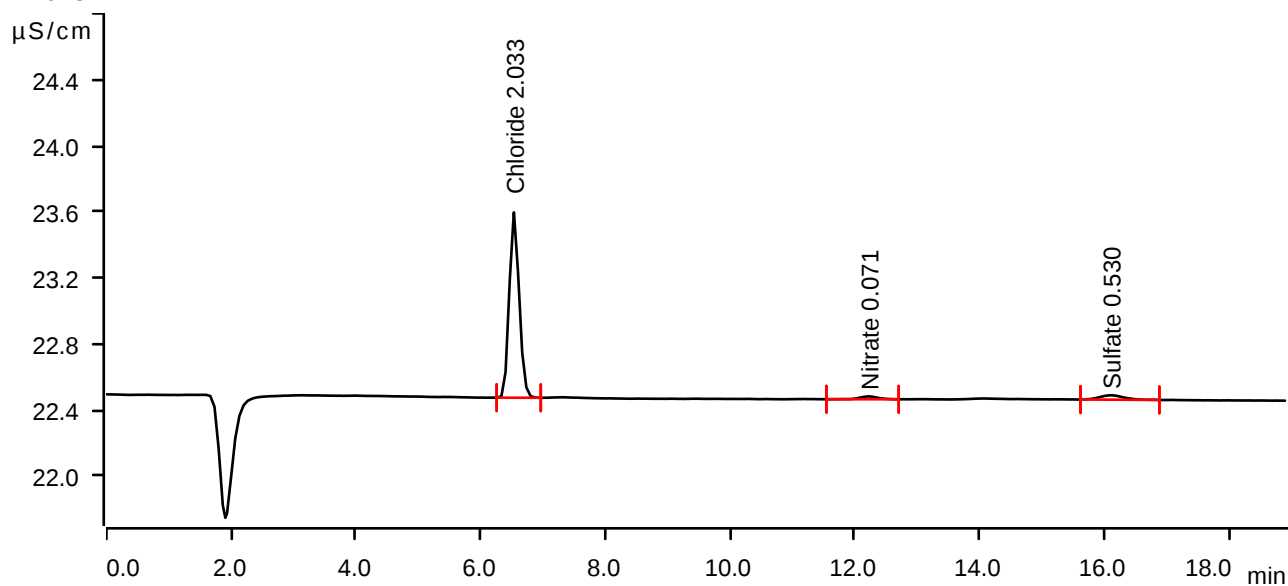

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.535	0.2065	1.121	2.033	Chloride
2	12.220	0.0059	0.017	0.071	Nitrate
3	16.098	0.0119	0.027	0.530	Sulfate


Sample data

Ident Q3202-11DLX2
Sample type Sample
Determination start 2025-09-25 16:01:27 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.16 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

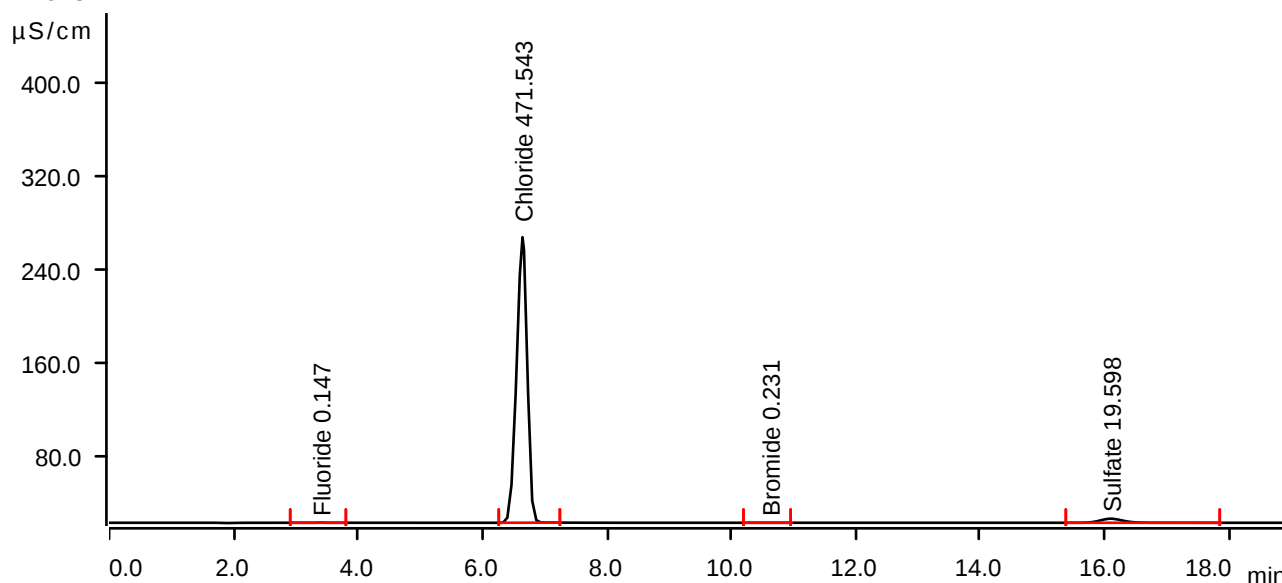

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.397	0.0178	0.125	0.147	Fluoride
2	6.645	48.5978	245.265	471.543	Chloride
3	10.617	0.0046	0.017	0.231	Bromide
4	16.097	1.5029	3.525	19.598	Sulfate


Sample data

Ident Q3202-11DL2X200
Sample type Sample
Determination start 2025-09-25 16:22:56 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.27 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

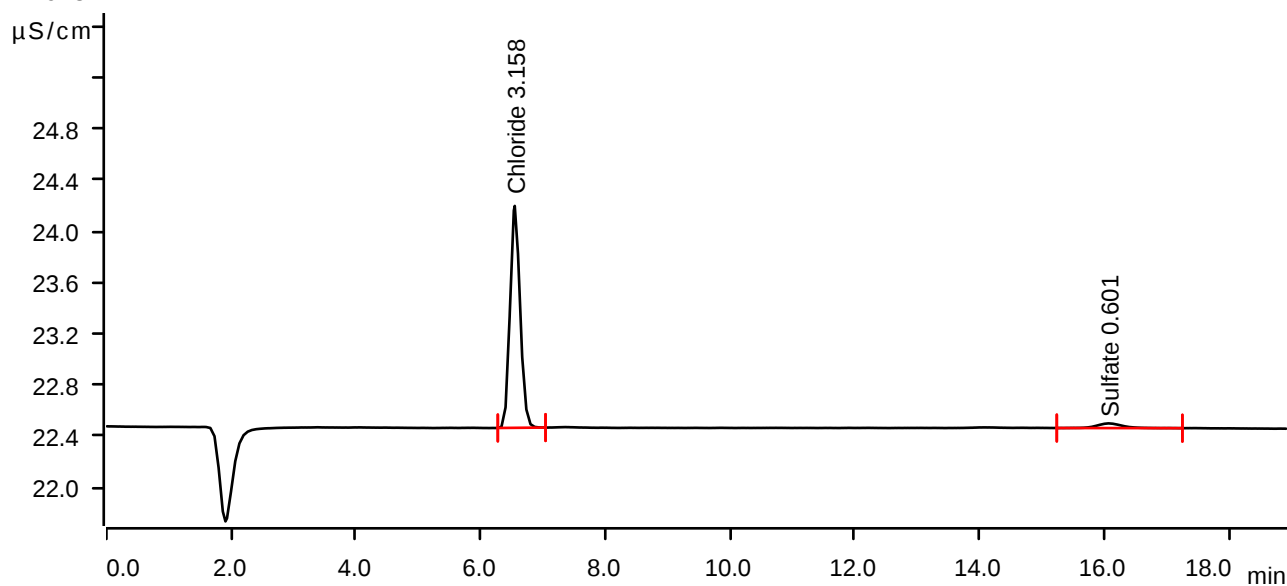

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.548	0.3225	1.733	3.158	Chloride
2	16.065	0.0174	0.037	0.601	Sulfate


Sample data

Ident Q3202-17DLX100
Sample type Sample
Determination start 2025-09-25 16:44:24 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.27 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

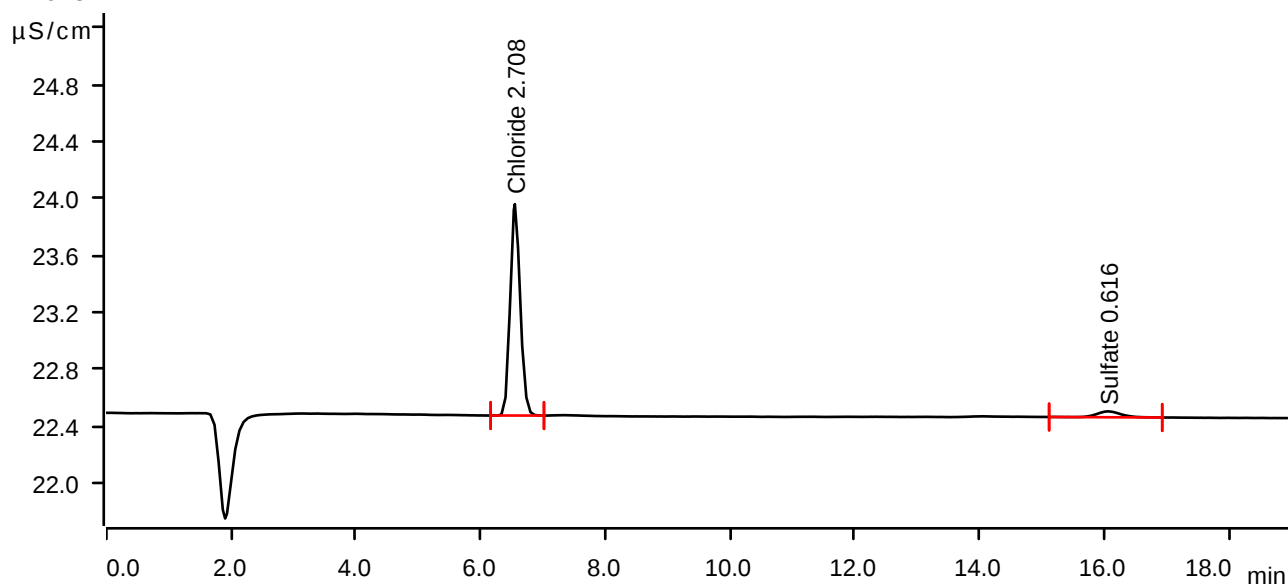

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.550	0.2761	1.486	2.708	Chloride
2	16.058	0.0186	0.042	0.616	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-09-25 17:05:50 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

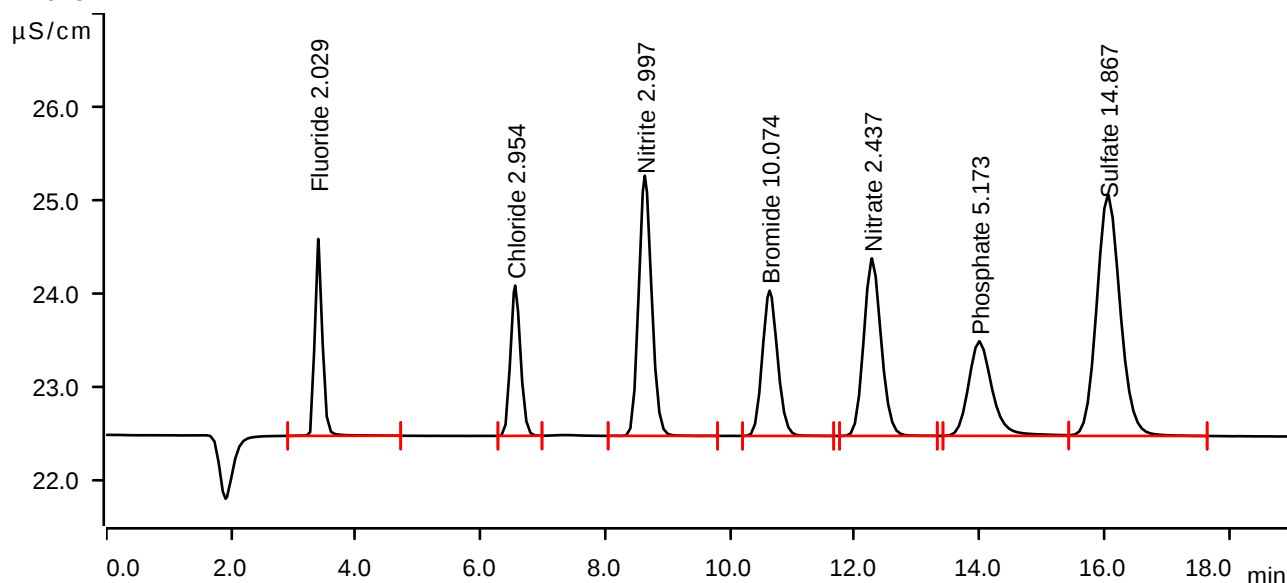

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.397	0.2966	2.114	2.029	Fluoride
2	6.555	0.3015	1.614	2.954	Chloride
3	8.633	0.6736	2.795	2.997	Nitrite
4	10.633	0.4419	1.560	10.074	Bromide
5	12.275	0.6166	1.906	2.437	Nitrate
6	13.995	0.4481	1.015	5.173	Phosphate
7	16.058	1.1330	2.590	14.867	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-09-25 17:27:09 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions