

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092925\
 Data File : VX047870.D
 Acq On : 29 Sep 2025 09:48
 Operator : JC/MD
 Sample : VX0929WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0929WBL01

Quant Time: Sep 30 01:15:03 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 17 06:39:58 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.538	168	151039	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.745	114	304108	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	305847	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	151711	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	118516	49.296	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	98.600%
35) Dibromofluoromethane	5.373	113	99558	48.815	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.620%
50) Toluene-d8	8.635	98	342151	48.483	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	96.960%
62) 4-Bromofluorobenzene	11.067	95	142267	53.118	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	106.240%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092925\
Data File : VX047870.D
Acq On : 29 Sep 2025 09:48
Operator : JC/MD
Sample : VX0929WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0929WBL01


Quant Time: Sep 30 01:15:03 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 17 06:39:58 2025
Response via : Initial Calibration

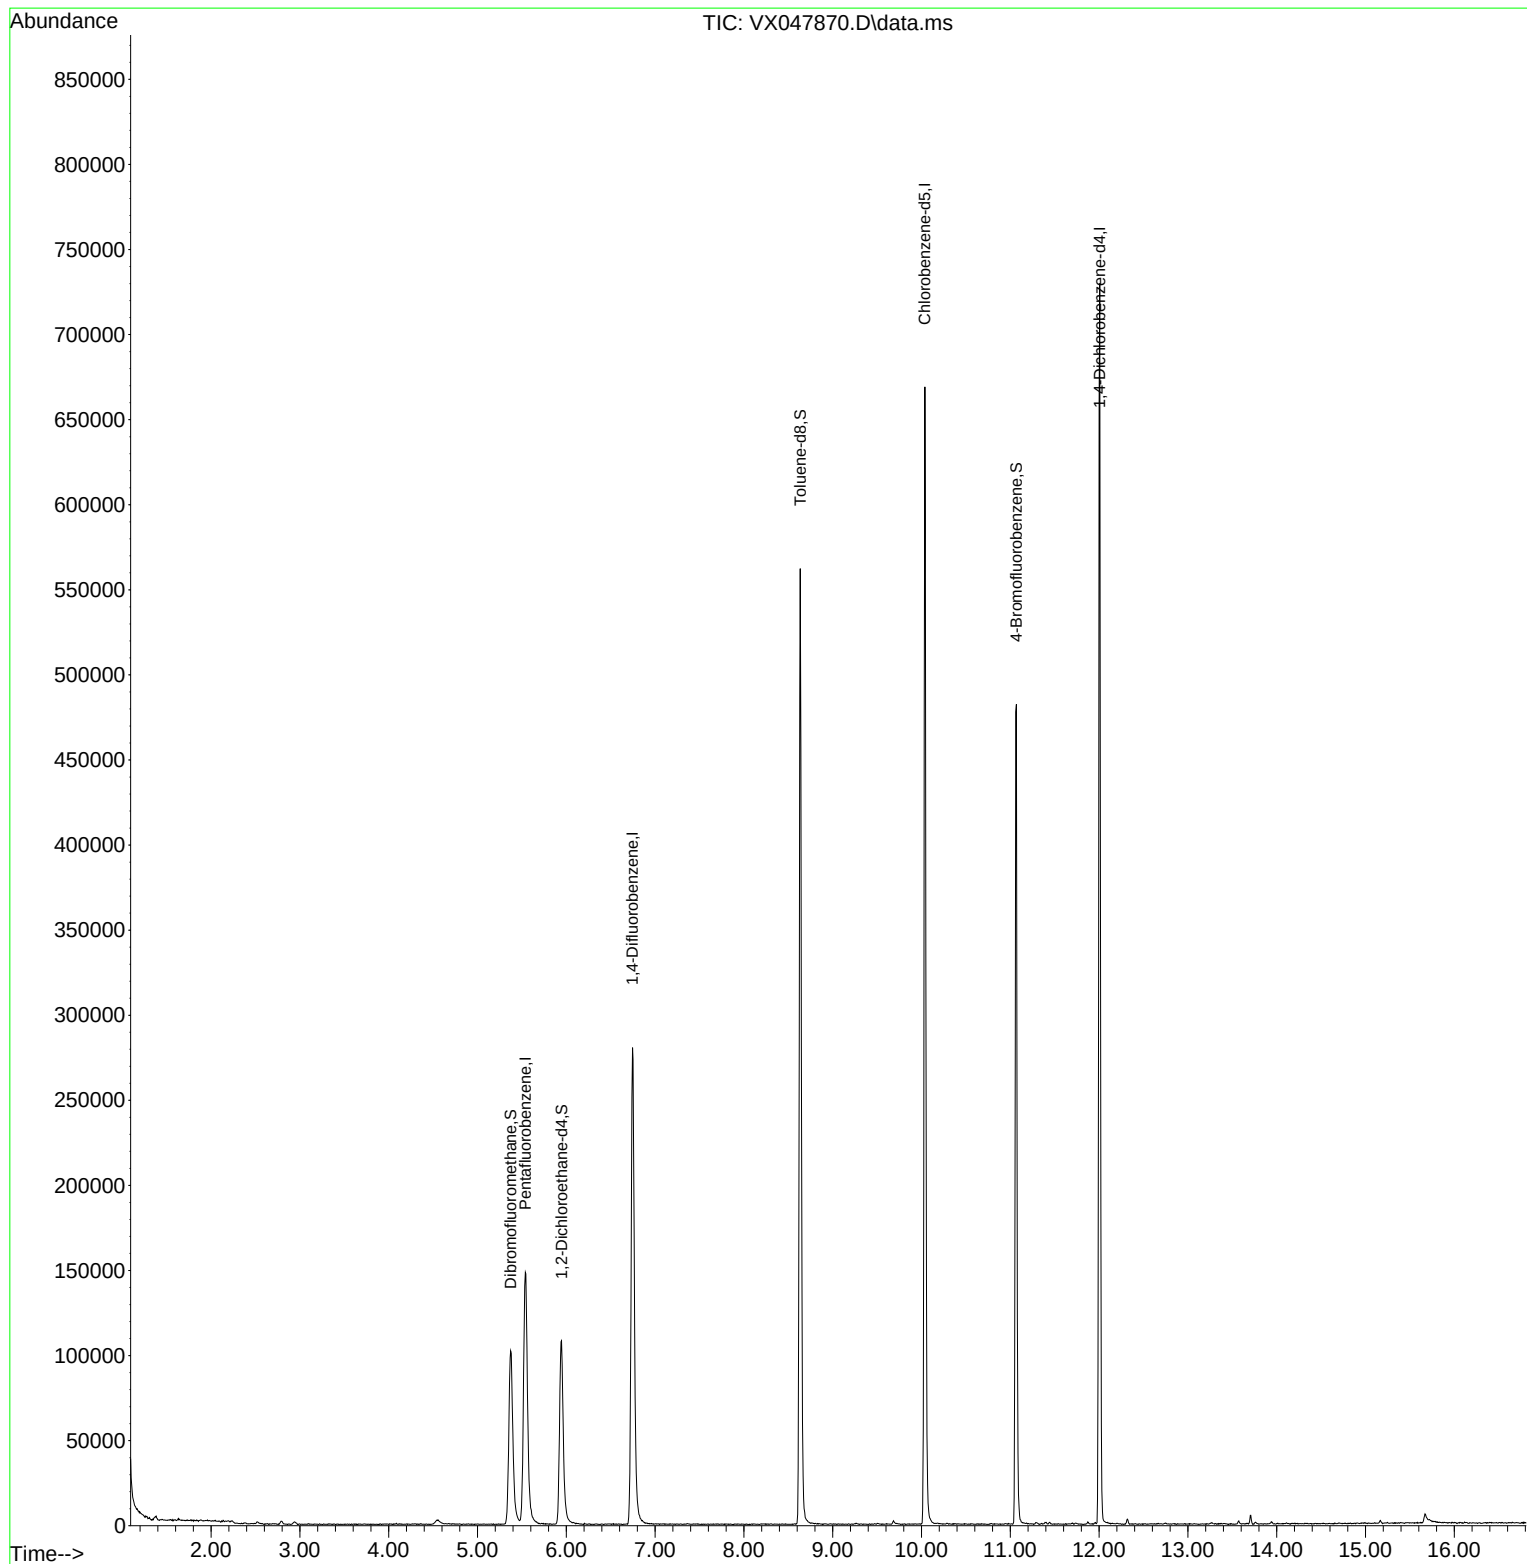



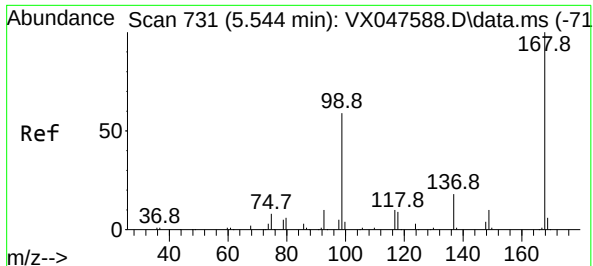


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.538 min Scan# 713
Delta R.T. -0.006 min
Lab File: VX047870.D
Acq: 29 Sep 2025 09:48

Instrument :
MSVOA_X
ClientSampleId :
VX0929WBL01



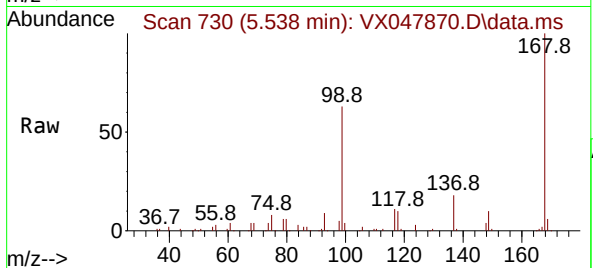



Tgt Ion:168 Resp: 151039
Ion Ratio Lower Upper
168 100
99 62.8 48.8 73.2

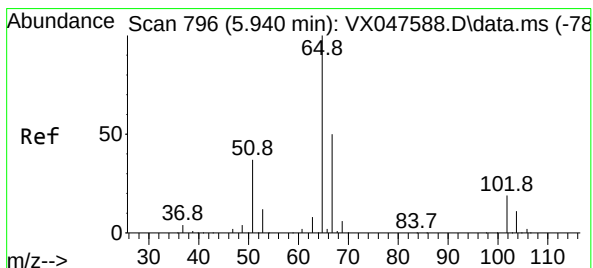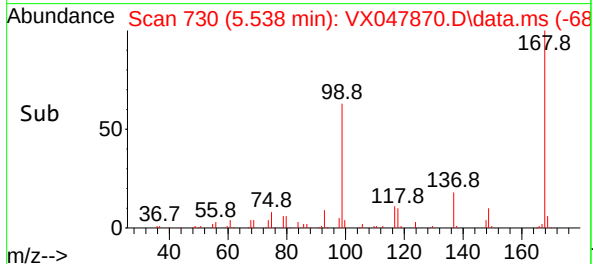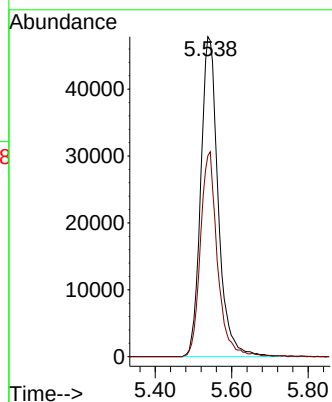

#33
1,2-Dichloroethane-d4
Concen: 49.296 ug/l
RT: 5.946 min Scan# 797
Delta R.T. 0.006 min
Lab File: VX047870.D
Acq: 29 Sep 2025 09:48

Tgt Ion: 65 Resp: 118516
Ion Ratio Lower Upper
65 100
67 50.8 0.0 103.0


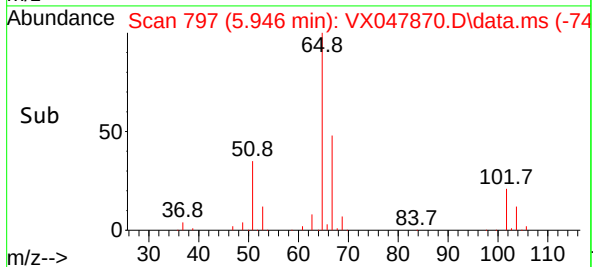
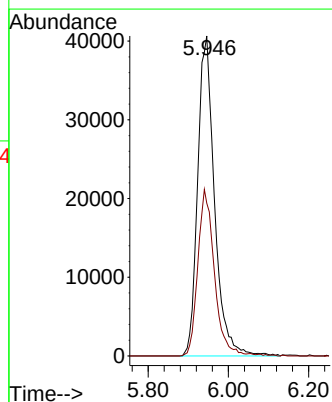
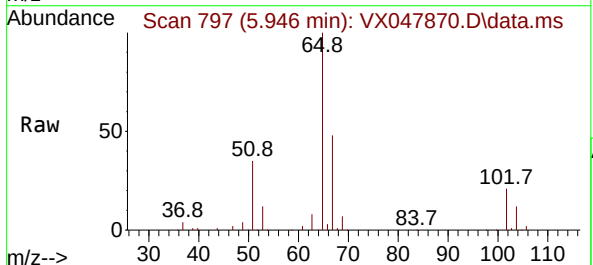


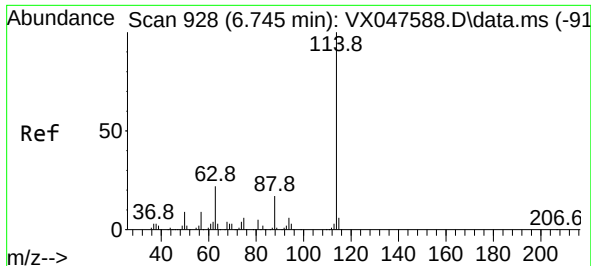

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.745 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX047870.D
Acq: 29 Sep 2025 09:48




Instrument :
MSVOA_X
ClientSampleId :
VX0929WBL01


Tgt Ion:114 Resp: 304108
Ion Ratio Lower Upper
114 100
63 21.7 0.0 44.0
88 16.4 0.0 34.2

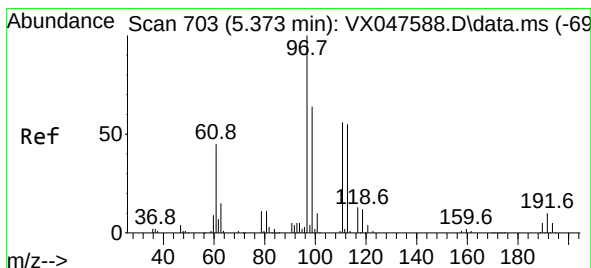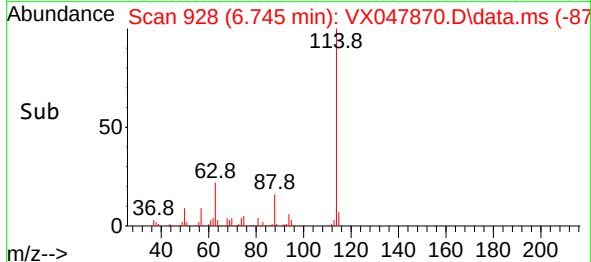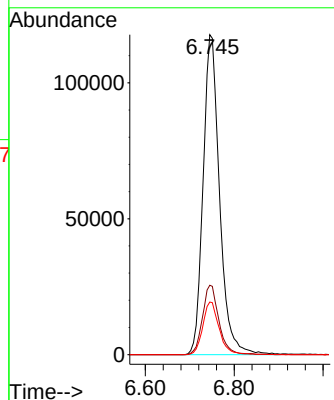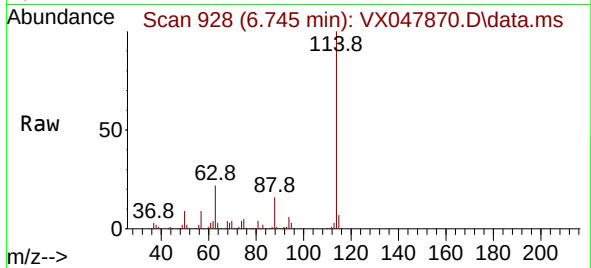

#35
Dibromofluoromethane
Concen: 48.815 ug/l
RT: 5.373 min Scan# 703
Delta R.T. 0.000 min
Lab File: VX047870.D
Acq: 29 Sep 2025 09:48

Tgt Ion:113 Resp: 99558
Ion Ratio Lower Upper
113 100
111 103.8 80.9 121.3
192 18.4 14.2 21.4


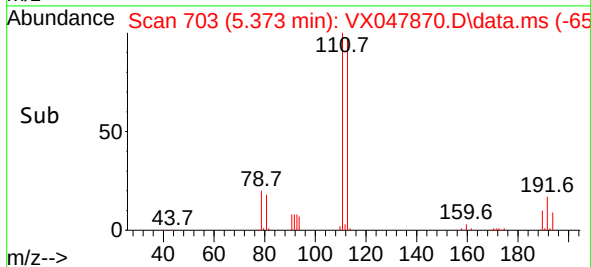
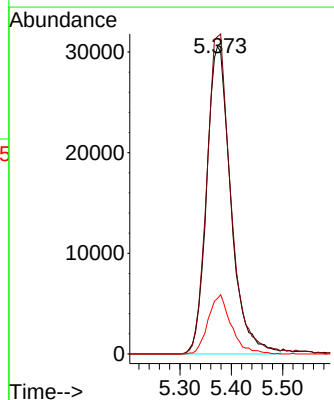
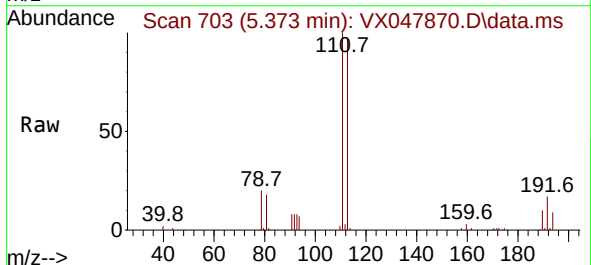


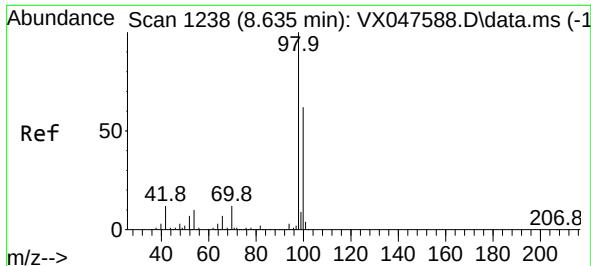

#50
Toluene-d8
Concen: 48.483 ug/l
RT: 8.635 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX047870.D
Acq: 29 Sep 2025 09:48




Instrument :
MSVOA_X
ClientSampleId :
VX0929WBL01


Tgt Ion: 98 Resp: 342151
Ion Ratio Lower Upper
98 100
100 66.5 53.0 79.4

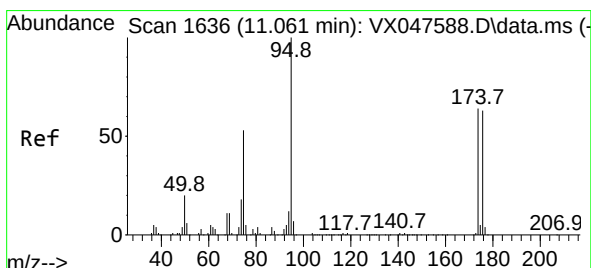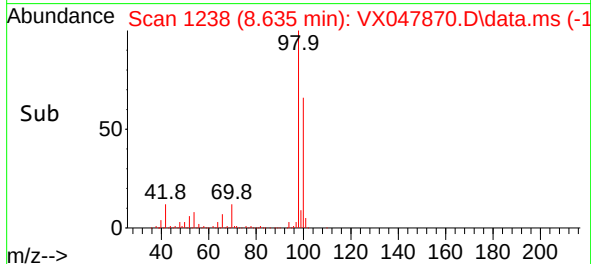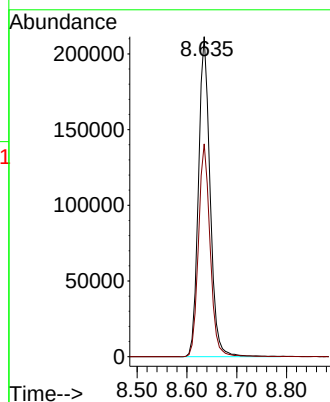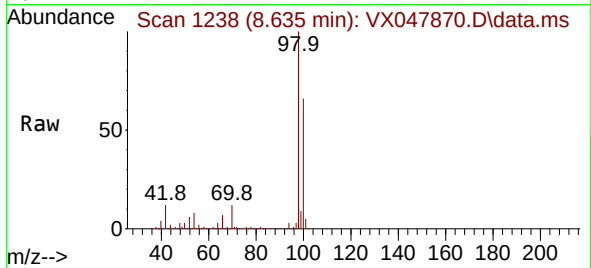

#62
4-Bromofluorobenzene
Concen: 53.118 ug/l
RT: 11.067 min Scan# 1637
Delta R.T. 0.006 min
Lab File: VX047870.D
Acq: 29 Sep 2025 09:48

Tgt Ion: 95 Resp: 142267
Ion Ratio Lower Upper
95 100
174 72.5 0.0 141.6
176 69.8 0.0 138.4

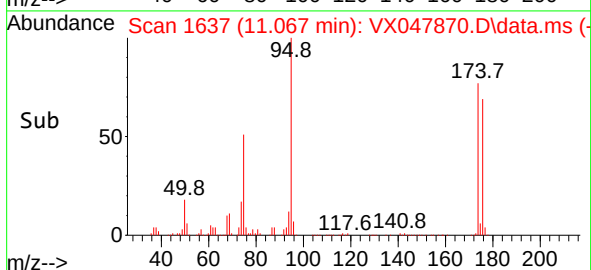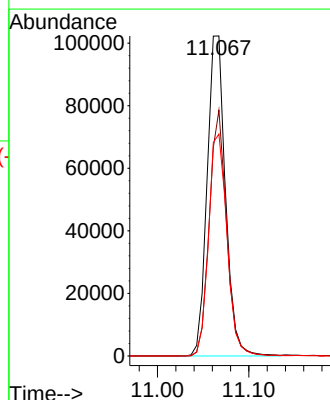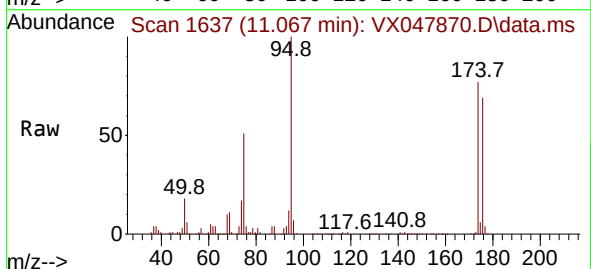

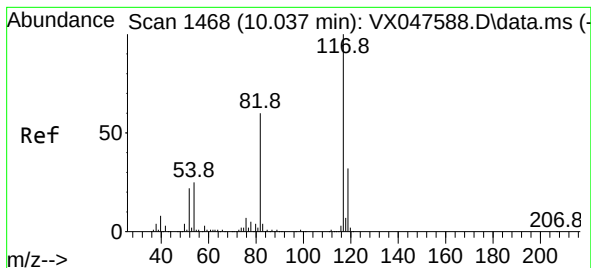

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.037 min Scan# 1468

Delta R.T. 0.000 min

Lab File: VX047870.D

Acq: 29 Sep 2025 09:48

Instrument :

MSVOA_X

ClientSampleId :

VX0929WBL01





Tgt Ion:117 Resp: 305847

Ion Ratio Lower Upper

117 100

82 57.6 47.8 71.6

119 32.2 25.2 37.8

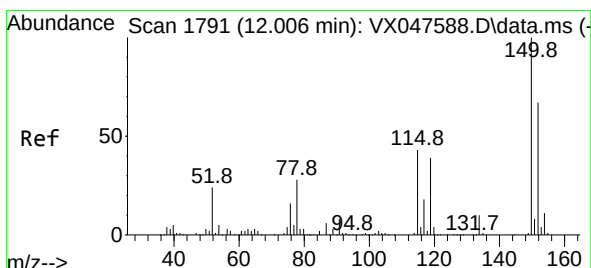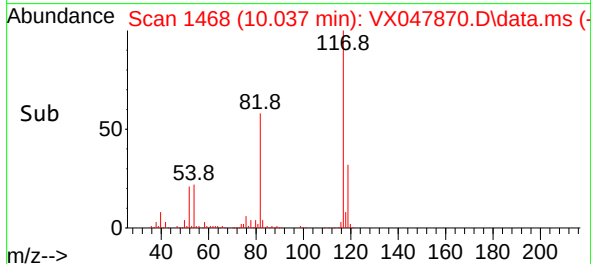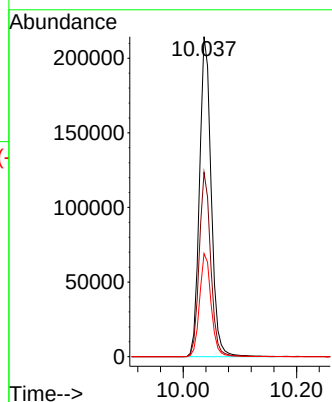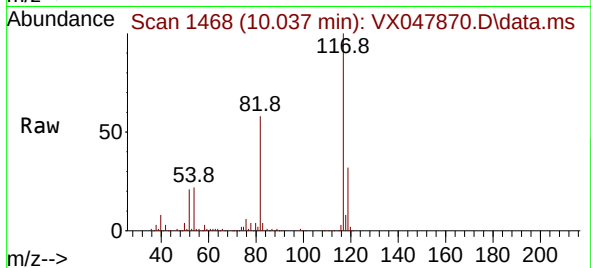

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.006 min Scan# 1791

Delta R.T. 0.000 min

Lab File: VX047870.D

Acq: 29 Sep 2025 09:48

Tgt Ion:152 Resp: 151711

Ion Ratio Lower Upper

152 100

115 61.5 44.9 134.5

150 154.9 0.0 352.0

