


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092925\
Data File : BF143819.D
Acq On : 29 Sep 2025 10:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF092325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 24 05:00:00 2025

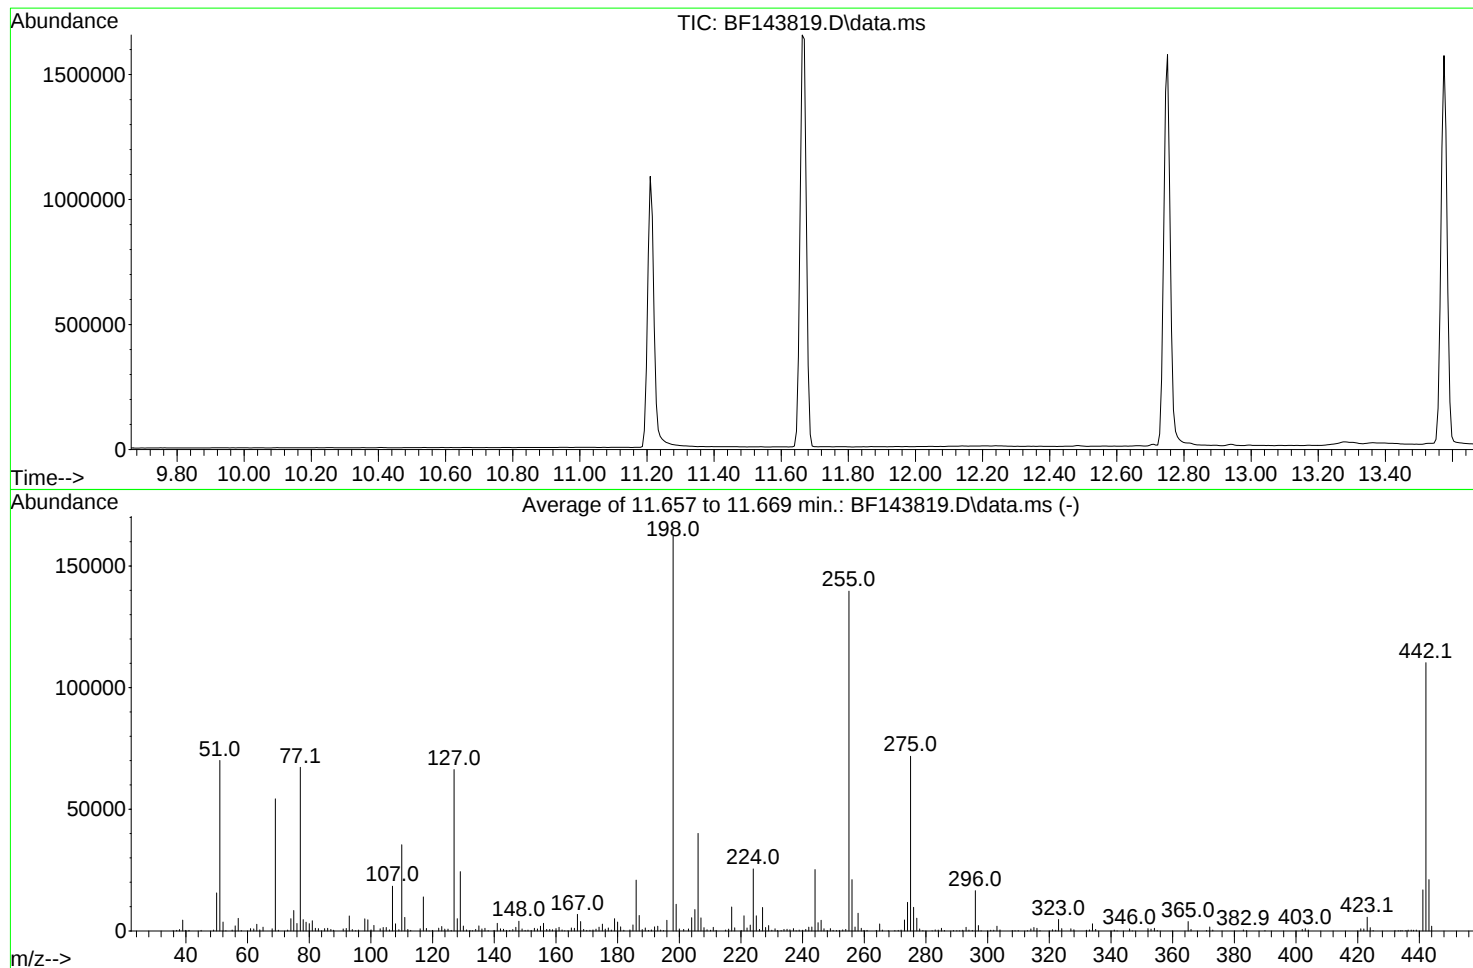




AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1603

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	883	PASS
69	69	100	100	100.0	54331	PASS
70	69	0.00	2	0.5	287	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	162325	PASS
199	198	5	9	6.7	10944	PASS
365	198	1	100	2.4	3827	PASS
441	443	0.01	150	80.1	16905	PASS
442	442	100	100	100.0	110304	PASS
443	442	15	24	19.1	21109	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092925\
Data File : BF143819.D
Acq On : 29 Sep 2025 10:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 29 11:22:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF092325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 24 05:00:00 2025
Response via : Initial Calibration

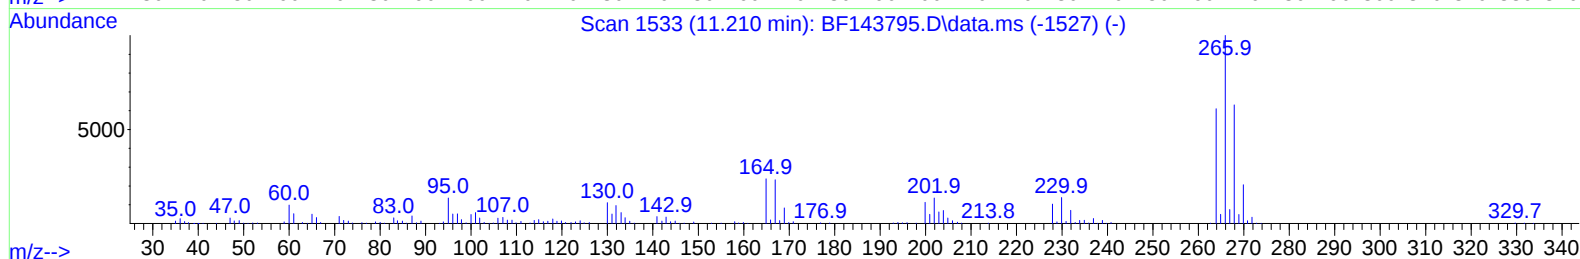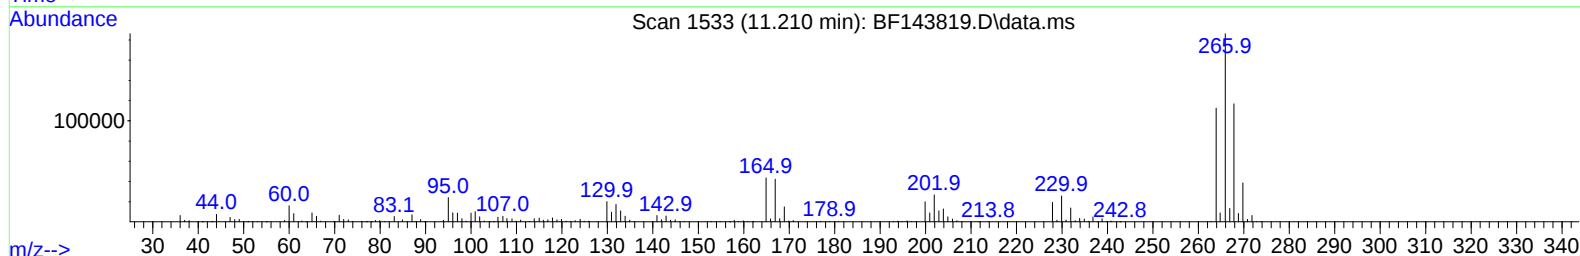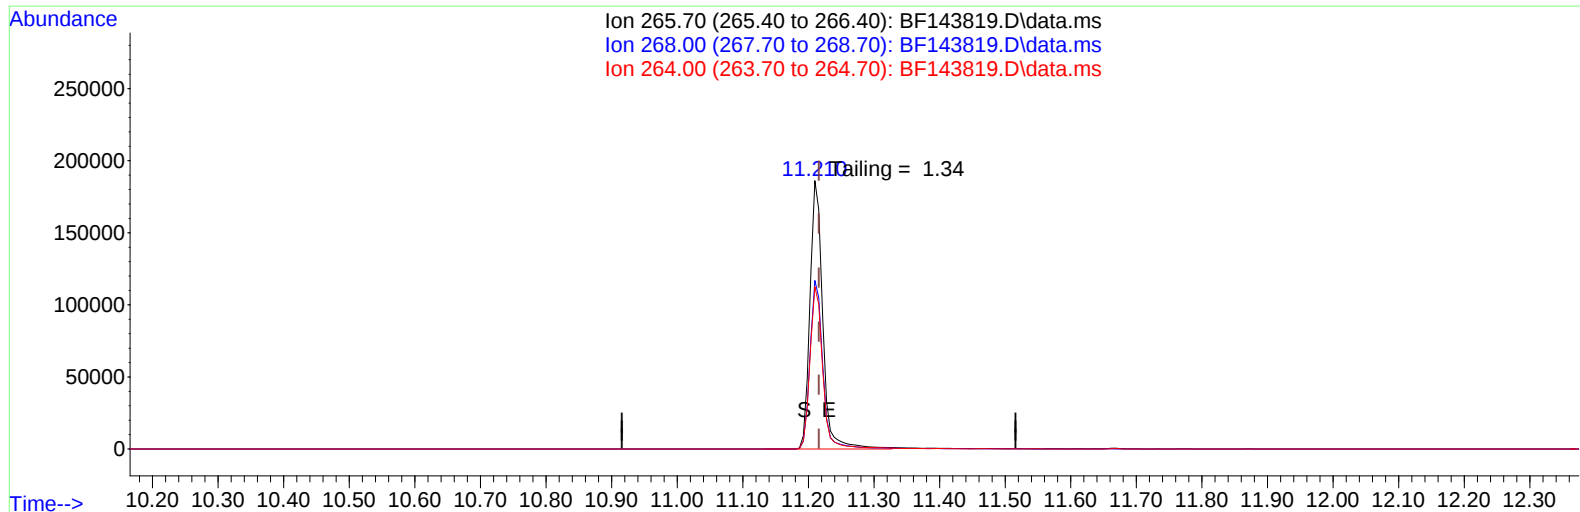

TIC: BF143819.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.006) 28093.51 ng




response 254856

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.78
264.00	61.00	60.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092925\
Data File : BF143819.D
Acq On : 29 Sep 2025 10:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 29 11:22:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF092325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 24 05:00:00 2025
Response via : Initial Calibration

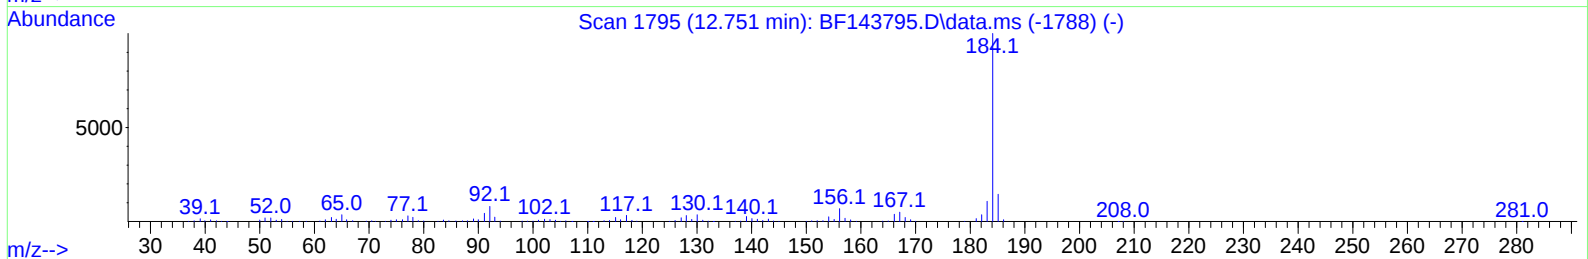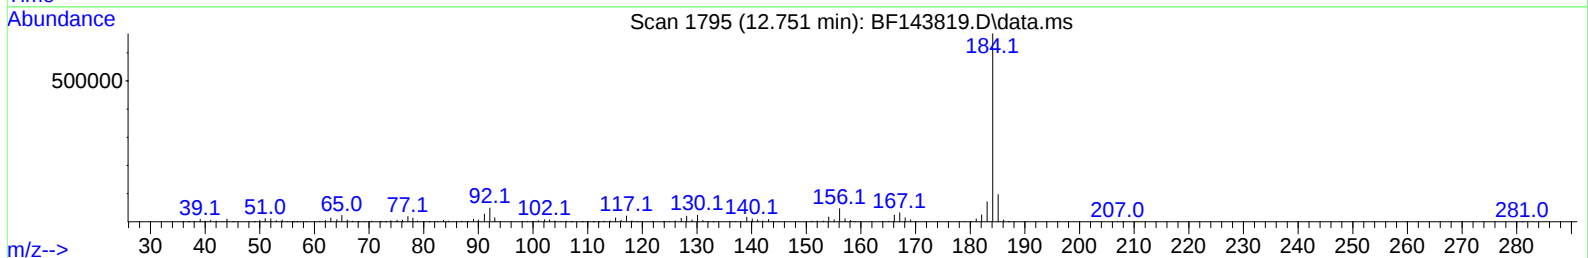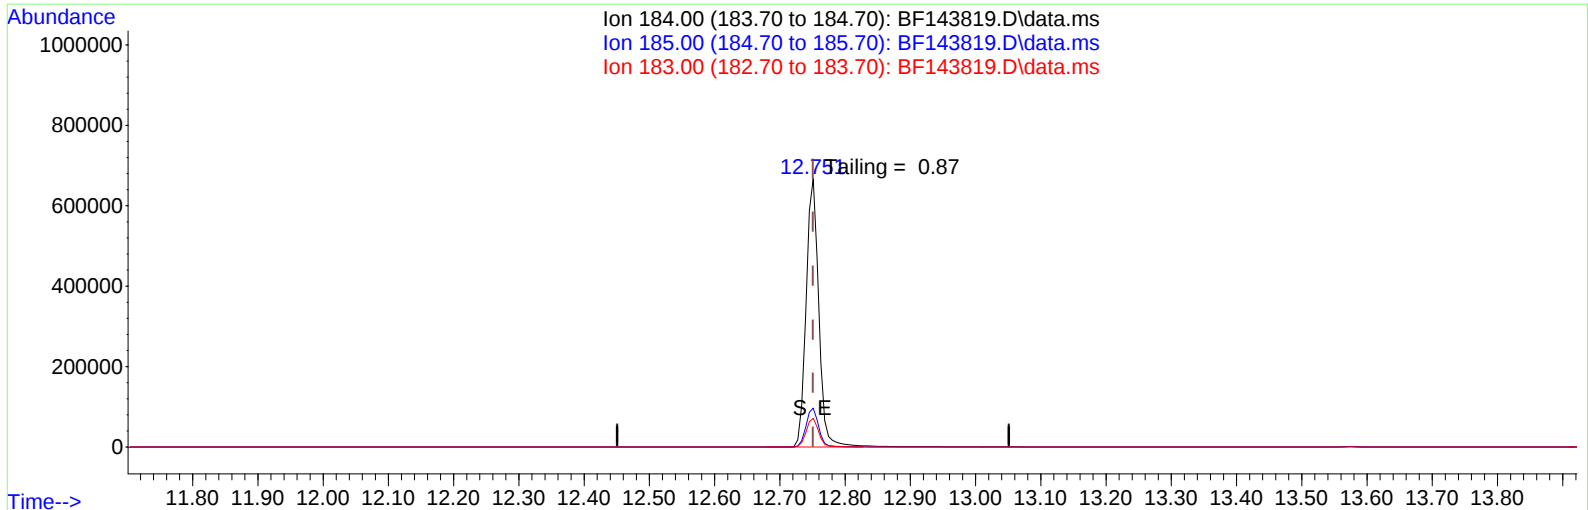

TIC: BF143819.D\data.ms

(77) Benzidine

12.751min (+ 0.000) 0.00 ng

response 903640

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.52
183.00	10.80	10.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/29/2025	BNA_F	<u>BF143819.D</u>
Compound Name	Response	Retention Time
DDT	376595	13.574
DDD	3571	13.274
DDE	1951	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5522	382117	1.45

Instrument :
BNA_F
ClientSampleId :
DFTPP