
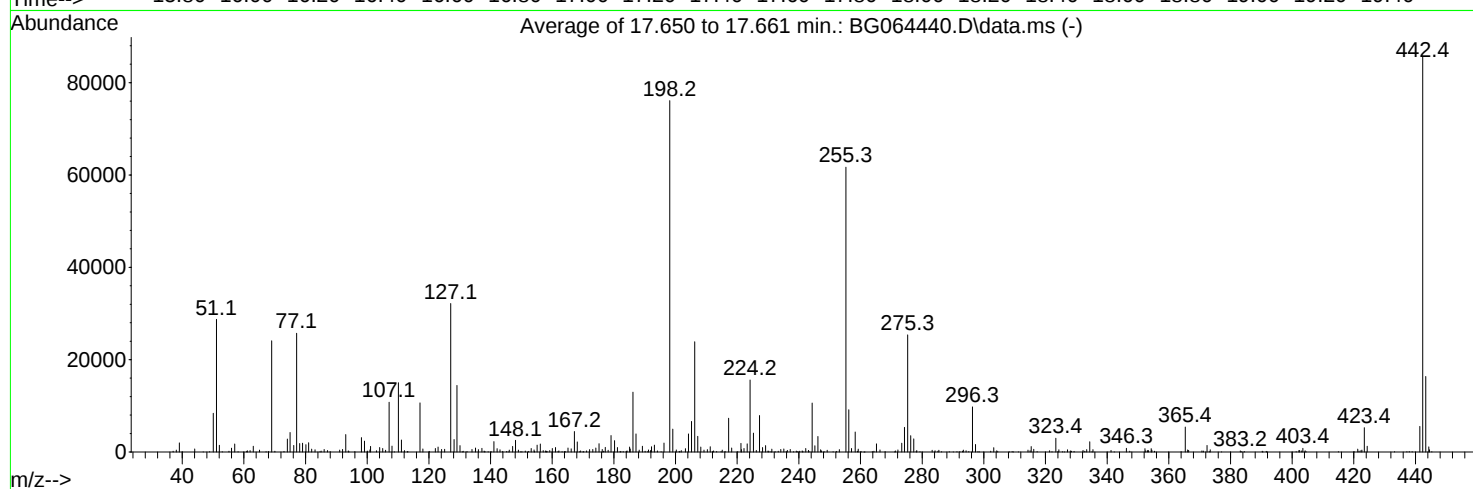


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092525\
Data File : BG064440.D
Acq On : 25 Sep 2025 11:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG092525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Sep 29 18:04:12 2025

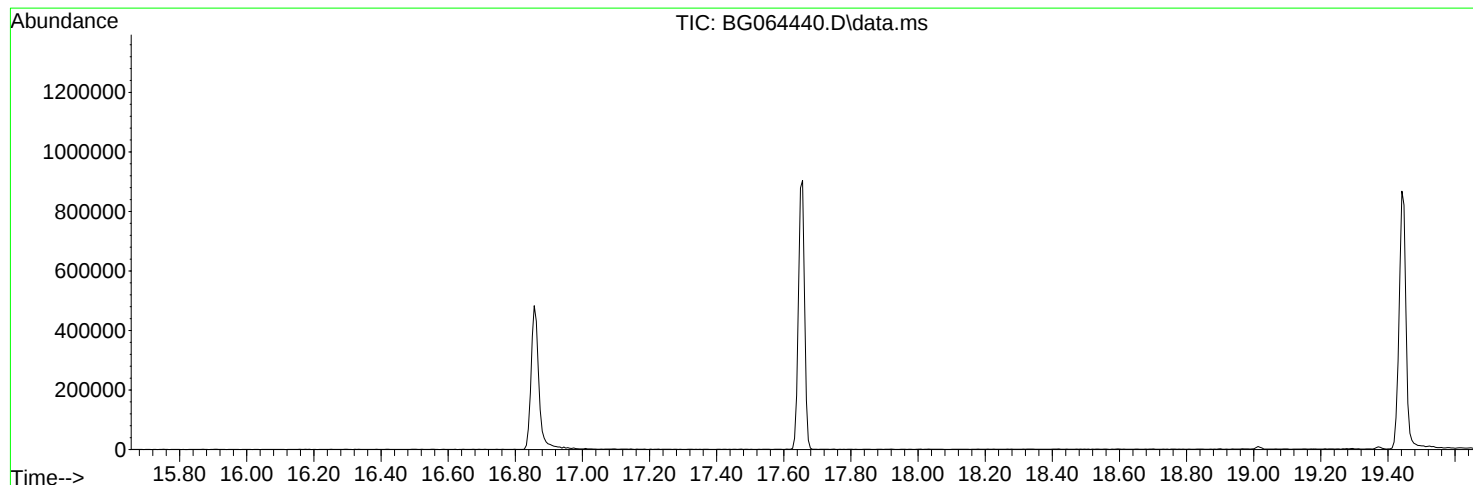




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	0.4	96	PASS
69	69	100	100	100.0	24100	PASS
70	69	0.00	2	0.8	182	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	76131	PASS
199	198	5	9	6.5	4946	PASS
365	198	1	100	7.1	5416	PASS
441	443	0.01	150	34.0	5552	PASS
442	442	100	100	100.0	85525	PASS
443	442	15	24	19.1	16349	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092525\
Data File : BG064440.D
Acq On : 25 Sep 2025 11:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 25 18:46:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG092525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 25 17:35:42 2025
Response via : Initial Calibration

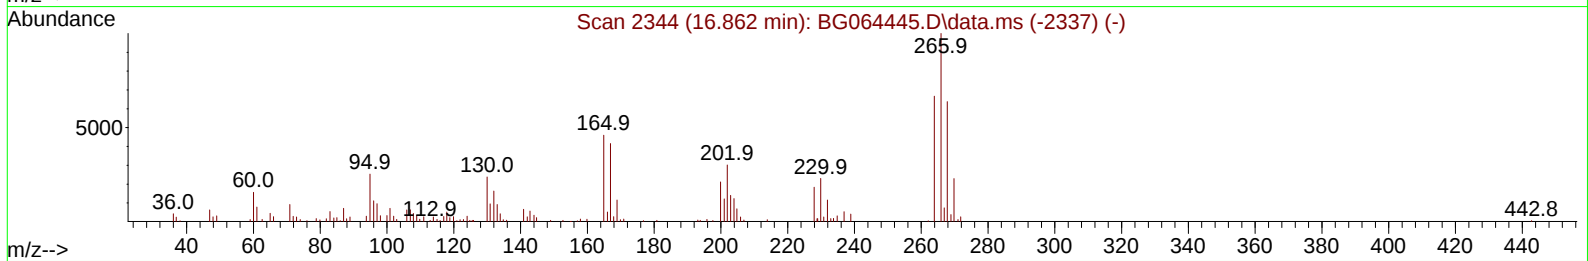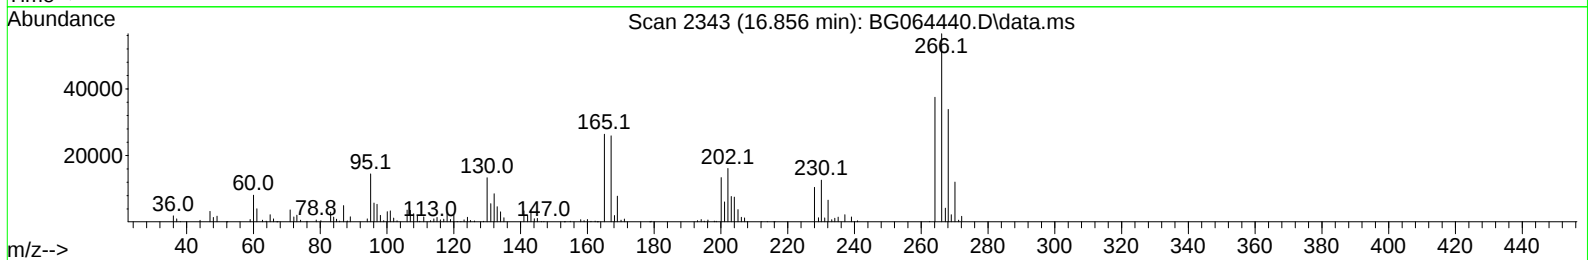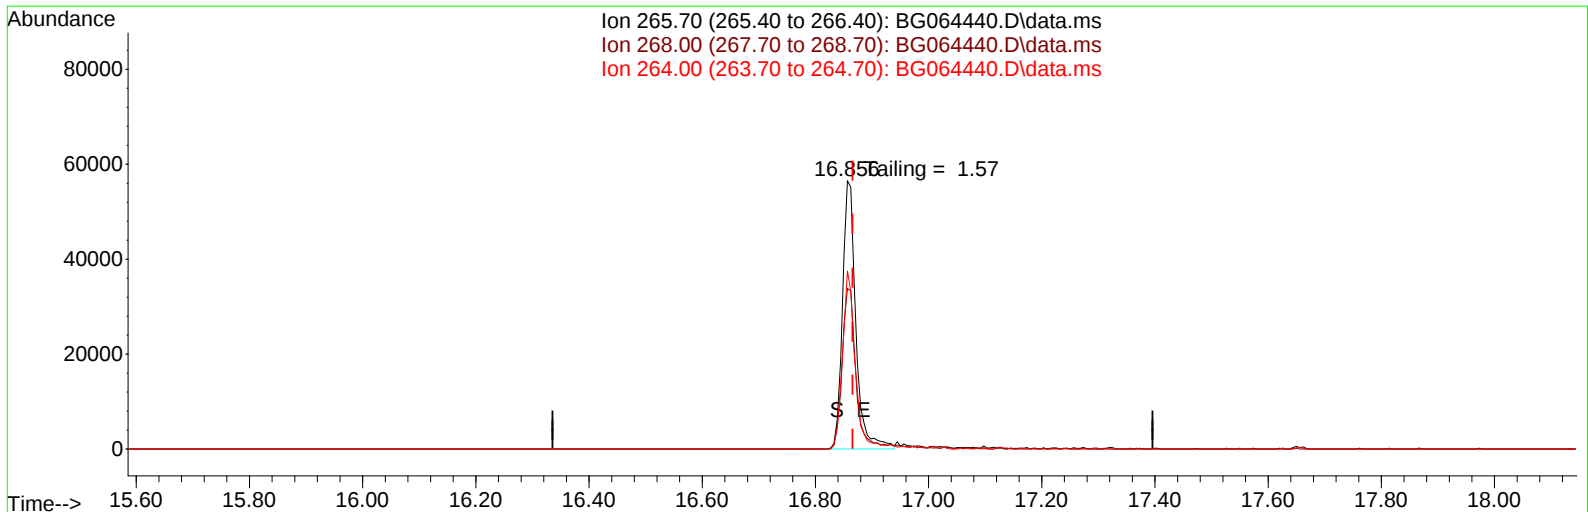

TIC: BG064440.D\data.ms

(70) Pentachlorophenol (C)

16.856min (-0.009) 185440.68 ng




response 92957

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	59.83
264.00	66.70	66.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092525\
Data File : BG064440.D
Acq On : 25 Sep 2025 11:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 25 18:46:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG092525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 25 17:35:42 2025
Response via : Initial Calibration

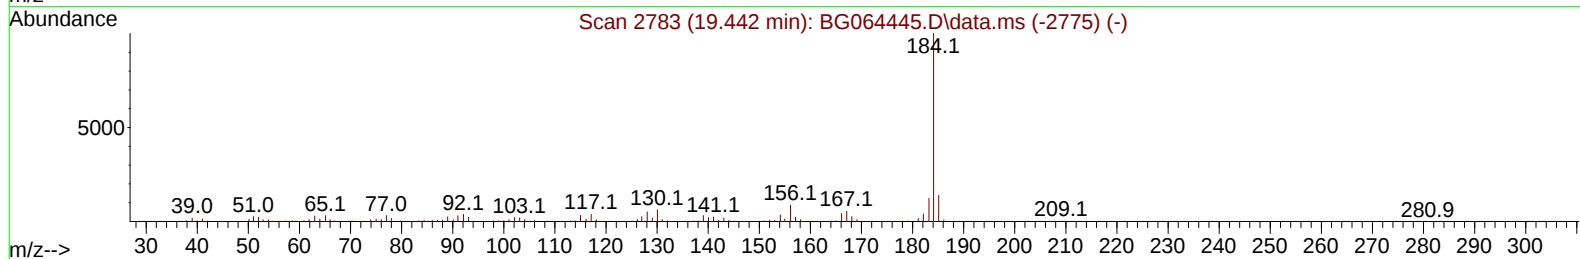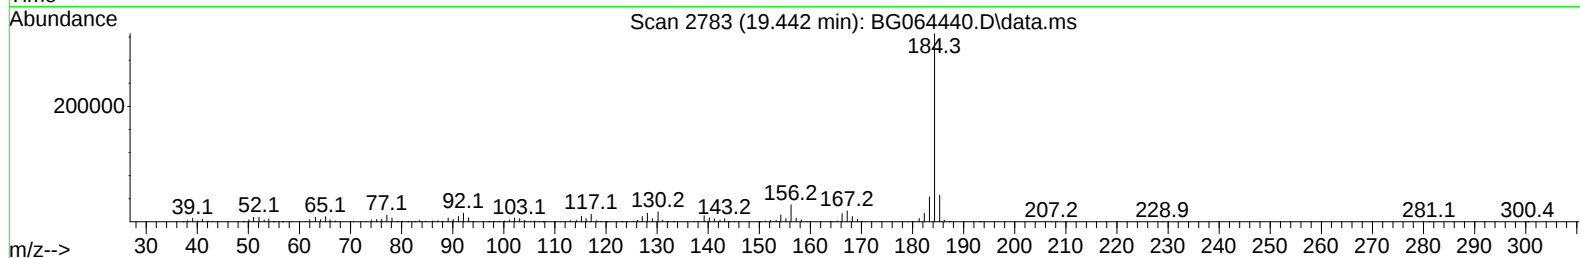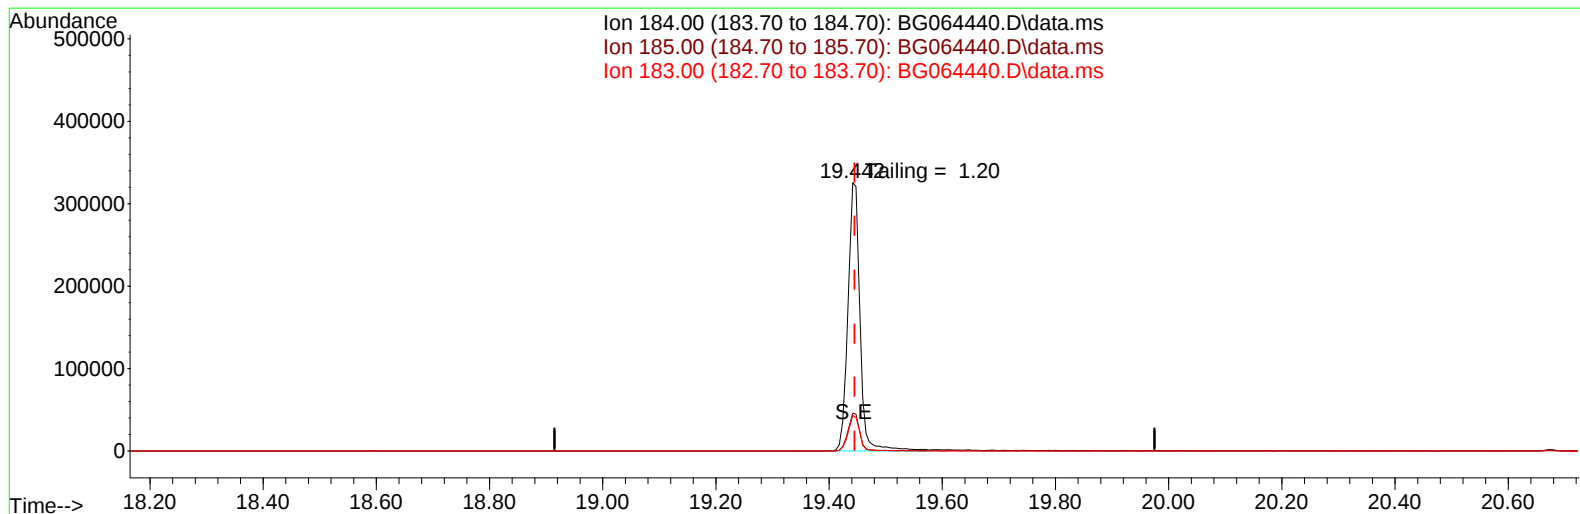

TIC: BG064440.D\data.ms

(77) Benzidine

19.442min (-0.003) 322131.38 ng

response 481159

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.07
183.00	12.30	13.25
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/25/2025	BNA_G	<u>BG064440.D</u>
Compound Name	Response	Retention Time
DDT	305253	20.676
DDD	3808	20.241
DDE	194	19.724
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4002	309255	1.29

Instrument :
BNA_G
ClientSampleId :
DFTPP