


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092925\
Data File : BG064455.D
Acq On : 29 Sep 2025 11:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG092525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Sep 29 18:04:12 2025

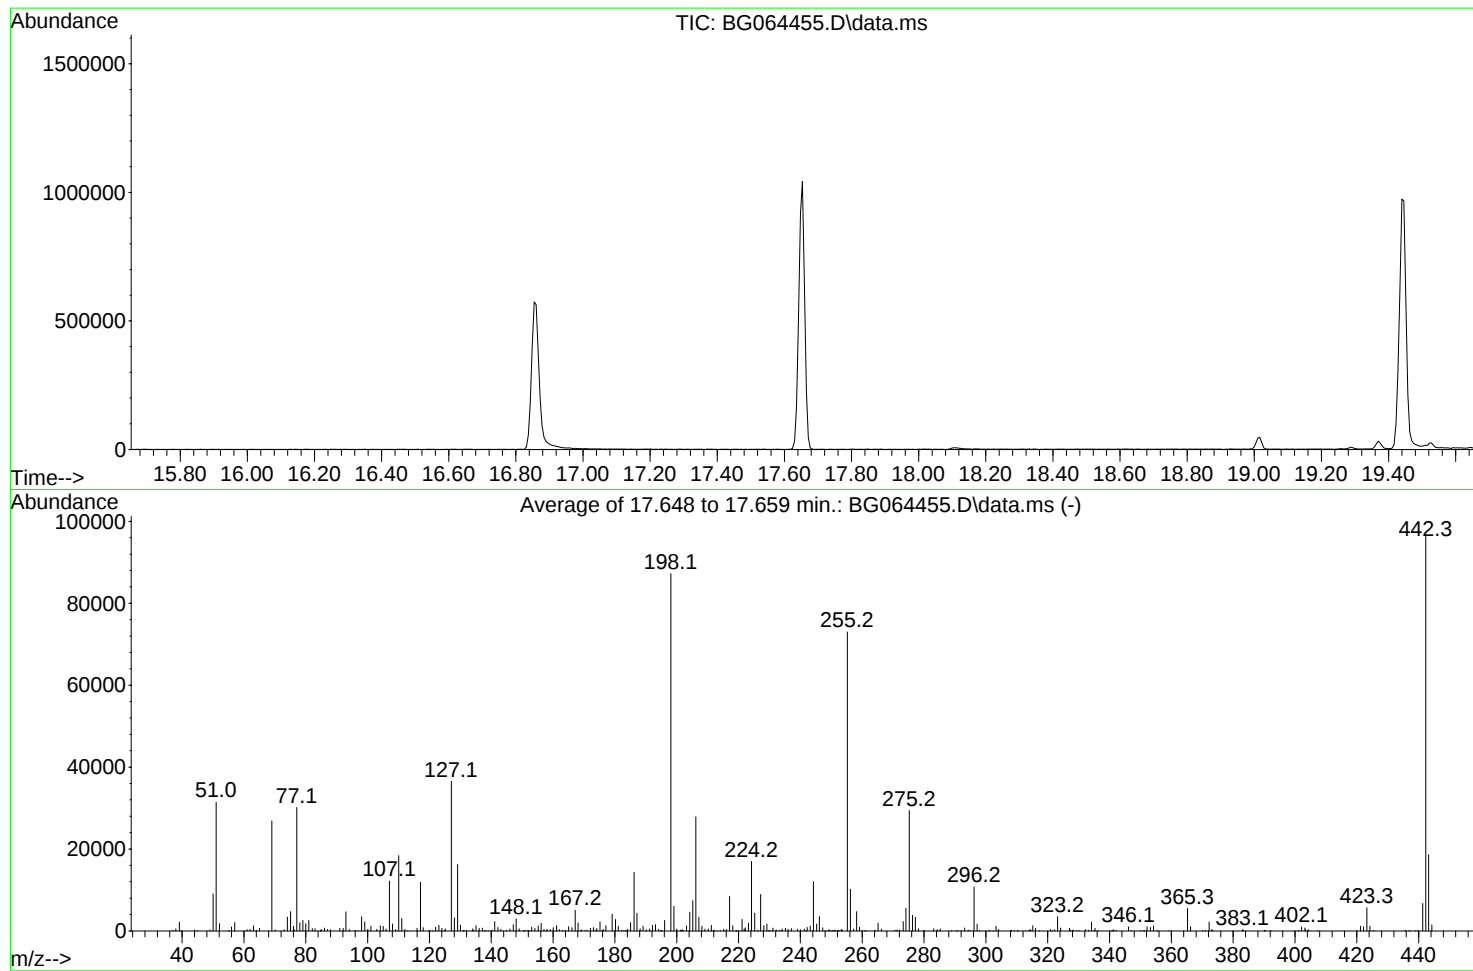




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	26872	PASS
70	69	0.00	2	0.9	246	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	87269	PASS
199	198	5	9	6.9	5996	PASS
365	198	1	100	6.3	5510	PASS
441	443	0.01	150	36.0	6691	PASS
442	442	100	100	100.0	96408	PASS
443	442	15	24	19.3	18588	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092925\
Data File : BG064455.D
Acq On : 29 Sep 2025 11:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 29 19:15:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG092525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 18:04:12 2025
Response via : Initial Calibration

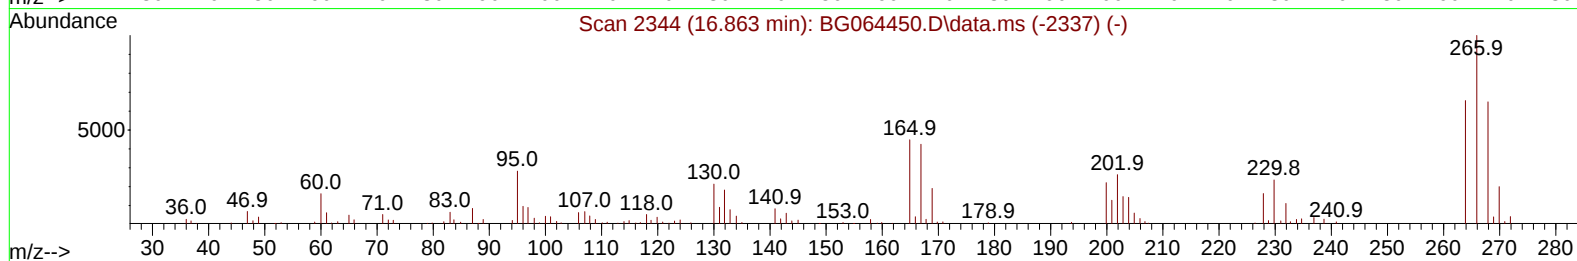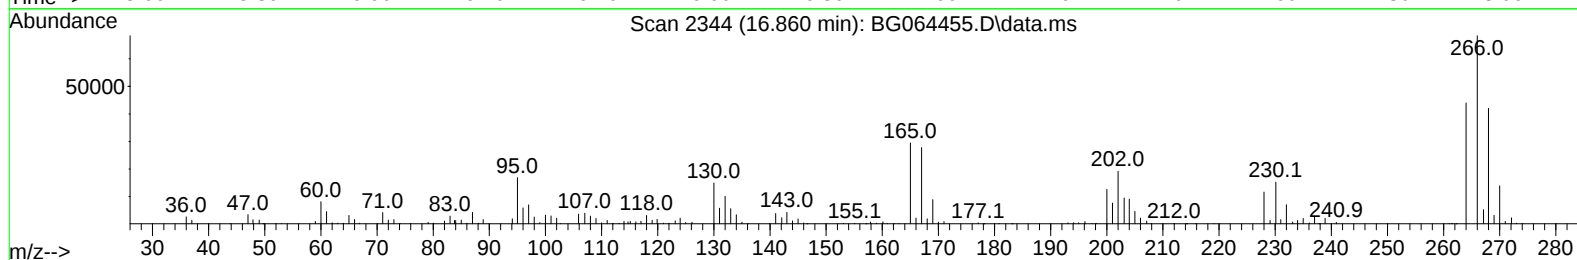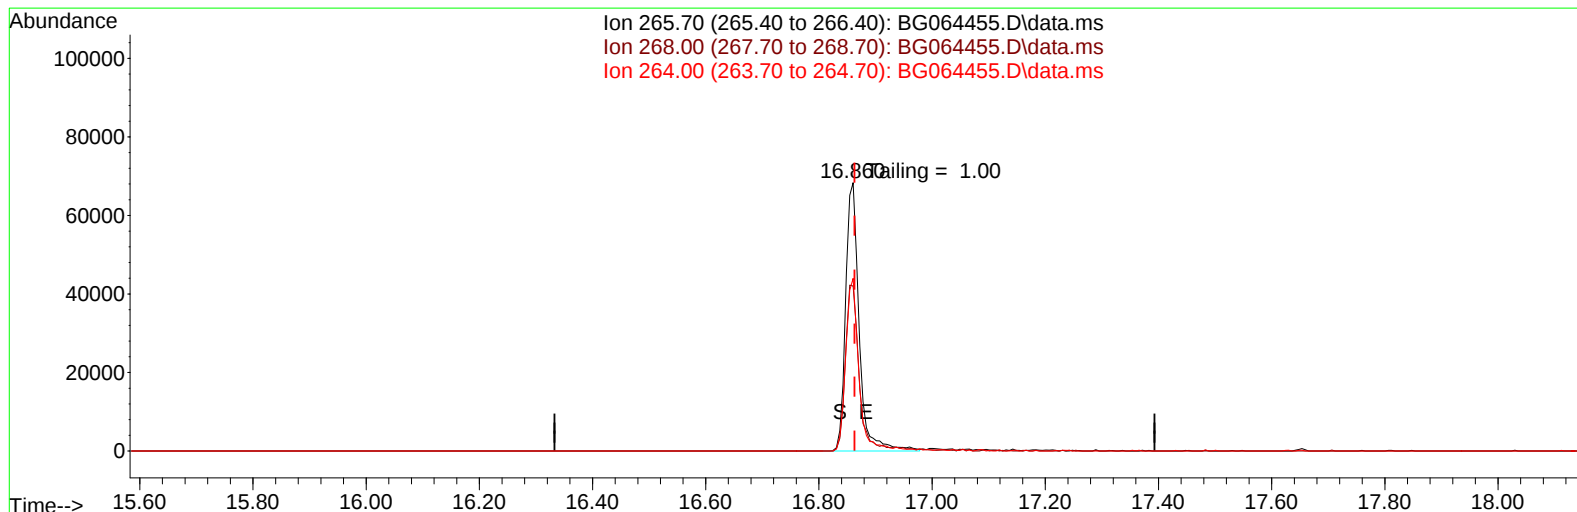

TIC: BG064455.D\data.ms

(70) Pentachlorophenol (C)

16.860min (-0.002) 151423.59 ng




response 113326

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	61.46
264.00	65.50	64.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092925\
Data File : BG064455.D
Acq On : 29 Sep 2025 11:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 29 19:15:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG092525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 18:04:12 2025
Response via : Initial Calibration

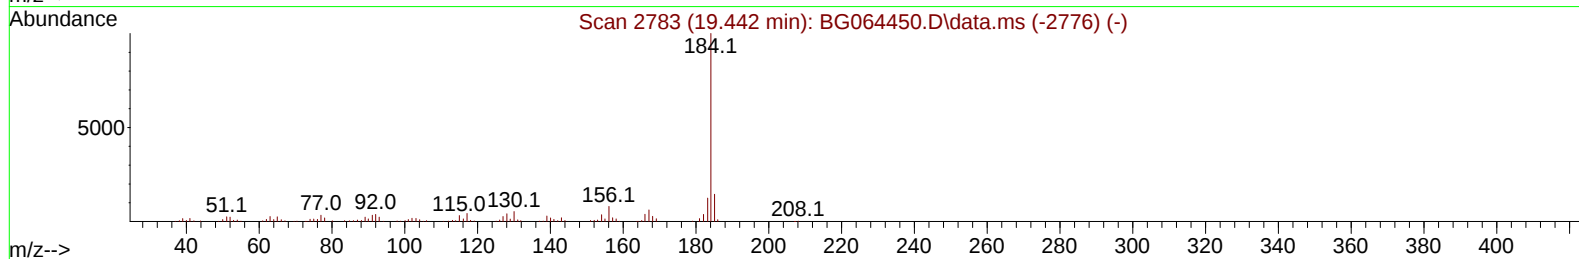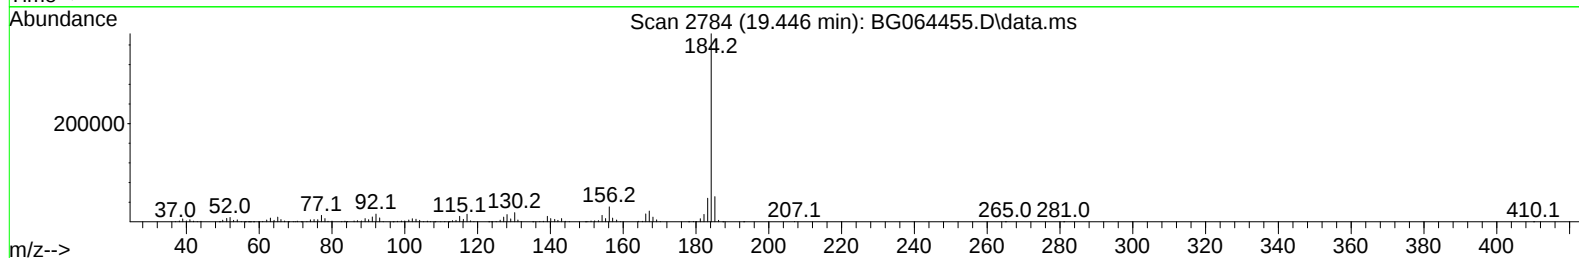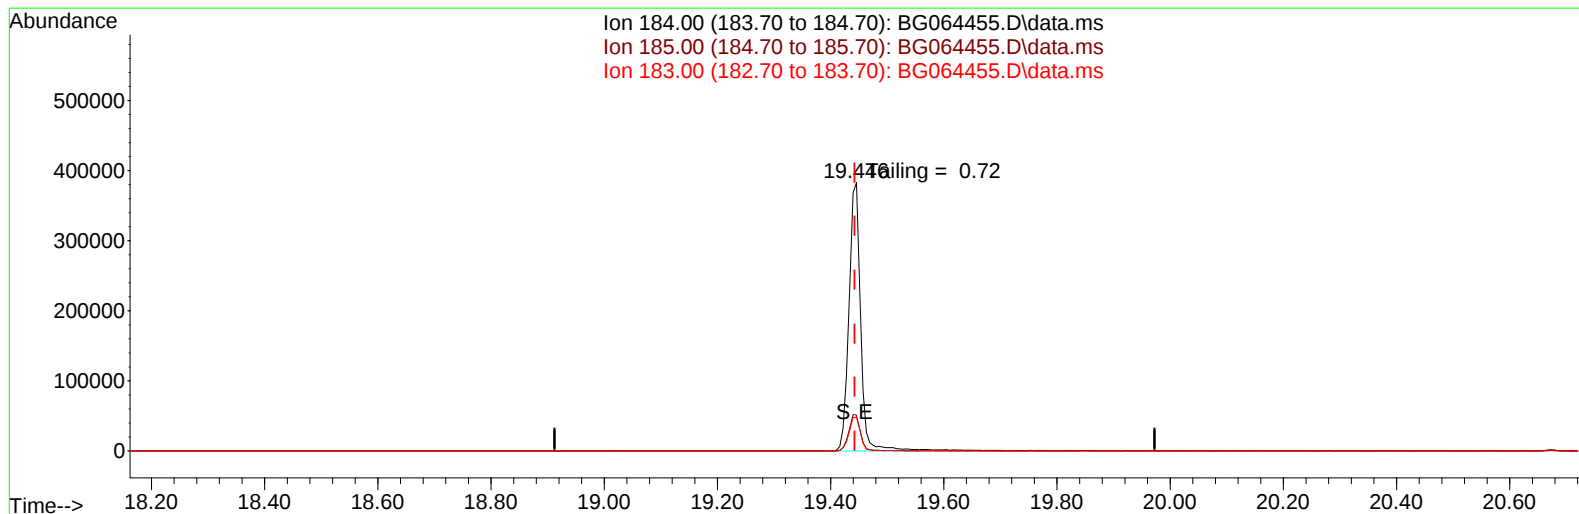

TIC: BG064455.D\data.ms

(77) Benzidine

19.446min (+ 0.003) 35719.25 ng

response 544294

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.37
183.00	12.50	12.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/29/2025	BNA_G	<u>BG064440.D</u>
Compound Name	Response	Retention Time
DDT	364482	20.674
DDD	4920	20.233
DDE	334	19.728
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5254	369736	1.42

Instrument :
BNA_G
ClientSampleId :
DFTPP