

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100325\
 Data File : VX047995.D
 Acq On : 03 Oct 2025 15:34
 Operator : JC/MD
 Sample : Q3226-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SAMPLE-MANAGEMENT

Quant Time: Oct 03 23:50:51 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 17 06:39:58 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	127919	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.751	114	256789	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	267564	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	136370	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.940	65	107493	52.792	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	105.580%
35) Dibromofluoromethane	5.379	113	86753	50.374	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	100.740%
50) Toluene-d8	8.635	98	296223	49.710	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	99.420%
62) 4-Bromofluorobenzene	11.067	95	125293	55.401	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	110.800%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100325\
Data File : VX047995.D
Acq On : 03 Oct 2025 15:34
Operator : JC/MD
Sample : Q3226-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAGEMENT

Quant Time: Oct 03 23:50:51 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 17 06:39:58 2025
Response via : Initial Calibration



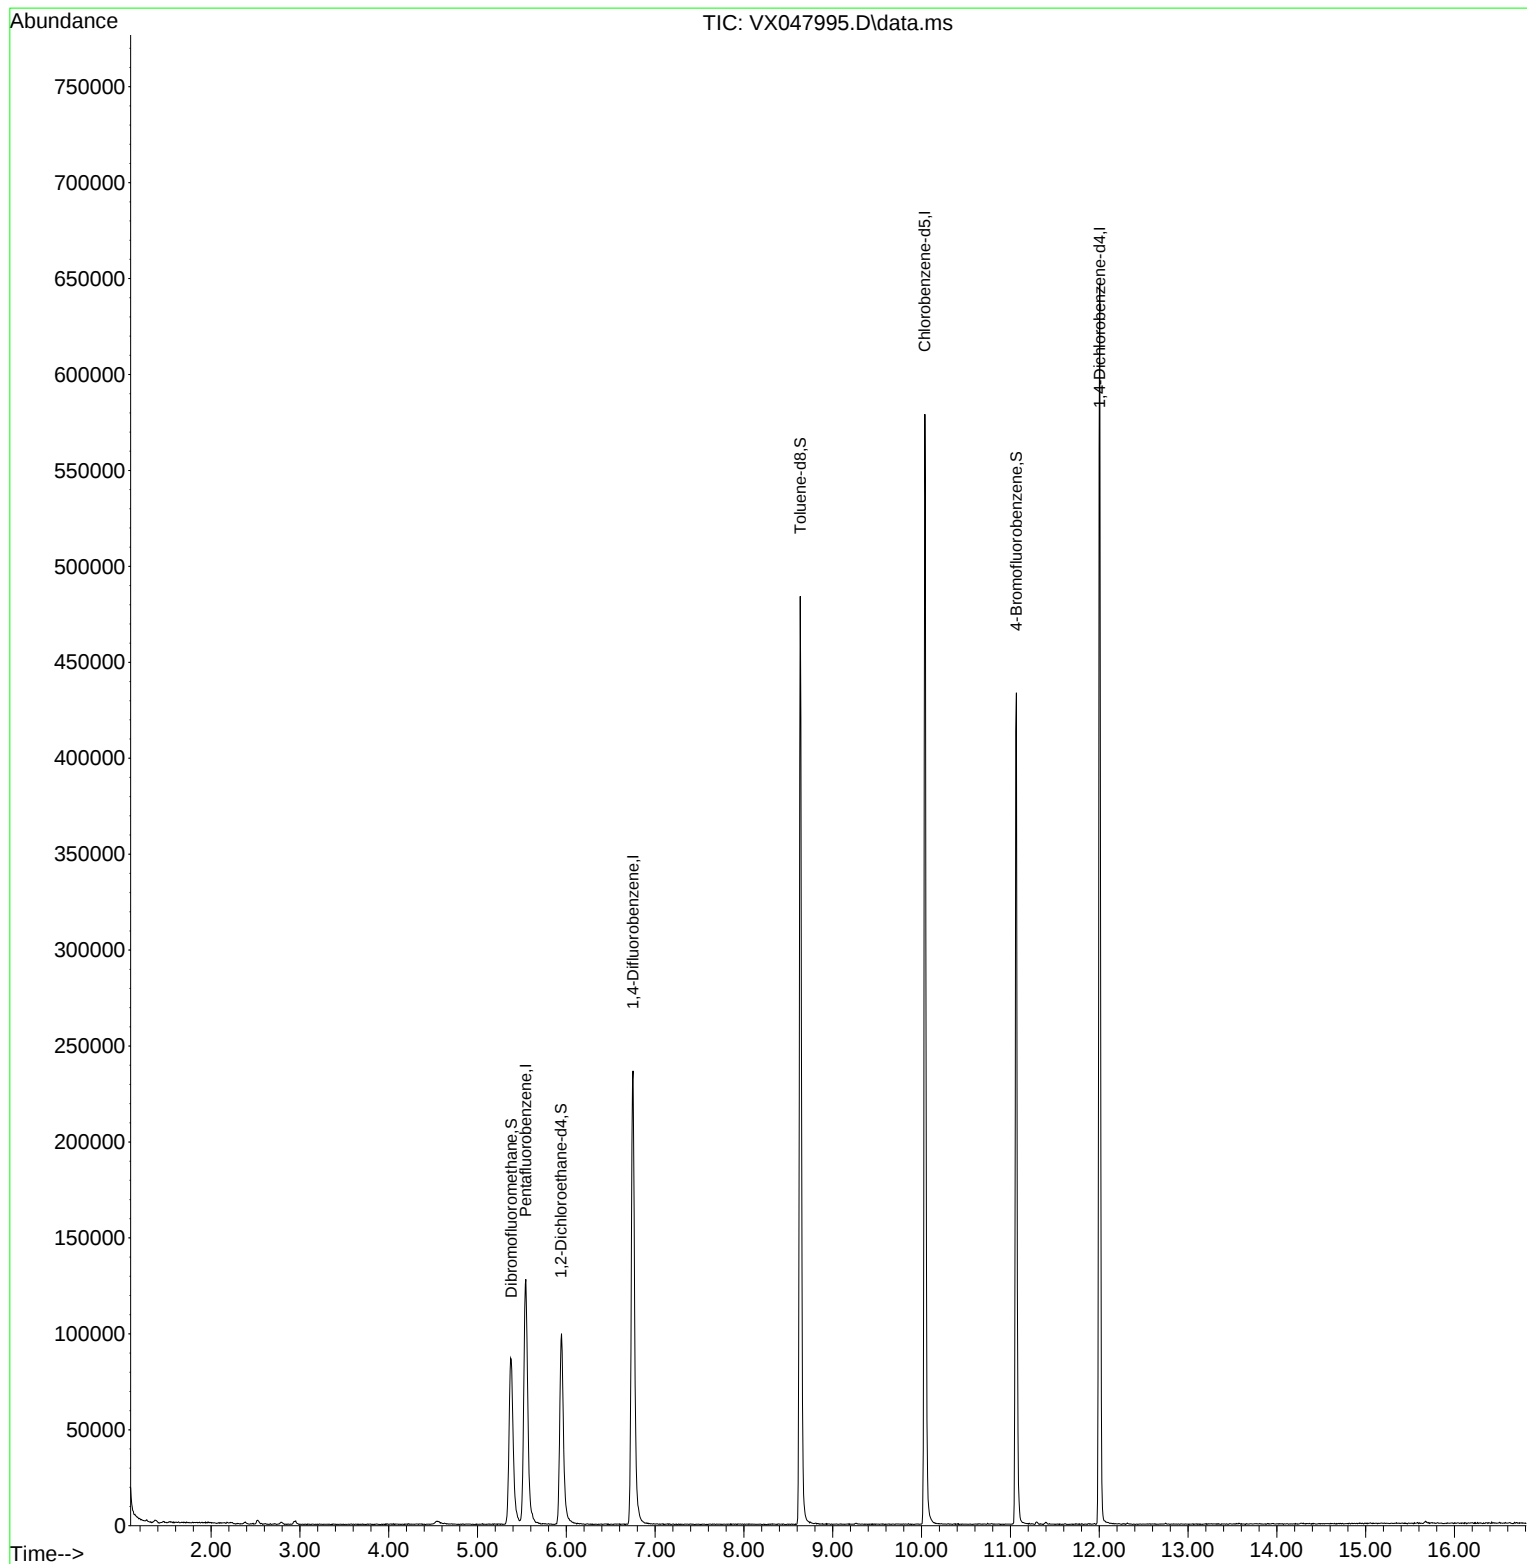




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.000 min
Lab File: VX047995.D
Acq: 03 Oct 2025 15:34




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAGEMENT

Tgt Ion:168 Resp: 127919
Ion Ratio Lower Upper
168 100
99 62.2 48.8 73.2

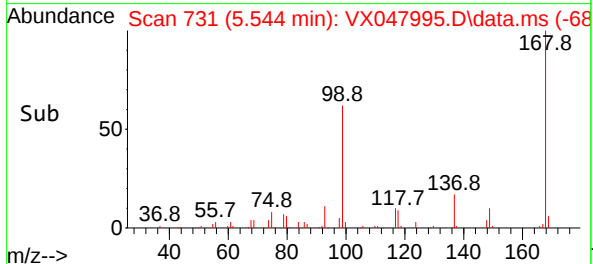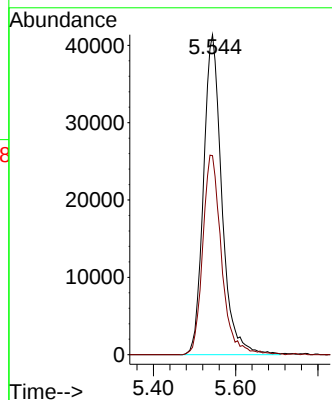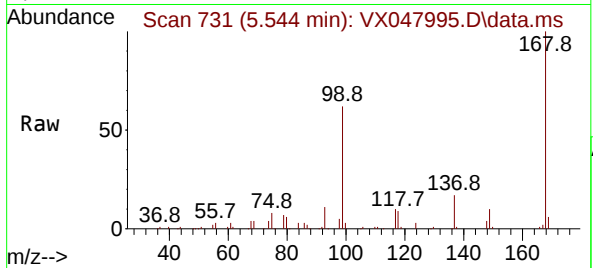

#33
1,2-Dichloroethane-d4
Concen: 52.792 ug/l
RT: 5.940 min Scan# 796
Delta R.T. -0.000 min
Lab File: VX047995.D
Acq: 03 Oct 2025 15:34

Tgt Ion: 65 Resp: 107493
Ion Ratio Lower Upper
65 100
67 52.3 0.0 103.0

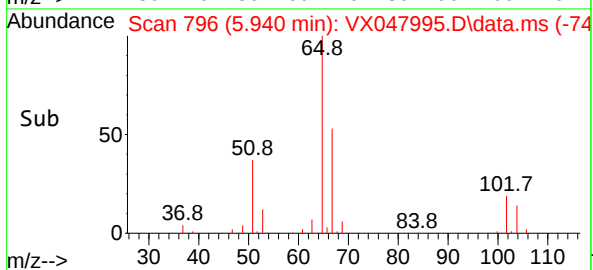
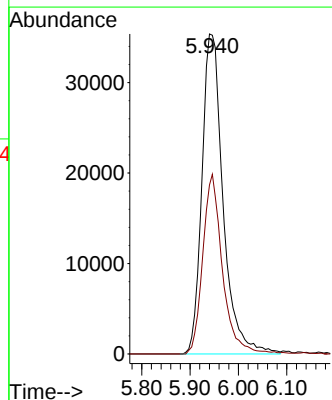
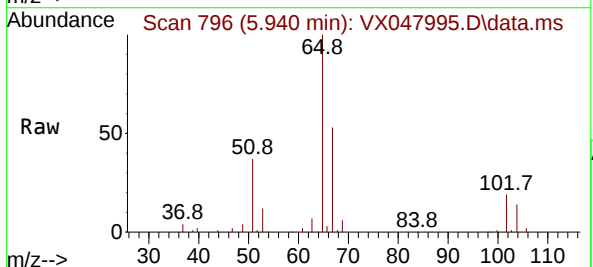




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.751 min Scan# 91
Delta R.T. 0.006 min
Lab File: VX047995.D
Acq: 03 Oct 2025 15:34




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAGEMENT

Tgt Ion:114 Resp: 256789
Ion Ratio Lower Upper
114 100
63 22.1 0.0 44.0
88 16.7 0.0 34.2

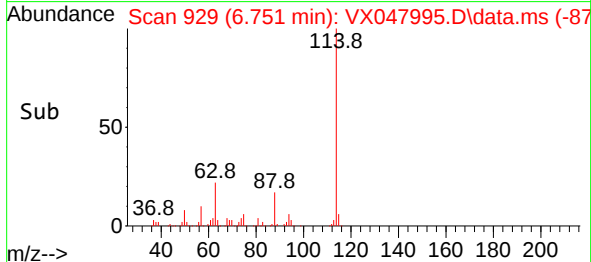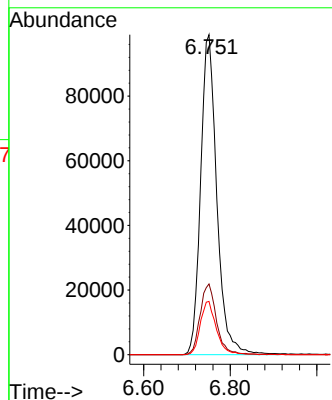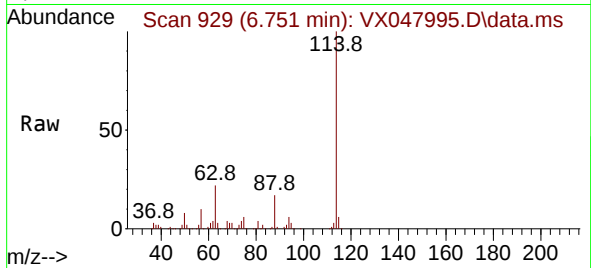

#35
Dibromofluoromethane
Concen: 50.374 ug/l
RT: 5.379 min Scan# 704
Delta R.T. 0.006 min
Lab File: VX047995.D
Acq: 03 Oct 2025 15:34

Tgt Ion:113 Resp: 86753
Ion Ratio Lower Upper
113 100
111 102.0 80.9 121.3
192 17.2 14.2 21.4

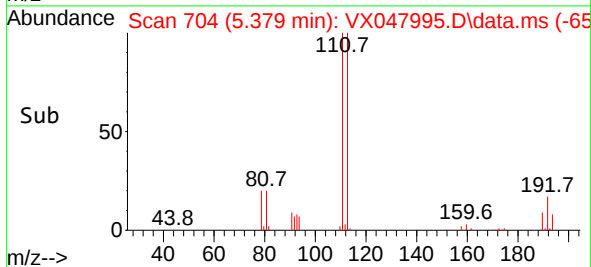
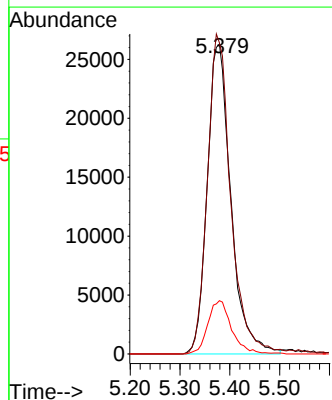
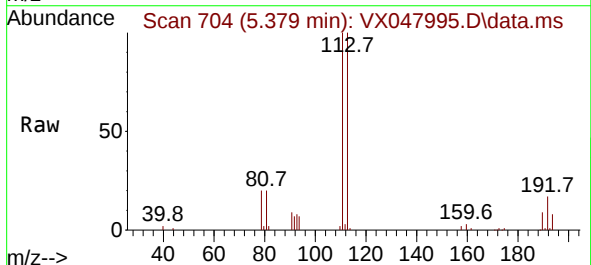




#50
Toluene-d8
Concen: 49.710 ug/l
RT: 8.635 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX047995.D
Acq: 03 Oct 2025 15:34




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAGEMENT

Tgt Ion: 98 Resp: 296223
Ion Ratio Lower Upper
98 100
100 65.9 53.0 79.4

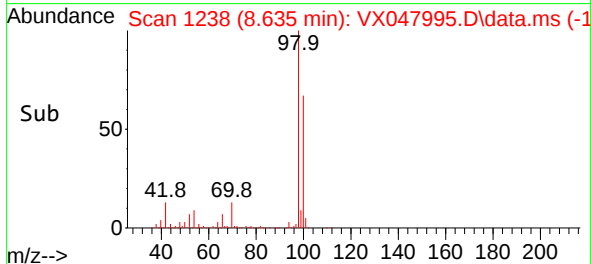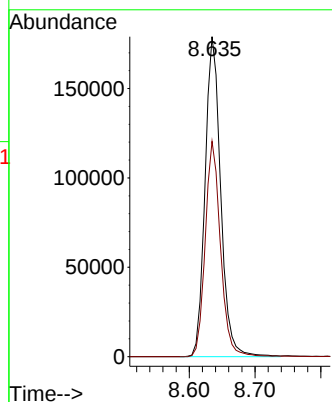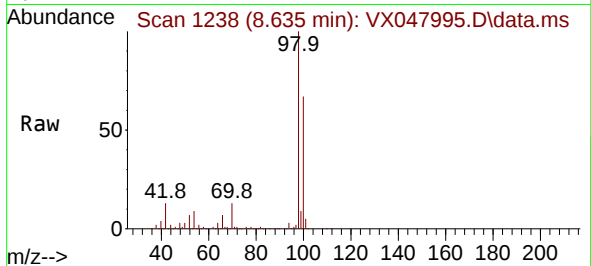

#62
4-Bromofluorobenzene
Concen: 55.401 ug/l
RT: 11.067 min Scan# 1637
Delta R.T. 0.006 min
Lab File: VX047995.D
Acq: 03 Oct 2025 15:34

Tgt Ion: 95 Resp: 125293
Ion Ratio Lower Upper
95 100
174 72.9 0.0 141.6
176 68.3 0.0 138.4


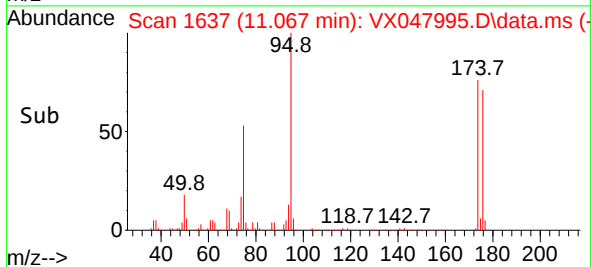
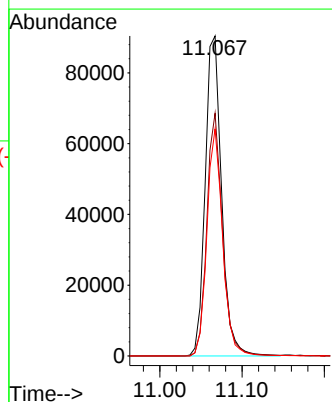
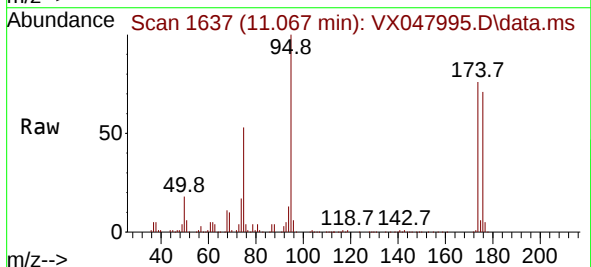




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.037 min Scan# 1468
Delta R.T. -0.000 min
Lab File: VX047995.D
Acq: 03 Oct 2025 15:34

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAGEMENT

Tgt Ion:117 Resp: 267564
Ion Ratio Lower Upper
117 100
82 59.0 47.8 71.6
119 31.2 25.2 37.8

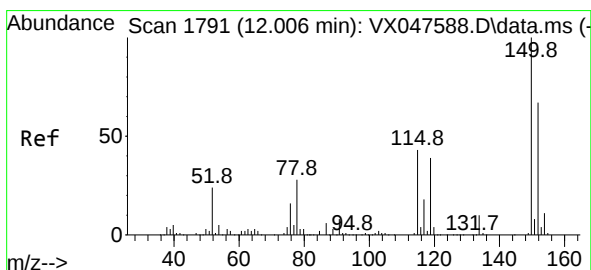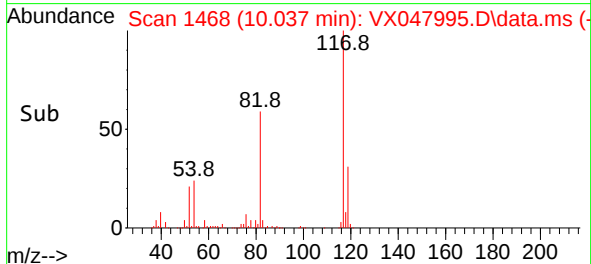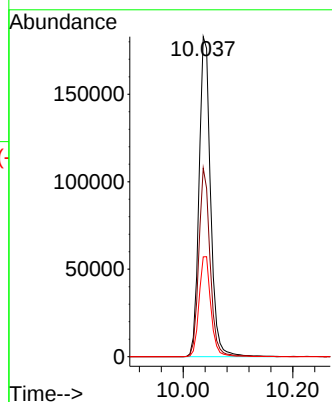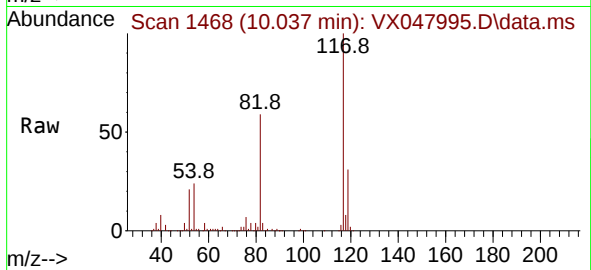

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. -0.000 min
Lab File: VX047995.D
Acq: 03 Oct 2025 15:34

Tgt Ion:152 Resp: 136370
Ion Ratio Lower Upper
152 100
115 61.7 44.9 134.5
150 154.5 0.0 352.0

