


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100625\
Data File : BN038021.D
Acq On : 06 Oct 2025 22:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 24 11:00:01 2025

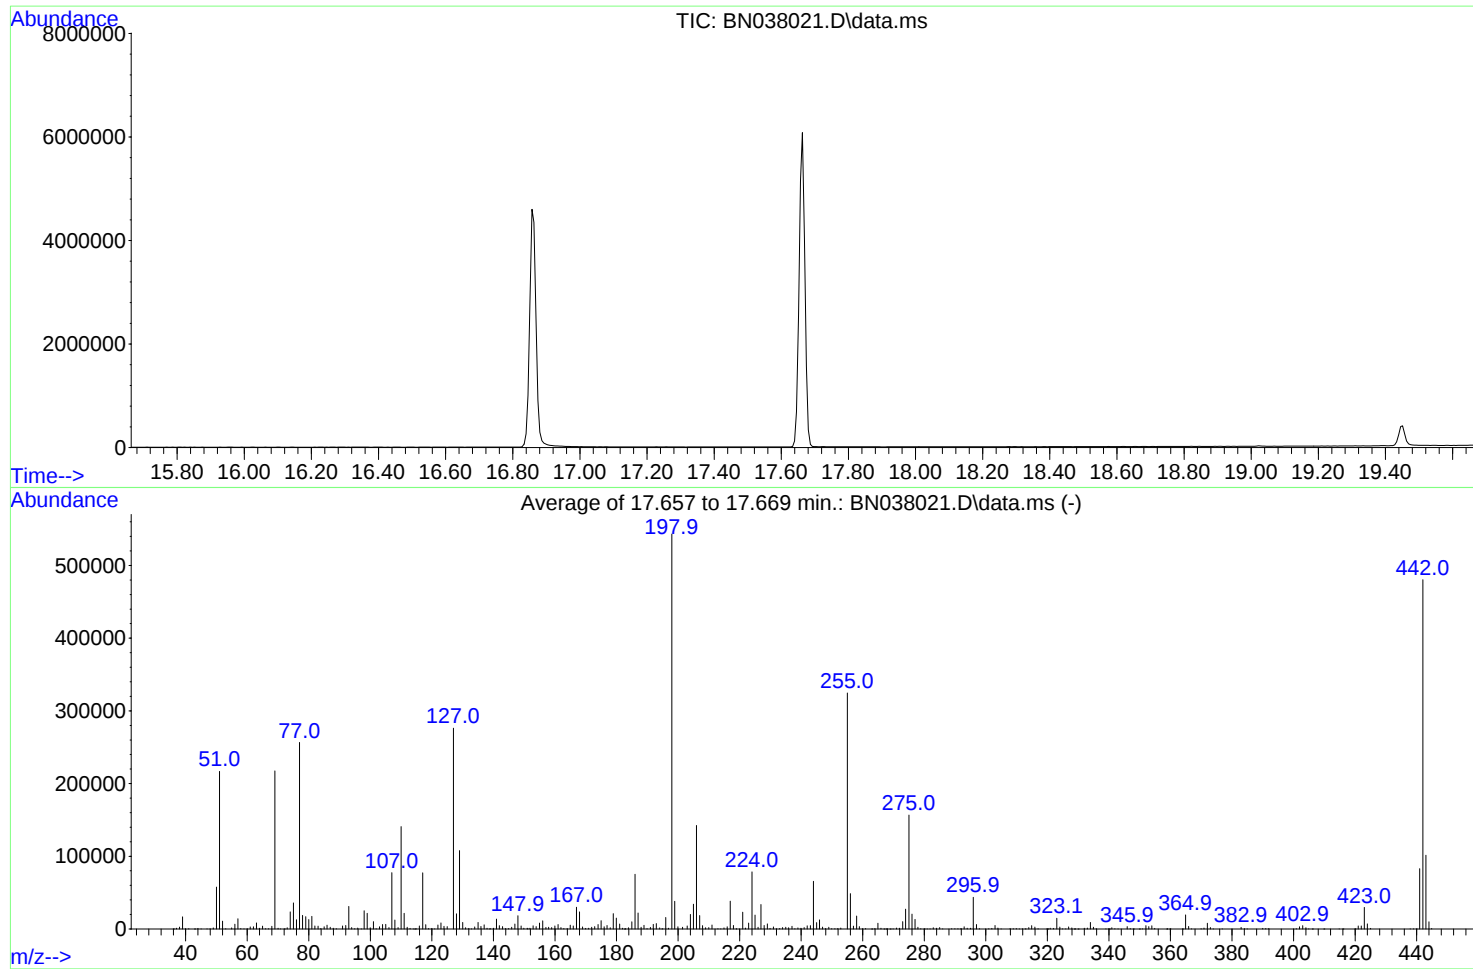

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2469

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	3833	PASS
69	69	100	100	100.0	217387	PASS
70	69	0.00	2	0.5	1053	PASS
197	198	0.00	2	0.2	1130	PASS
198	198	100	100	100.0	543040	PASS
199	198	5	9	7.0	38141	PASS
365	198	1	100	3.5	19270	PASS
441	443	0.01	150	81.7	82901	PASS
442	442	100	100	100.0	480363	PASS
443	442	15	24	21.1	101427	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/6/2025	BNA_N	<u>BN038021.D</u>
Compound Name	Response	Retention Time
DDT	1680193	20.698
DDD	6164	20.315
DDE	438	19.757
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6602	1686795	0.39

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100625\
Data File : BN038021.D
Acq On : 06 Oct 2025 22:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 07 01:36:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

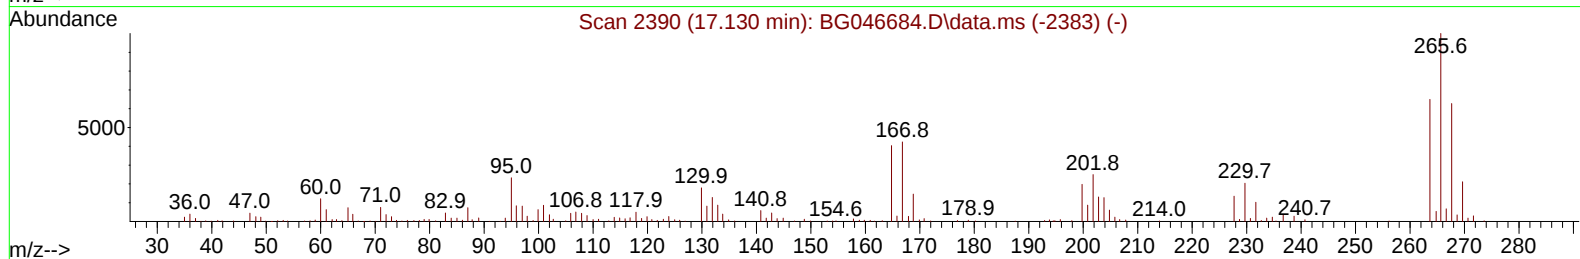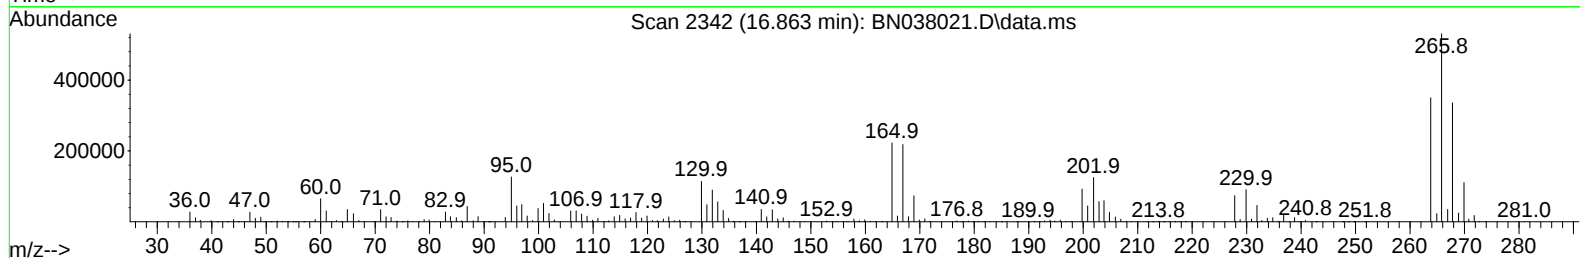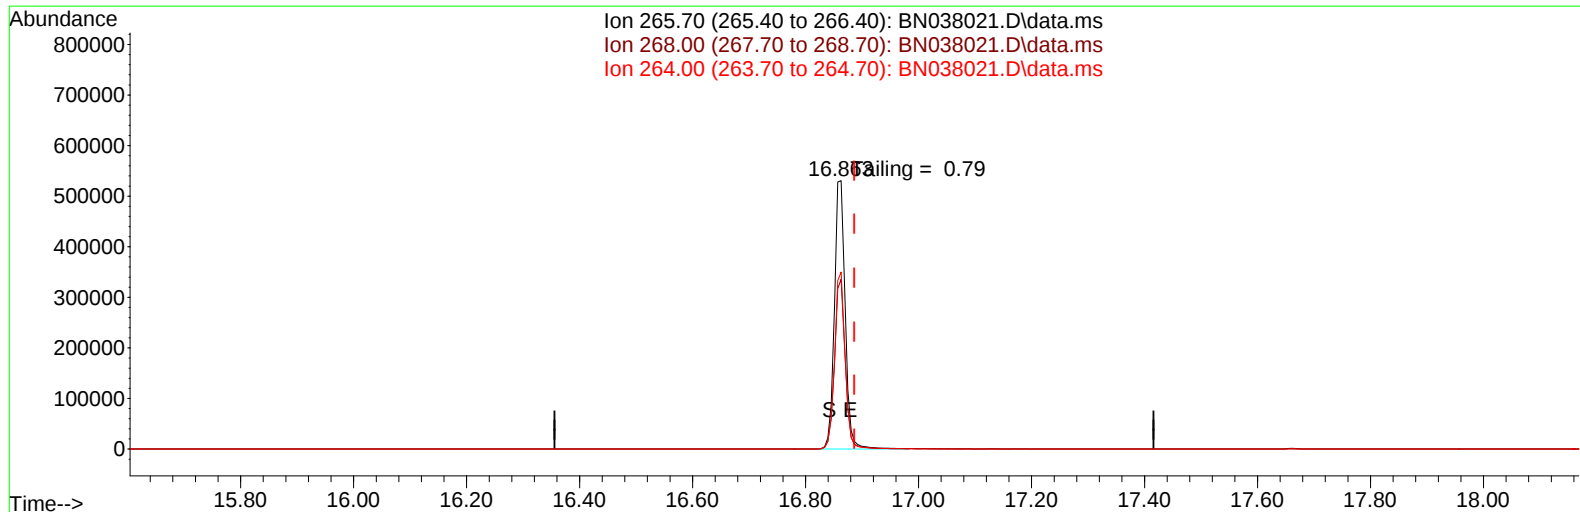

TIC: BN038021.D\data.ms

(70) Pentachlorophenol (C)

16.863min (-0.023) 25768.22 ng




response 704341

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.25
264.00	61.60	65.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100625\
Data File : BN038021.D
Acq On : 06 Oct 2025 22:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 07 01:36:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

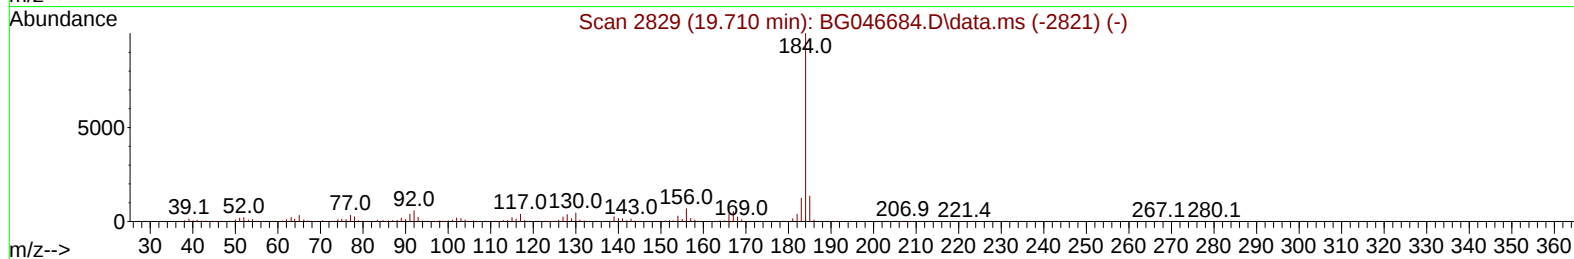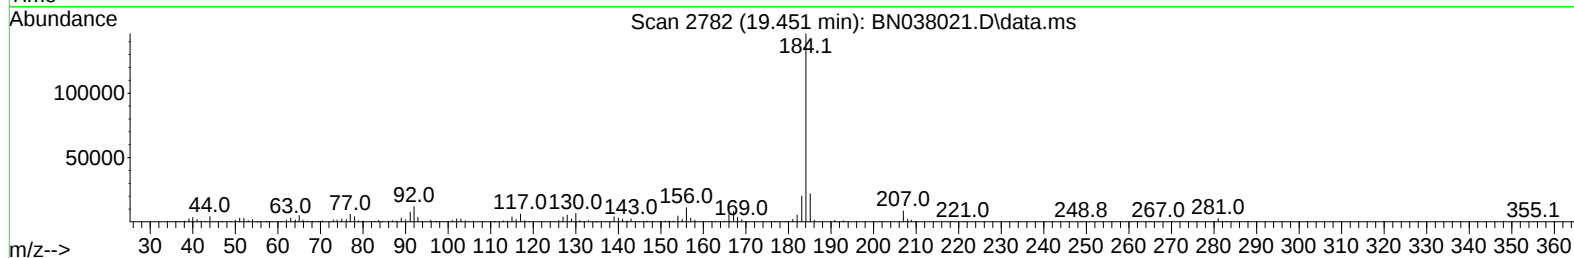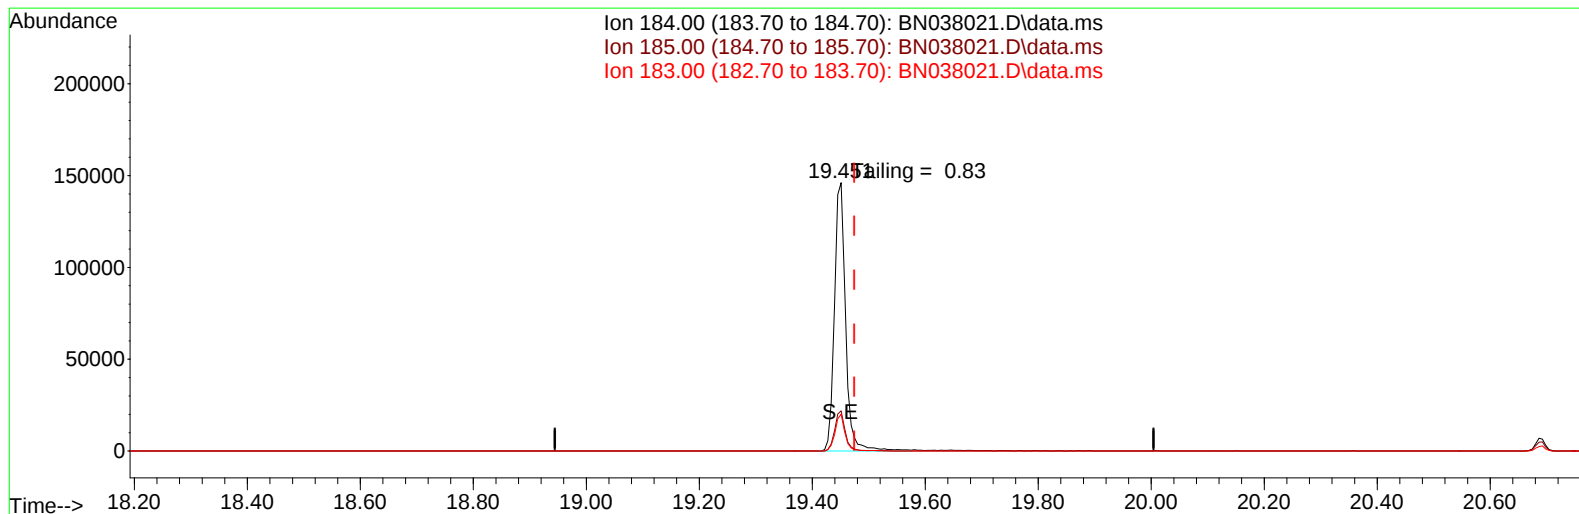

TIC: BN038021.D\data.ms

(77) Benzidine

19.451min (-0.023) 0.00 ng

response 201168

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.96
183.00	13.20	13.71
0.00	0.00	0.00