


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF093025\
Data File : BF143829.D
Acq On : 30 Sep 2025 12:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF092325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 24 05:00:00 2025

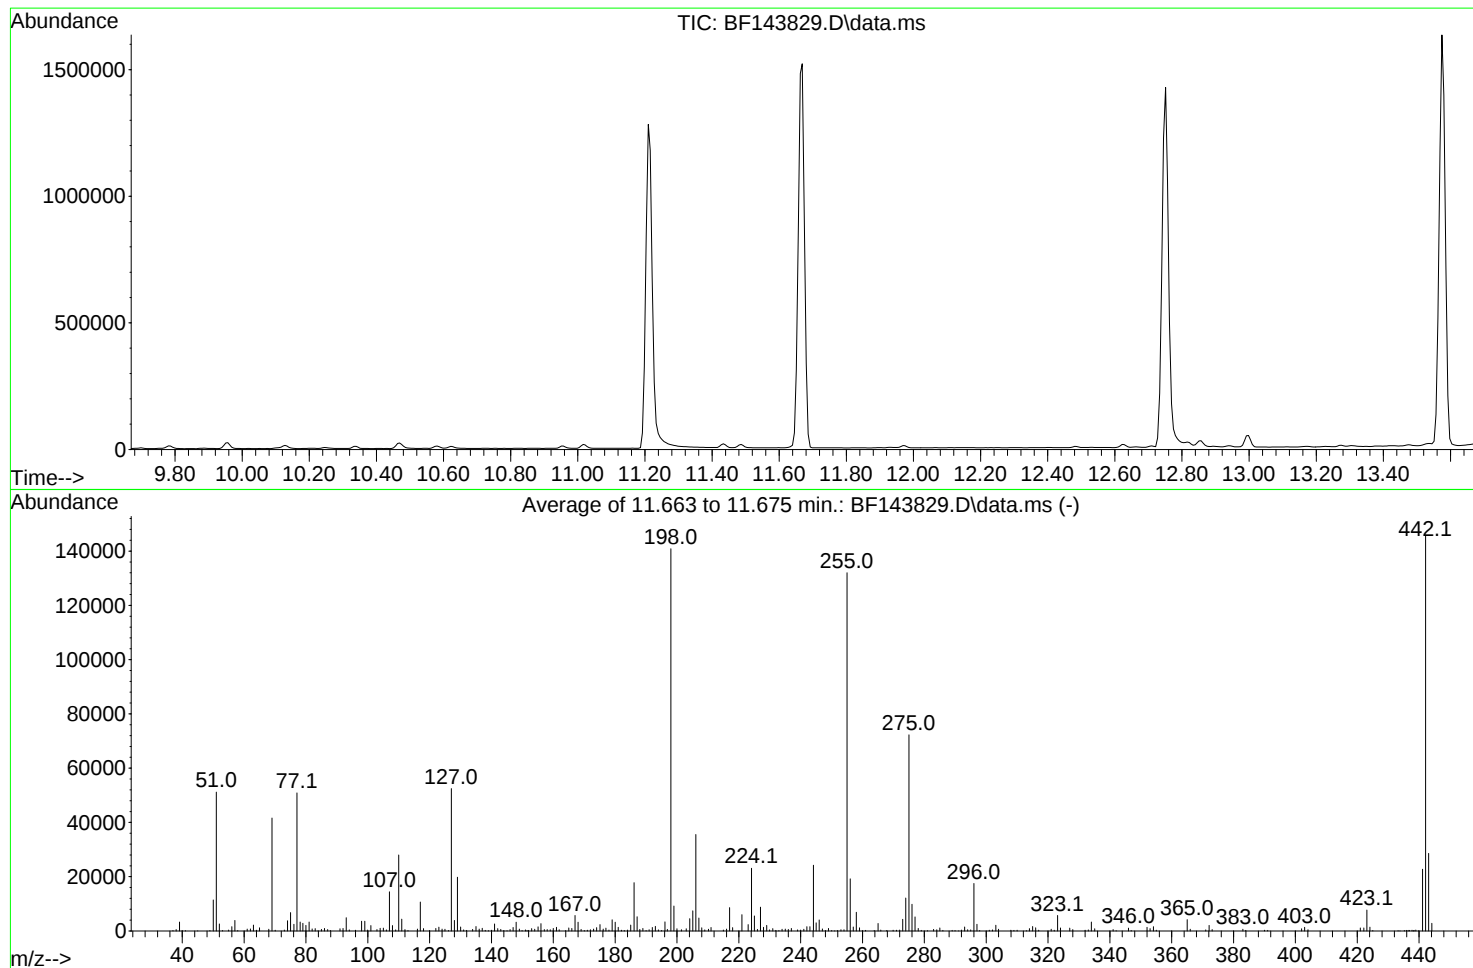




AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1603

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.5	642	PASS
69	69	100	100	100.0	41624	PASS
70	69	0.00	2	0.6	249	PASS
197	198	0.00	2	0.4	591	PASS
198	198	100	100	100.0	140891	PASS
199	198	5	9	6.5	9207	PASS
365	198	1	100	3.0	4182	PASS
441	443	0.01	150	79.6	22741	PASS
442	442	100	100	100.0	145544	PASS
443	442	15	24	19.6	28576	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF093025\
Data File : BF143829.D
Acq On : 30 Sep 2025 12:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 30 13:05:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF092325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 24 05:00:00 2025
Response via : Initial Calibration

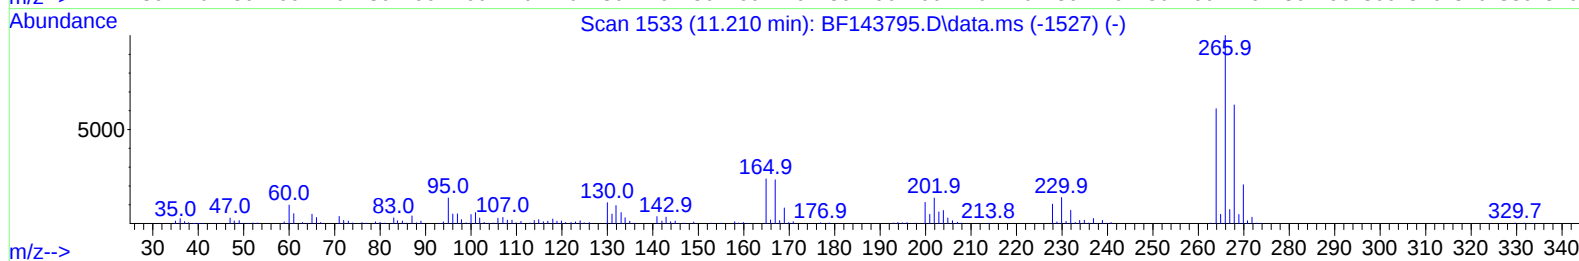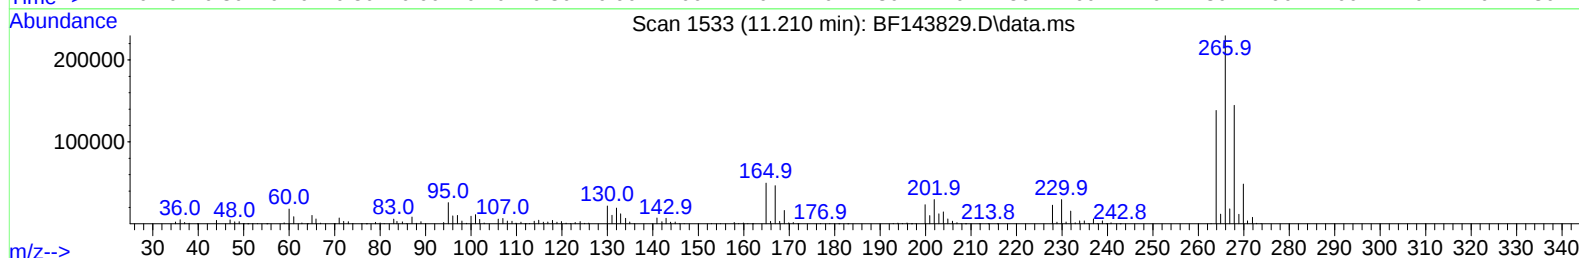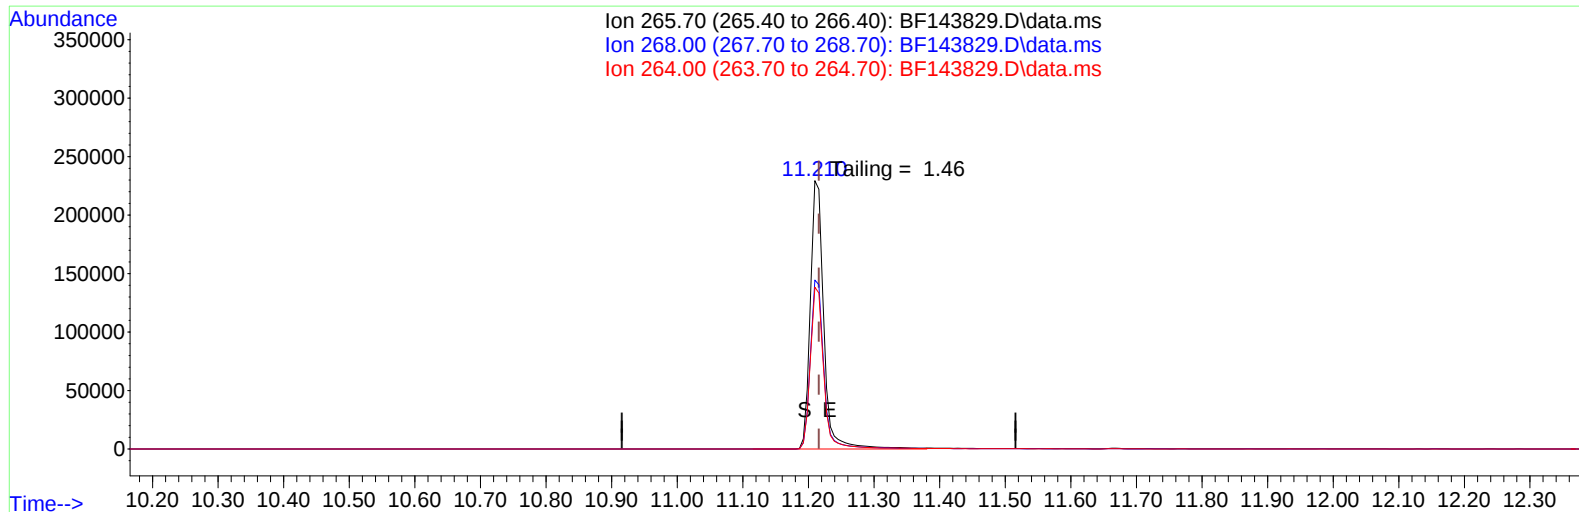

TIC: BF143829.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.006) 35352.24 ng




response 326491

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.97
264.00	61.00	60.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF093025\
Data File : BF143829.D
Acq On : 30 Sep 2025 12:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 30 13:05:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF092325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 24 05:00:00 2025
Response via : Initial Calibration

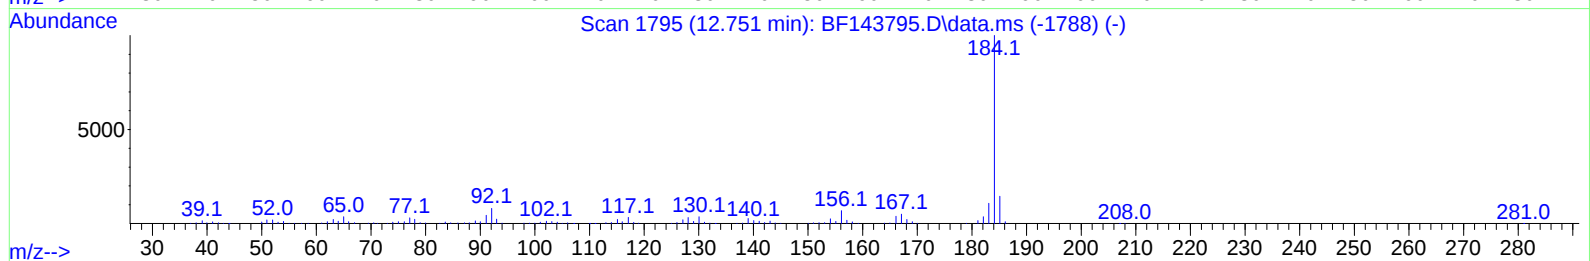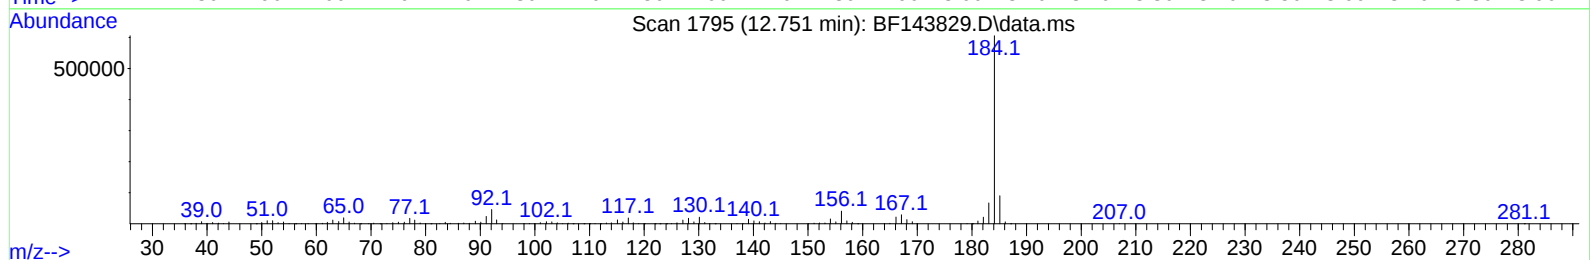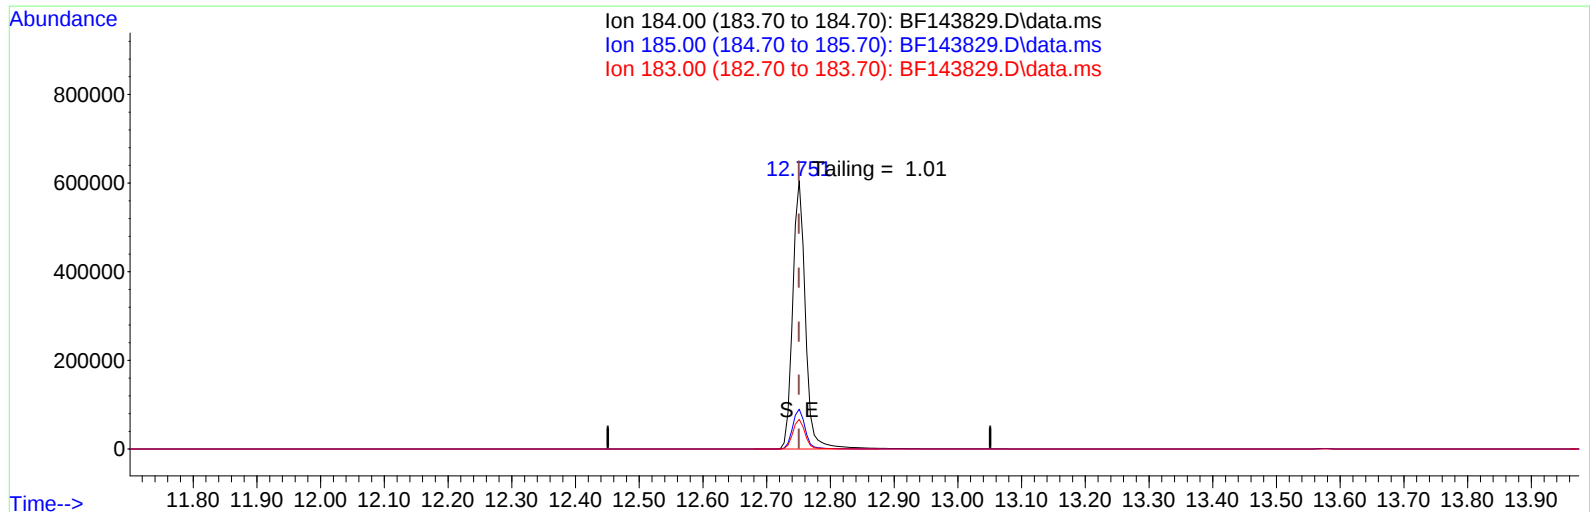

TIC: BF143829.D\data.ms

(77) Benzidine

12.751min (+ 0.000) 0.00 ng

response 840967

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.89
183.00	10.80	11.05
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/30/2025	BNA_F	<u>BF143829.D</u>
Compound Name	Response	Retention Time
DDT	440560	13.574
DDD	4133	13.274
DDE	1748	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5881	446441	1.32

Instrument :
BNA_F
ClientSampleId :
DFTPP