
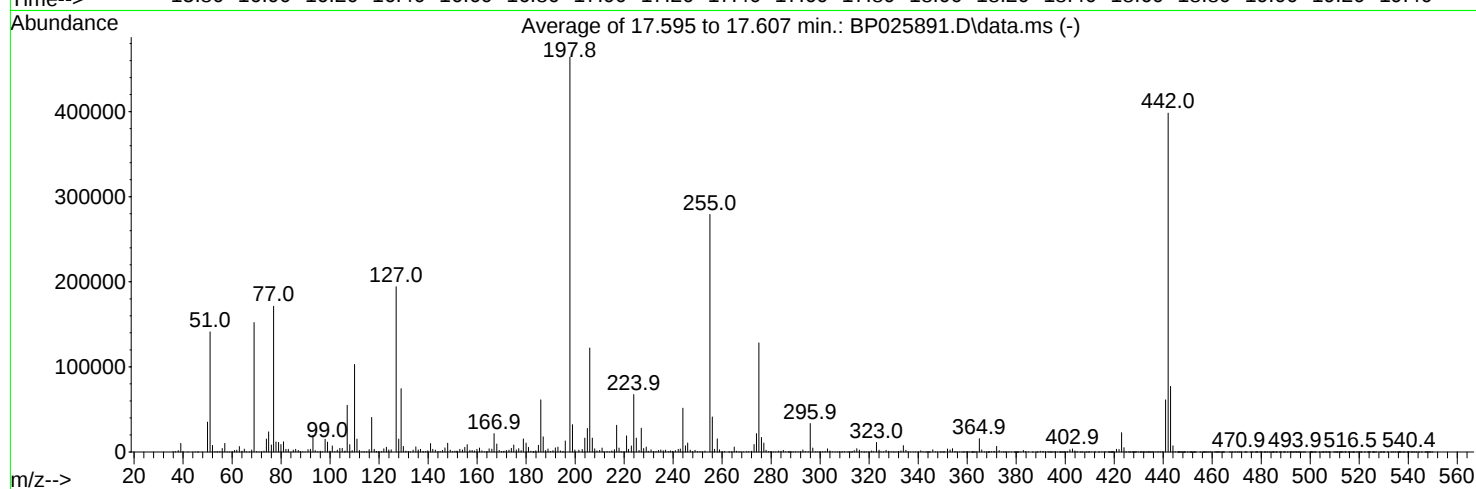


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093025\
Data File : BP025891.D
Acq On : 30 Sep 2025 14:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 11 16:45:04 2025

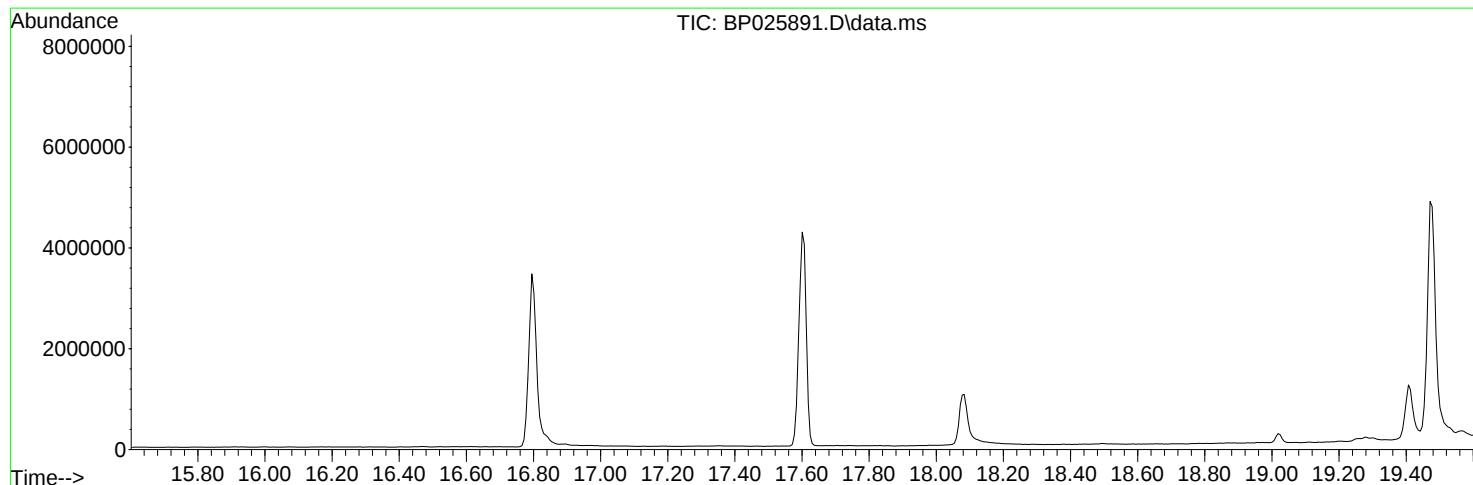




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2484

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	2402	PASS
69	69	100	100	100.0	152148	PASS
70	69	0.00	2	0.4	553	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	464126	PASS
199	198	5	9	6.9	32080	PASS
365	198	1	100	3.4	15595	PASS
441	443	0.01	150	79.6	61257	PASS
442	442	100	100	100.0	398208	PASS
443	442	15	24	19.3	76955	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093025\
Data File : BP025891.D
Acq On : 30 Sep 2025 14:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 30 15:07:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

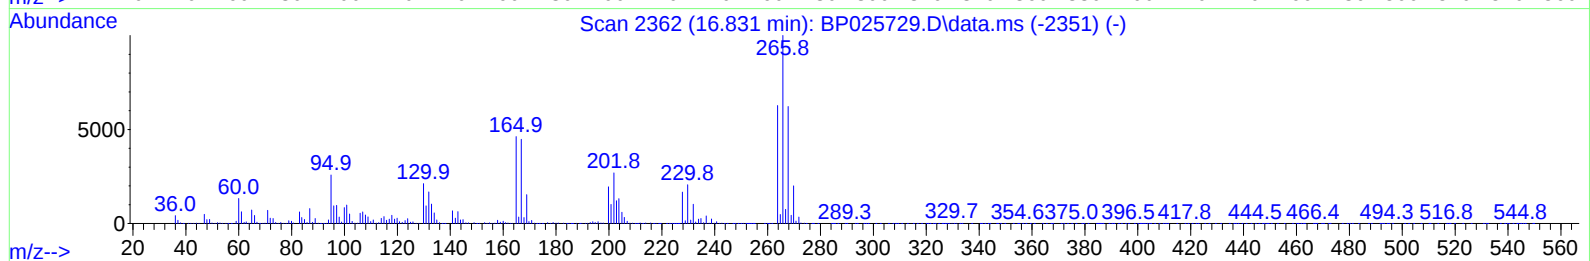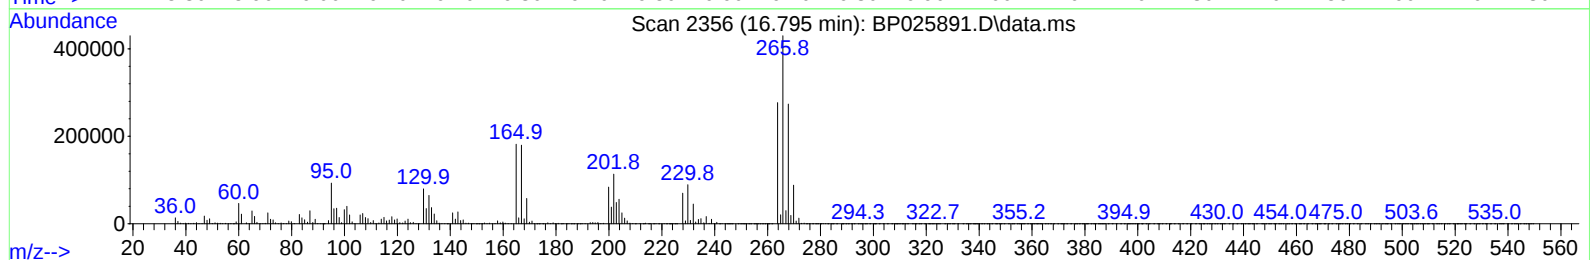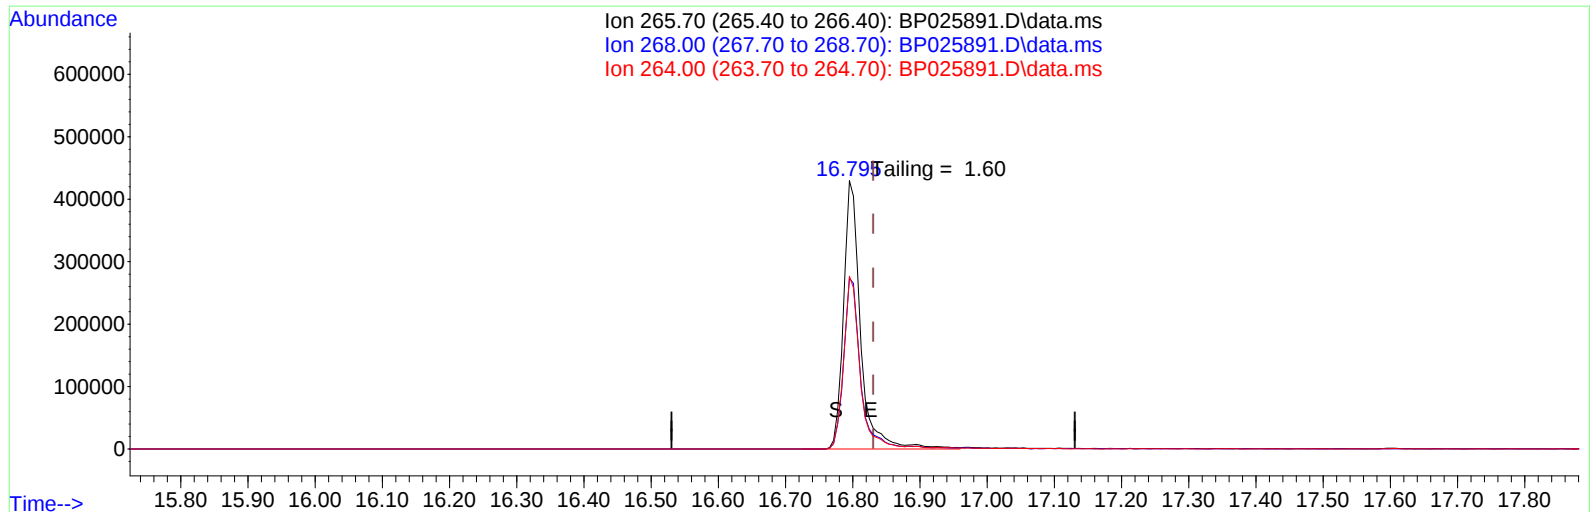

TIC: BP025891.D\data.ms

(70) Pentachlorophenol (C)

16.795min (-0.036) 1604261.33 ng




response 739379

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.70
264.00	62.70	64.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093025\
Data File : BP025891.D
Acq On : 30 Sep 2025 14:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 30 15:07:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

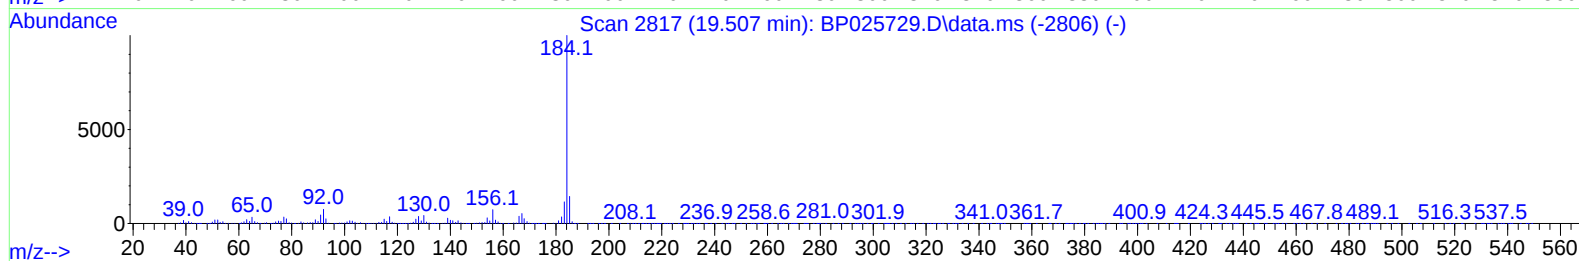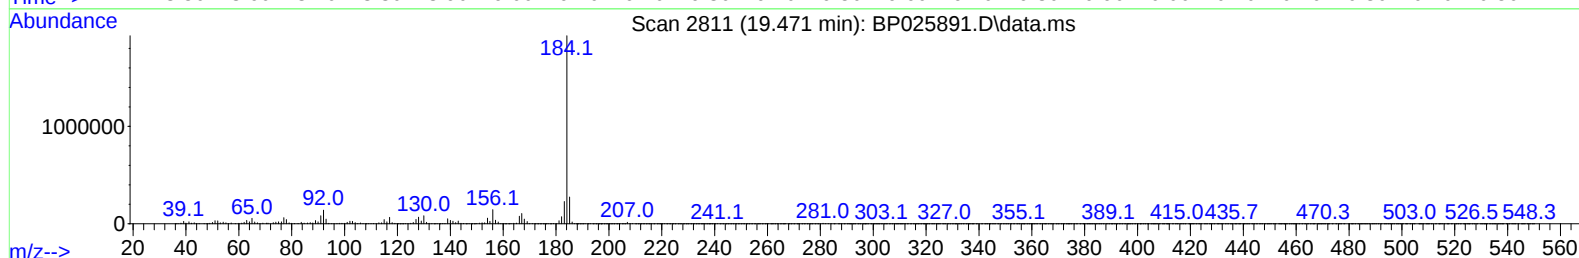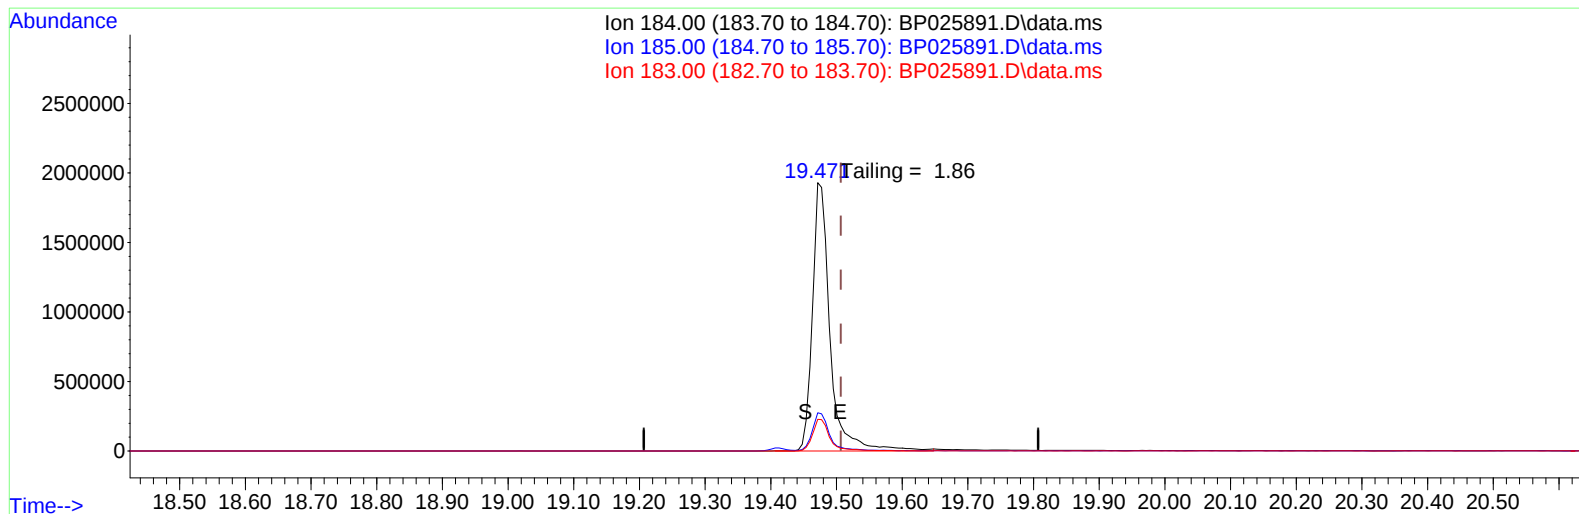

TIC: BP025891.D\data.ms

(77) Benzidine

19.471min (-0.036) 176773.01 ng

response 3574590

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.25
183.00	11.50	11.80
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/30/2025	BNA_P	<u>BP025891.D</u>
Compound Name	Response	Retention Time
DDT	2079365	20.765
DDD	58249	20.307
DDE	10109	19.765
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
68358	2147723	3.18

Instrument :
BNA_P
ClientSampleId :
DFTPP