


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100725\
Data File : BN038040.D
Acq On : 07 Oct 2025 10:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 24 11:00:01 2025

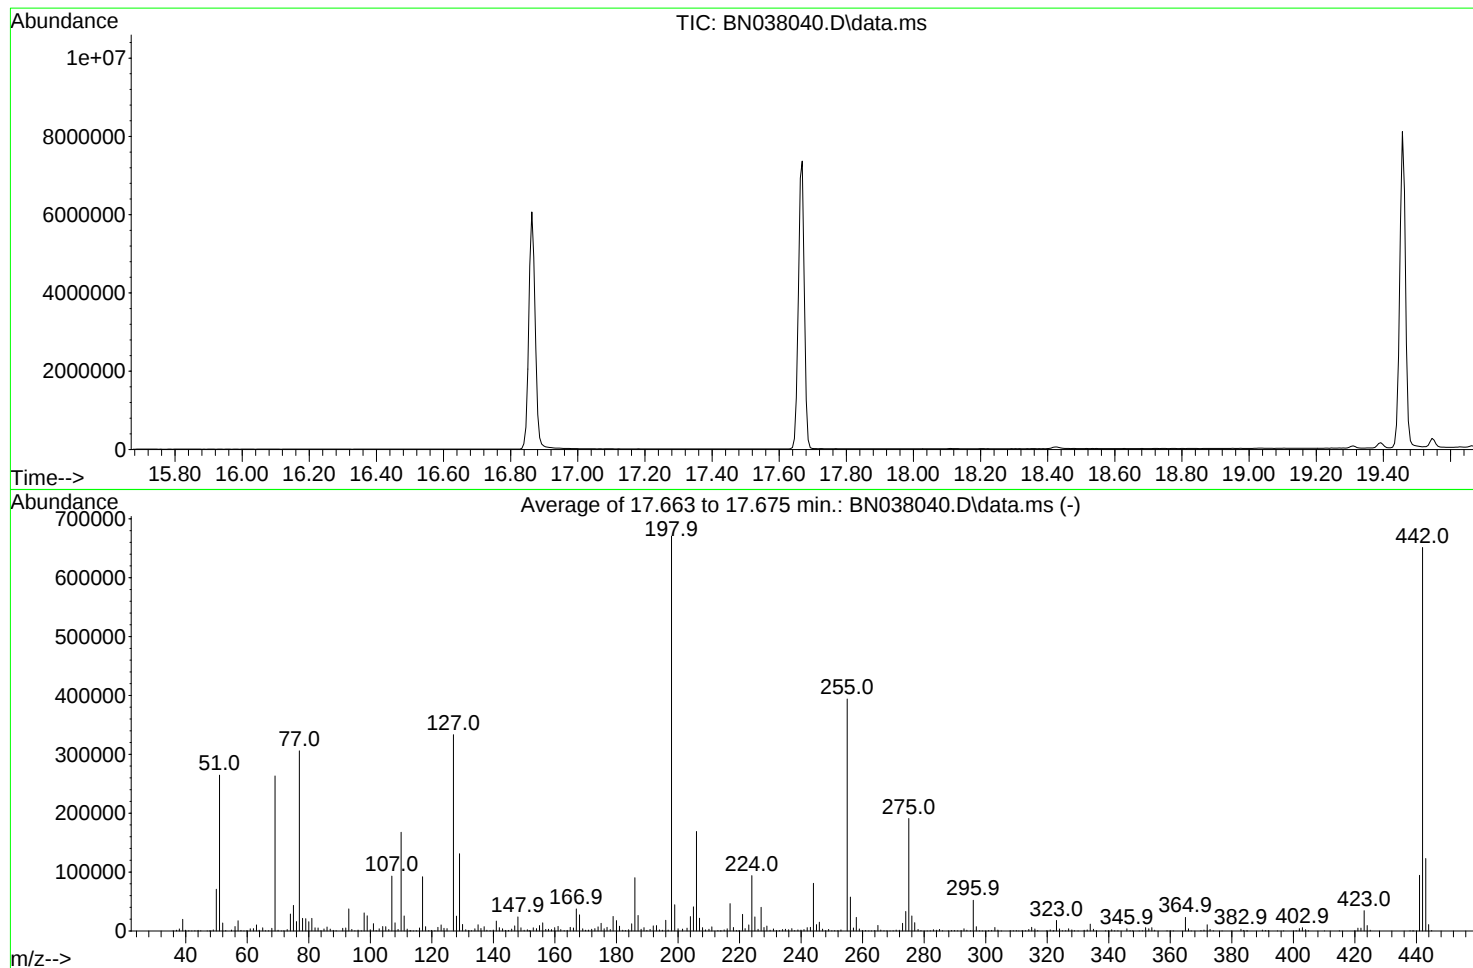




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2470

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	4415	PASS
69	69	100	100	100.0	263211	PASS
70	69	0.00	2	0.5	1365	PASS
197	198	0.00	2	0.2	1396	PASS
198	198	100	100	100.0	670699	PASS
199	198	5	9	6.6	44432	PASS
365	198	1	100	3.4	23117	PASS
441	443	0.01	150	76.8	94429	PASS
442	442	100	100	100.0	651413	PASS
443	442	15	24	18.9	123029	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100725\
Data File : BN038040.D
Acq On : 07 Oct 2025 10:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 07 11:58:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

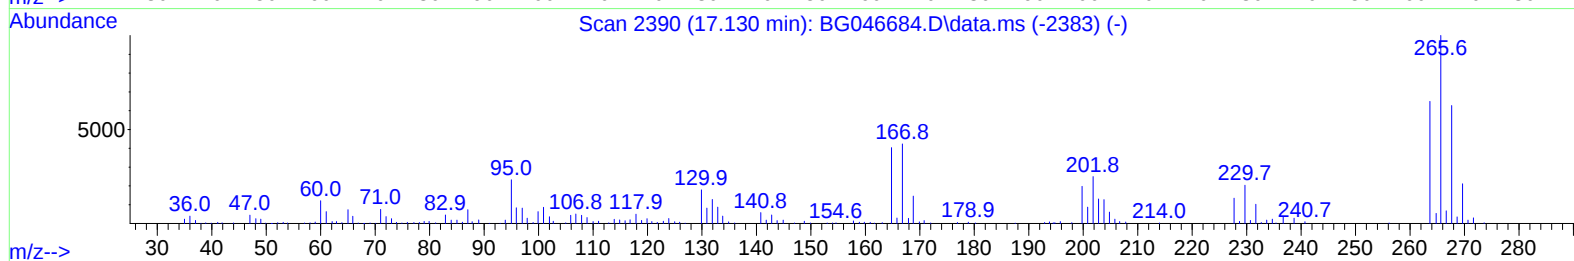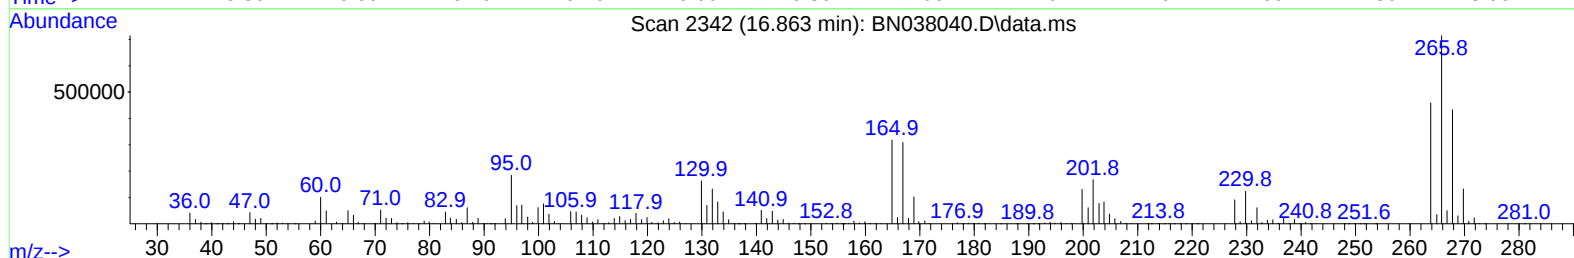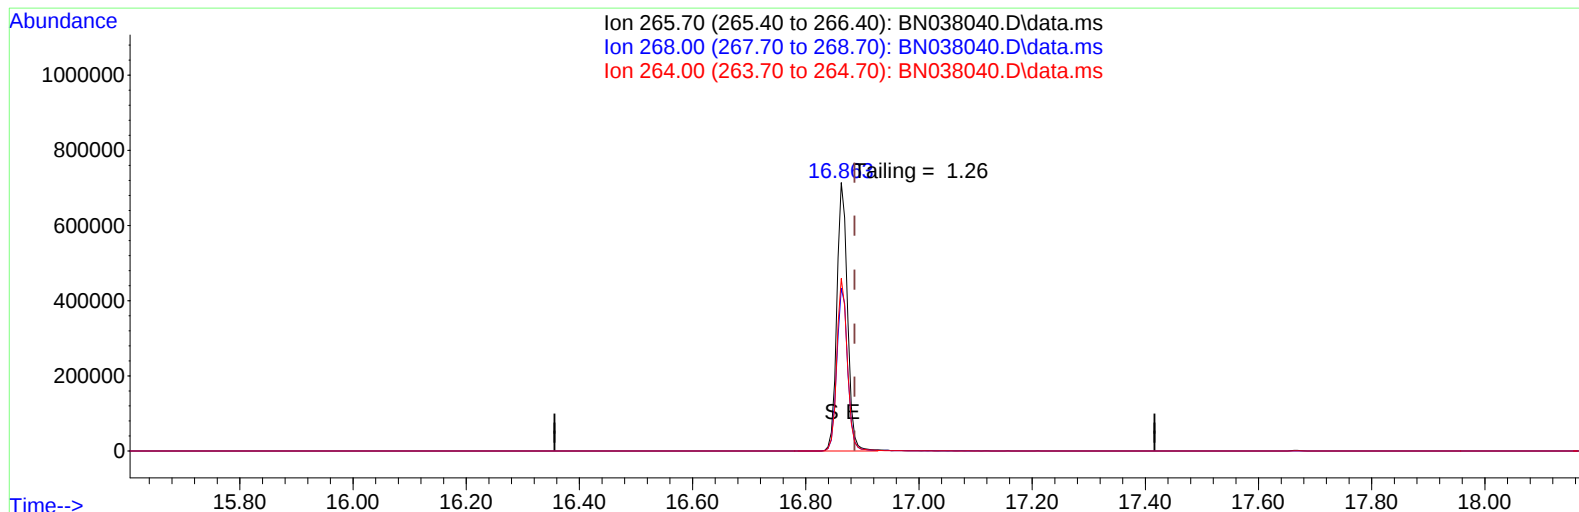

TIC: BN038040.D\data.ms

(70) Pentachlorophenol (C)

16.863min (-0.023) 28552.74 ng




response 938649

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.61
264.00	61.60	64.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100725\
Data File : BN038040.D
Acq On : 07 Oct 2025 10:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 07 11:58:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

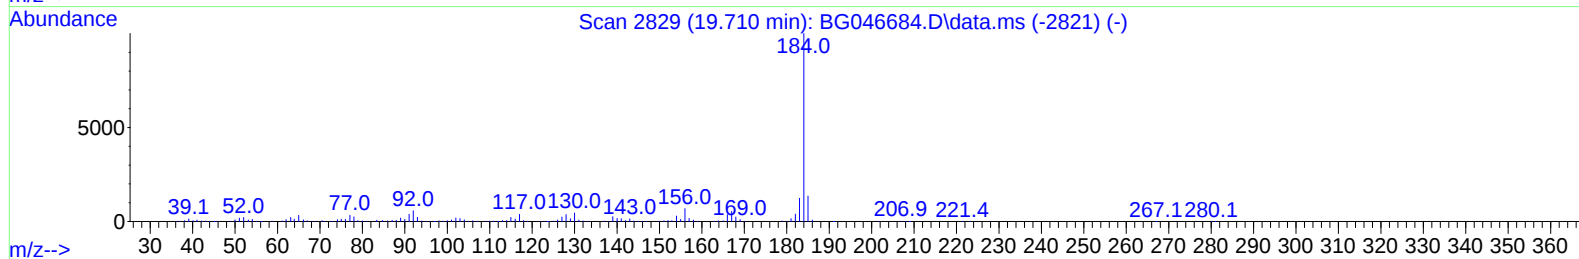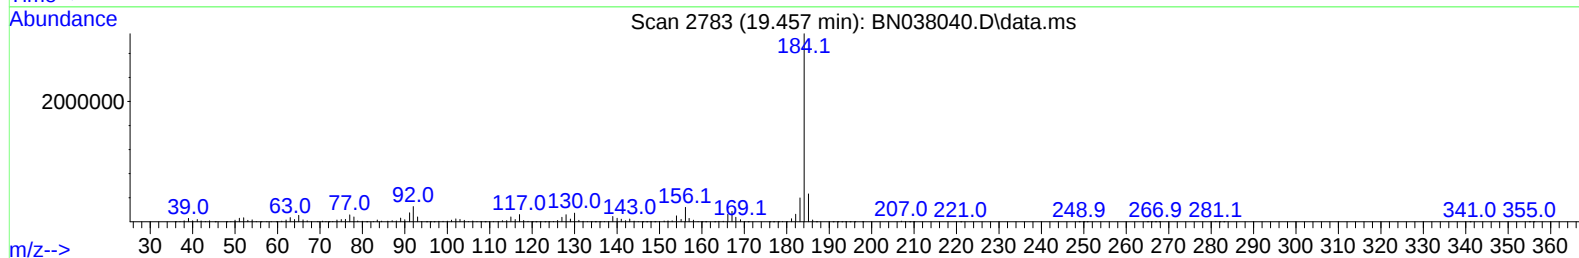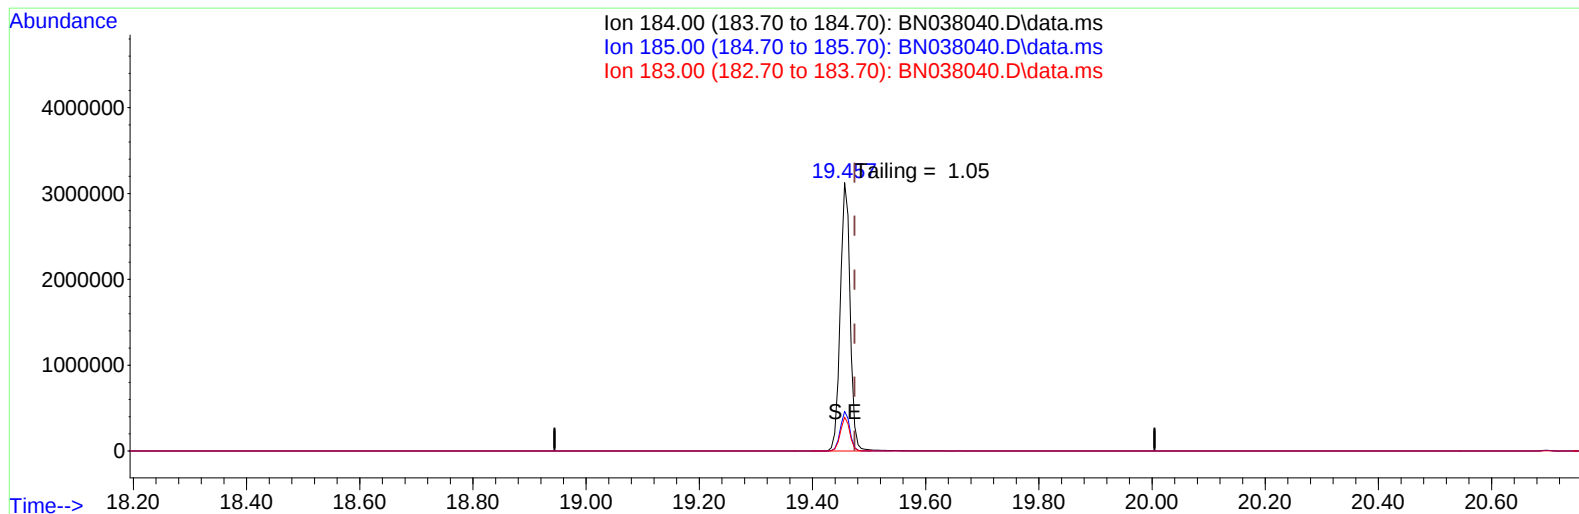

TIC: BN038040.D\data.ms

(77) Benzidine

19.457min (-0.017) 0.00 ng

response 3786107

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.80
183.00	13.20	12.66
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/7/2025	BNA_N	<u>BN038040.D</u>
Compound Name	Response	Retention Time
DDT	2140478	20.698
DDD	16098	20.257
DDE	520	19.751
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16618	2157096	0.77

Instrument :
BNA_N
ClientSampleId :
DFTPP