


Instrument IC-1										Analyst: RM	Method: 300.0 / 9056A		
Ident	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4	Method name	date time	Initial Analyst			
STD1	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-090925	9/9/2025 10:21	10 RM/IZ			
STD2	0.423	0.641	0.632	2.091	0.529	1.063	3.237	IC1-090925	9/9/2025 10:42	10 RM/IZ			
STD3	0.794	1.189	1.197	3.984	0.997	2.006	6.010	IC1-090925	9/9/2025 11:25	10 RM/IZ			
STD4	0.990	1.475	1.473	4.920	1.228	2.461	7.371	IC1-090925	9/9/2025 11:47	10 RM/IZ			
STD5	2.008	3.012	3.027	10.105	2.514	4.978	15.047	IC1-090925	9/9/2025 13:36	10 RM/IZ			
STD6	3.935	5.921	5.894	19.658	4.924	9.905	29.203	IC1-090925	9/9/2025 13:58	10 RM/IZ			
STD7	5.050	7.561	7.577	25.243	6.308	12.587	37.633	IC1-090925	9/9/2025 14:41	10 RM/IZ			
ICV	2.001	2.995	2.988	9.985	2.483	5.041	14.797	IC1-090925	9/9/2025 15:02	10 RM/IZ			
ICB	0.000	0.063	0.000	0.000	0.000	0.000	0.000	IC1-090925	9/9/2025 15:45	10 RM/IZ			
CCV	2.067	3.130	3.129	10.485	2.586	4.853	15.356	IC1-090925	9/30/2025 11:13	10 RM/IZ			
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-090925	9/30/2025 11:34	10 RM/IZ			
LB137383BLW	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-090925	9/30/2025 11:56	10 RM/IZ			
LB137383BSW	2.086	3.121	3.125	10.502	2.597	5.015	15.420	IC1-090925	9/30/2025 12:17	10 RM/IZ			
Q3254-01	0.095	166.573	0.000	0.000	3.228	0.000	27.763	IC1-090925	9/30/2025 13:41	10 RM/IZ			
Q3254-01MS	1.988	161.834	2.821	9.511	5.398	0.000	40.983	IC1-090925	9/30/2025 14:03	10 RM/IZ			
Q3254-01MSD	2.092	161.643	2.949	9.939	5.508	0.000	41.610	IC1-090925	9/30/2025 14:24	10 RM/IZ			
Q3254-03	0.221	551.450	0.000	0.530	0.000	0.000	33.048	IC1-090925	9/30/2025 14:46	10 RM/IZ			
Q3254-05	0.202	384.425	0.000	0.324	0.970	0.000	28.280	IC1-090925	9/30/2025 15:08	10 RM/IZ			
Q3254-07	0.222	551.586	0.000	0.529	0.000	0.000	33.228	IC1-090925	9/30/2025 15:29	10 RM/IZ			
CCV	2.071	3.081	3.098	10.391	2.562	5.273	15.243	IC1-090925	9/30/2025 15:51	10 RM/IZ			
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-090925	9/30/2025 16:12	10 RM/IZ			
Q3254-01DLX50	0.000	2.396	0.000	0.000	0.101	0.000	0.908	IC1-090925	9/30/2025 16:34	10 RM/IZ			
Q3254-03DLX100	0.000	3.687	0.000	0.000	0.000	0.000	0.791	IC1-090925	9/30/2025 16:55	10 RM/IZ			
Q3254-05DLX100	0.000	2.613	0.000	0.000	0.000	0.000	0.707	IC1-090925	9/30/2025 18:00	10 RM/IZ			
Q3254-07DLX100	0.000	3.741	0.000	0.000	0.000	0.000	0.774	IC1-090925	9/30/2025 18:21	10 RM/IZ			
CCV	2.070	3.087	3.099	10.400	2.560	5.225	15.261	IC1-090925	9/30/2025 19:04	10 RM/IZ			
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-090925	9/30/2025 19:26	10 RM/IZ			

Clear table

Instrument ID: IC-2 Analyst: IZ Method: 300.0 / 9056A									
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentratio n HPO4	concentrati on SO4	file name	Initial wt/ Final
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-090925	10 RM/IZ
STD2	0.4230	0.6410	0.6320	2.0910	0.5290	1.0630	3.2370	IC1-090925	10 RM/IZ
STD3	0.7940	1.1890	1.1970	3.9840	0.9970	2.0060	6.0100	IC1-090925	10 RM/IZ
STD4	0.9900	1.4750	1.4730	4.9200	1.2280	2.4610	7.3710	IC1-090925	10 RM/IZ
STD5	2.0080	3.0120	3.0270	10.1050	2.5140	4.9780	15.0470	IC1-090925	10 RM/IZ
STD6	3.9350	5.9210	5.8940	19.6580	4.9240	9.9050	29.2030	IC1-090925	10 RM/IZ
STD7	5.0500	7.5610	7.5770	25.2430	6.3080	12.5870	37.6330	IC1-090925	10 RM/IZ
date time	9/9/2025 10:21	9/9/2025 10:42	9/9/2025 11:25	9/9/2025 11:47	9/9/2025 13:36	9/9/2025 13:58	9/9/2025 14:41		
Analyst									
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000		
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000		
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000		
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000		
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000		
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000		
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000		
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4		
STD1									
STD2	5.7500	6.8333	5.3333	4.5500	5.8000	6.3000	7.9000		
STD3	-0.7500	-0.9167	-0.2500	-0.4000	-0.3000	0.3000	0.1667		
STD4	-1.0000	-1.6667	-1.8000	-1.6000	-1.7600	-1.5600	-1.7200		
STD5	0.4000	0.4000	0.9000	1.0500	0.5600	-0.4400	0.3133		
STD6	-1.6250	-1.3167	-1.7667	-1.7100	-1.5200	-0.9500	-2.6567		
STD7	1.0000	0.8133	1.0267	0.9720	0.9280	0.6960	1.7108		

Fluoride (Anions)

($\mu\text{S}/\text{cm}$) x min

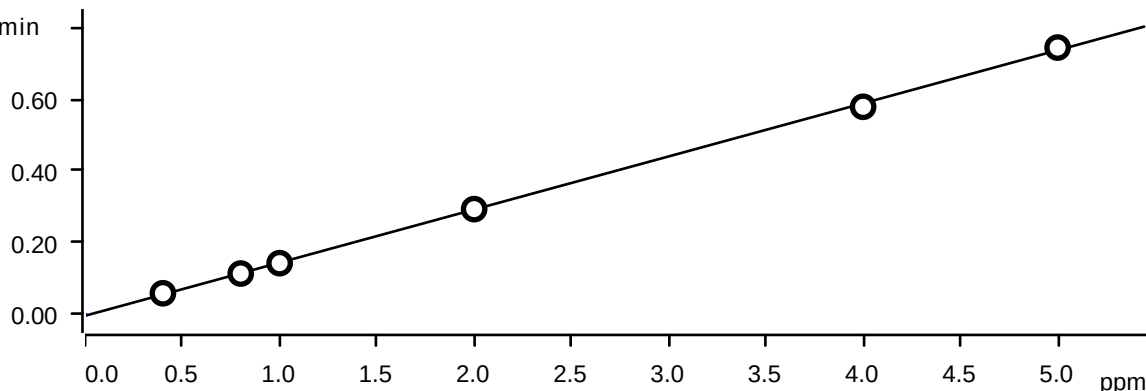

Function: $A = -3.91674E-3 + 0.0148053 \times Q$


Relative standard deviation 1.985504 %

Correlation coefficient 0.999790

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.059	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.114	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.143	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.293	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.579	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.744	STD7	2025-09-09 14:41:06 UTC-4	used

Chloride (Anions)

($\mu\text{S}/\text{cm}$) x min

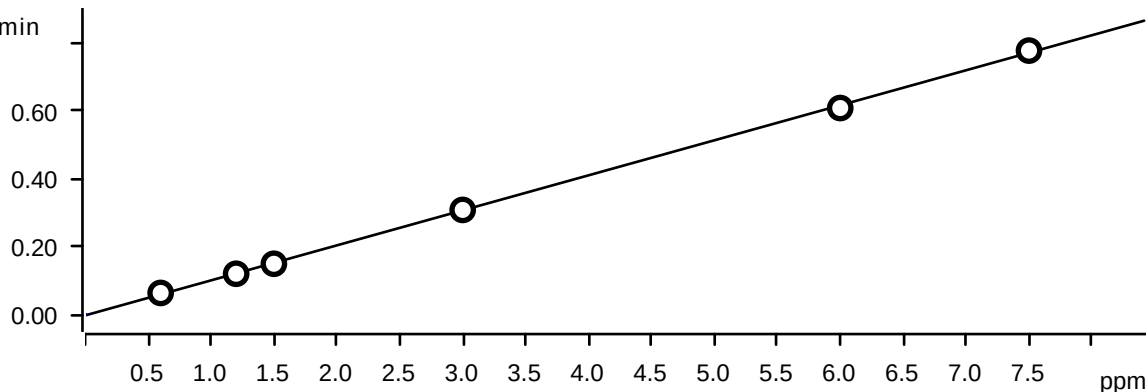


Function: $A = -2.97735E-3 + 0.0103068 \times Q$

Relative standard deviation 1.712968 %

Correlation coefficient 0.999843

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.063	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.120	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.149	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.307	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.607	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.776	STD7	2025-09-09 14:41:06 UTC-4	used

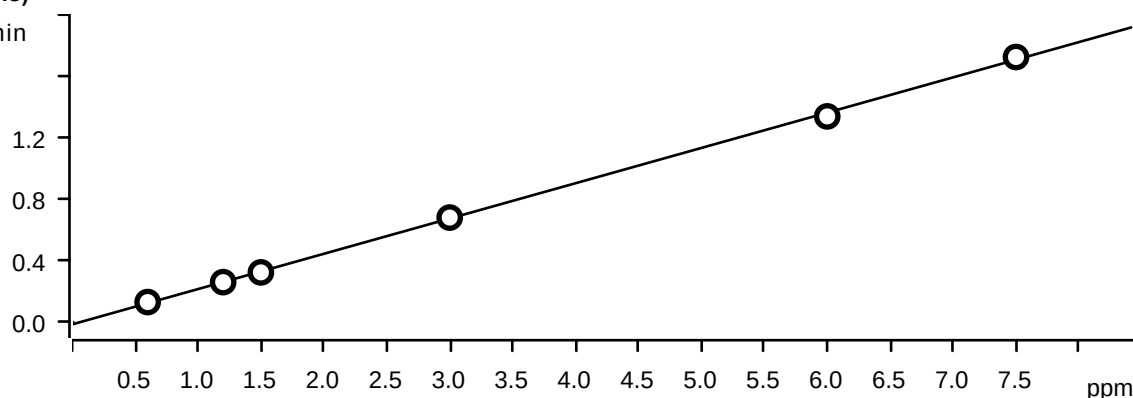Nitrite (Anions) $(\mu\text{S/cm}) \times \text{min}$ Function: $A = -0.0143669 + 0.0229543 \times Q$


Relative standard deviation 2.170764 %

Correlation coefficient 0.999753

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.131	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.260	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.324	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.681	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.339	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.725	STD7	2025-09-09 14:41:06 UTC-4	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

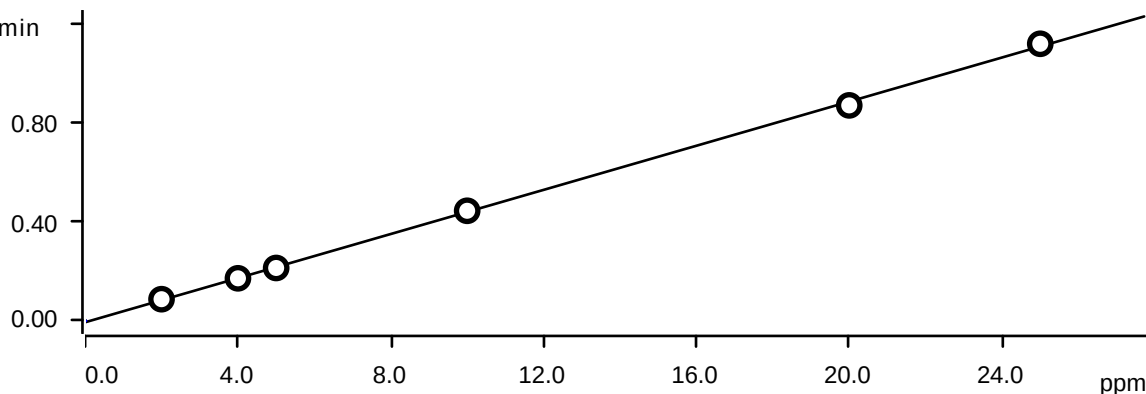

Function: $A = -5.68247E-3 + 4.44287E-3 \times Q$


Relative standard deviation: 2.066849 %

Correlation coefficient: 0.999773

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.087	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.171	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.213	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.443	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.868	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.116	STD7	2025-09-09 14:41:06 UTC-4	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

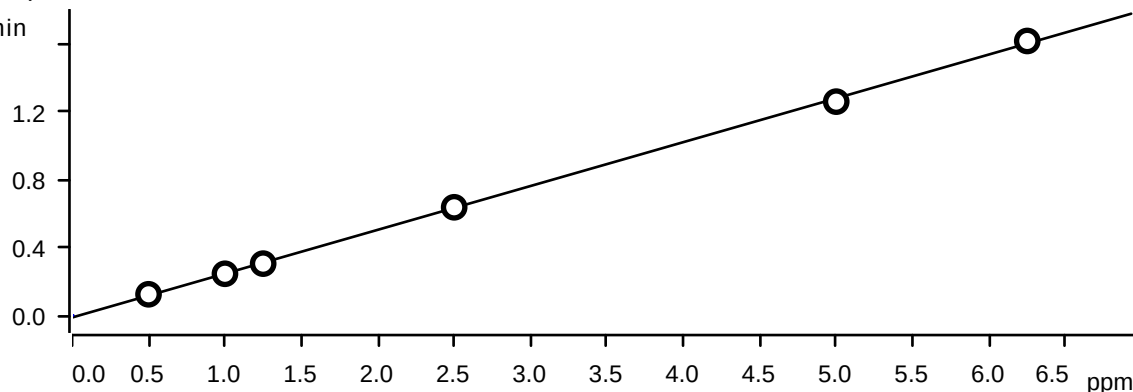


Function: $A = -0.0122982 + 0.0258010 \times Q$

Relative standard deviation: 1.914251 %

Correlation coefficient 0.999807

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.124	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.245	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.305	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.636	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.258	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.615	STD7	2025-09-09 14:41:06 UTC-4	used

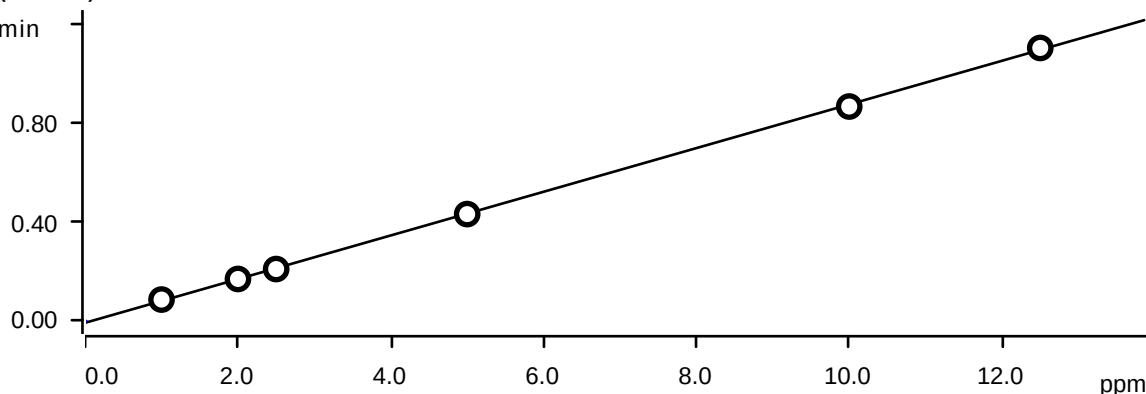
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -6.72192E-3 + 8.79335E-3 \times Q$

Relative standard deviation 1.384046 %

Correlation coefficient 0.999898

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.087	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.170	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.210	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.431	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.864	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.100	STD7	2025-09-09 14:41:06 UTC-4	used

Sulfate (Anions)

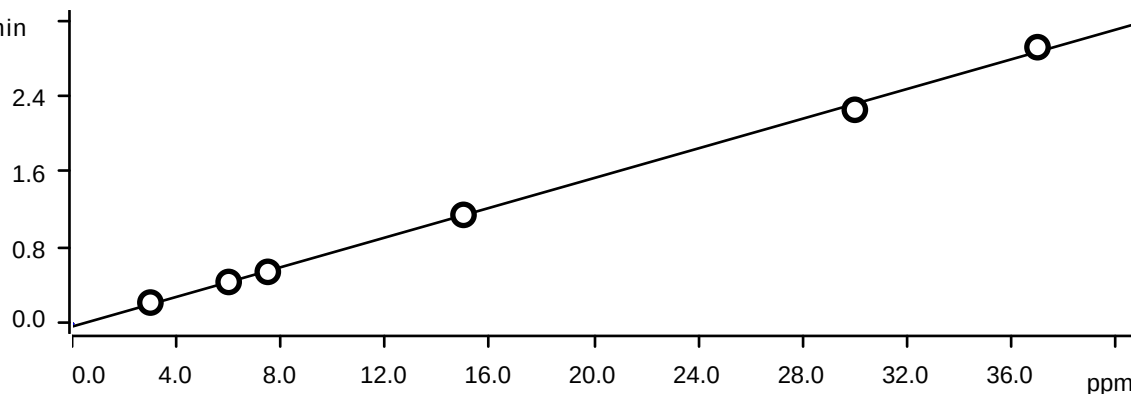 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0295615 + 7.81954E-3 \times Q$

Relative standard deviation 3.285067 %

Correlation coefficient 0.999433


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-09-09 10:21:26 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.224	STD2	2025-09-09 10:42:49 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.440	STD3	2025-09-09 11:25:44 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.547	STD4	2025-09-09 11:47:10 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.147	STD5	2025-09-09 13:36:36 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.254	STD6	2025-09-09 13:58:07 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.913	STD7	2025-09-09 14:41:06 UTC-4	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-09-09 10:21:26 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 13.06 MPa
Maximum pressure monitored yes
Temperature ---- °C

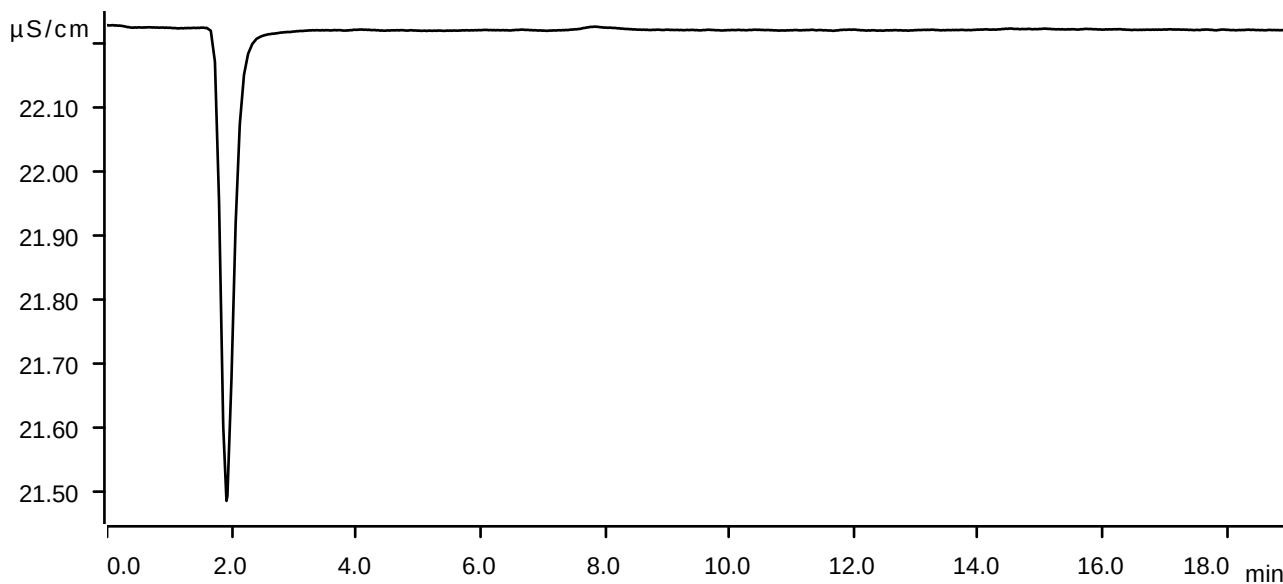Anions


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-09-09 10:42:49 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.84 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

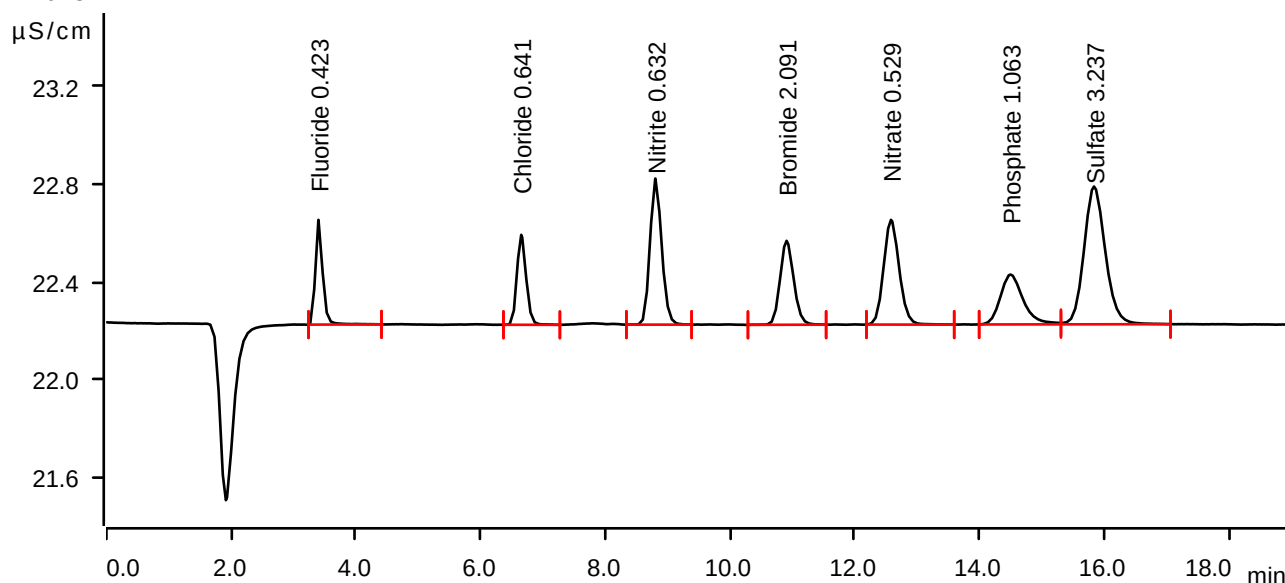

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.400	0.0587	0.429	0.423	Fluoride
2	6.652	0.0631	0.369	0.641	Chloride
3	8.803	0.1306	0.599	0.632	Nitrite
4	10.907	0.0872	0.344	2.091	Bromide
5	12.580	0.1242	0.430	0.529	Nitrate
6	14.497	0.0867	0.205	1.063	Phosphate
7	15.835	0.2236	0.565	3.237	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-09-09 11:25:44 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.67 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

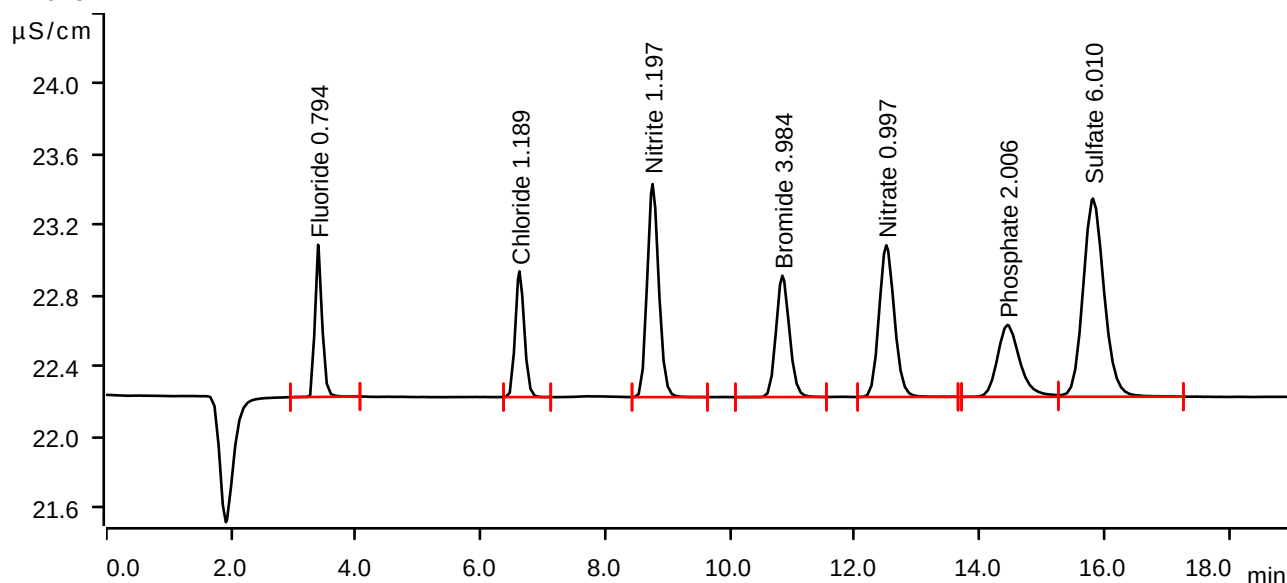

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.395	0.1137	0.861	0.794	Fluoride
2	6.623	0.1196	0.712	1.189	Chloride
3	8.758	0.2603	1.206	1.197	Nitrite
4	10.838	0.1713	0.687	3.984	Bromide
5	12.505	0.2450	0.859	0.997	Nitrate
6	14.448	0.1697	0.407	2.006	Phosphate
7	15.818	0.4404	1.122	6.010	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-09-09 11:47:10 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.61 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

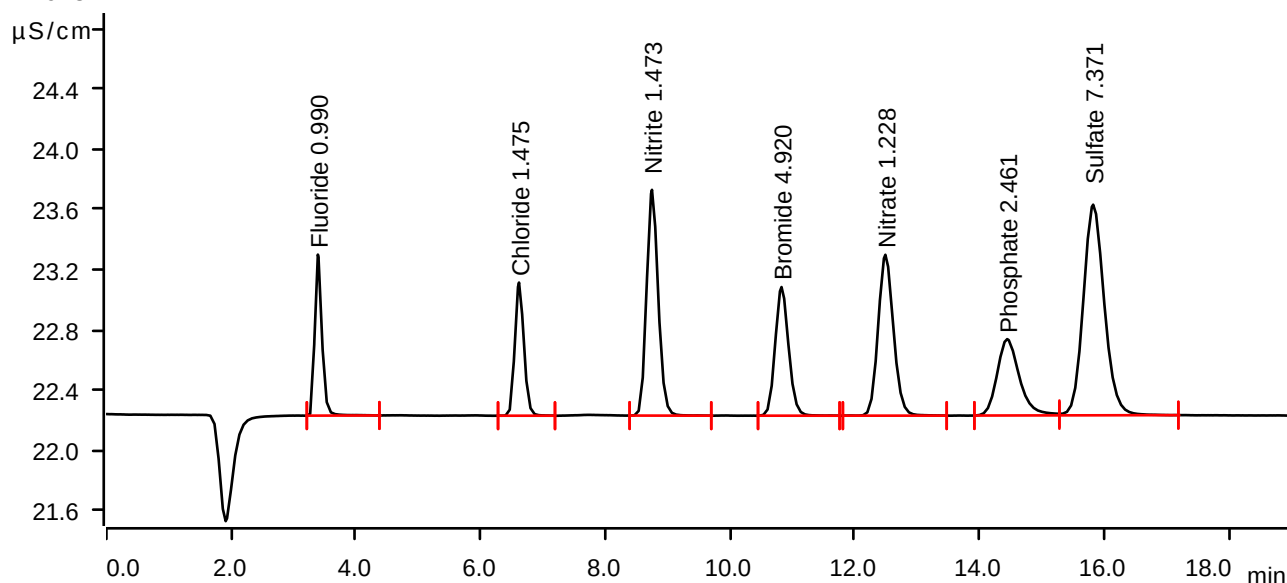

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.392	0.1426	1.068	0.990	Fluoride
2	6.617	0.1490	0.884	1.475	Chloride
3	8.748	0.3238	1.499	1.473	Nitrite
4	10.825	0.2129	0.854	4.920	Bromide
5	12.490	0.3046	1.068	1.228	Nitrate
6	14.443	0.2097	0.507	2.461	Phosphate
7	15.822	0.5468	1.398	7.371	Sulfate


Sample data

Ident STD5
 Sample type Standard 5
 Determination start 2025-09-09 13:36:36 UTC-4
 Method IC1-090925
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 12.50 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

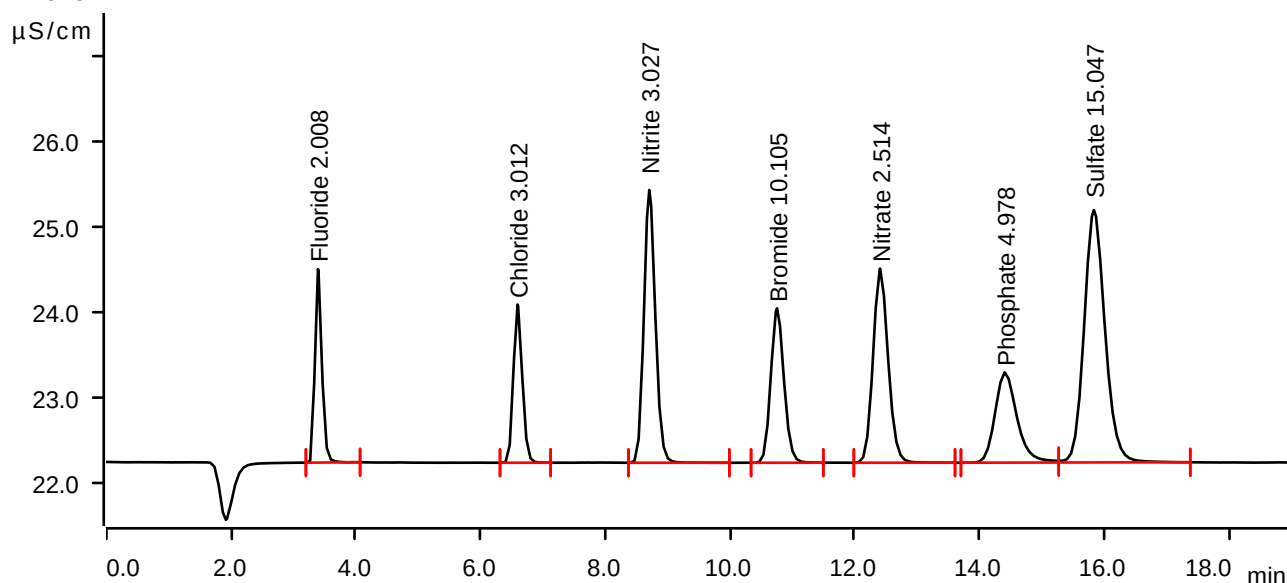

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.393	0.2933	2.266	2.008	Fluoride
2	6.593	0.3075	1.854	3.012	Chloride
3	8.705	0.6805	3.195	3.027	Nitrite
4	10.753	0.4432	1.809	10.105	Bromide
5	12.407	0.6363	2.273	2.514	Nitrate
6	14.405	0.4310	1.057	4.978	Phosphate
7	15.833	1.1470	2.956	15.047	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-09-09 13:58:07 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

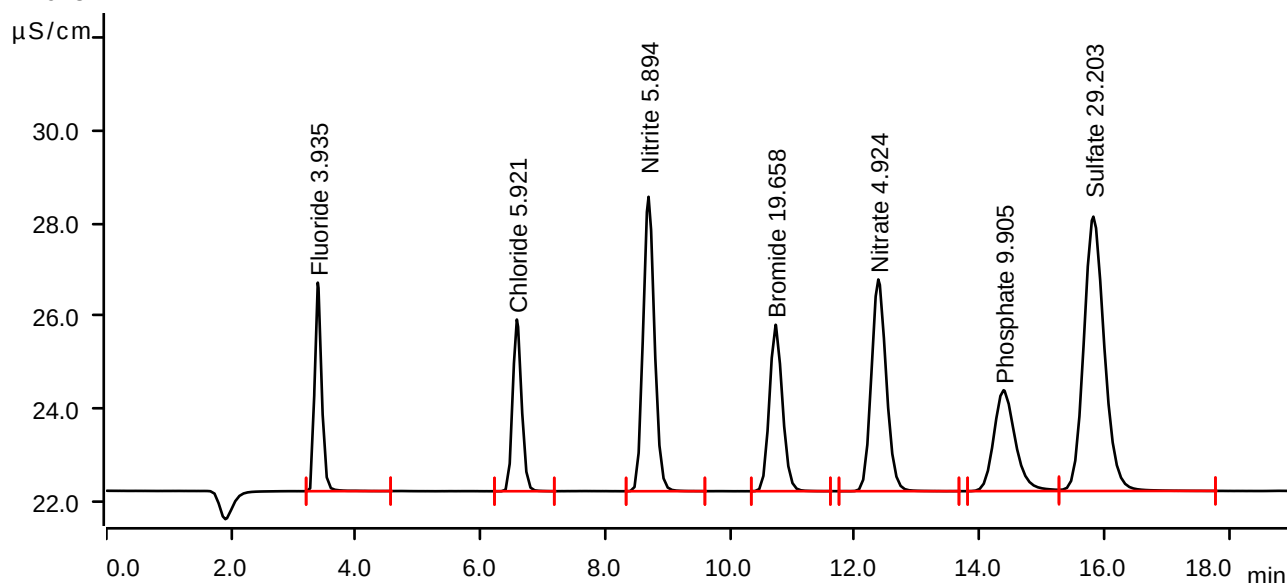

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.390	0.5787	4.477	3.935	Fluoride
2	6.582	0.6073	3.687	5.921	Chloride
3	8.693	1.3385	6.323	5.894	Nitrite
4	10.730	0.8677	3.574	19.658	Bromide
5	12.377	1.2581	4.546	4.924	Nitrate
6	14.385	0.8642	2.167	9.905	Phosphate
7	15.825	2.2540	5.893	29.203	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-09-09 14:41:06 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

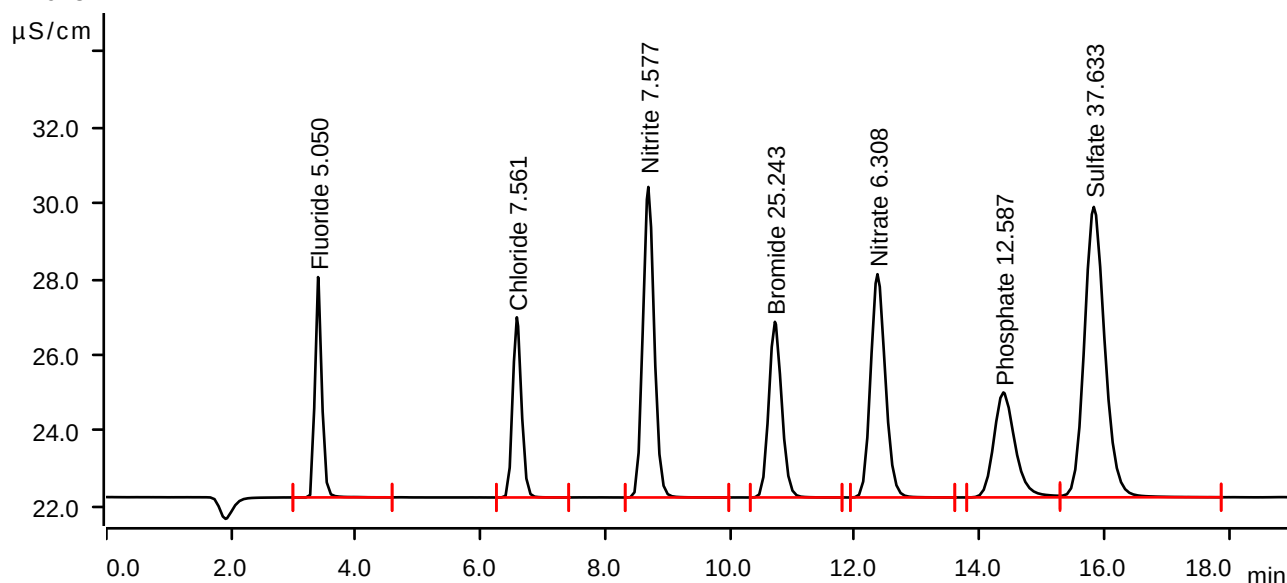

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.395	0.7438	5.806	5.050	Fluoride
2	6.582	0.7764	4.748	7.561	Chloride
3	8.690	1.7250	8.184	7.577	Nitrite
4	10.718	1.1158	4.629	25.243	Bromide
5	12.363	1.6152	5.884	6.308	Nitrate
6	14.382	1.1001	2.766	12.587	Phosphate
7	15.832	2.9131	7.654	37.633	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-09-09 15:02:34 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.50 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

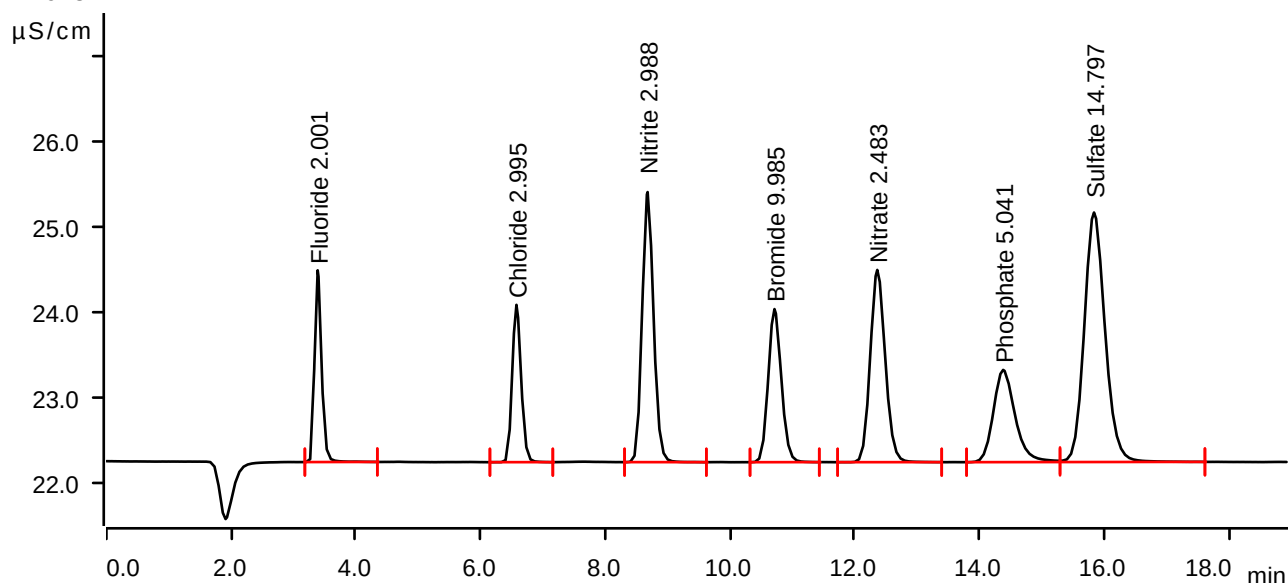

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.388	0.2923	2.246	2.001	Fluoride
2	6.575	0.3057	1.843	2.995	Chloride
3	8.678	0.6715	3.164	2.988	Nitrite
4	10.712	0.4379	1.793	9.985	Bromide
5	12.360	0.6282	2.252	2.483	Nitrate
6	14.378	0.4365	1.080	5.041	Phosphate
7	15.835	1.1275	2.923	14.797	Sulfate


Sample data

Ident ICB
Sample type Sample
Determination start 2025-09-09 15:45:30 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

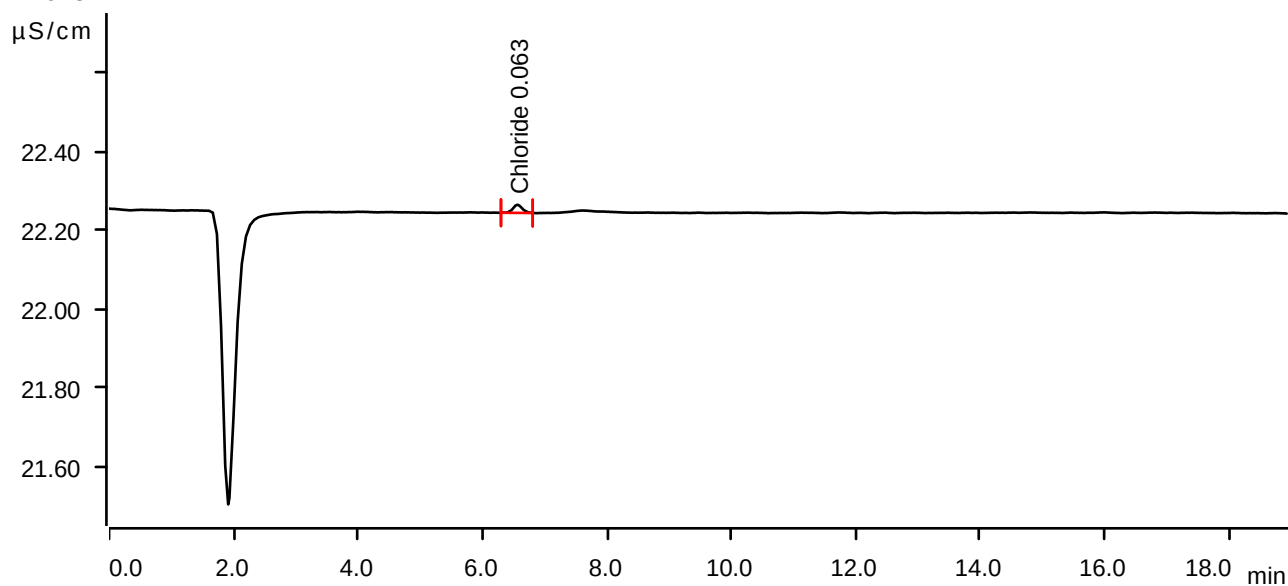

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.568	0.0036	0.021	0.063	Chloride


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-09-30 11:13:26 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 13.18 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

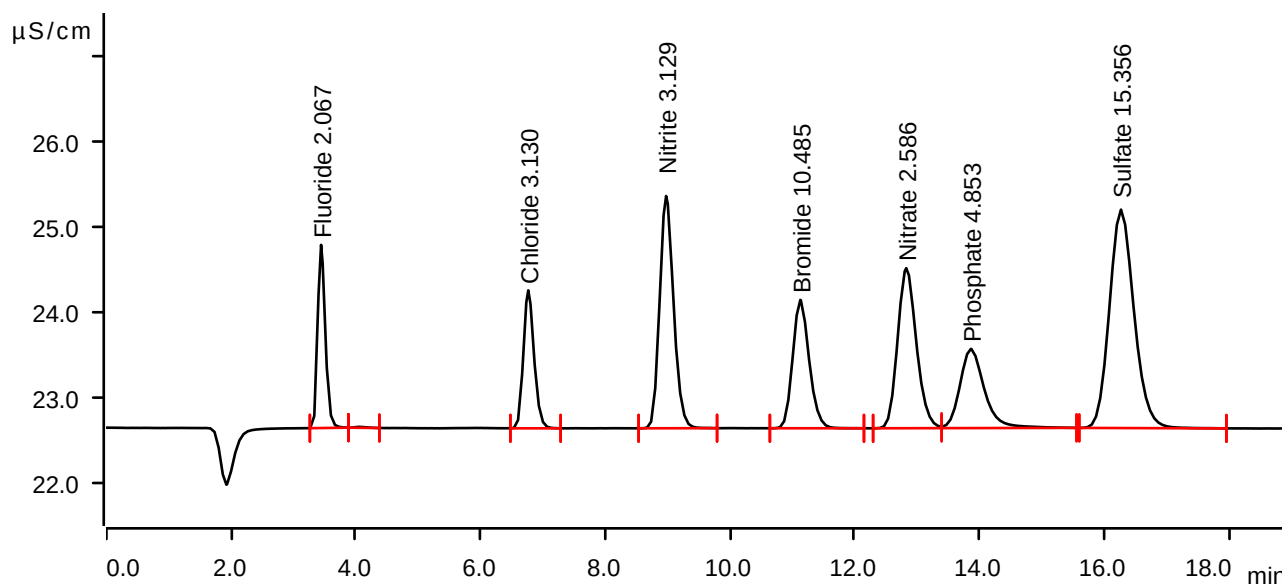


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.443	0.3021	2.145	2.067	Fluoride
2	4.052	0.0022	0.010	invalid	
3	6.765	0.3196	1.616	3.130	Chloride
4	8.975	0.7039	2.721	3.129	Nitrite
5	11.127	0.4602	1.504	10.485	Bromide
6	12.825	0.6550	1.875	2.586	Nitrate
7	13.862	0.4200	0.928	4.853	Phosphate
8	16.267	1.1712	2.558	15.356	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-09-30 11:34:57 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 13.06 MPa
Maximum pressure monitored yes
Temperature ---- °C

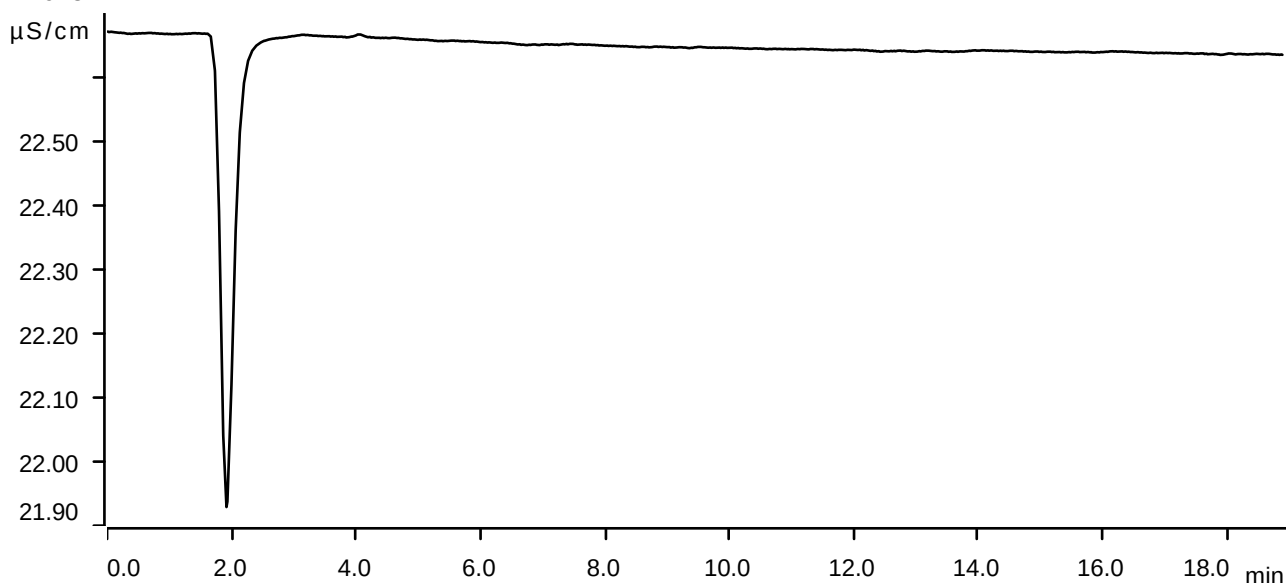Anions


Sample data

Ident LB137383BLW
Sample type Sample
Determination start 2025-09-30 11:56:28 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 13.06 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

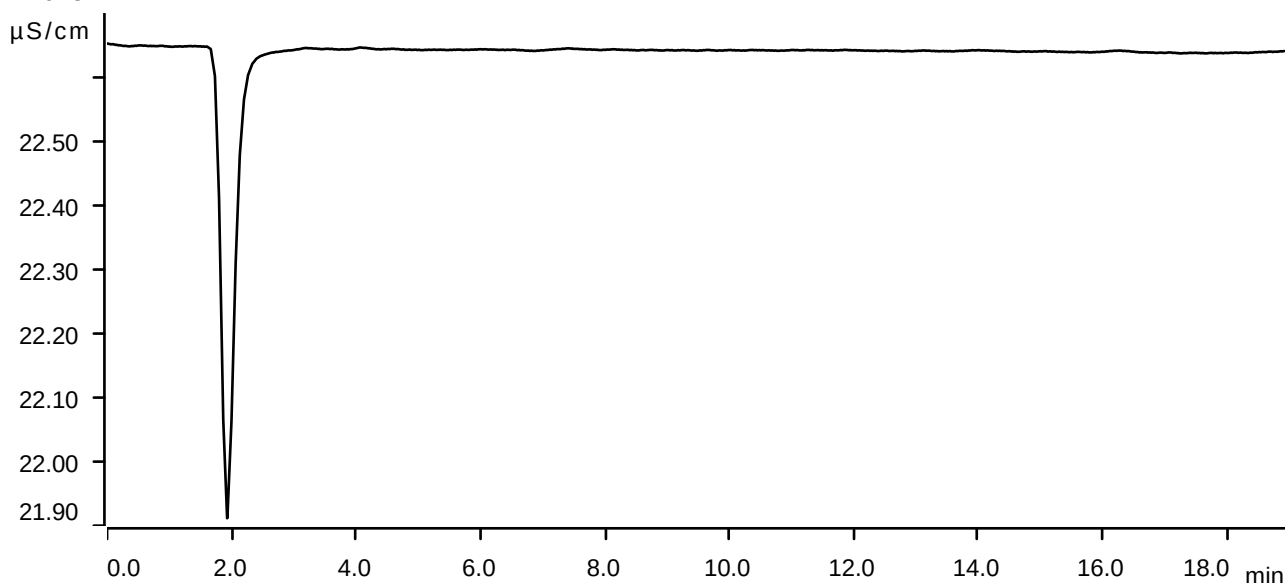


Sample data

Ident LB137383BSW
Sample type Check standard 1
Determination start 2025-09-30 12:17:59 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 13.06 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

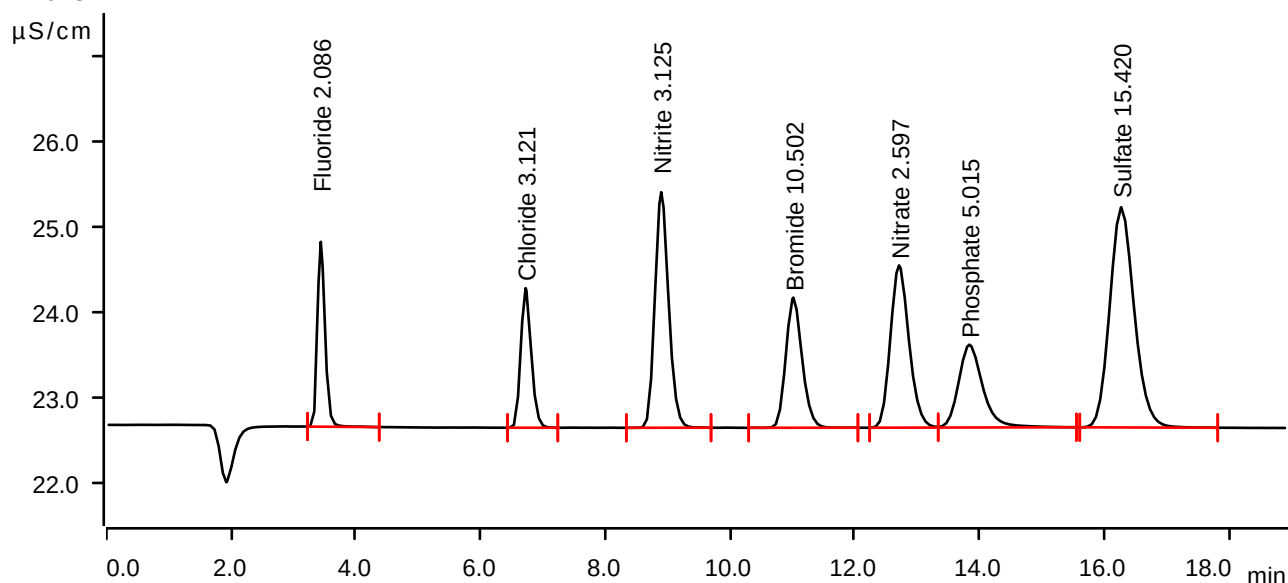

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.438	0.3049	2.165	2.086	Fluoride
2	6.722	0.3187	1.636	3.121	Chloride
3	8.897	0.7031	2.759	3.125	Nitrite
4	11.015	0.4609	1.524	10.502	Bromide
5	12.708	0.6579	1.901	2.597	Nitrate
6	13.835	0.4343	0.970	5.015	Phosphate
7	16.272	1.1762	2.579	15.420	Sulfate


Sample data

Ident Q3254-01
Sample type Sample
Determination start 2025-09-30 13:41:45 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 13.12 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

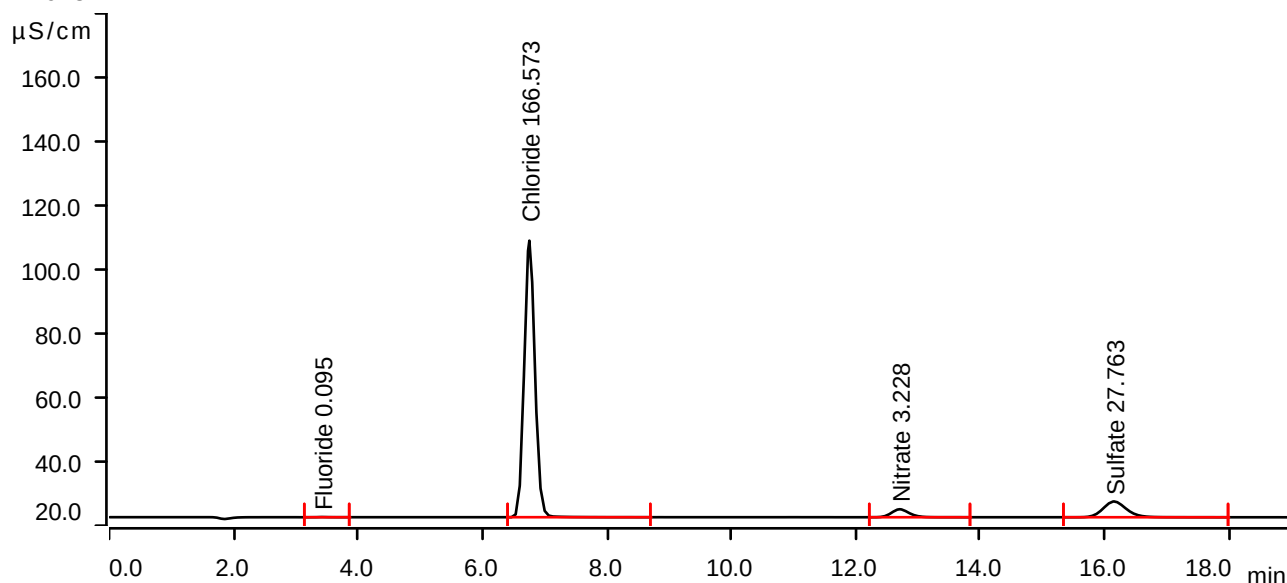

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.423	0.0102	0.059	0.095	Fluoride
2	6.755	17.1653	86.391	166.573	Chloride
3	12.707	0.8206	2.496	3.228	Nitrate
4	16.150	2.1414	4.933	27.763	Sulfate


Sample data

Ident Q3254-01MS
Sample type Sample
Determination start 2025-09-30 14:03:23 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 13.06 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

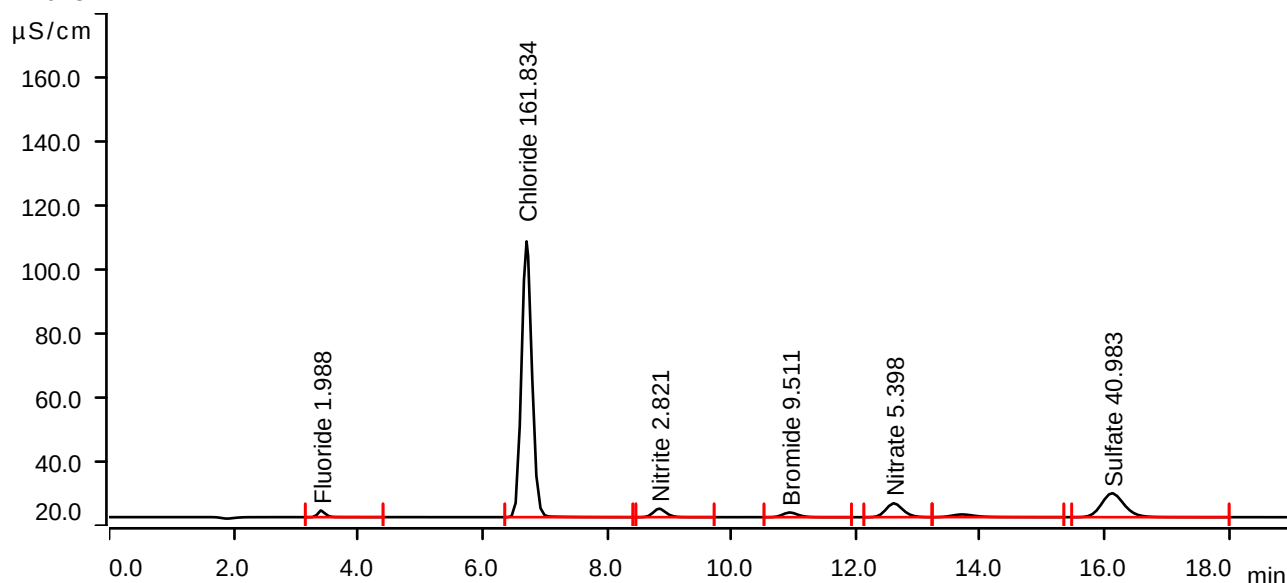

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.408	0.2904	2.082	1.988	Fluoride
2	6.710	16.6769	86.143	161.834	Chloride
3	8.842	0.6331	2.642	2.821	Nitrite
4	10.940	0.4169	1.474	9.511	Bromide
5	12.612	1.3804	4.324	5.398	Nitrate
6	13.708	0.3634	0.842	invalid	
7	16.118	3.1751	7.462	40.983	Sulfate


Sample data

Ident Q3254-01MSD
Sample type Sample
Determination start 2025-09-30 14:24:57 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.89 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

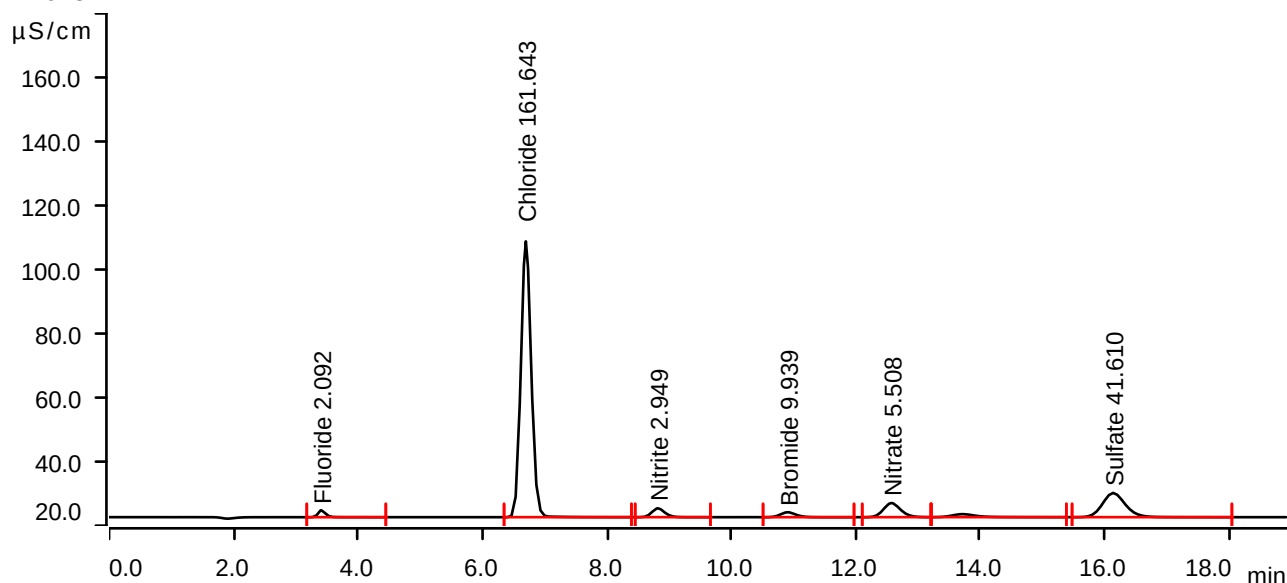

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.412	0.3058	2.179	2.092	Fluoride
2	6.698	16.6572	86.162	161.643	Chloride
3	8.820	0.6626	2.768	2.949	Nitrite
4	10.905	0.4359	1.543	9.939	Bromide
5	12.573	1.4088	4.419	5.508	Nitrate
6	13.715	0.4092	0.942	invalid	
7	16.137	3.2241	7.564	41.610	Sulfate


Sample data

Ident Q3254-03
Sample type Sample
Determination start 2025-09-30 14:46:32 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.89 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

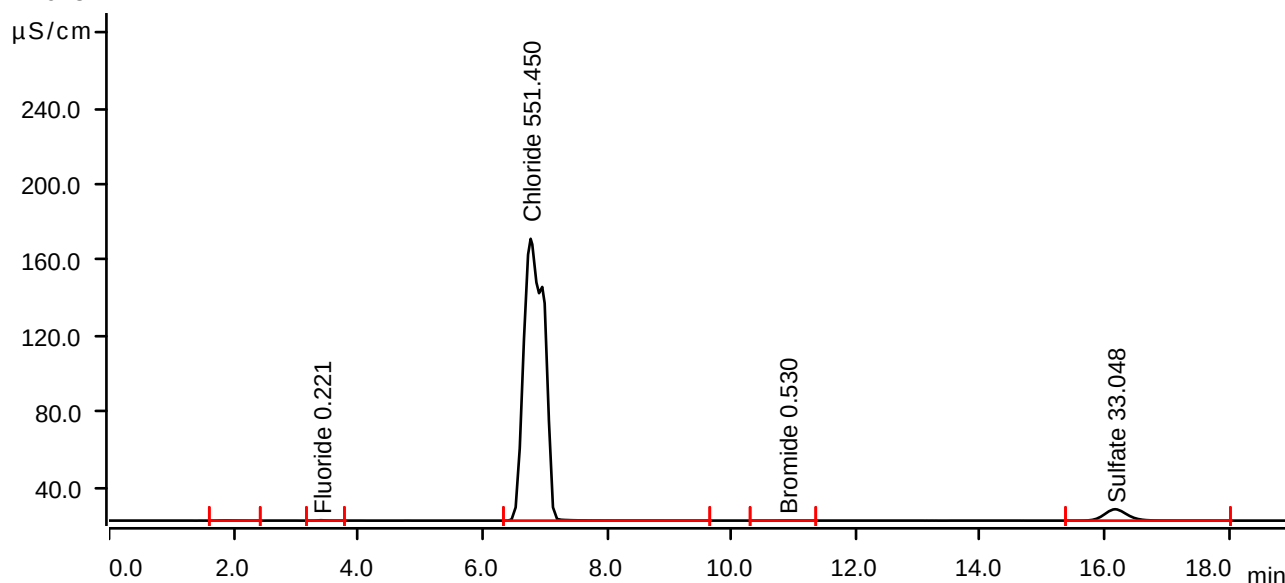

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.867	0.0362	0.125	invalid	
2	3.407	0.0288	0.200	0.221	Fluoride
3	6.775	56.8337	148.573	551.450	Chloride
4	10.895	0.0179	0.063	0.530	Bromide
5	16.167	2.5547	5.996	33.048	Sulfate


Sample data

Ident Q3254-05
Sample type Sample
Determination start 2025-09-30 15:08:07 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.84 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

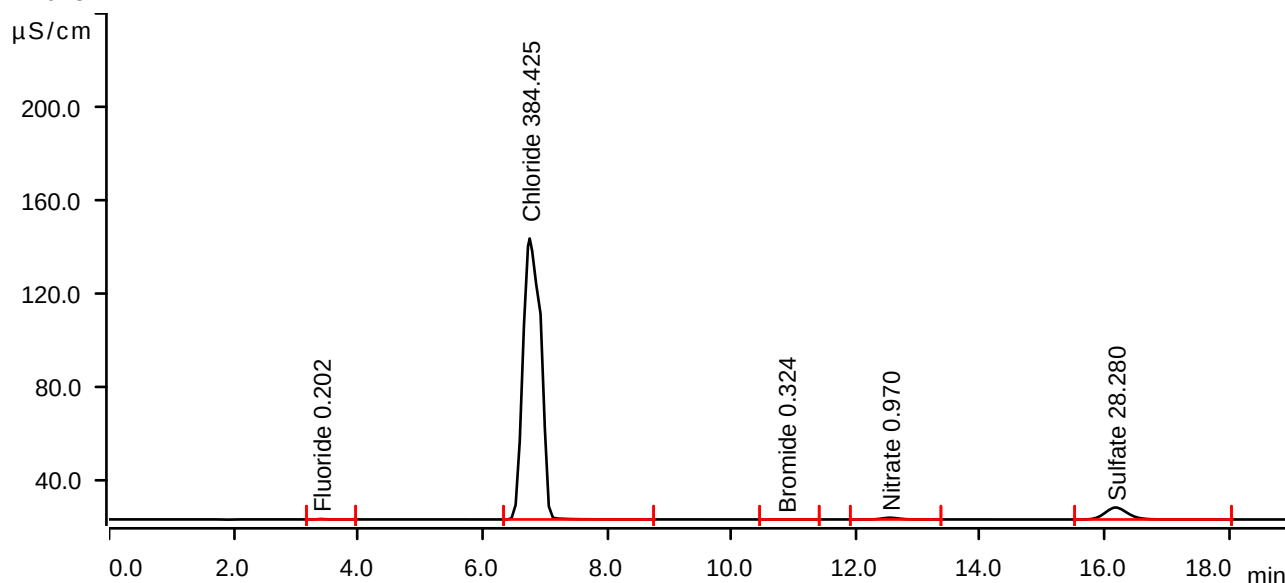

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.405	0.0260	0.175	0.202	Fluoride
2	6.760	39.6188	120.684	384.425	Chloride
3	10.877	0.0087	0.030	0.324	Bromide
4	12.548	0.2379	0.745	0.970	Nitrate
5	16.175	2.1818	5.150	28.280	Sulfate


Sample data

Ident Q3254-07
Sample type Sample
Determination start 2025-09-30 15:29:42 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 13.06 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

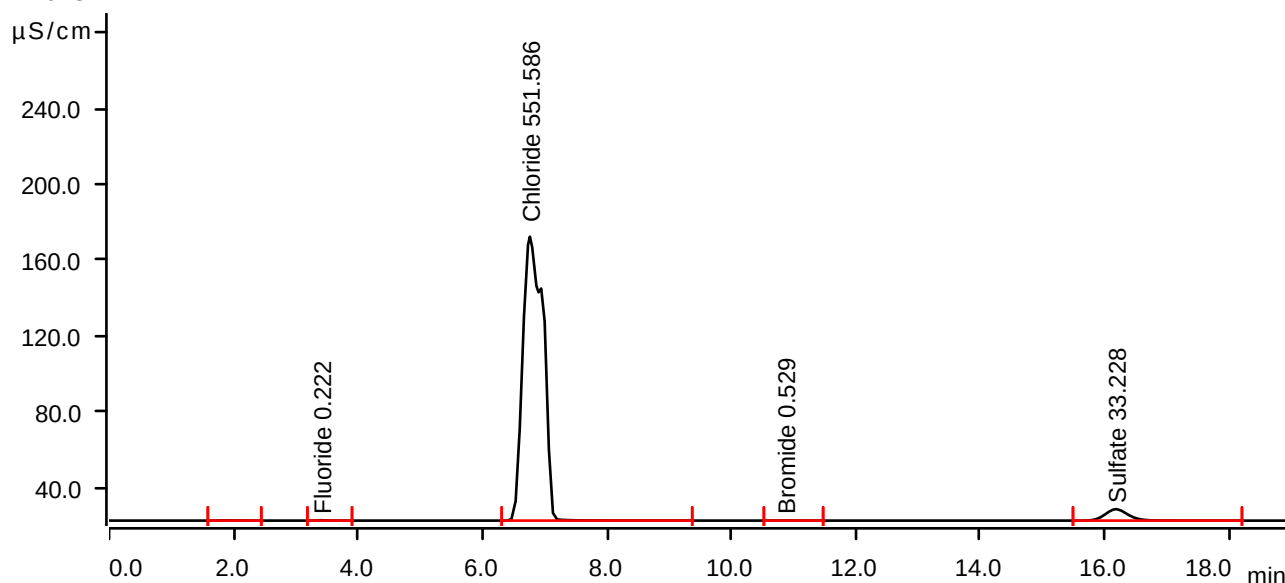

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.873	0.0363	0.125	invalid	
2	3.410	0.0290	0.199	0.222	Fluoride
3	6.763	56.8477	149.679	551.586	Chloride
4	10.865	0.0178	0.062	0.529	Bromide
5	16.180	2.5687	6.022	33.228	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-09-30 15:51:16 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.95 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

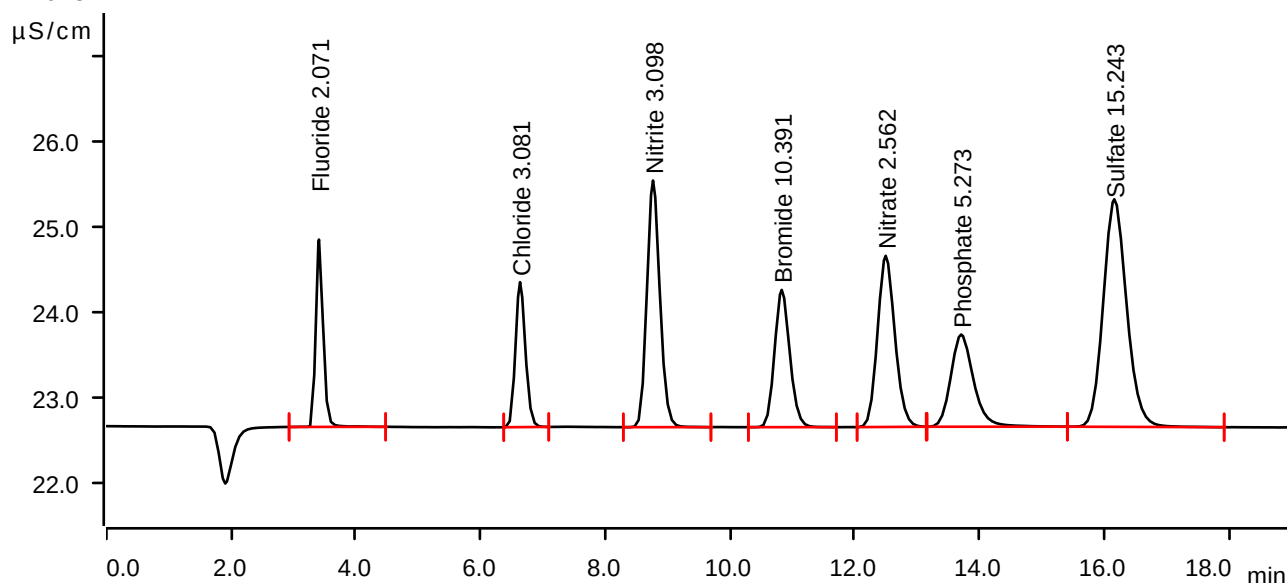


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.410	0.3027	2.194	2.071	Fluoride
2	6.633	0.3145	1.698	3.081	Chloride
3	8.765	0.6967	2.889	3.098	Nitrite
4	10.828	0.4560	1.608	10.391	Bromide
5	12.495	0.6487	2.005	2.562	Nitrate
6	13.705	0.4569	1.080	5.273	Phosphate
7	16.160	1.1623	2.666	15.243	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-09-30 16:12:46 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.67 MPa
Maximum pressure monitored yes
Temperature ---- °C

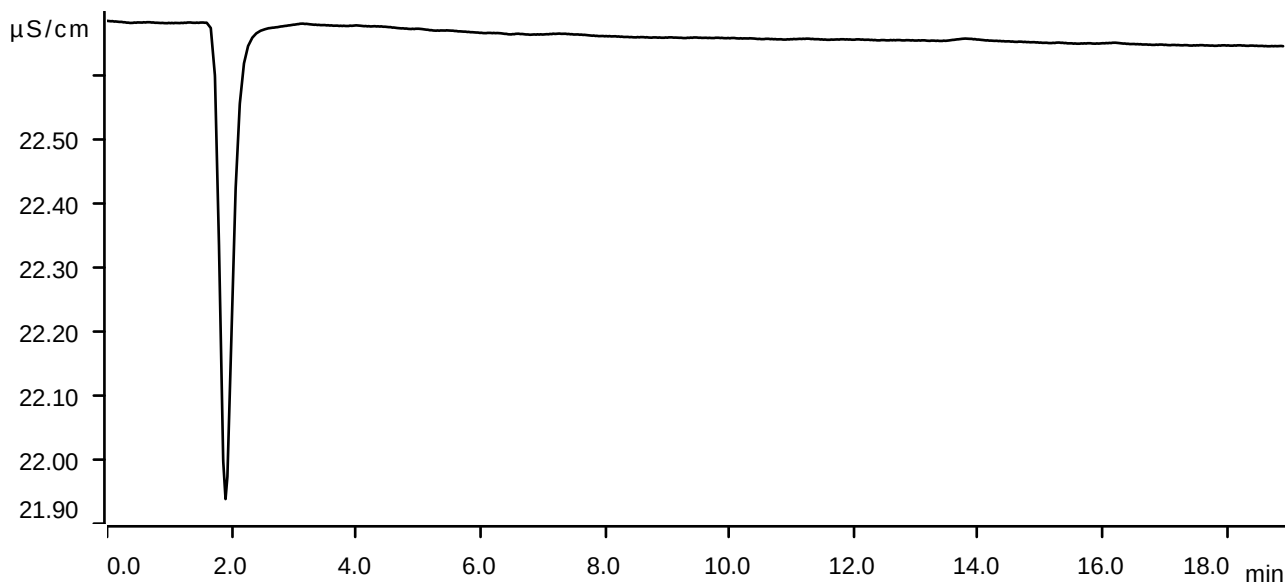Anions


Sample data

Ident Q3254-01DLX50
Sample type Sample
Determination start 2025-09-30 16:34:16 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 13.01 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

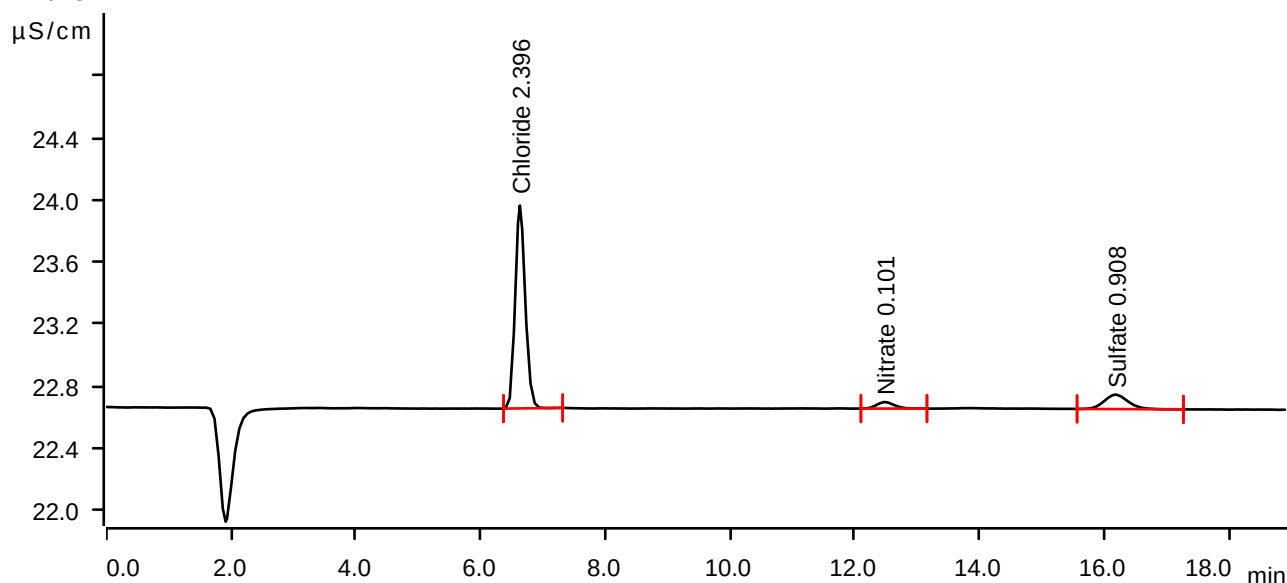

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.630	0.2440	1.307	2.396	Chloride
2	12.475	0.0138	0.042	0.101	Nitrate
3	16.185	0.0415	0.093	0.908	Sulfate


Sample data

Ident Q3254-03DLX100
Sample type Sample
Determination start 2025-09-30 16:55:49 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 13.06 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

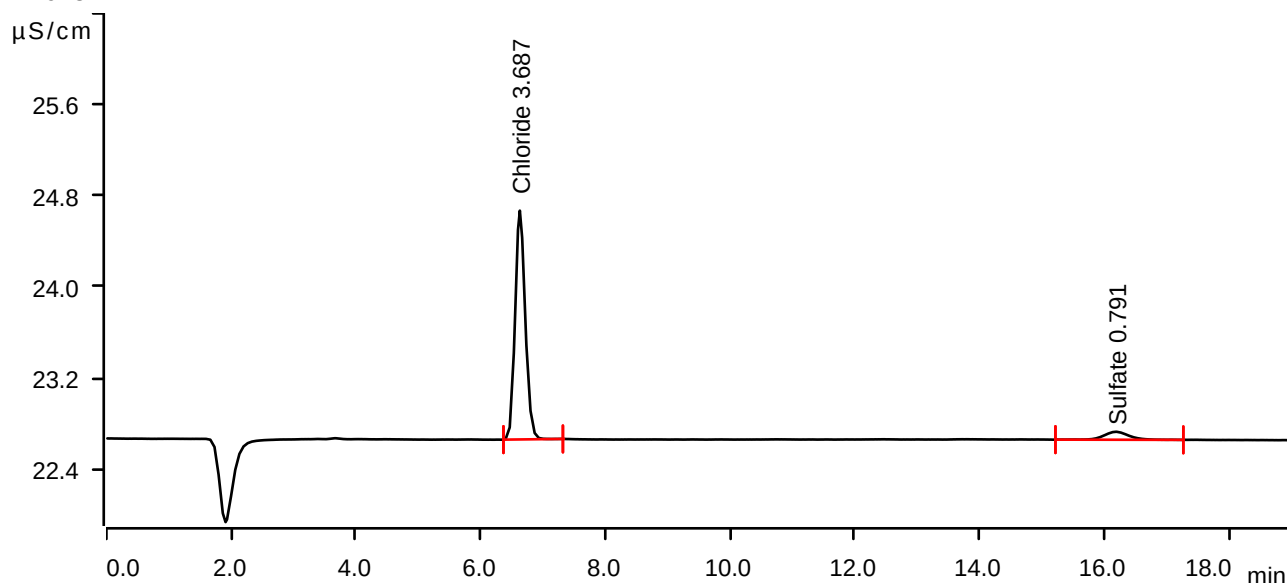

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.630	0.3770	2.010	3.687	Chloride
2	16.190	0.0323	0.070	0.791	Sulfate


Sample data

Ident Q3254-05DLX100
Sample type Sample
Determination start 2025-09-30 18:00:11 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.67 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

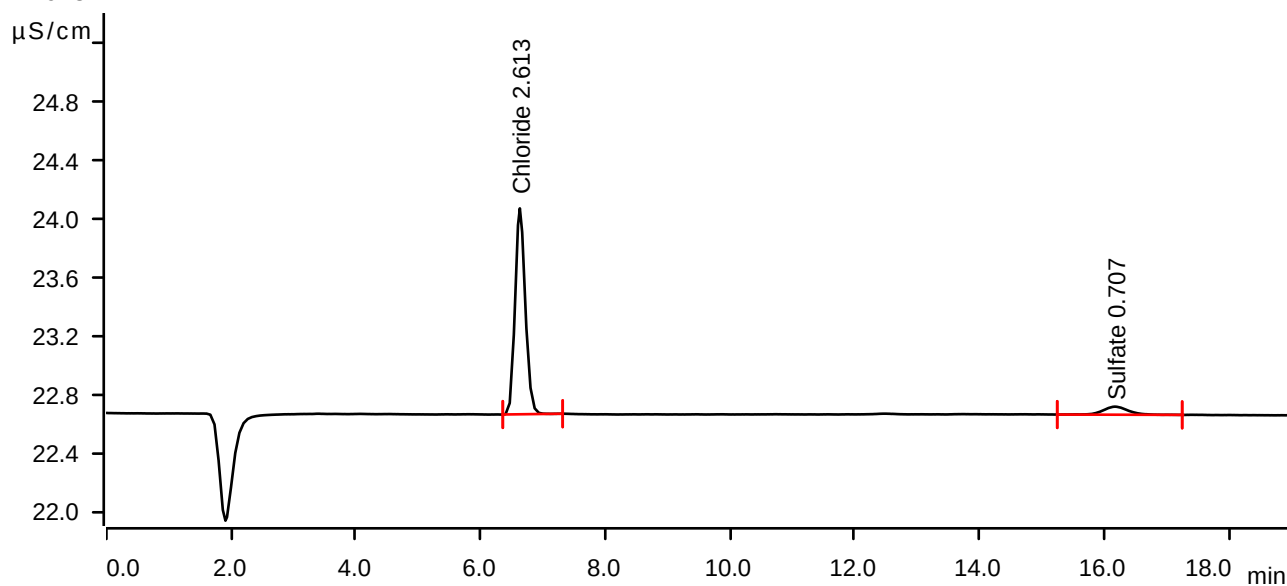

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.630	0.2664	1.407	2.613	Chloride
2	16.172	0.0257	0.055	0.707	Sulfate


Sample data

Ident Q3254-07DLX100
Sample type Sample
Determination start 2025-09-30 18:21:42 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.78 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

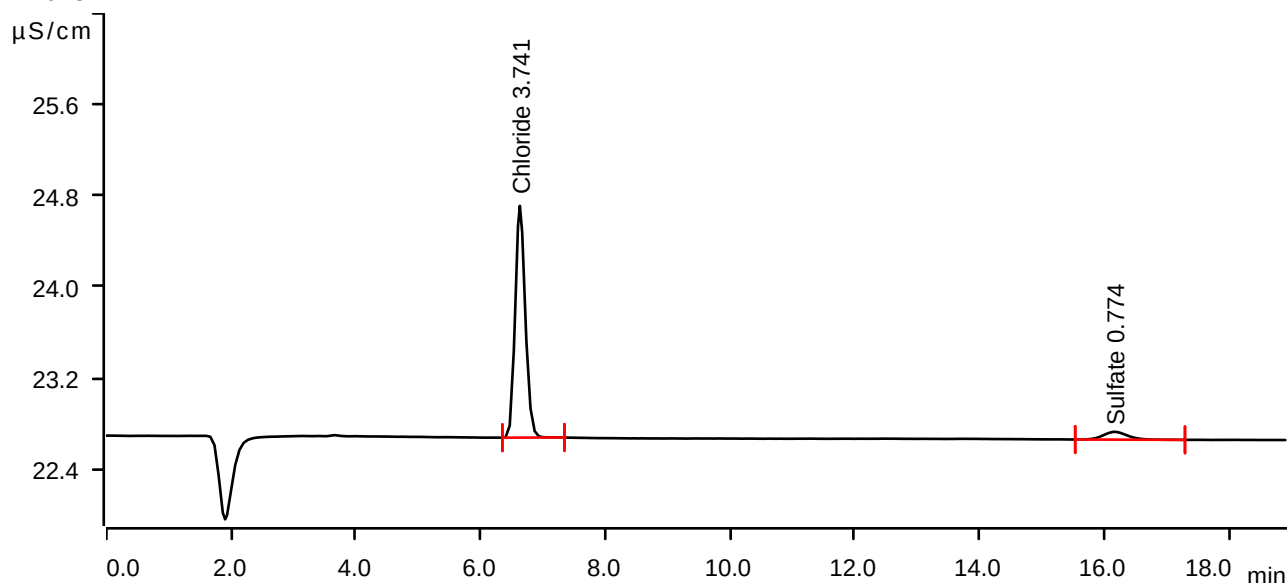

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.630	0.3826	2.036	3.741	Chloride
2	16.160	0.0310	0.069	0.774	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-09-30 19:04:41 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.73 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

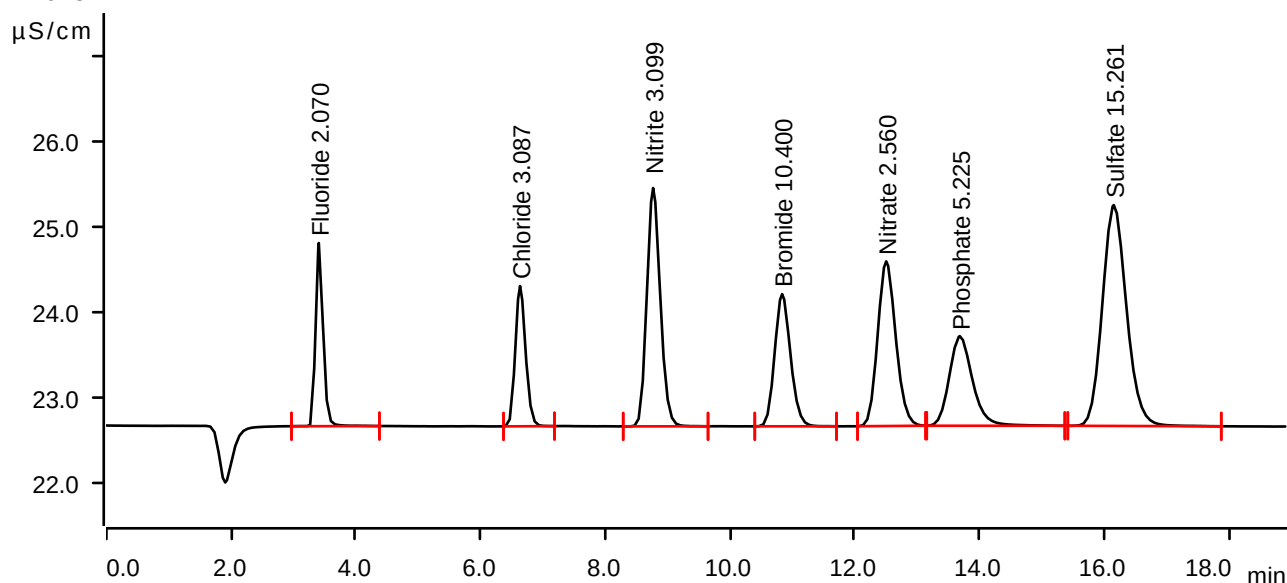

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.407	0.3026	2.145	2.070	Fluoride
2	6.633	0.3151	1.643	3.087	Chloride
3	8.767	0.6970	2.792	3.099	Nitrite
4	10.835	0.4564	1.549	10.400	Bromide
5	12.503	0.6481	1.929	2.560	Nitrate
6	13.685	0.4528	1.050	5.225	Phosphate
7	16.152	1.1638	2.588	15.261	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2025-09-30 19:26:12 UTC-4
Method IC1-090925
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.84 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

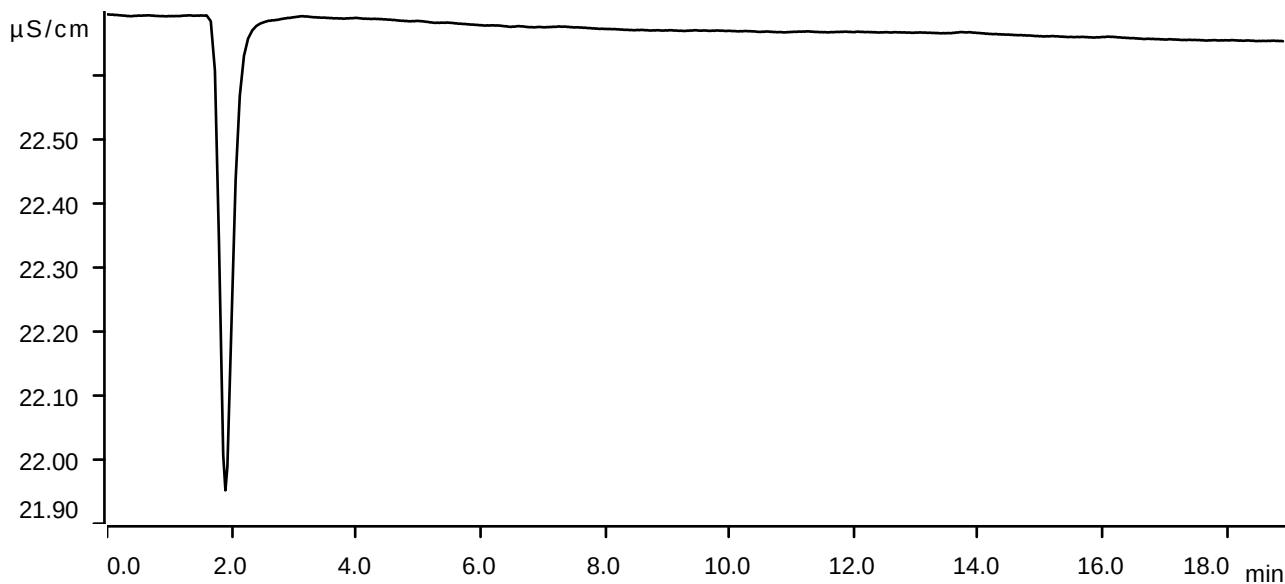

WORKLIST(Hardcopy Internal Chain)

LB 137383

WorkList Name : Anions-093025

WorkList ID : 192180

Department : Wet-Chemistry

Date : 09-30-2025 13:15:47

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q3254-01	MW-1	Water	Anions Group1	Cool 4 deg C	LOCK01	D31	09/29/2025	300.0
Q3254-03	MW-2	Water	Anions Group1	Cool 4 deg C	LOCK01	D31	09/29/2025	300.0
Q3254-05	MW-3	Water	Anions Group1	Cool 4 deg C	LOCK01	D31	09/29/2025	300.0
Q3254-07	MW-4	Water	Anions Group1	Cool 4 deg C	LOCK01	D31	09/29/2025	300.0

Date/Time 09/30/25 13:25
 Raw Sample Received by: 12(wc)
 Raw Sample Relinquished by: 20(wc)

Date/Time 09/30/25 14:20
 Raw Sample Received by: 20(wc)
 Raw Sample Relinquished by: 12(wc)