
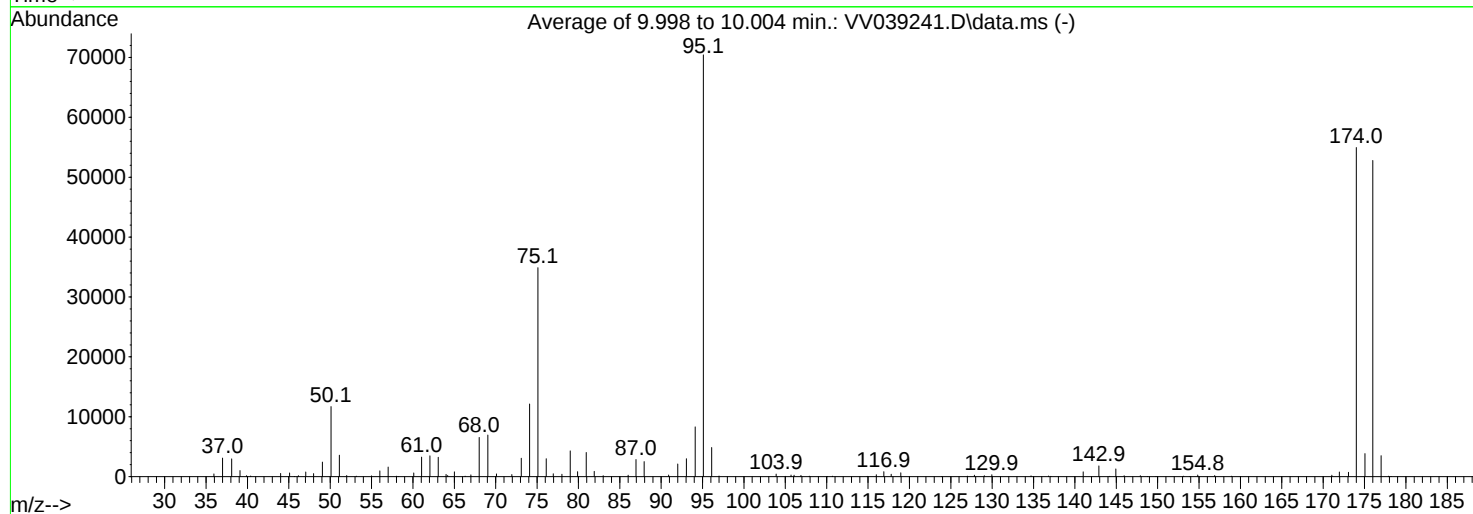


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100325\
Data File : VV039241.D
Acq On : 03 Oct 2025 08:26
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V092225W.M
Title : SW846 8260
Last Update : Wed Sep 24 08:08:08 2025

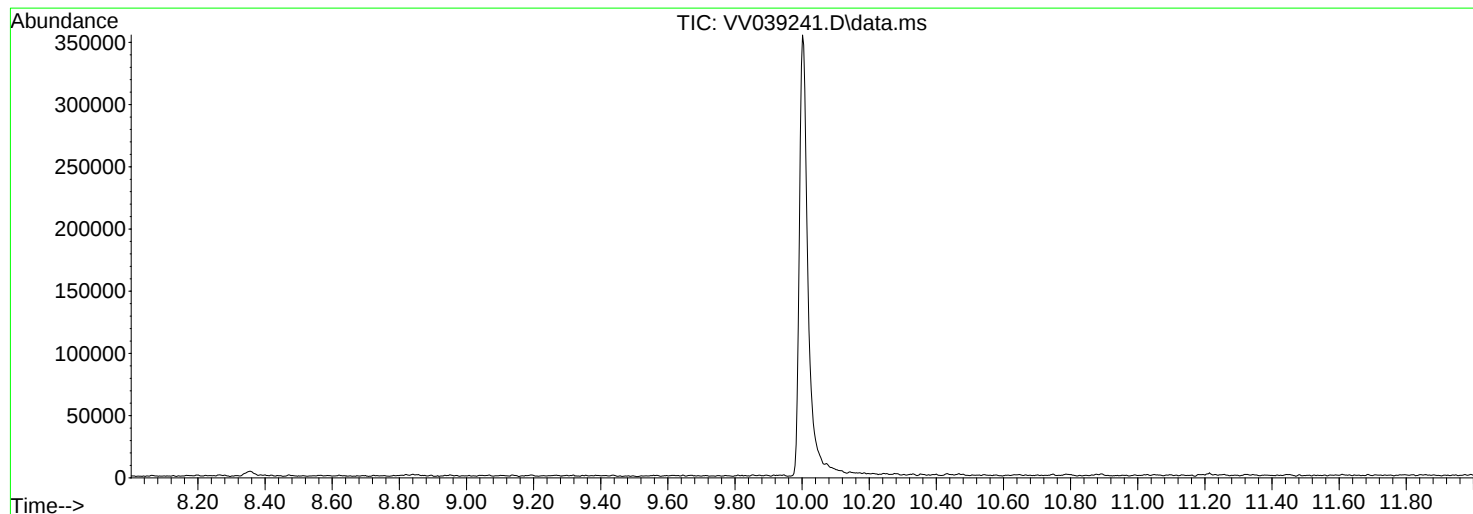

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.6	11702	PASS
75	95	30	60	49.5	34896	PASS
95	95	100	100	100.0	70432	PASS
96	95	5	9	6.9	4879	PASS
173	174	0.00	2	1.3	733	PASS
174	95	50	100	78.0	54968	PASS
175	174	5	9	7.0	3851	PASS
176	174	95	101	96.0	52784	PASS
177	176	5	9	6.6	3489	PASS