


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100125\
Data File : BP025900.D
Acq On : 01 Oct 2025 14:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 11 16:45:04 2025

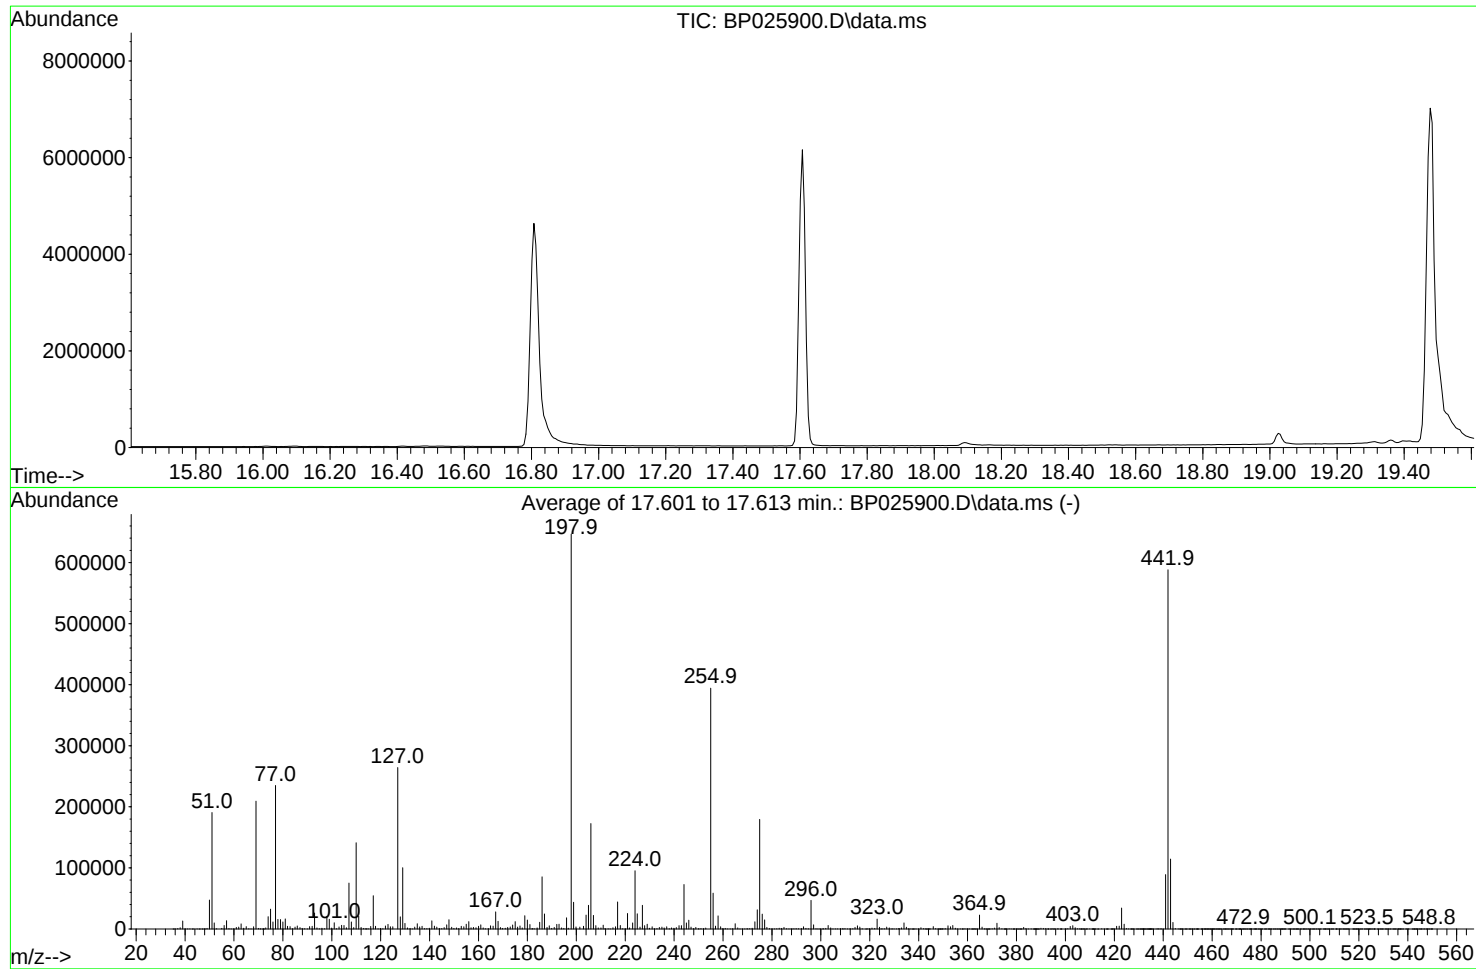




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2485

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	3503	PASS
69	69	100	100	100.0	209399	PASS
70	69	0.00	2	0.4	889	PASS
197	198	0.00	2	0.2	1235	PASS
198	198	100	100	100.0	646684	PASS
199	198	5	9	6.7	43570	PASS
365	198	1	100	3.5	22672	PASS
441	443	0.01	150	77.9	89072	PASS
442	442	100	100	100.0	588220	PASS
443	442	15	24	19.4	114301	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100125\
Data File : BP025900.D
Acq On : 01 Oct 2025 14:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Oct 01 14:49:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

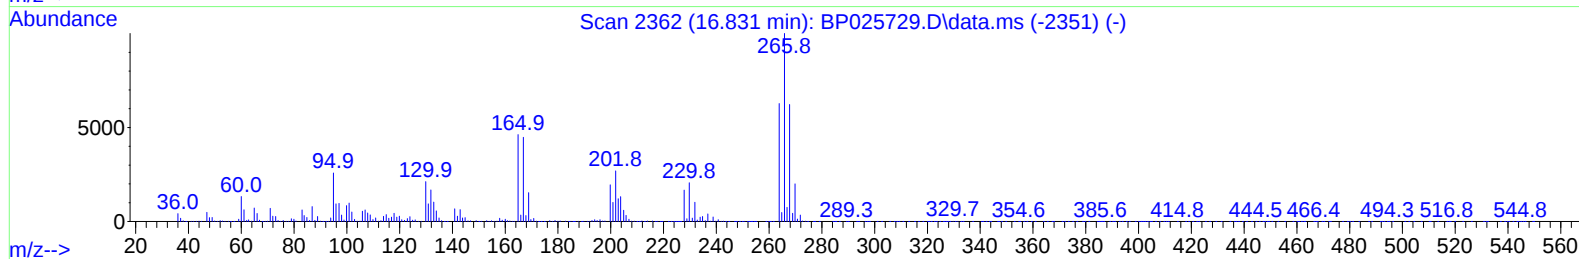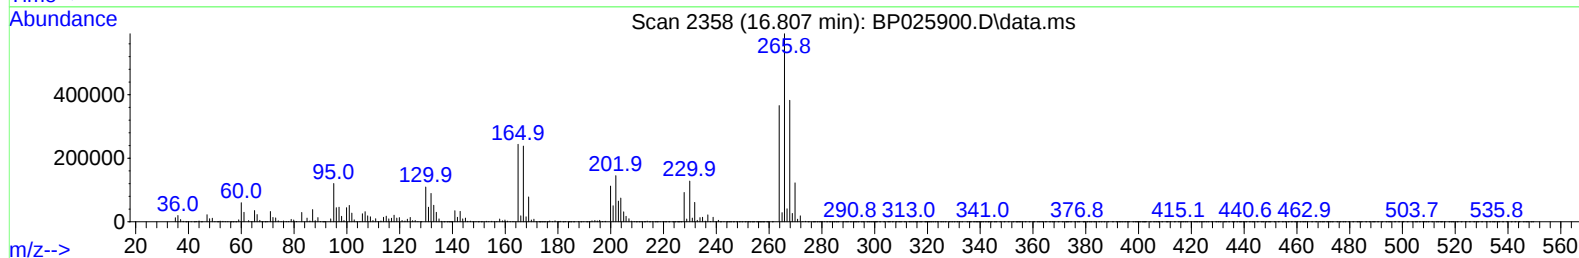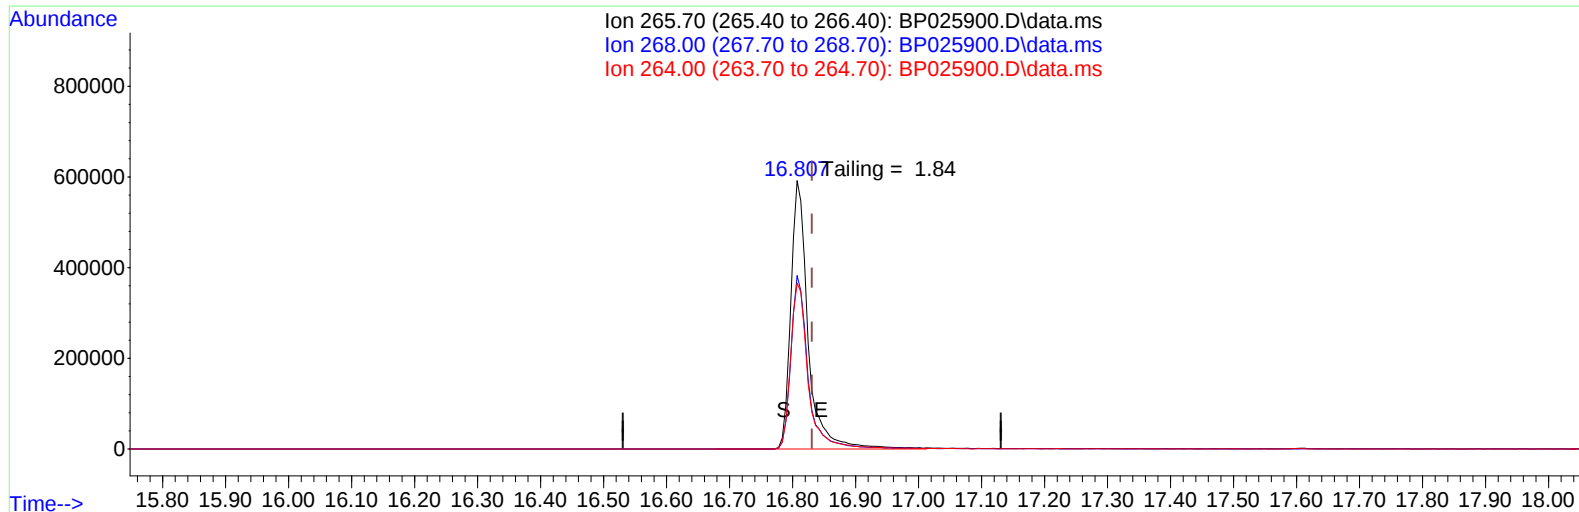

TIC: BP025900.D\data.ms

(70) Pentachlorophenol (C)

16.807min (-0.024) 6411668.82 ng




response 1140541

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.61
264.00	62.70	61.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100125\
Data File : BP025900.D
Acq On : 01 Oct 2025 14:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Oct 01 14:49:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

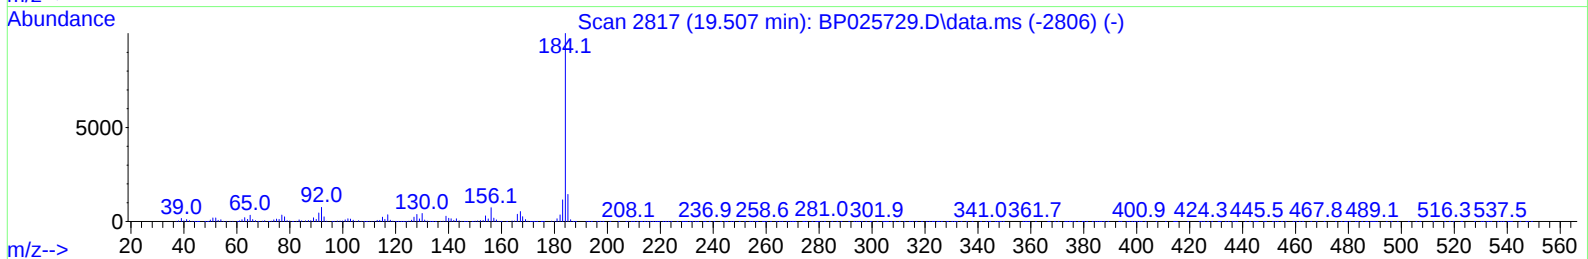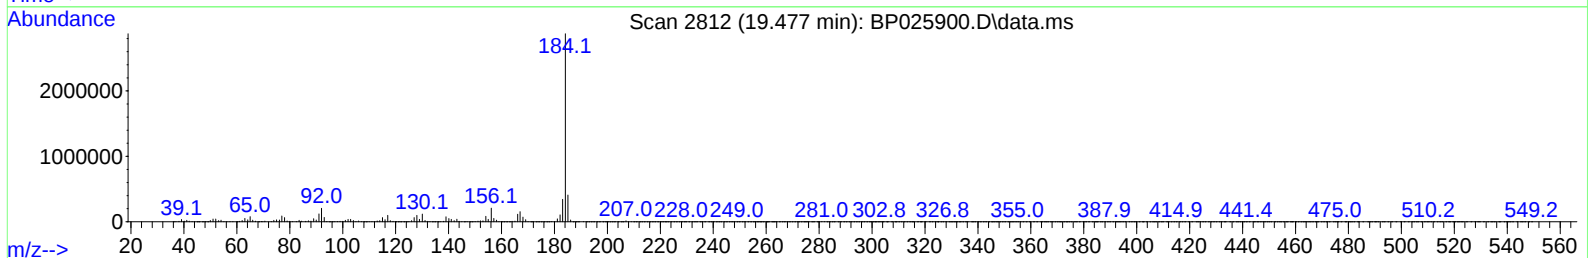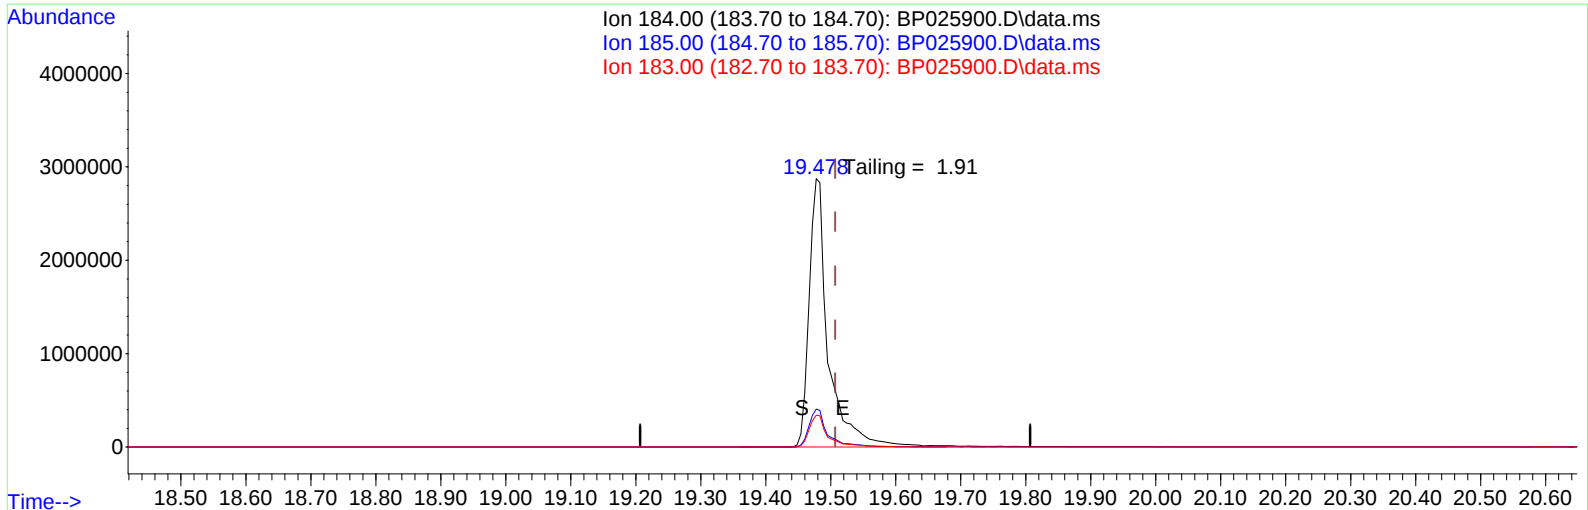

TIC: BP025900.D\data.ms

(77) Benzidine

19.477min (-0.029) 106666.91 ng

response 5893204

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.17
183.00	11.50	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/1/2025	BNA_P	<u>BP025900.D</u>
Compound Name	Response	Retention Time
DDT	2500492	20.76
DDD	64248	20.307
DDE	13790	19.766
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
78038	2578530	3.03

Instrument :
BNA_P
ClientSampleId :
DFTPP