

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100125\
 Data File : BP025902.D
 Acq On : 01 Oct 2025 15:49
 Operator : CG/JU
 Sample : PB169936BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB169936BL

Quant Time: Oct 01 16:12:27 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 11 16:45:04 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.743	152	202580	20.000	ng	-0.02
21) Naphthalene-d8	10.507	136	767867	20.000	ng	-0.02
39) Acenaphthene-d10	14.354	164	474978	20.000	ng	-0.02
64) Phenanthrene-d10	17.160	188	939544	20.000	ng	-0.02
76) Chrysene-d12	21.613	240	929664	20.000	ng	-0.03
86) Perylene-d12	24.960	264	989236	20.000	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.384	112	1857870	147.979	ng	0.00
7) Phenol-d6	6.949	99	2291905	137.340	ng	0.00
23) Nitrobenzene-d5	8.890	82	1467343	84.293	ng	-0.01
42) 2,4,6-Tribromophenol	15.872	330	908244	153.306	ng	-0.04
45) 2-Fluorobiphenyl	12.960	172	3207426	89.914	ng	-0.03
79) Terphenyl-d14	19.877	244	4828161	93.429	ng	-0.04


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100125\
Data File : BP025902.D
Acq On : 01 Oct 2025 15:49
Operator : CG/JU
Sample : PB169936BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB169936BL

Quant Time: Oct 01 16:12:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration




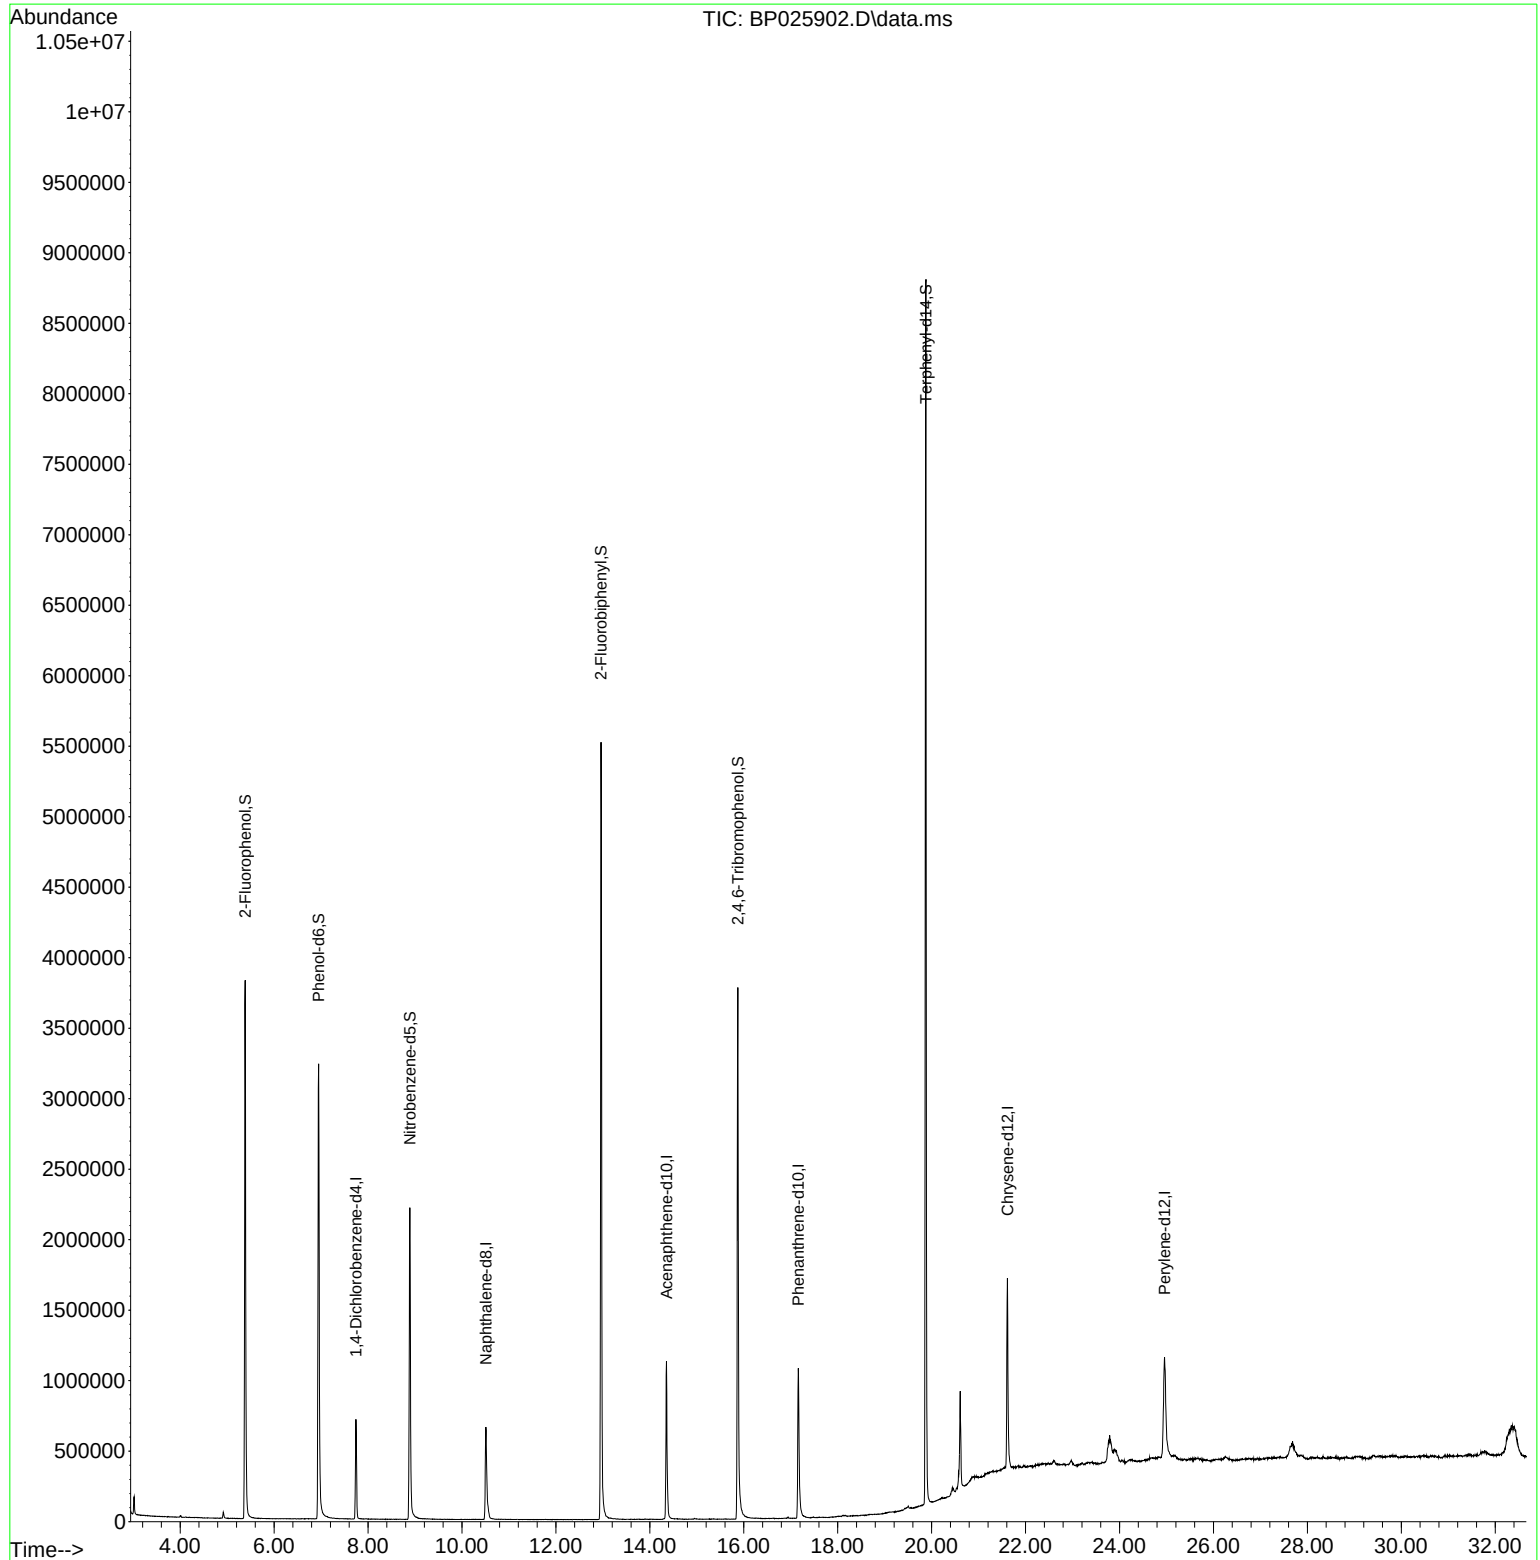




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.743 min Scan# 81
Delta R.T. -0.017 min
Lab File: BP025902.D
Acq: 01 Oct 2025 15:49




Instrument :
BNA_P
ClientSampleId :
PB169936BL


Tgt Ion:152 Resp: 202580
Ion Ratio Lower Upper
152 100
150 157.8 124.3 186.5
115 64.5 50.3 75.5

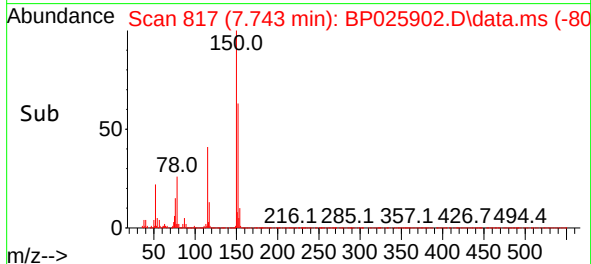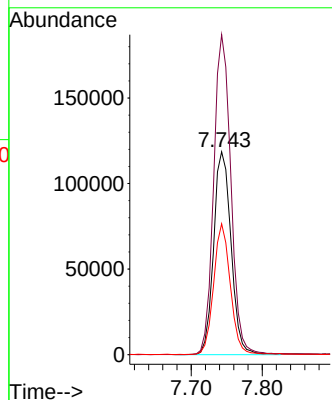

#5
2-Fluorophenol
Concen: 147.979 ng
RT: 5.384 min Scan# 416
Delta R.T. -0.000 min
Lab File: BP025902.D
Acq: 01 Oct 2025 15:49

Tgt Ion:112 Resp: 1857870
Ion Ratio Lower Upper
112 100
64 59.4 50.2 75.4
63 30.2 26.7 40.1


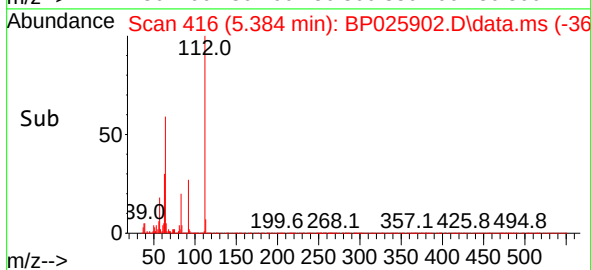
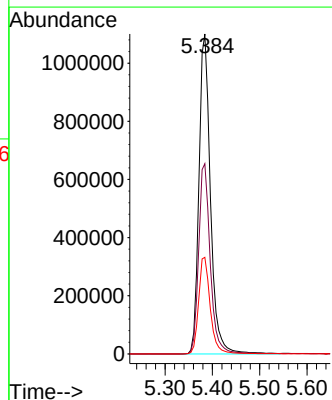
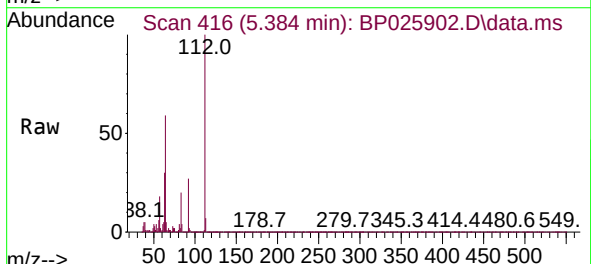




#7
Phenol-d6
Concen: 137.340 ng
RT: 6.949 min Scan# 682
Delta R.T. -0.000 min
Lab File: BP025902.D
Acq: 01 Oct 2025 15:49




Instrument :
BNA_P
ClientSampleId :
PB169936BL


Tgt Ion: 99 Resp: 2291905
Ion Ratio Lower Upper
99 100
42 16.9 15.6 23.4
71 35.4 28.6 43.0

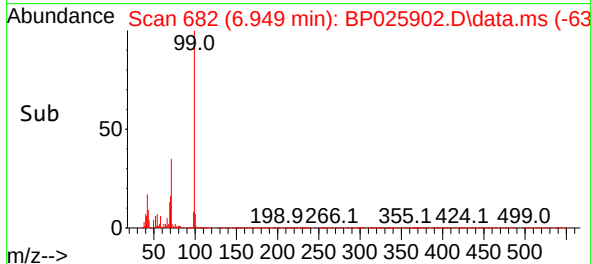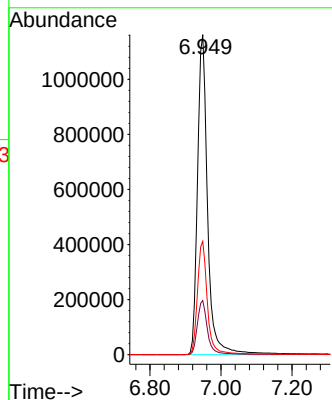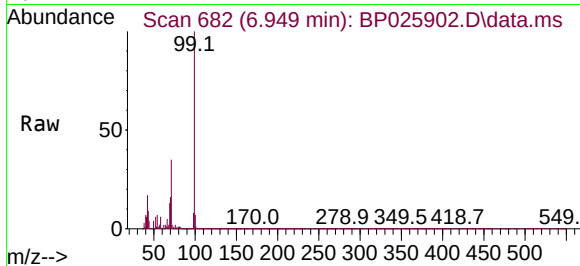

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.507 min Scan# 1287
Delta R.T. -0.018 min
Lab File: BP025902.D
Acq: 01 Oct 2025 15:49

Tgt Ion:136 Resp: 767867
Ion Ratio Lower Upper
136 100
137 10.9 8.7 13.1
54 8.8 7.5 11.3
68 5.8 5.0 7.6


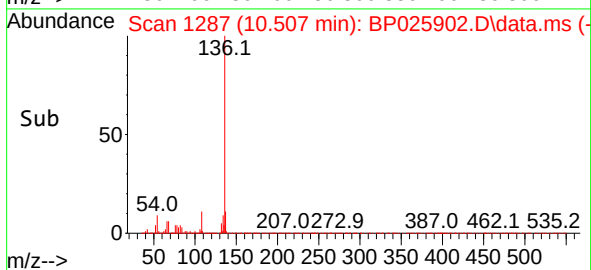
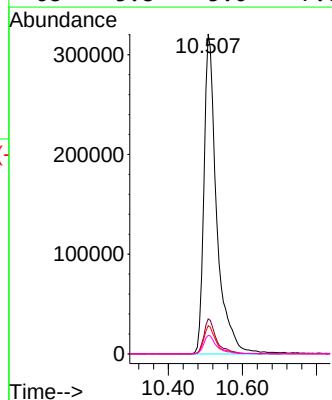
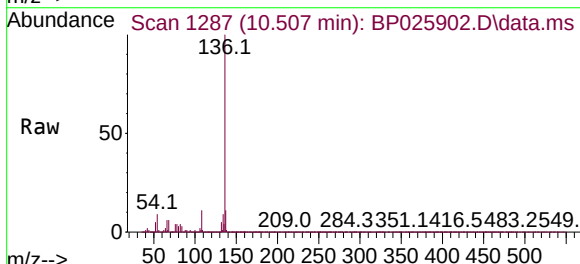




#23
Nitrobenzene-d5
Concen: 84.293 ng
RT: 8.890 min Scan# 1014
Delta R.T. -0.012 min
Lab File: BP025902.D
Acq: 01 Oct 2025 15:49




Instrument :
BNA_P
ClientSampleId :
PB169936BL


Tgt Ion: 82 Resp: 1467343
Ion Ratio Lower Upper
82 100
128 42.8 32.9 49.3
54 48.7 43.4 65.2

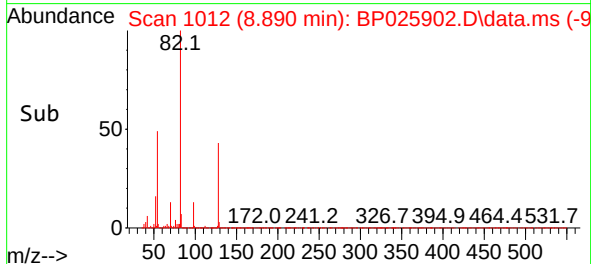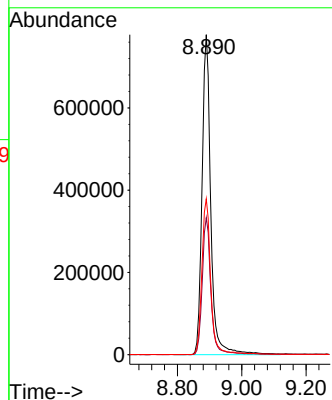

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.354 min Scan# 1941
Delta R.T. -0.024 min
Lab File: BP025902.D
Acq: 01 Oct 2025 15:49

Tgt Ion: 164 Resp: 474978
Ion Ratio Lower Upper
164 100
162 99.6 80.6 120.8
160 43.2 35.0 52.6

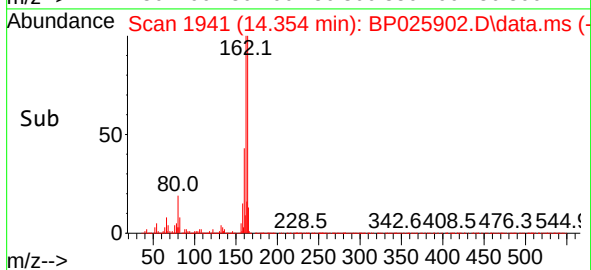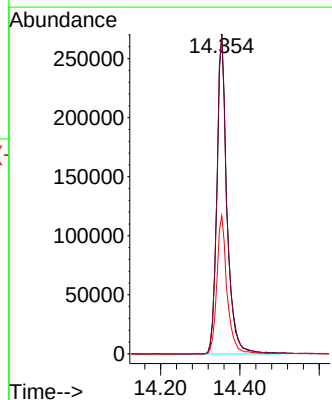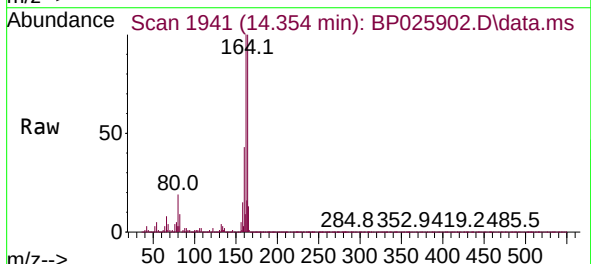

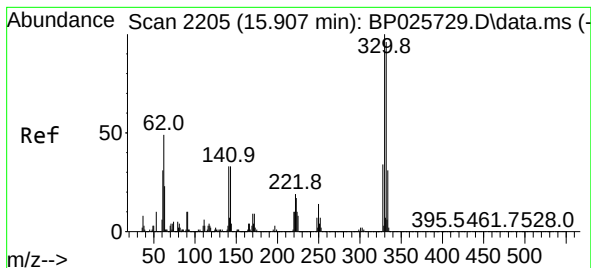

#42

2,4,6-Tribromophenol

Concen: 153.306 ng

RT: 15.872 min Scan# 21

Delta R.T. -0.035 min

Lab File: BP025902.D

Acq: 01 Oct 2025 15:49

Instrument :

BNA_P

ClientSampleId :

PB169936BL





Tgt Ion:330 Resp: 908244

Ion Ratio Lower Upper

330 100

332 97.9 76.9 115.3

141 33.3 31.0 46.4

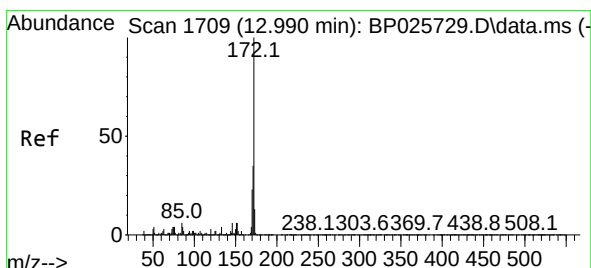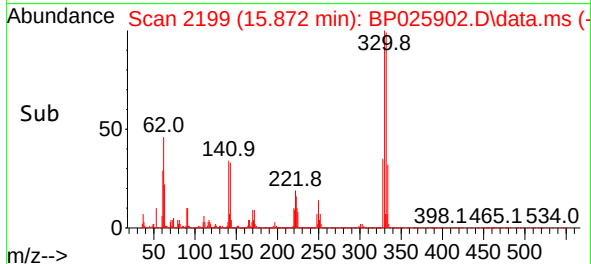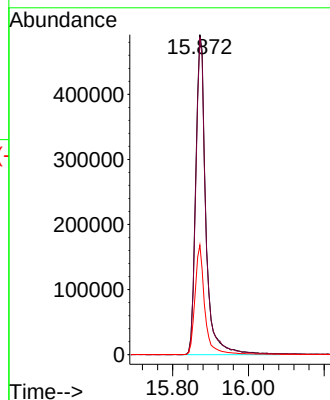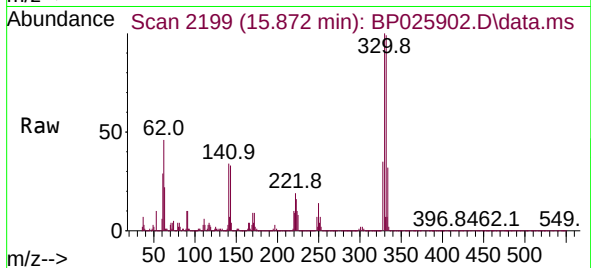

#45

2-Fluorobiphenyl

Concen: 89.914 ng

RT: 12.960 min Scan# 1704

Delta R.T. -0.029 min

Lab File: BP025902.D

Acq: 01 Oct 2025 15:49




Tgt Ion:172 Resp: 3207426


Ion Ratio Lower Upper

172 100

171 34.6 27.8 41.6

170 22.7 18.6 27.8

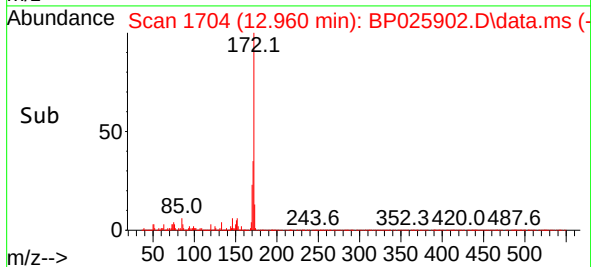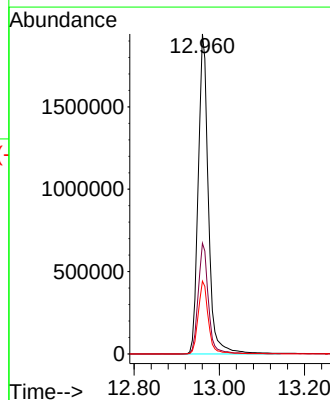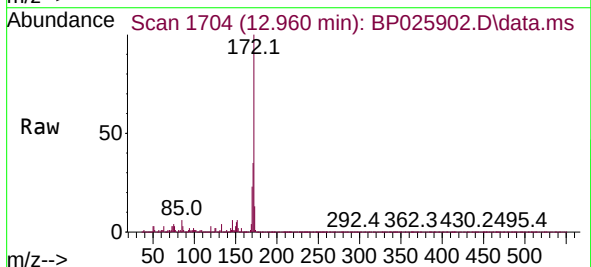



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.160 min Scan# 24

Delta R.T. -0.024 min

Lab File: BP025902.D

Acq: 01 Oct 2025 15:49

Instrument :

BNA_P

ClientSampleId :

PB169936BL





Tgt Ion:188 Resp: 939544

Ion Ratio Lower Upper

188 100

94 9.1 7.4 11.0

80 10.0 7.7 11.5

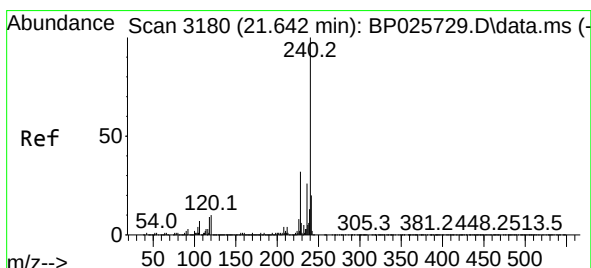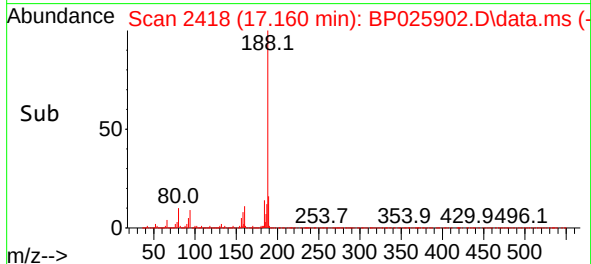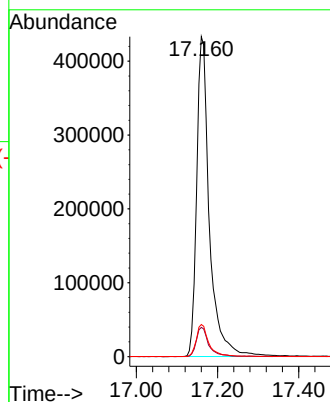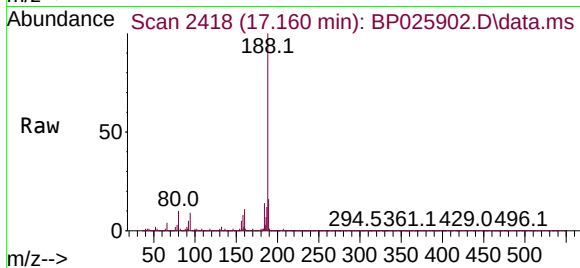

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.613 min Scan# 3175

Delta R.T. -0.029 min

Lab File: BP025902.D

Acq: 01 Oct 2025 15:49




Tgt Ion:240 Resp: 929664


Ion Ratio Lower Upper

240 100

120 9.5 8.0 12.0

236 25.0 20.7 31.1


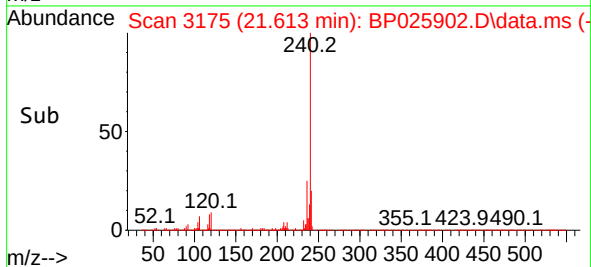
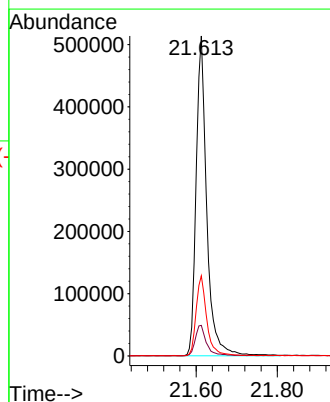
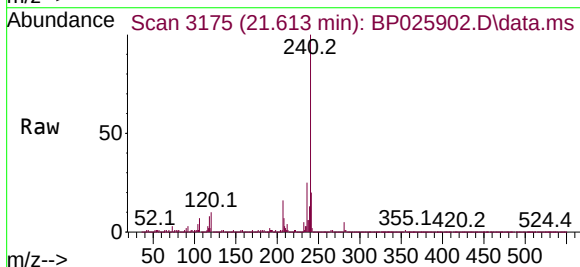




#79
 Terphenyl-d14
 Concen: 93.429 ng
 RT: 19.877 min Scan# 2886
 Delta R.T. -0.035 min
 Lab File: BP025902.D
 Acq: 01 Oct 2025 15:49

Instrument :
 BNA_P
 ClientSampleId :
 PB169936BL

Tgt Ion:244 Resp: 4828161
 Ion Ratio Lower Upper
 244 100
 212 7.2 5.9 8.9
 122 9.0 7.1 10.7

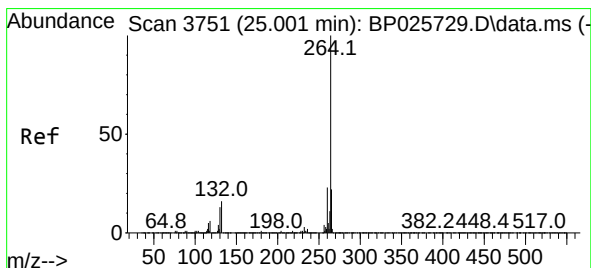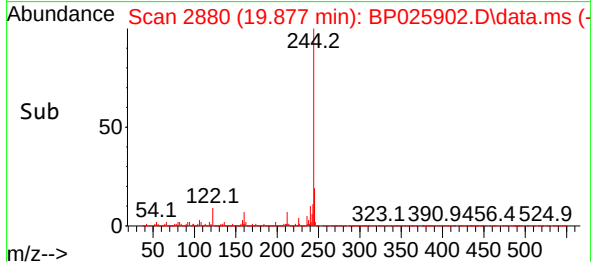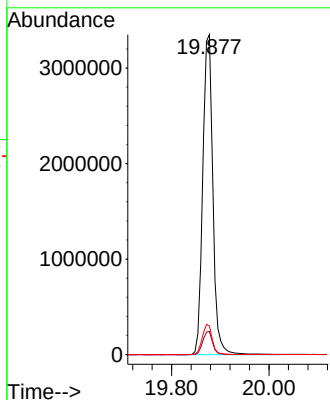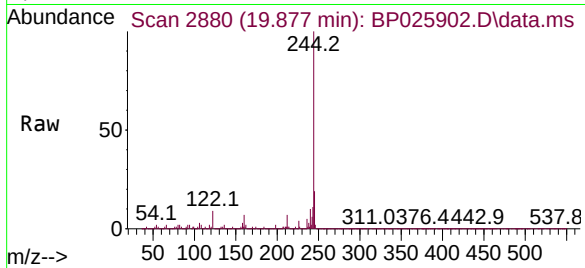

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.960 min Scan# 3744
 Delta R.T. -0.041 min
 Lab File: BP025902.D
 Acq: 01 Oct 2025 15:49

Tgt Ion:264 Resp: 989236
 Ion Ratio Lower Upper
 264 100
 260 22.6 18.3 27.5
 265 22.6 17.3 25.9

