

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100625\
 Data File : PS031954.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2025 10:15
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 03:00:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 09 13:56:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.286	7.747	1611.8E6	411.2E6	447.529	452.416
Target Compounds							
1) T	Dalapon	0.000	2.648f	0	54137765	N.D.	19.214
2) T	3,5-DICHL...	6.452	0.000	356840	0	<MDL	N.D. #
3) T	4-Nitroph...	7.082	0.000	4425161	0	4.011	N.D. #
7) T	MCPA	7.812	0.000	1129675	0	<MDL	N.D. #
8) T	DICHLORPROP	8.177	0.000	117531	0	<MDL	N.D. #
10) T	Pentachlo...	8.707	9.512	9057846	4424356	<MDL	<MDL #
11) T	2,4,5-TP ...	9.303	9.920f	4472258	1649274	<MDL	<MDL #
12) T	2,4,5-T	9.598	0.000	2272623	0	<MDL	N.D. #
13) T	2,4-DB	10.162	0.000	500114	0	<MDL	N.D. #
14) T	DINOSEB	11.348	0.000	8074532	0	<MDL	N.D. #
15) T	Picloram	11.179	0.000	1867745	0	<MDL	N.D. #
16) T	DCPA	11.651	12.308	5815555	2035617	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100625\
Data File : PS031954.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2025 10:15
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 03:00:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
Quant Title : 8080.M
QLast Update : Tue Sep 09 13:56:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

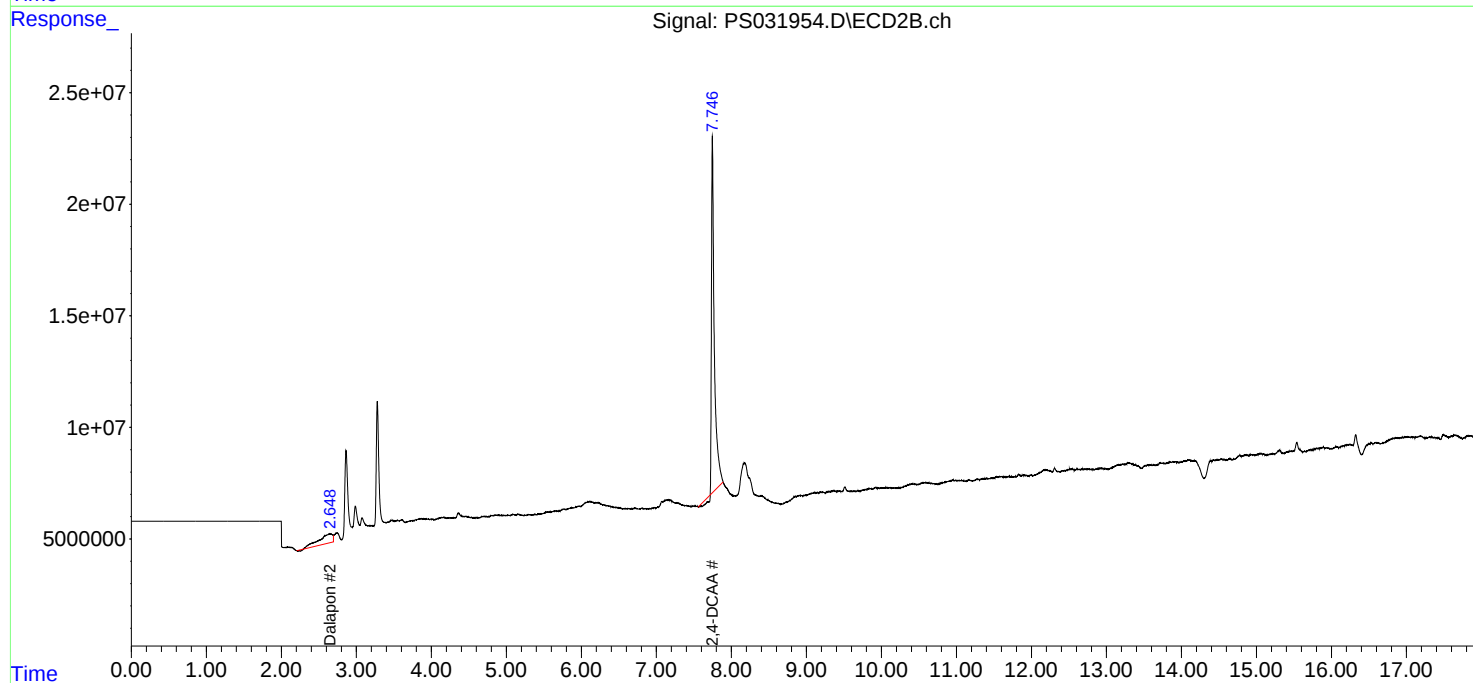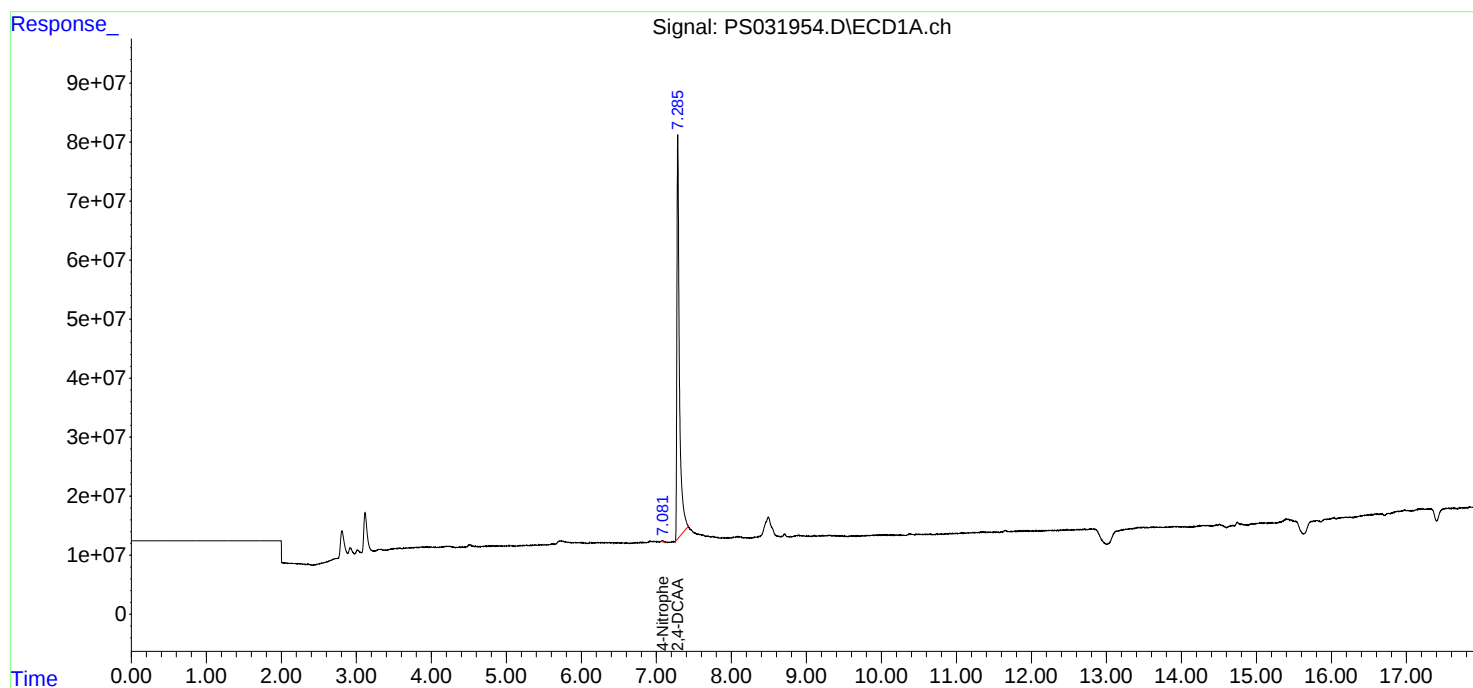


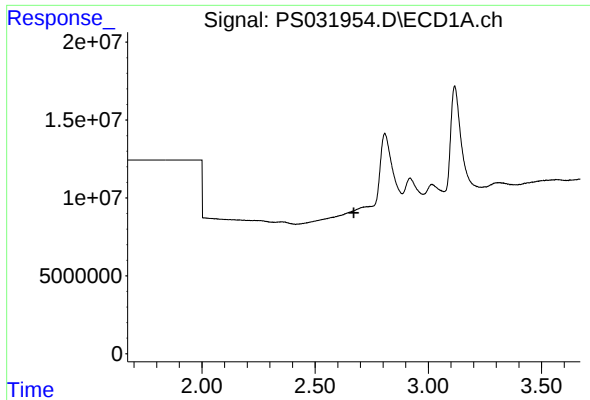

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

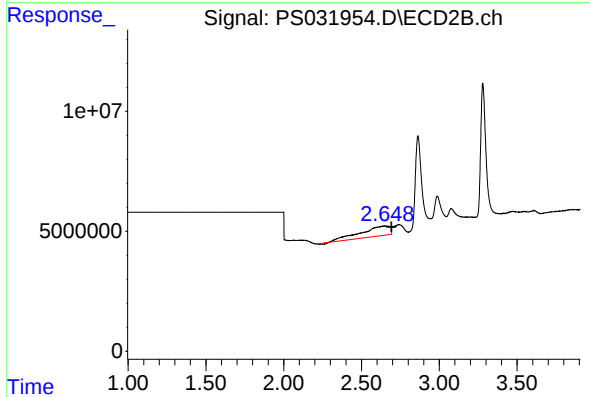


#1 Dalapon

R.T.: 2.648 min
Delta R.T.: -0.043 min
Response: 54137765
Conc: 19.21 ng/ml

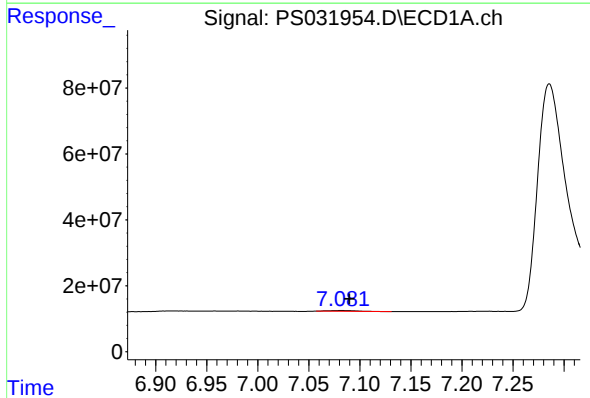


#3 4-Nitrophenol

R.T.: 7.082 min
Delta R.T.: -0.008 min
Response: 4425161
Conc: 4.01 ng/ml

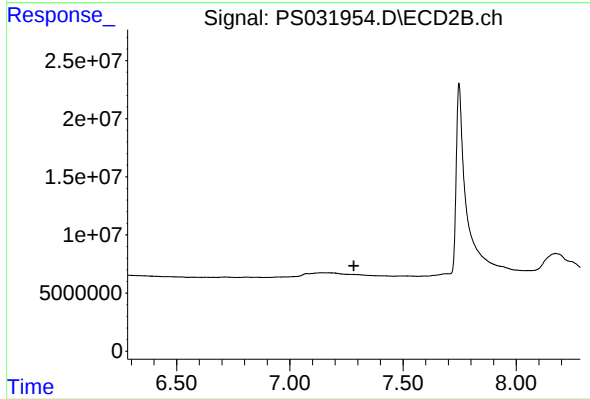

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.283 min
Response: 0
Conc: N.D.

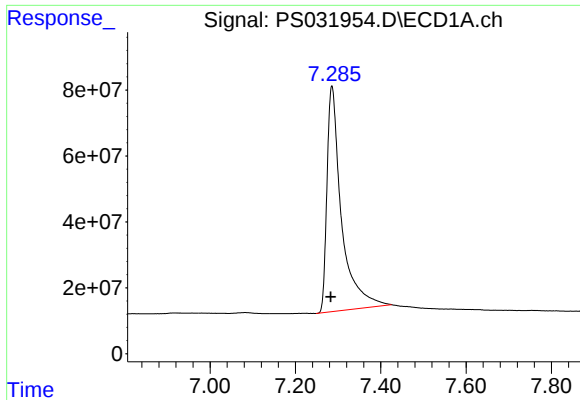

#4 2,4-DCAA

R.T.: 7.286 min
Delta R.T.: 0.002 min
Response: 1611788723
Conc: 447.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

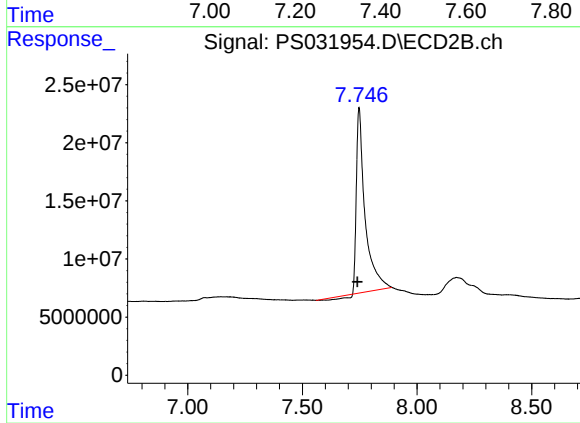

#4 2,4-DCAA

R.T.: 7.747 min
Delta R.T.: 0.007 min
Response: 411200553
Conc: 452.42 ng/ml