

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100225\
 Data File : PL097501.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2025 15:09
 Operator : AR\AJ
 Sample : Q3266-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ENV-3-6FT

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/03/2025
 Supervised By : mohammad ahmed 10/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 04:59:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.524	2.823	52875054	72910491	11.680m	11.088
28) SA Decachlor...	8.991	7.979	52452923	45975068	16.030m	8.078 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100225\
Data File : PL097501.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2025 15:09
Operator : AR\AJ
Sample : Q3266-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
ENV-3-6FT


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/03/2025
Supervised By : mohammad ahmed 10/04/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 04:59:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

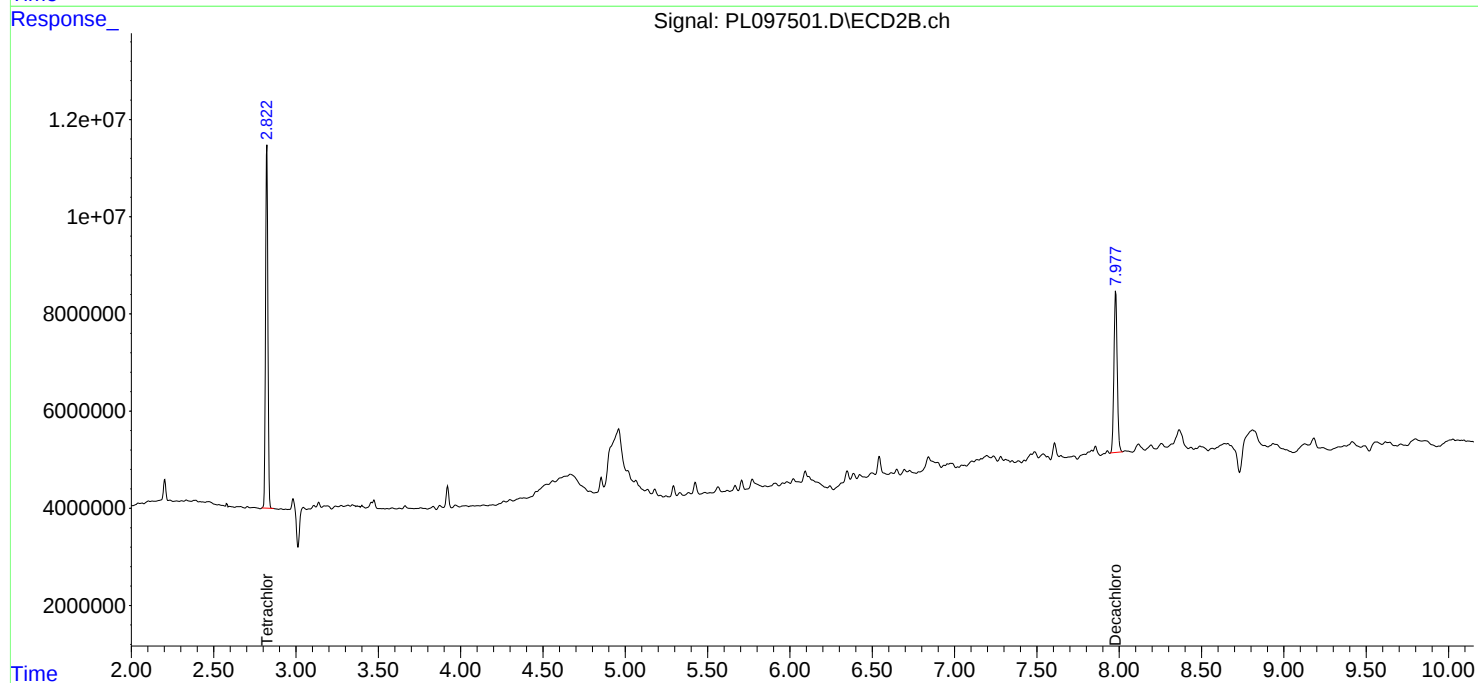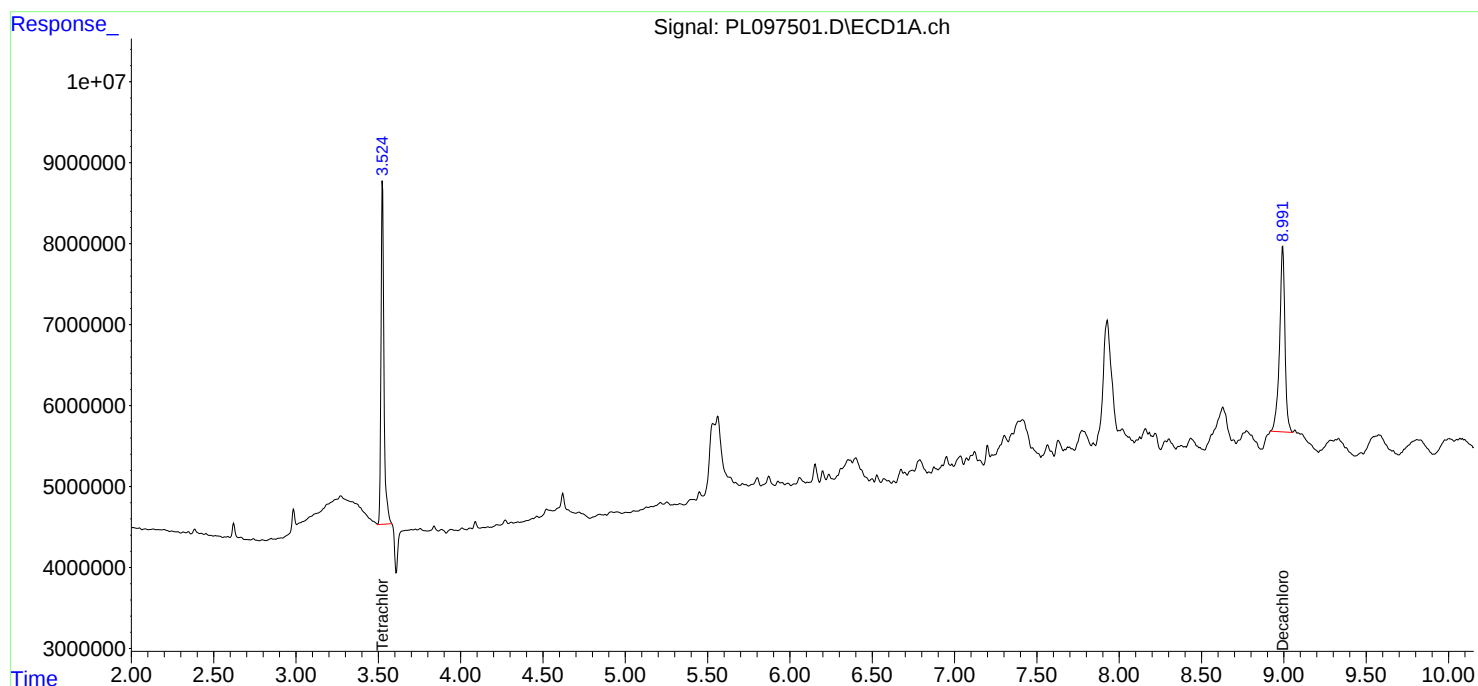

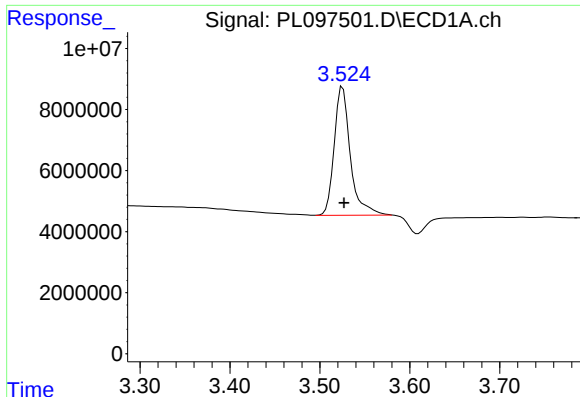


#1 Tetrachloro-m-xylene

R.T.: 3.524 min
Delta R.T.: -0.003 min
Response: 52875054
Conc: 11.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
ENV-3-6FT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/03/2025
Supervised By :mohammad ahmed 10/04/2025

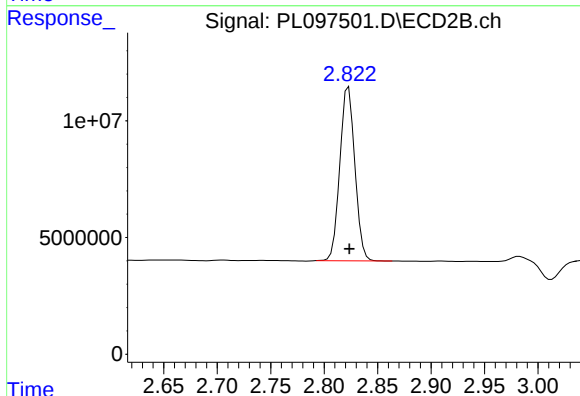


#1 Tetrachloro-m-xylene

R.T.: 2.823 min
Delta R.T.: 0.000 min
Response: 72910491
Conc: 11.09 ng/ml

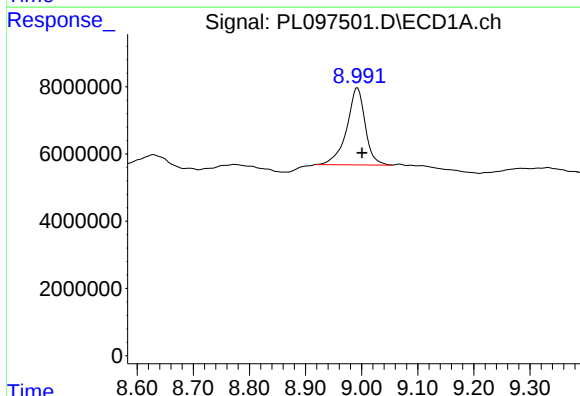

#28 Decachlorobiphenyl

R.T.: 8.991 min
Delta R.T.: -0.010 min
Response: 52452923
Conc: 16.03 ng/ml m

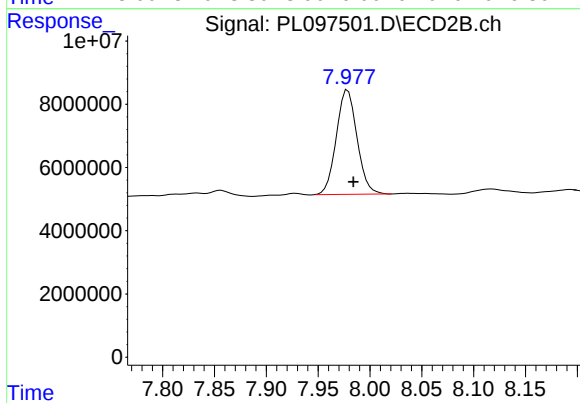

#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.005 min
Response: 45975068
Conc: 8.08 ng/ml