

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100225\
 Data File : PL097502.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2025 15:23
 Operator : AR\AJ
 Sample : Q3266-01MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ENV-4-6FT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 04:59:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.525	2.823	72988997	76701057	16.122	11.665 #
28)	SA Decachlor...	8.995	7.979	36142283	55810878	11.045	9.806
Target Compounds							
9)	A Endosulfan I	0.000	5.180f	0	10541100	N.D.	1.372 #
10)	B gamma-Chl...	0.000	5.017f	0	13231335	N.D.	1.515 #
12)	B 4,4'-DDE	6.152	5.293	10573543	11232402	2.219	1.462 #
13)	MA Dieldrin	0.000	5.426	0	15382746	N.D.	1.881 #
14)	MA Endrin	0.000	5.708	0	3169072	N.D.	0.422 #
15)	B Endosulfa...	0.000	5.984	0	8543196	N.D.	1.202 #
16)	A 4,4'-DDD	6.676	0.000	10123314	0	2.685	N.D. #
17)	MA 4,4'-DDT	6.975	6.095	8298131	22545733	1.963	3.258 #
20)	A Methoxychlor	0.000	6.697f	0	10932469	N.D.	2.900 #
25)	Chlordane-3	0.000	5.017f	0	13231335	N.D.	14.797 #
27)	Chlordane-5	0.000	5.984f	0	8543196	N.D.	28.655 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100225\
Data File : PL097502.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2025 15:23
Operator : AR\AJ
Sample : Q3266-01MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ENV-4-6FT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 04:59:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

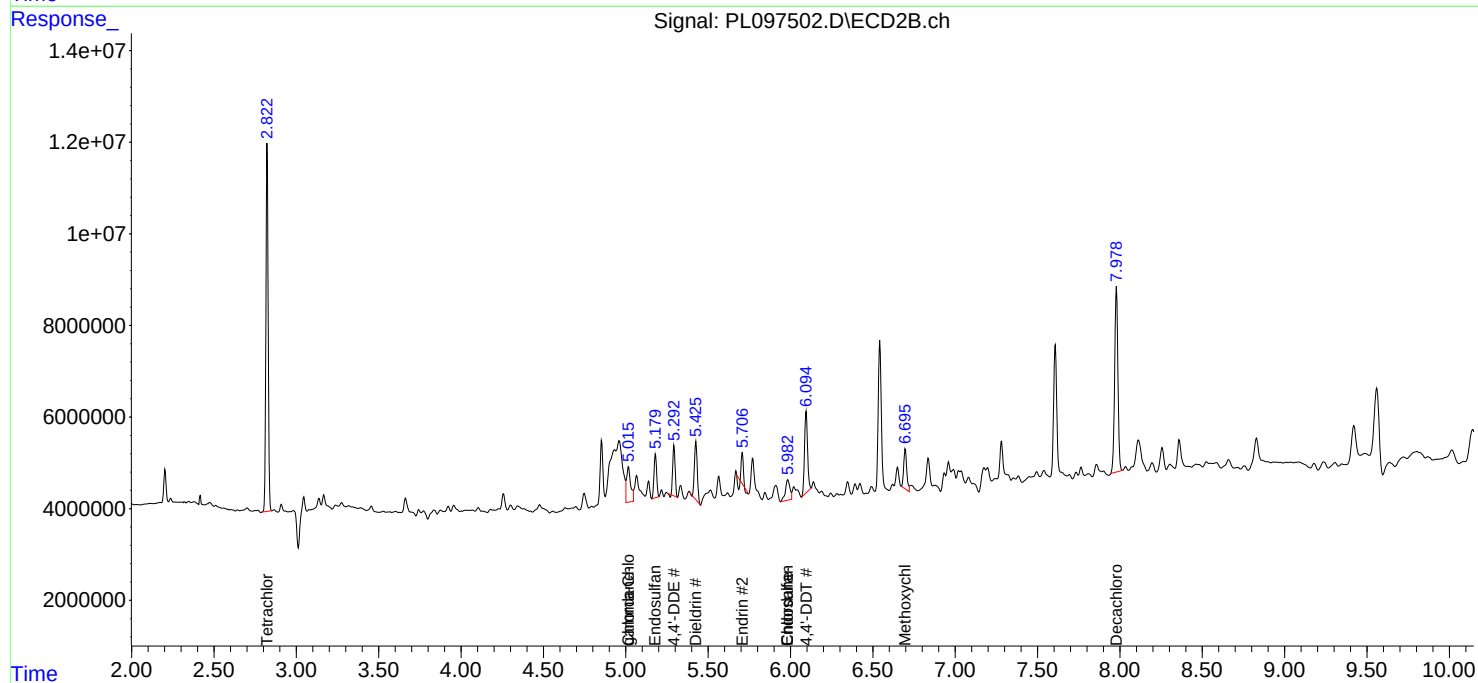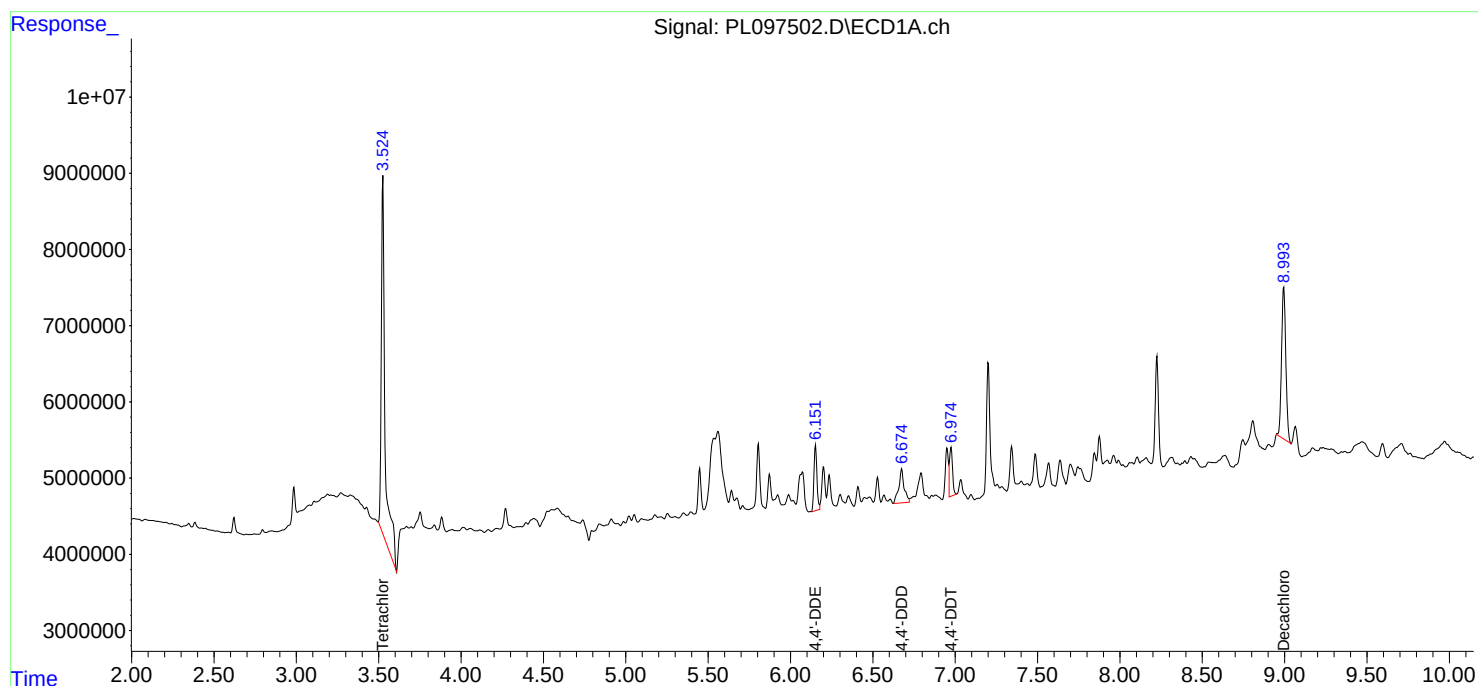


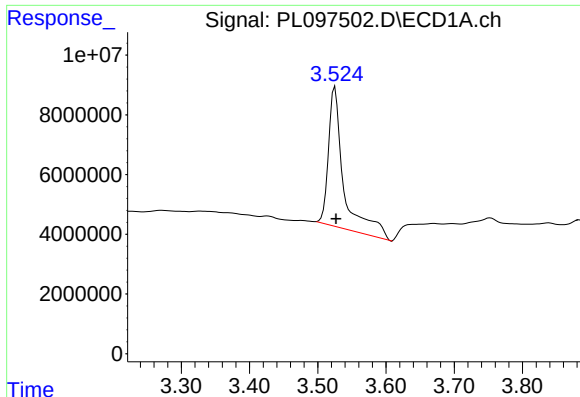

#1 Tetrachloro-m-xylene


R.T.: 3.525 min
Delta R.T.: -0.002 min
Response: 72988997
Conc: 16.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
ENV-4-6FT

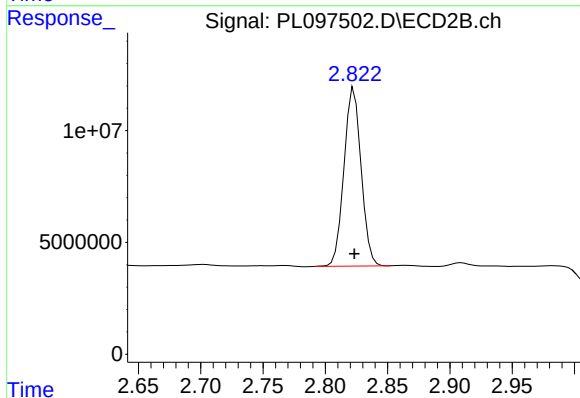


#1 Tetrachloro-m-xylene

R.T.: 2.823 min
Delta R.T.: 0.000 min
Response: 76701057
Conc: 11.66 ng/ml

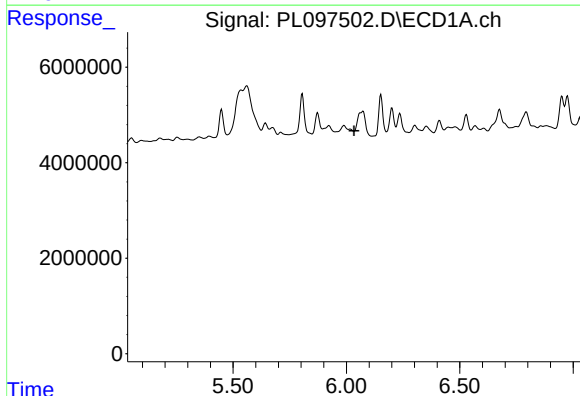


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.033 min
Response: 0
Conc: N.D.

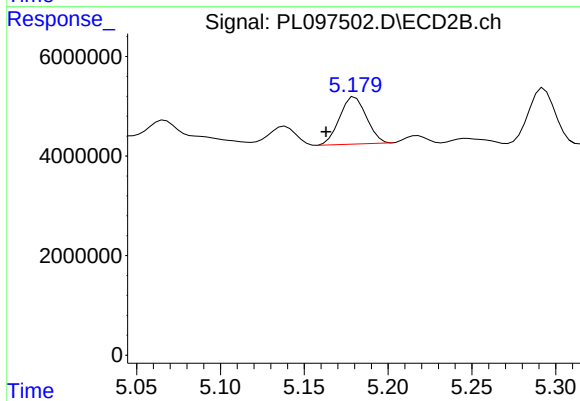

#9 Endosulfan I


R.T.: 5.180 min
Delta R.T.: 0.017 min
Response: 10541100
Conc: 1.37 ng/ml

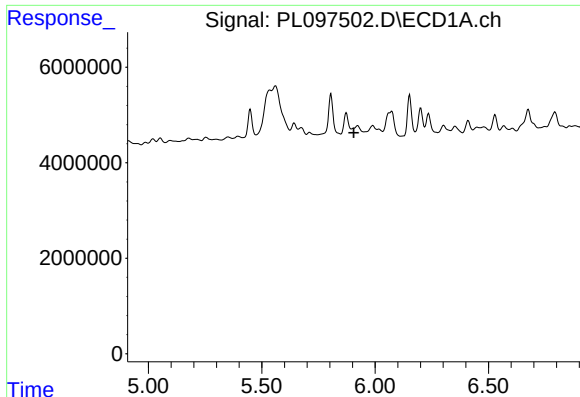

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.905 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
ENV-4-6FT

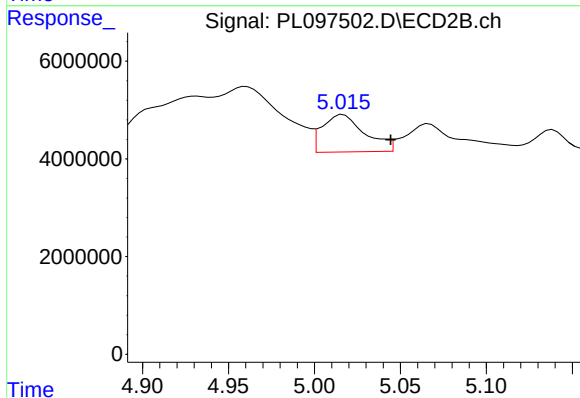


#10 gamma-Chlordane

R.T.: 5.017 min
Delta R.T.: -0.028 min
Response: 13231335
Conc: 1.51 ng/ml

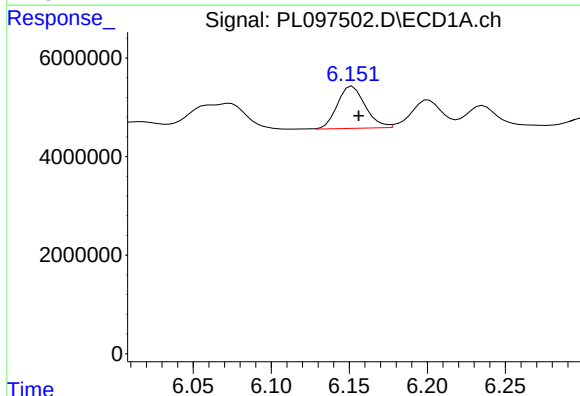


#12 4,4'-DDE

R.T.: 6.152 min
Delta R.T.: -0.004 min
Response: 10573543
Conc: 2.22 ng/ml

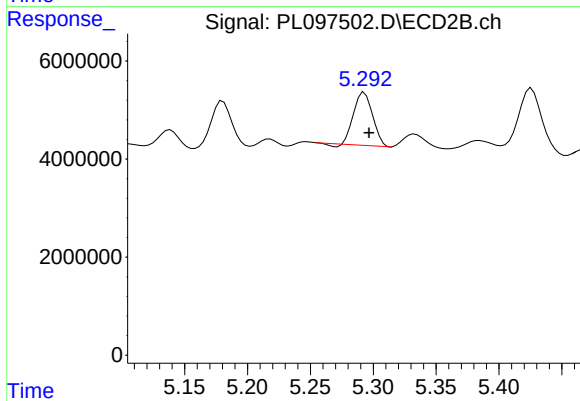

#12 4,4'-DDE


R.T.: 5.293 min
Delta R.T.: -0.004 min
Response: 11232402
Conc: 1.46 ng/ml

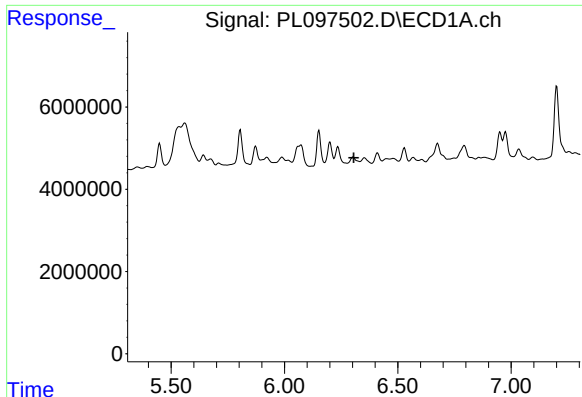

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.306 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
ENV-4-6FT

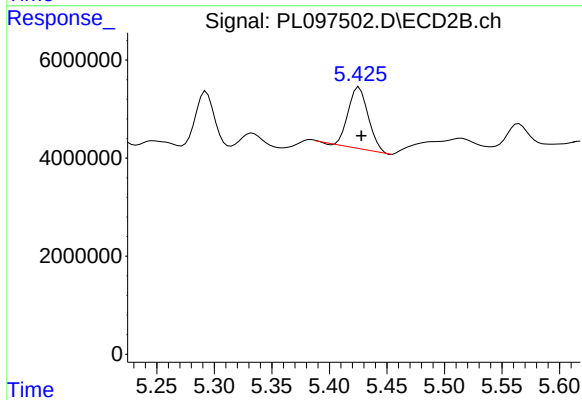


#13 Dieldrin

R.T.: 5.426 min
Delta R.T.: -0.002 min
Response: 15382746
Conc: 1.88 ng/ml

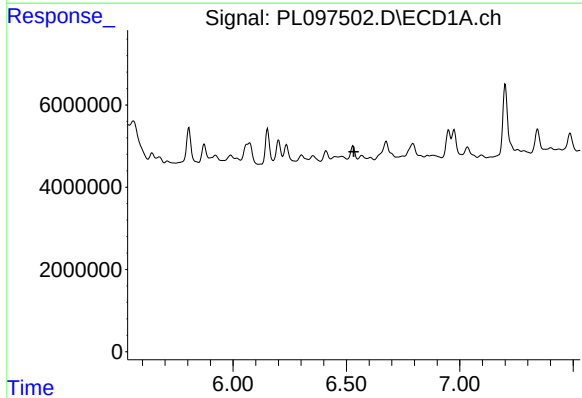


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.532 min
Response: 0
Conc: N.D.

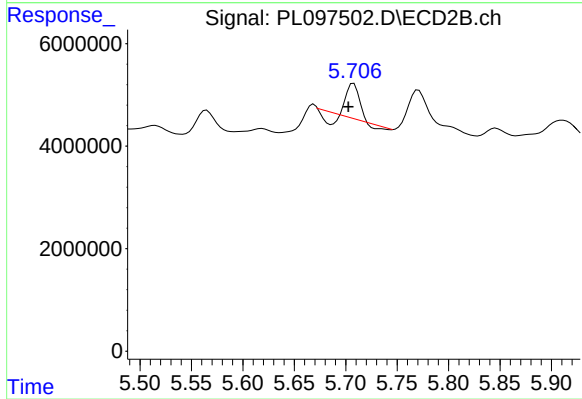

#14 Endrin


R.T.: 5.708 min
Delta R.T.: 0.005 min
Response: 3169072
Conc: 0.42 ng/ml

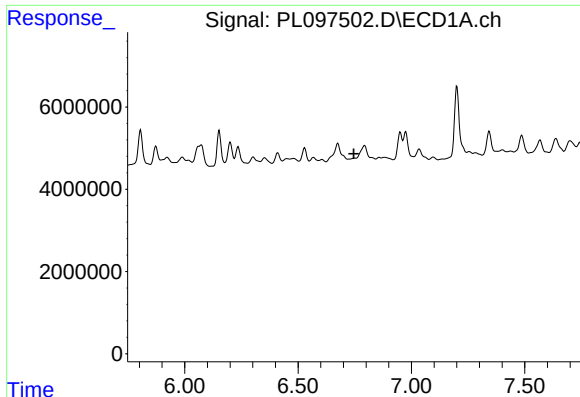

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.745 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
ENV-4-6FT

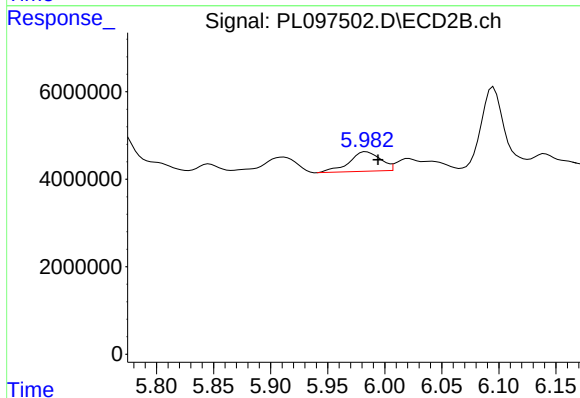


#15 Endosulfan II

R.T.: 5.984 min
Delta R.T.: -0.011 min
Response: 8543196
Conc: 1.20 ng/ml

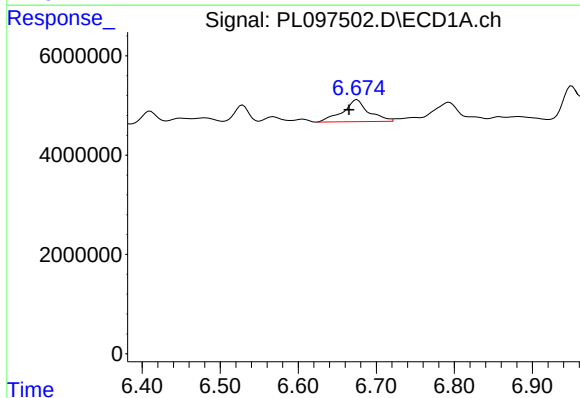


#16 4,4'-DDD

R.T.: 6.676 min
Delta R.T.: 0.011 min
Response: 10123314
Conc: 2.68 ng/ml

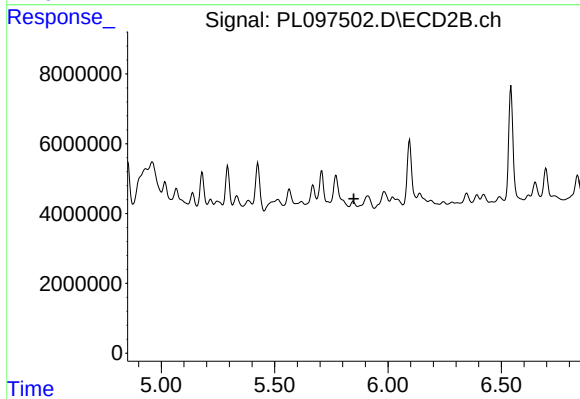

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.850 min
Response: 0
Conc: N.D.

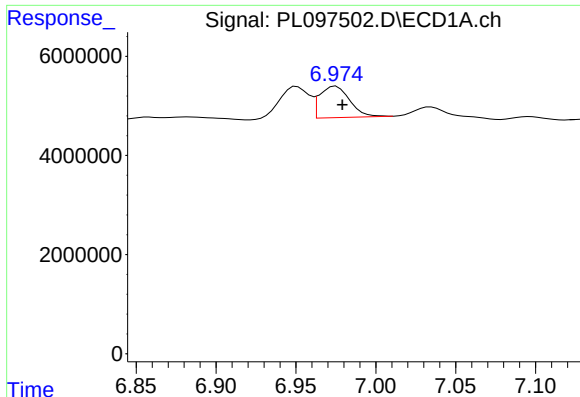

#17 4,4'-DDT


R.T.: 6.975 min
Delta R.T.: -0.004 min
Response: 8298131
Conc: 1.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
ENV-4-6FT

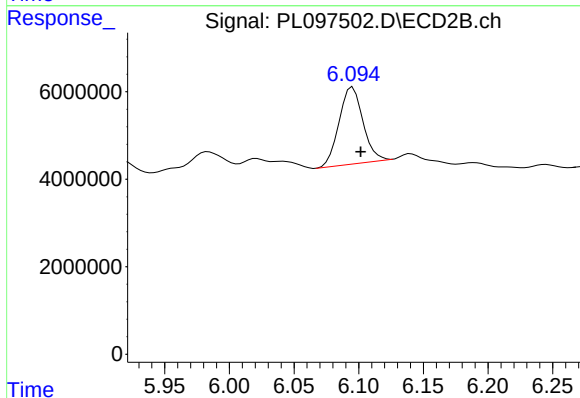


#17 4,4'-DDT

R.T.: 6.095 min
Delta R.T.: -0.006 min
Response: 22545733
Conc: 3.26 ng/ml

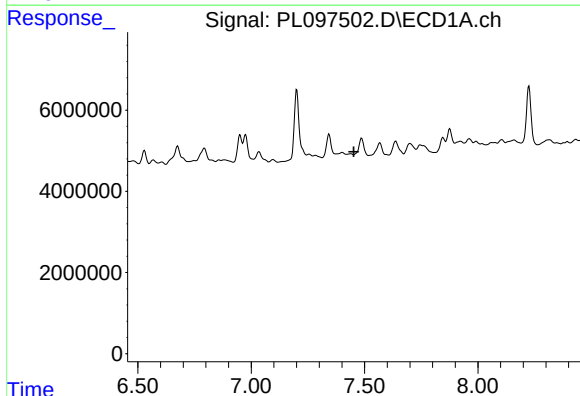


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.452 min
Response: 0
Conc: N.D.

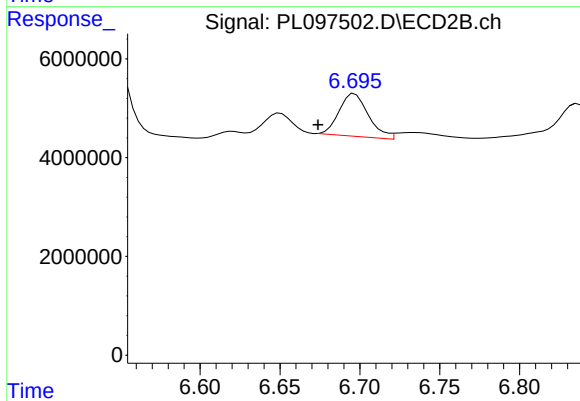

#20 Methoxychlor


R.T.: 6.697 min
Delta R.T.: 0.023 min
Response: 10932469
Conc: 2.90 ng/ml

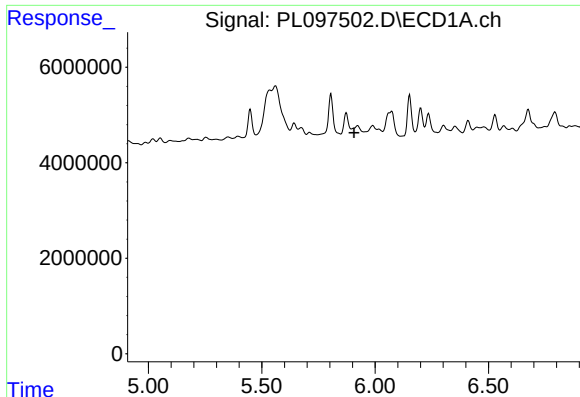

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.907 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
ENV-4-6FT

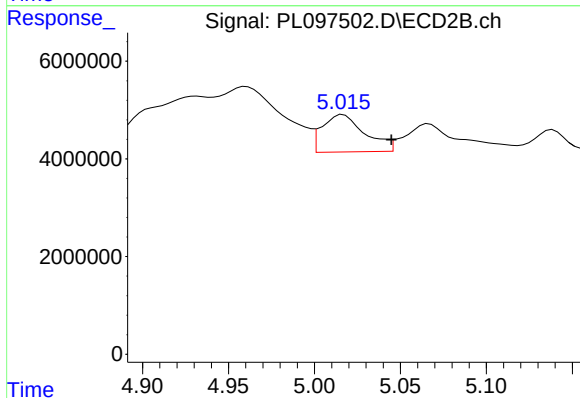


#25 Chlordane-3

R.T.: 5.017 min
Delta R.T.: -0.028 min
Response: 13231335
Conc: 14.80 ng/ml

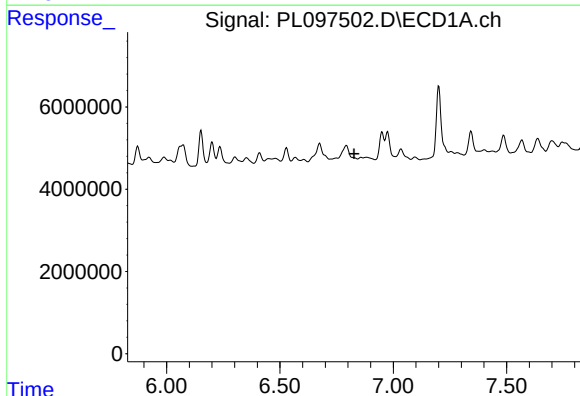


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.828 min
Response: 0
Conc: N.D.

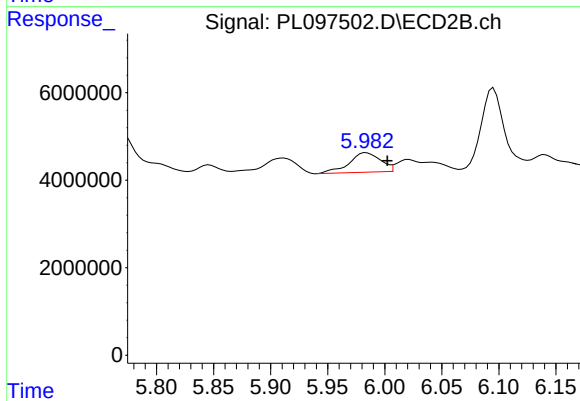

#27 Chlordane-5


R.T.: 5.984 min
Delta R.T.: -0.019 min
Response: 8543196
Conc: 28.65 ng/ml

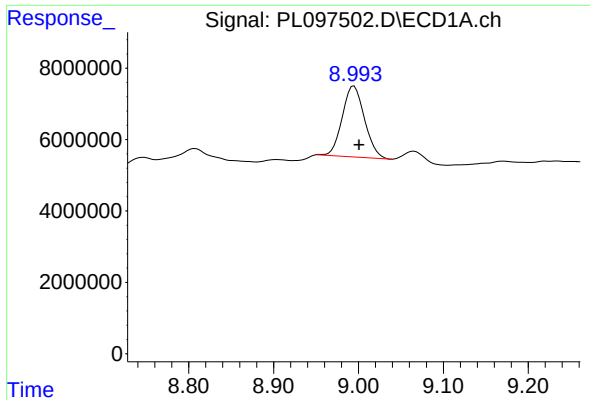

#28 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: -0.006 min
Response: 36142283
Conc: 11.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
ENV-4-6FT

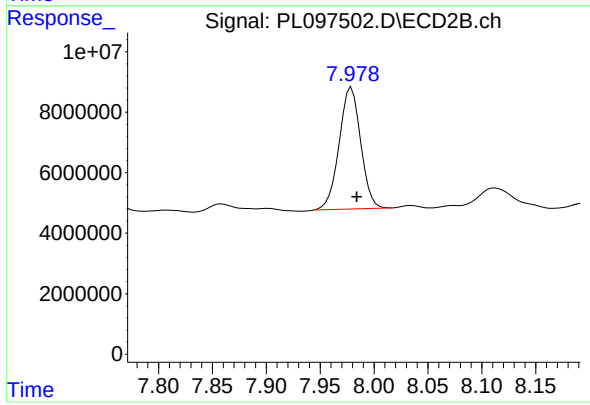

#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.005 min
Response: 55810878
Conc: 9.81 ng/ml